

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072020\
 Data File : PL060038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2020 16:30
 Operator : DD\AJ
 Sample : PB130316BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB130316BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 01:22:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.465	4.012	41030040	57285290	21.213	21.615
28) SA Decachlor...	8.225	9.102	36050352	44526072	21.914	21.290
Target Compounds						
4) MA Heptachlor	0.000	5.204	0	44883	N.D.	0.013 #
9) A Endosulfan I	0.000	6.245	0	9191332	N.D.	3.446 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072020\
Data File : PL060038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2020 16:30
Operator : DD\AJ
Sample : PB130316BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB130316BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 01:22:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

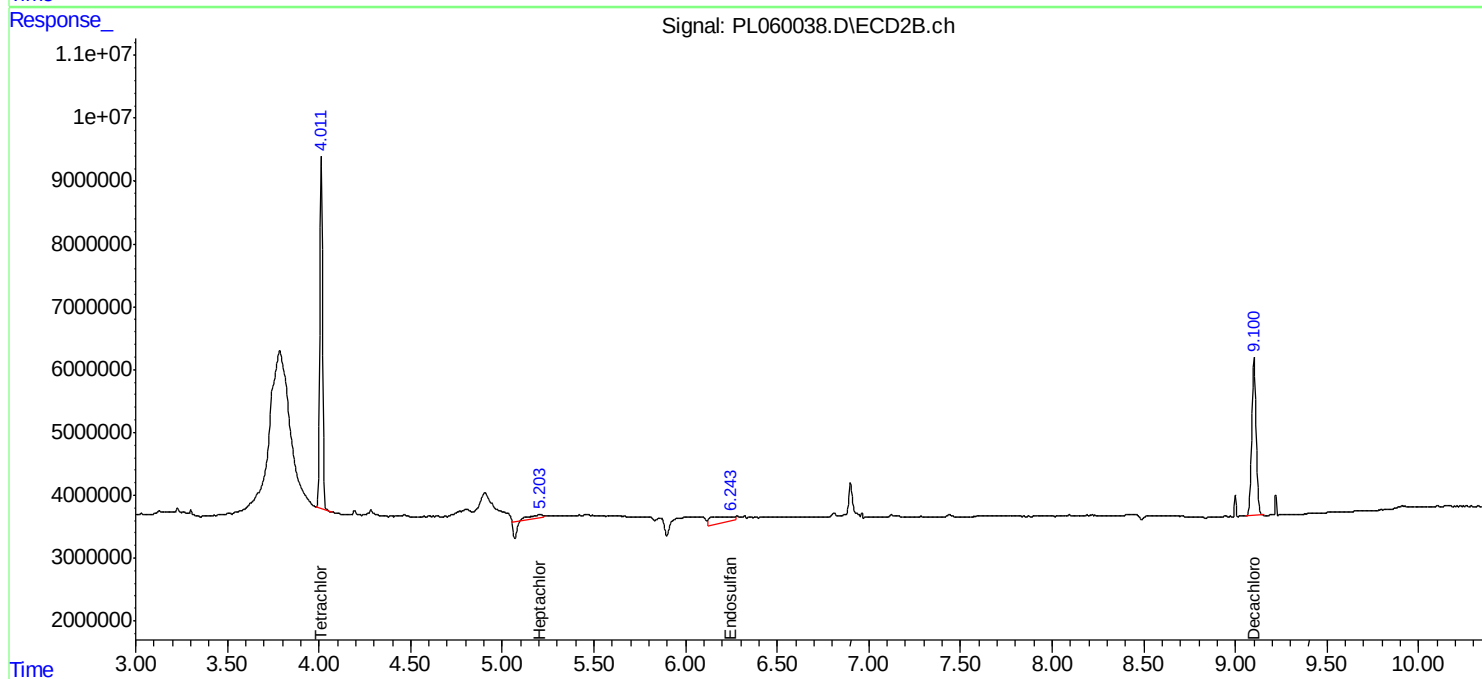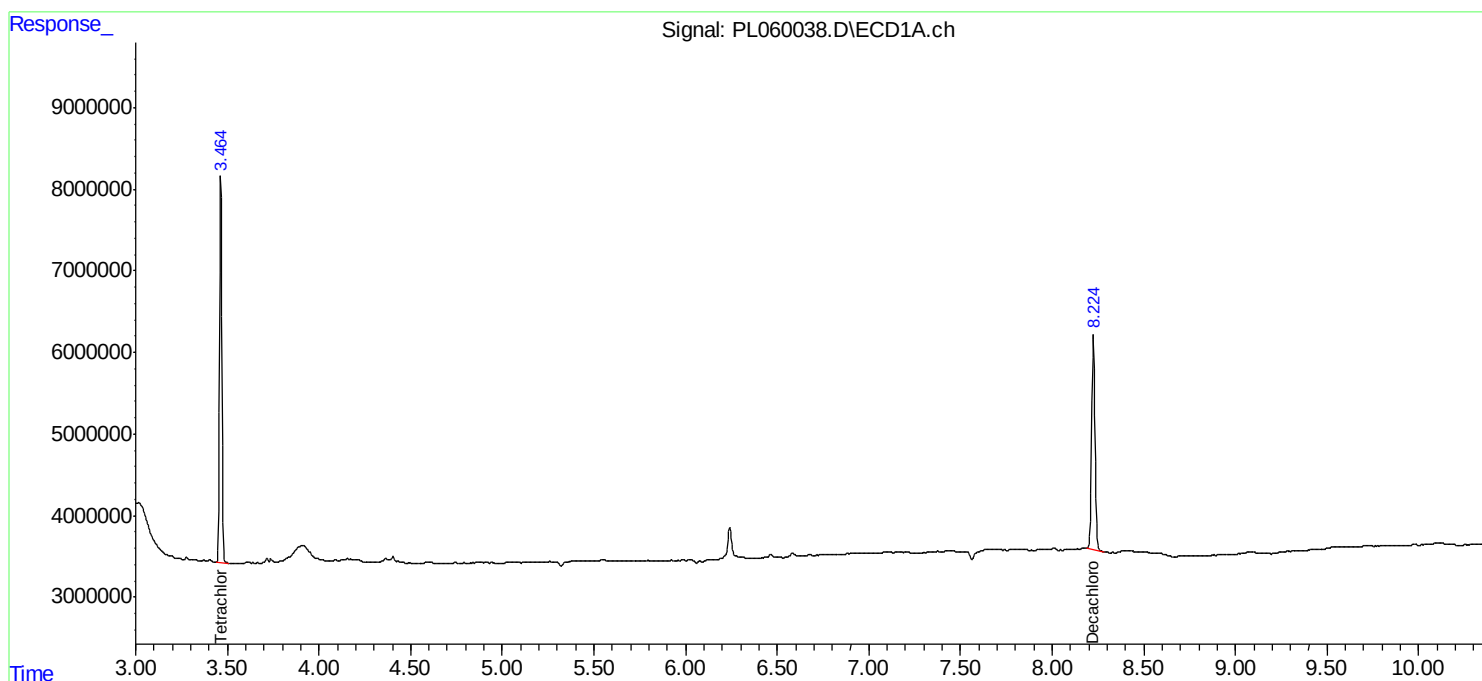


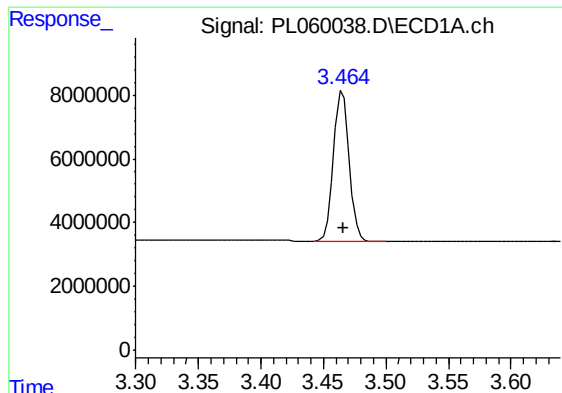

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 41030040
Conc: 21.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB130316BL

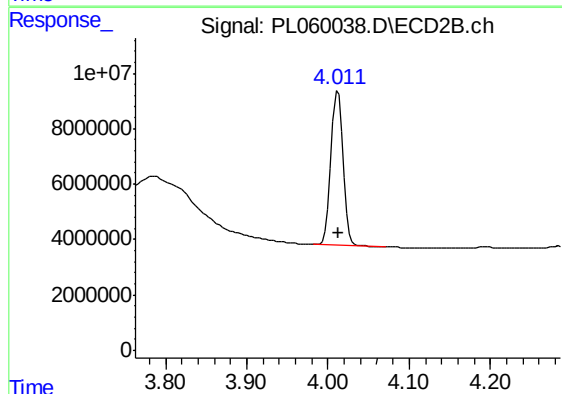


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 57285290
Conc: 21.62 ng/ml

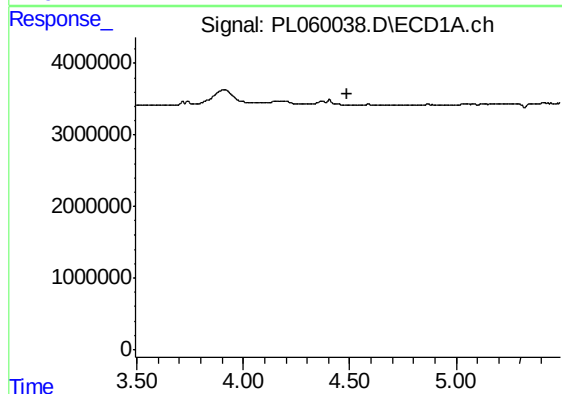


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

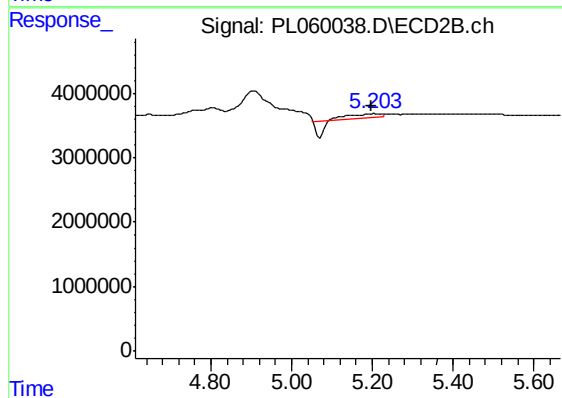

#4 Heptachlor


R.T.: 5.204 min
Delta R.T.: 0.006 min
Response: 44883
Conc: 0.01 ng/ml

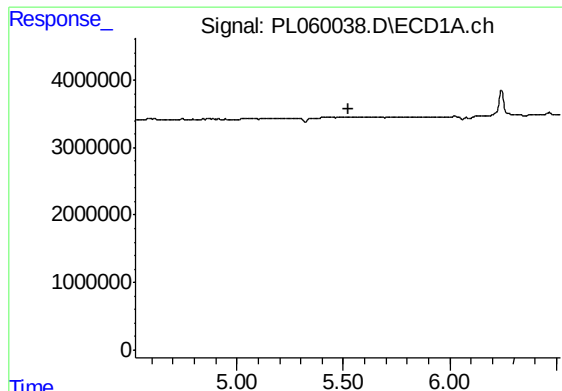

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB130316BL

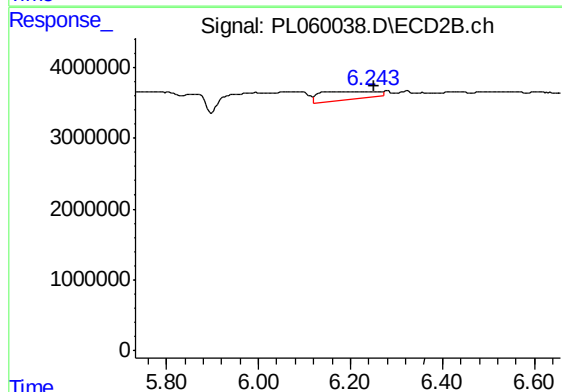


#9 Endosulfan I

R.T.: 6.245 min
Delta R.T.: -0.005 min
Response: 9191332
Conc: 3.45 ng/ml

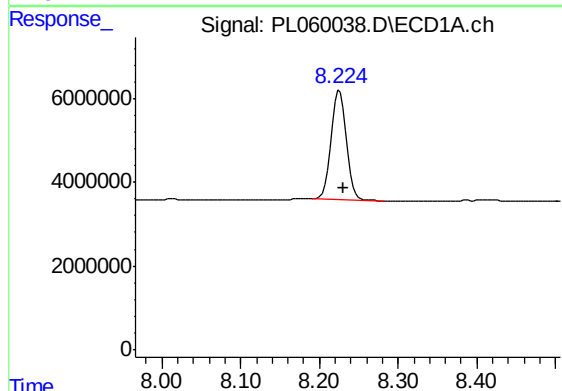

#28 Decachlorobiphenyl

R.T.: 8.225 min
Delta R.T.: -0.006 min
Response: 36050352
Conc: 21.91 ng/ml

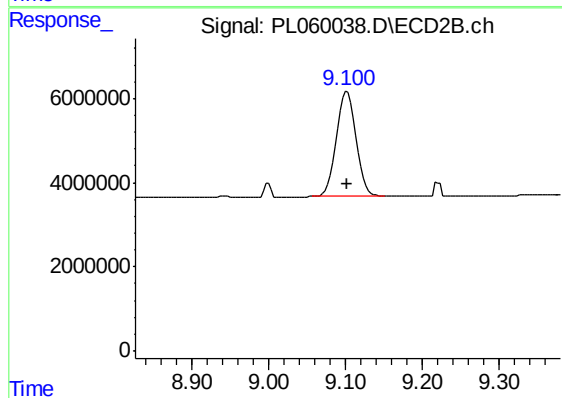

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: -0.001 min
Response: 44526072
Conc: 21.29 ng/ml