

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072020\
 Data File : PL060040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2020 16:58
 Operator : DD\AJ
 Sample : PB130316TB
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB130316TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 01:23:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.013	42285591	59320947	21.862	22.384
28)	SA Decachlor...	8.226	9.101	35551821	44244833	21.611	21.156
Target Compounds							
4)	MA Heptachlor	0.000	5.205	0	5872821	N.D.	1.746 #
9)	A Endosulfan I	0.000	6.256	0	1917633	N.D.	0.719 #
11)	B alpha-Chl...	0.000	6.199	0	1169559	N.D.	0.409 #
22)	Mirex	0.000	8.191f	0	688832	N.D.	0.373 #
26)	Chlordane-4	0.000	6.199	0	1169559	N.D.	2.527 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072020\
Data File : PL060040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2020 16:58
Operator : DD\AJ
Sample : PB130316TB
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB130316TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 01:23:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

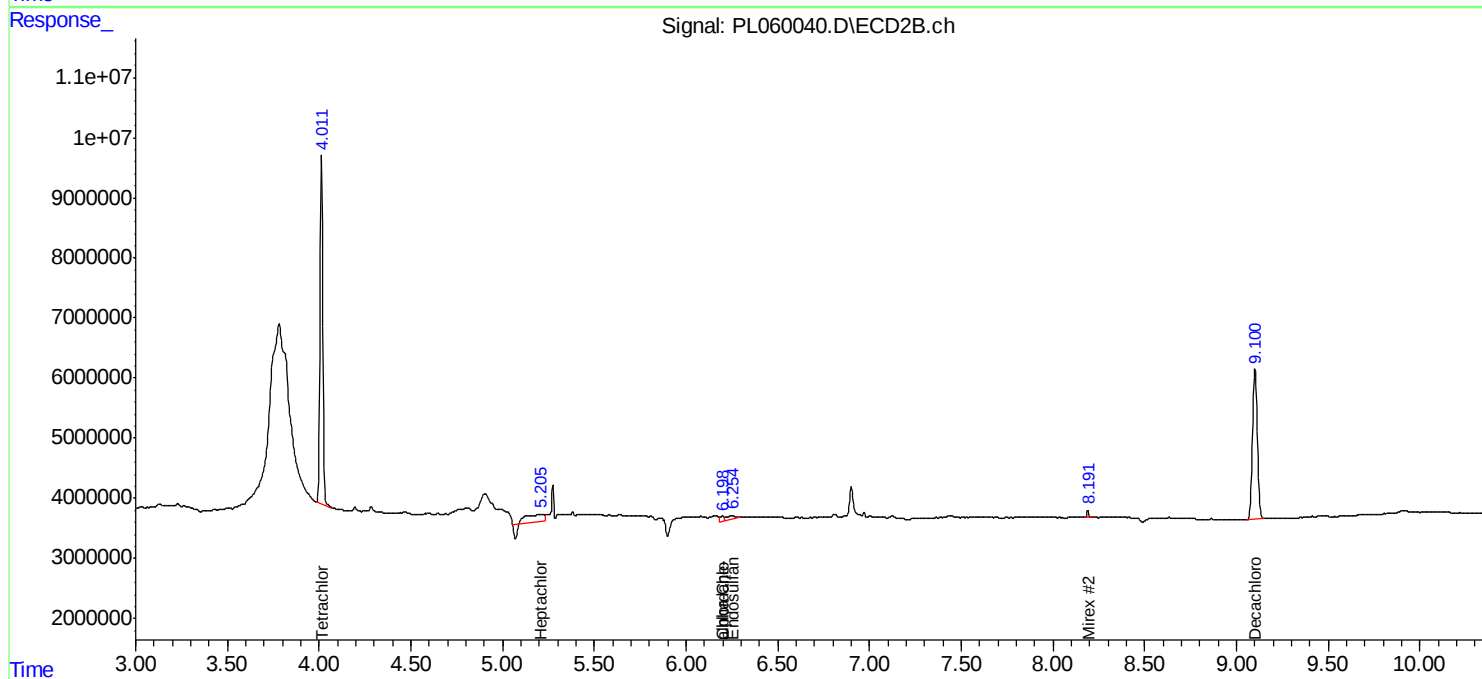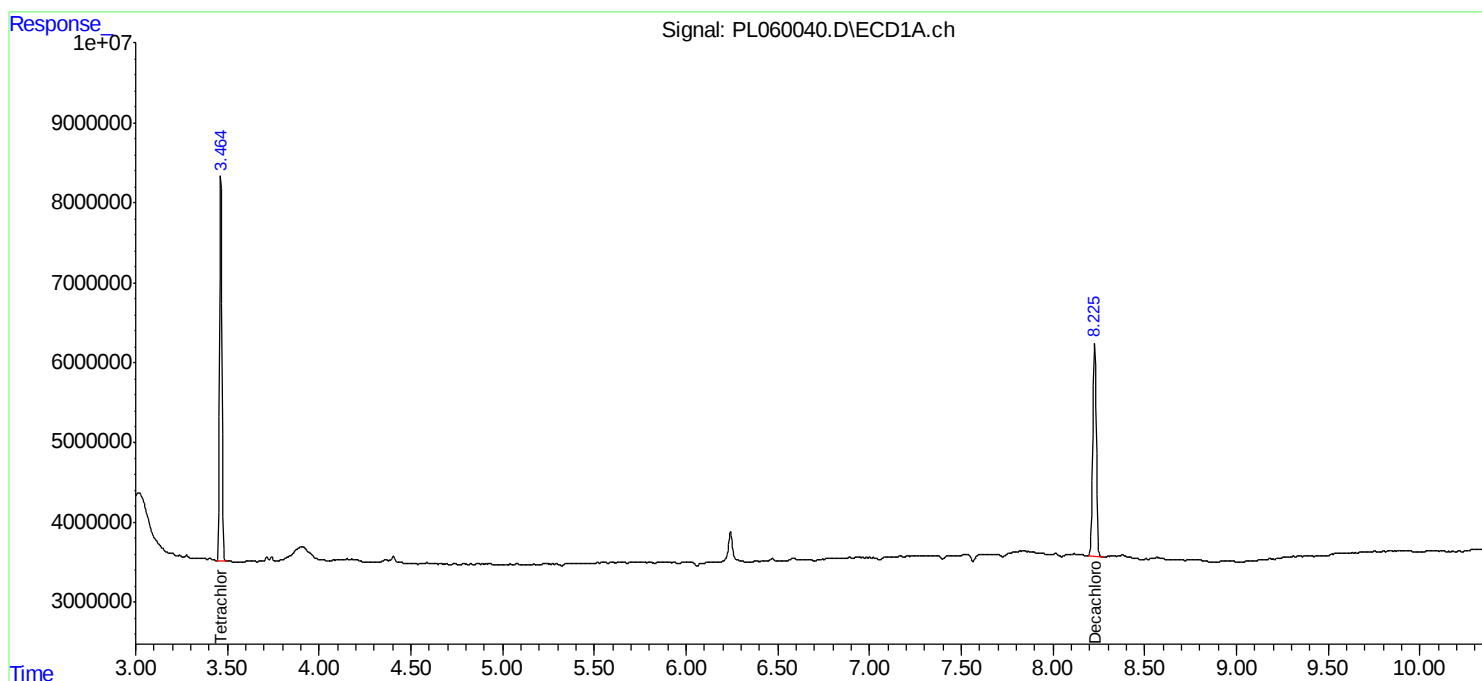


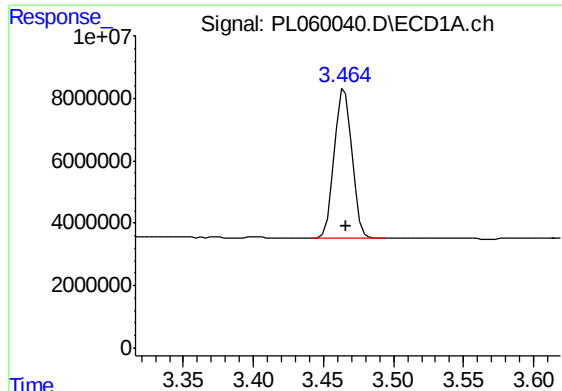

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 42285591
Conc: 21.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB130316TB

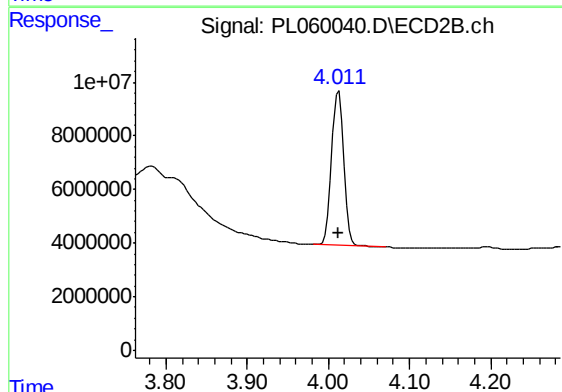


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 59320947
Conc: 22.38 ng/ml

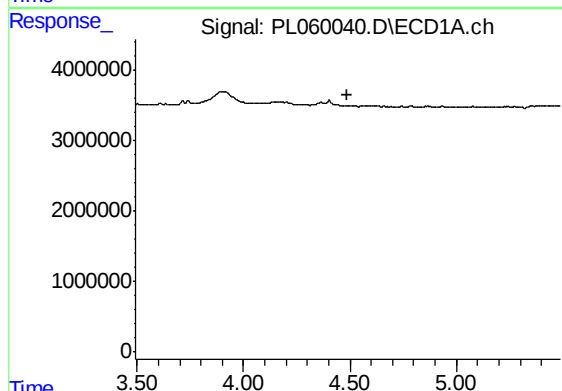


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

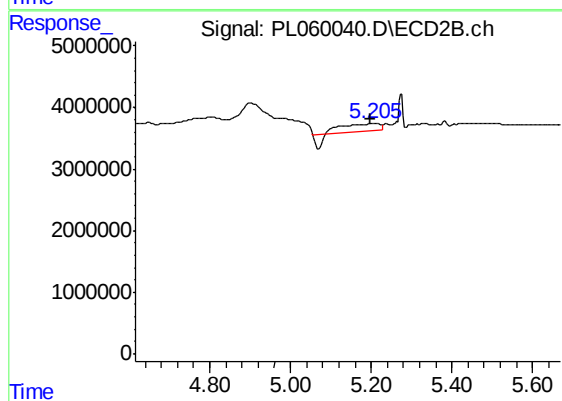

#4 Heptachlor


R.T.: 5.205 min
Delta R.T.: 0.007 min
Response: 5872821
Conc: 1.75 ng/ml

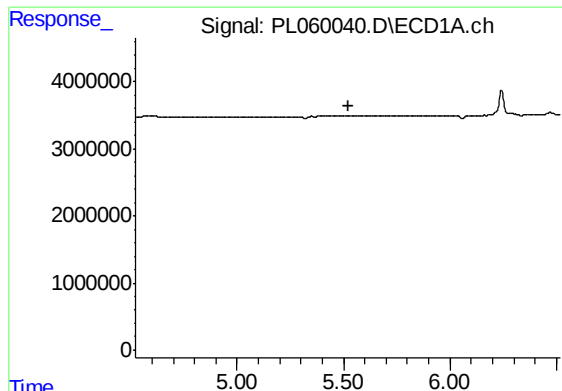

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB130316TB

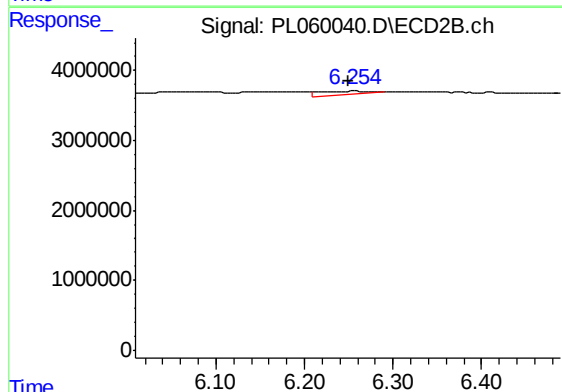


#9 Endosulfan I

R.T.: 6.256 min
Delta R.T.: 0.006 min
Response: 1917633
Conc: 0.72 ng/ml

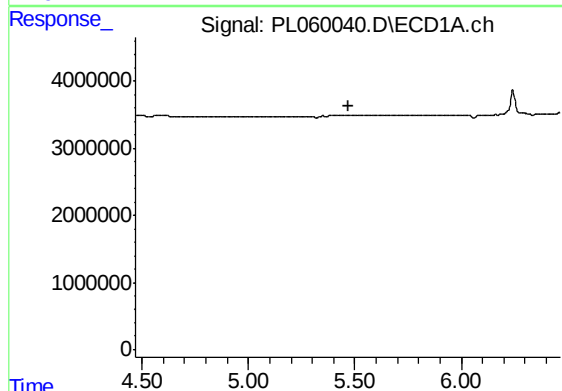


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.469 min
Response: 0
Conc: N.D.

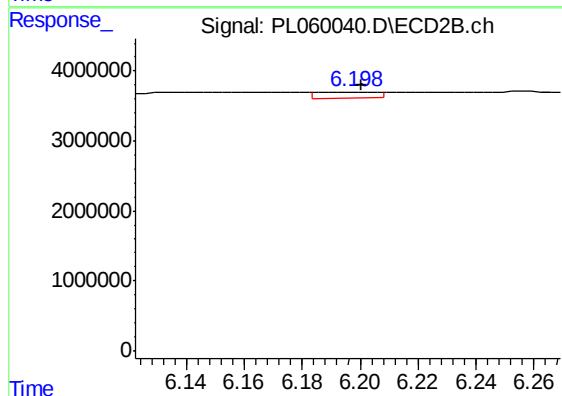

#11 alpha-Chlordane


R.T.: 6.199 min
Delta R.T.: -0.002 min
Response: 1169559
Conc: 0.41 ng/ml

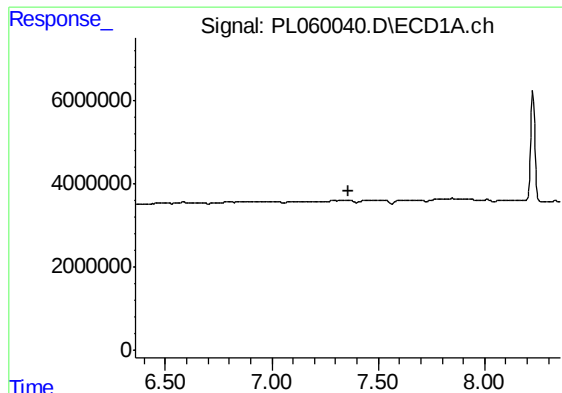

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 7.359 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB130316TB

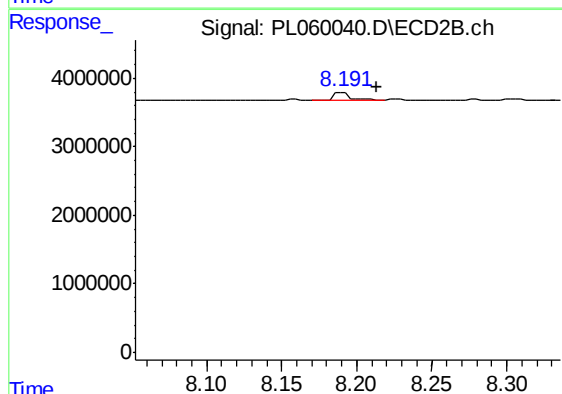


#22 Mirex

R.T.: 8.191 min
Delta R.T.: -0.021 min
Response: 688832
Conc: 0.37 ng/ml

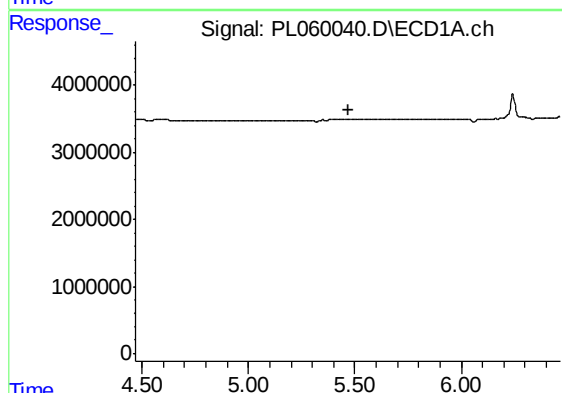


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.469 min
Response: 0
Conc: N.D.

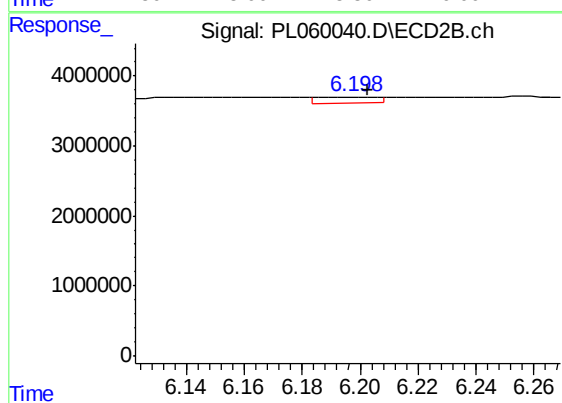

#26 Chlordane-4


R.T.: 6.199 min
Delta R.T.: -0.004 min
Response: 1169559
Conc: 2.53 ng/ml

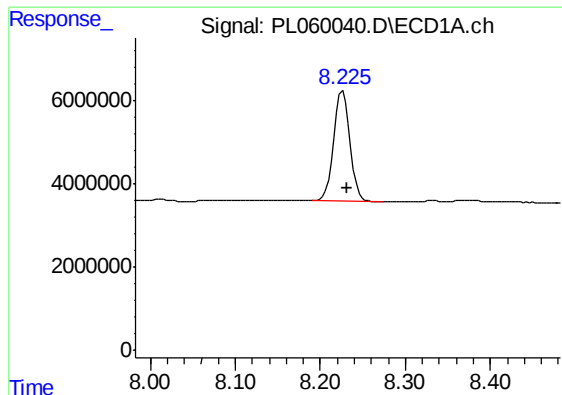

#28 Decachlorobiphenyl

R.T.: 8.226 min
Delta R.T.: -0.005 min
Response: 35551821
Conc: 21.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB130316TB

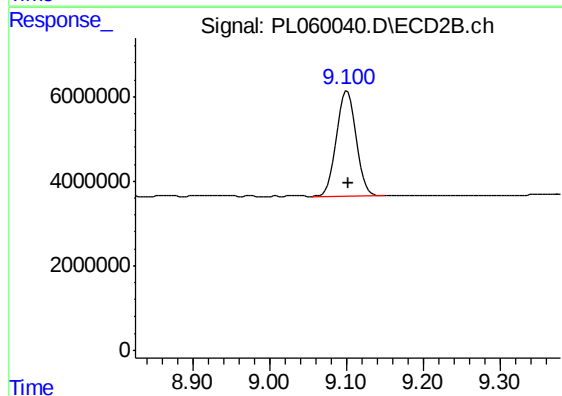

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: -0.001 min
Response: 44244833
Conc: 21.16 ng/ml