

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068258.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 08:57
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 05:44:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	8.044	0	3390720	N.D. 2.999 #
10) B	gamma-Chl...	7.386f	8.280f	188211	1769991	0.328 1.572 #
14) MA	Endrin	8.100f	0.000	501764	0	1.003 N.D. #
25)	Chlordane-3	7.386	8.280f	188211	1769991	3.495 11.429 #
27)	Chlordane-5	0.000	9.281	0	411666	N.D. 12.844 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068258.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 08:57
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 05:44:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

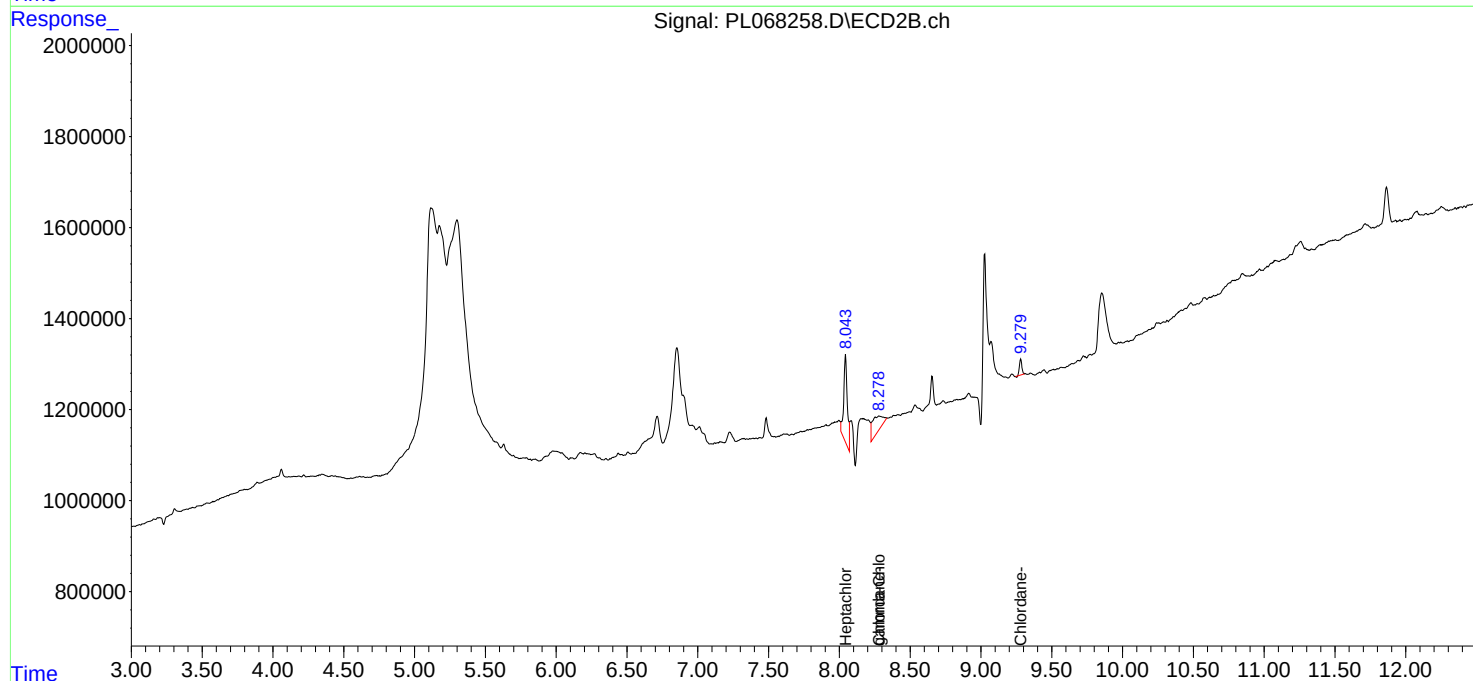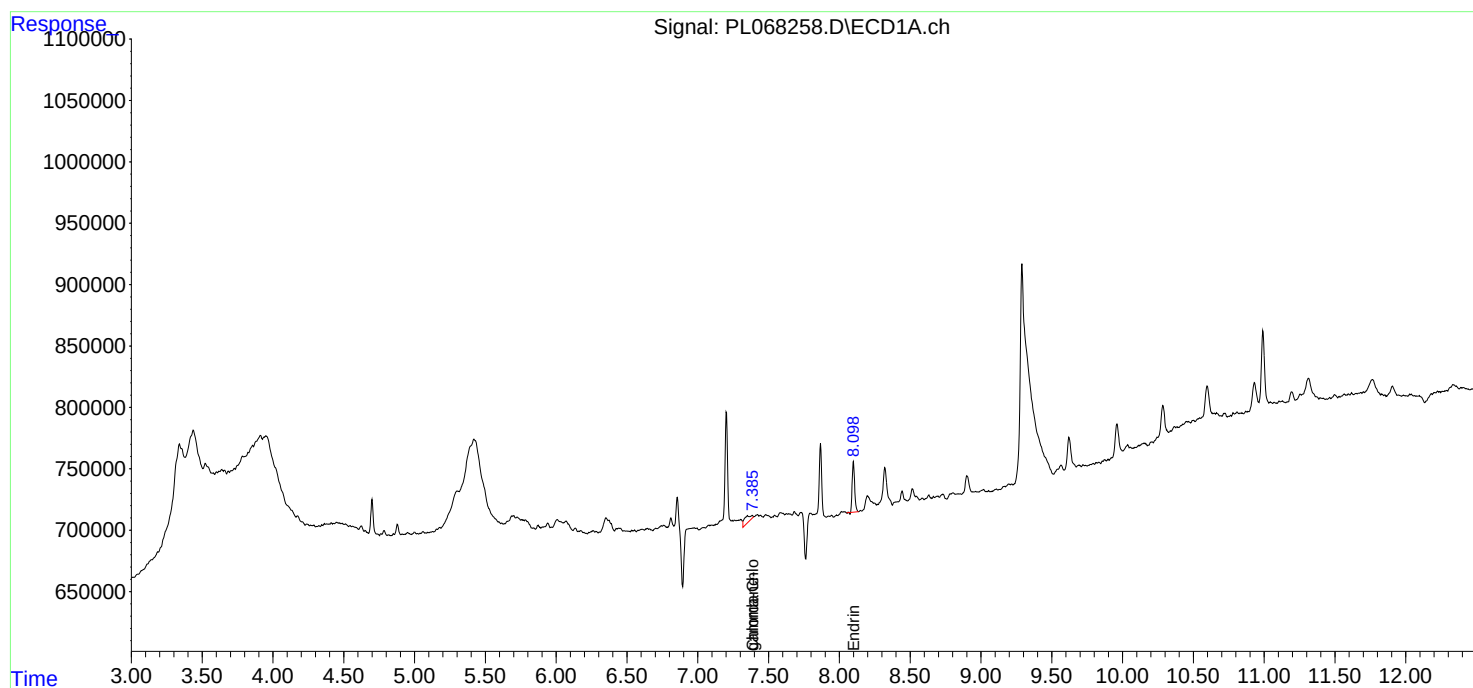


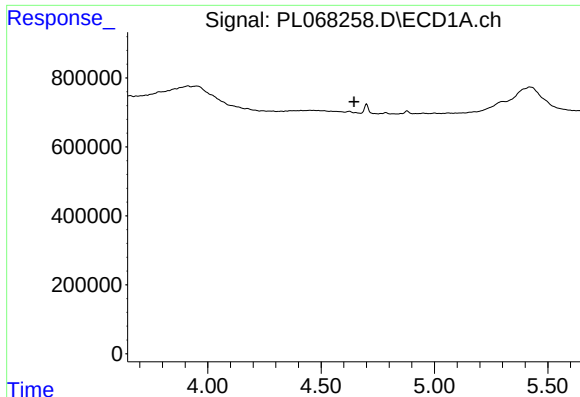

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

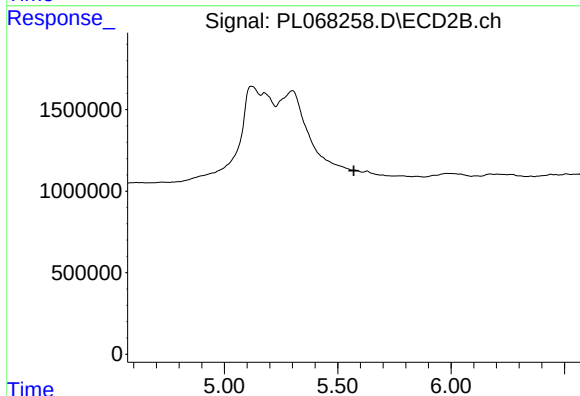


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.571 min
Response: 0
Conc: N.D.

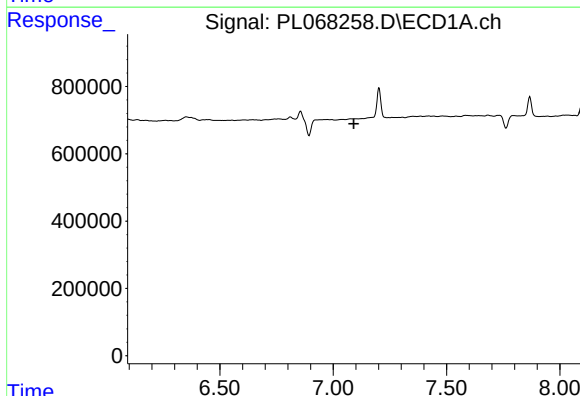


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

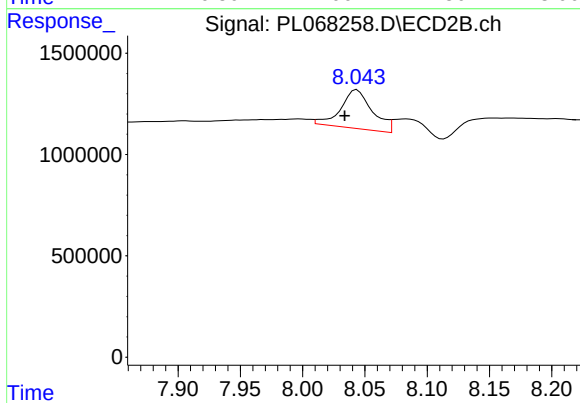

#8 Heptachlor epoxide


R.T.: 8.044 min
Delta R.T.: 0.010 min
Response: 3390720
Conc: 3.00 ng/ml

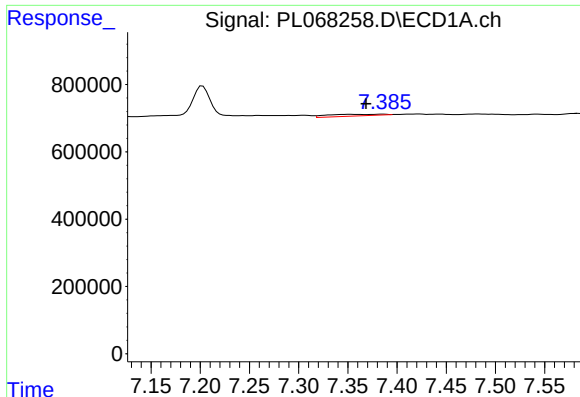

#10 gamma-Chlordane


R.T.: 7.386 min
Delta R.T.: 0.017 min
Response: 188211
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

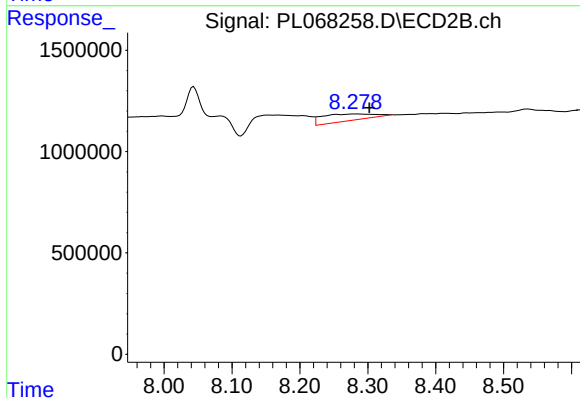


#10 gamma-Chlordane

R.T.: 8.280 min
Delta R.T.: -0.023 min
Response: 1769991
Conc: 1.57 ng/ml

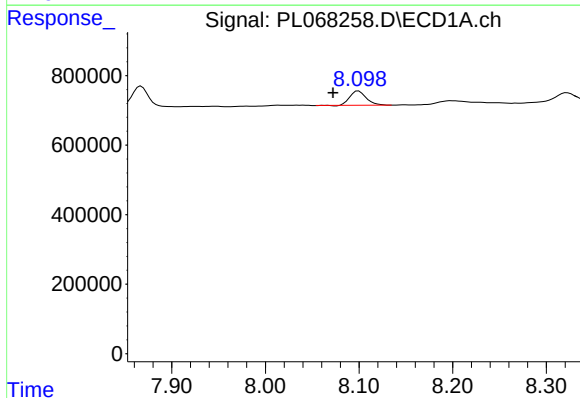


#14 Endrin

R.T.: 8.100 min
Delta R.T.: 0.027 min
Response: 501764
Conc: 1.00 ng/ml

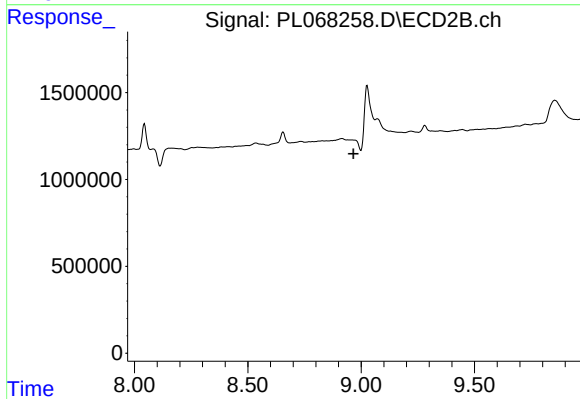

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.966 min
Response: 0
Conc: N.D.

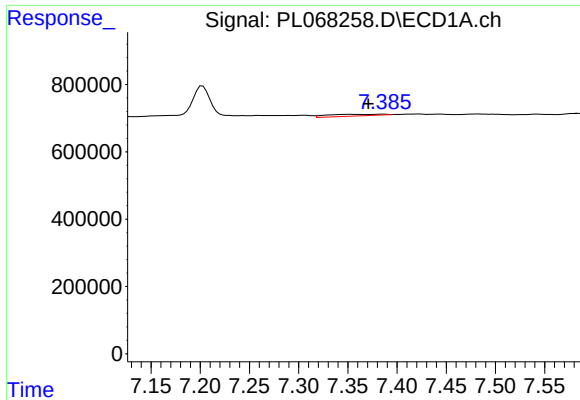

#25 Chlordane-3


R.T.: 7.386 min
Delta R.T.: 0.015 min
Response: 188211
Conc: 3.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

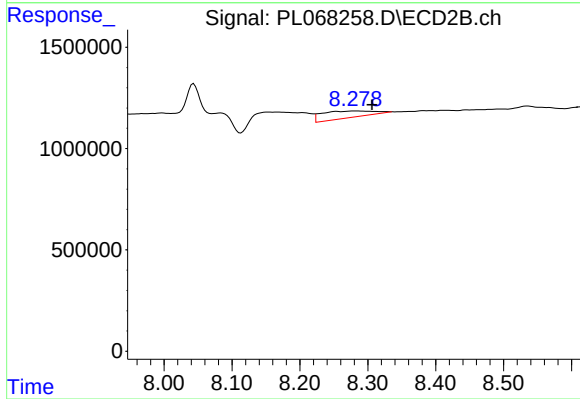


#25 Chlordane-3

R.T.: 8.280 min
Delta R.T.: -0.027 min
Response: 1769991
Conc: 11.43 ng/ml

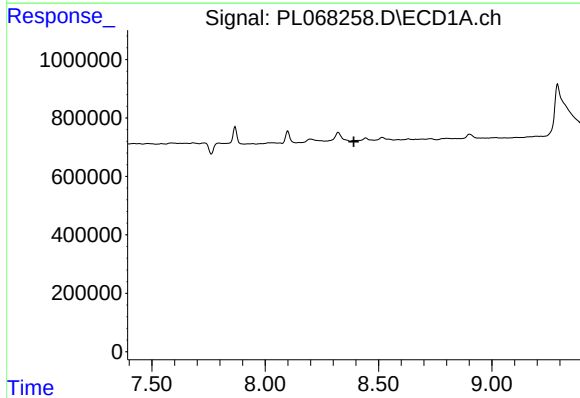


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 8.391 min
Response: 0
Conc: N.D.

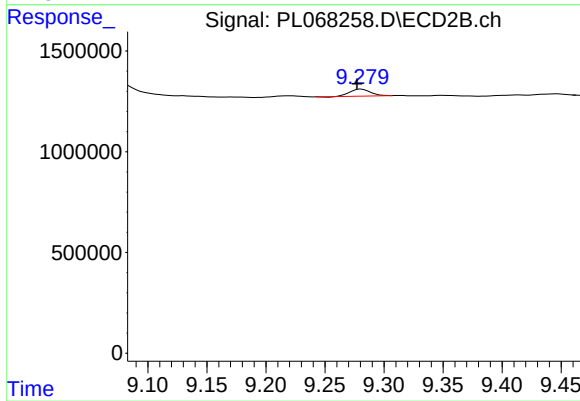

#27 Chlordane-5


R.T.: 9.281 min
Delta R.T.: 0.003 min
Response: 411666
Conc: 12.84 ng/ml

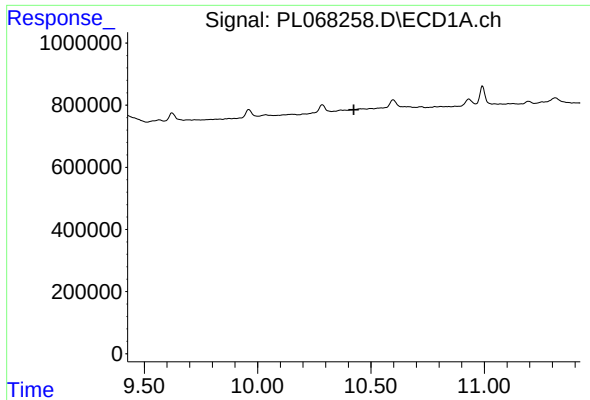

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

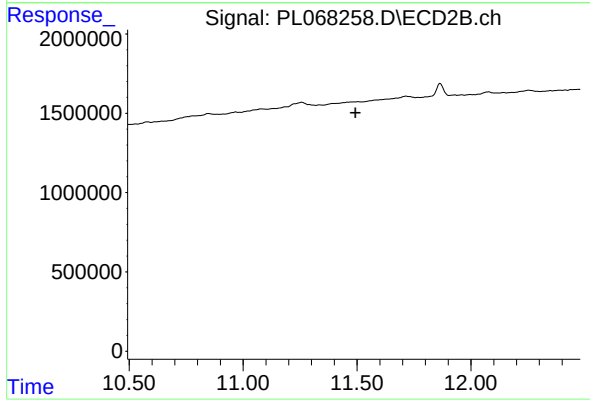

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.492 min
Response: 0
Conc: N.D.