

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068261.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 09:47
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 11:04:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:03:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.646	5.574	51838660	105.9E6	97.100	97.506
28)	SA Decachlor...	10.428	11.499	50565715	85759968	90.795	92.223
Target Compounds							
23)	Chlordane-1	5.979	6.958	14788365	38900822	971.914	978.218
24)	Chlordane-2	6.668	7.550	19819130	40510482	931.179	937.480
25)	Chlordane-3	7.372	8.307	54089194	159.7E6	992.498	992.660
26)	Chlordane-4	7.440	8.390	56667486	189.5E6	990.557	975.504
27)	Chlordane-5	8.391	9.278	19933122	32625729	984.599	970.068



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068261.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 09:47
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 11:04:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:03:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

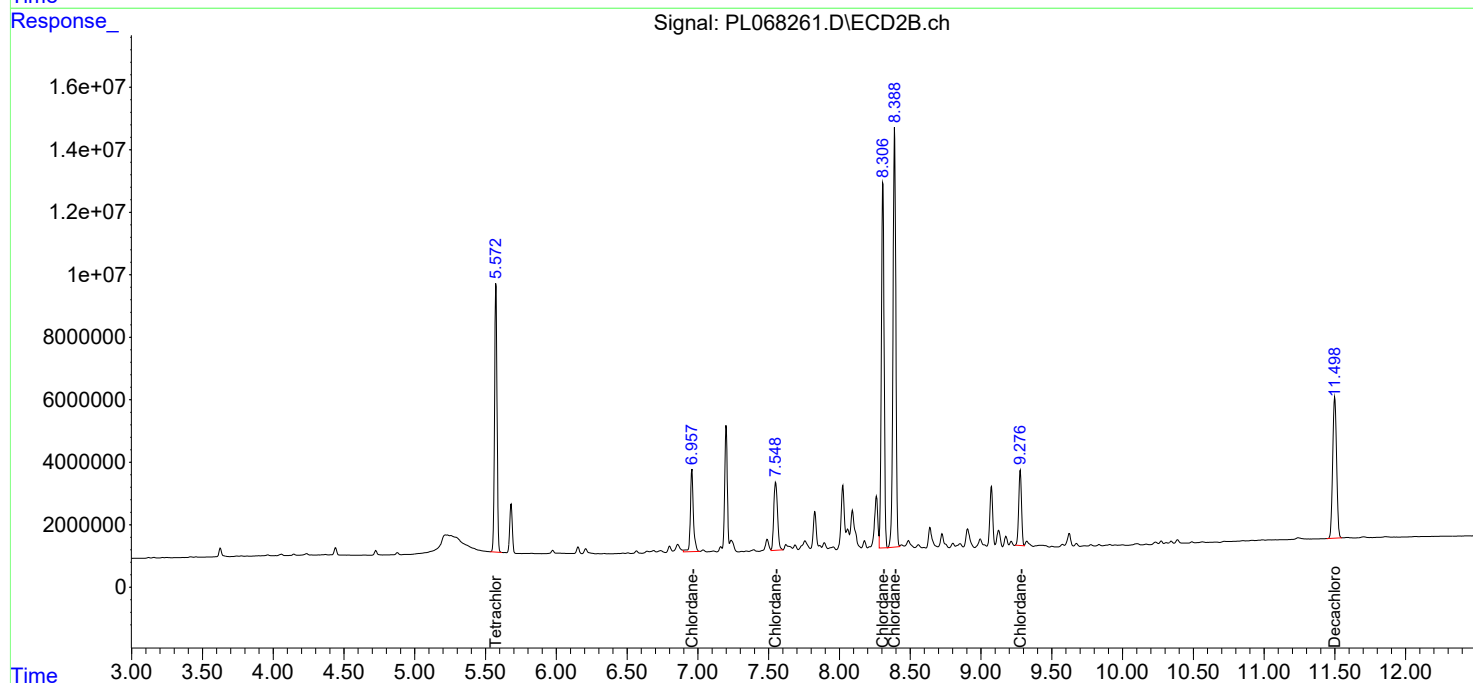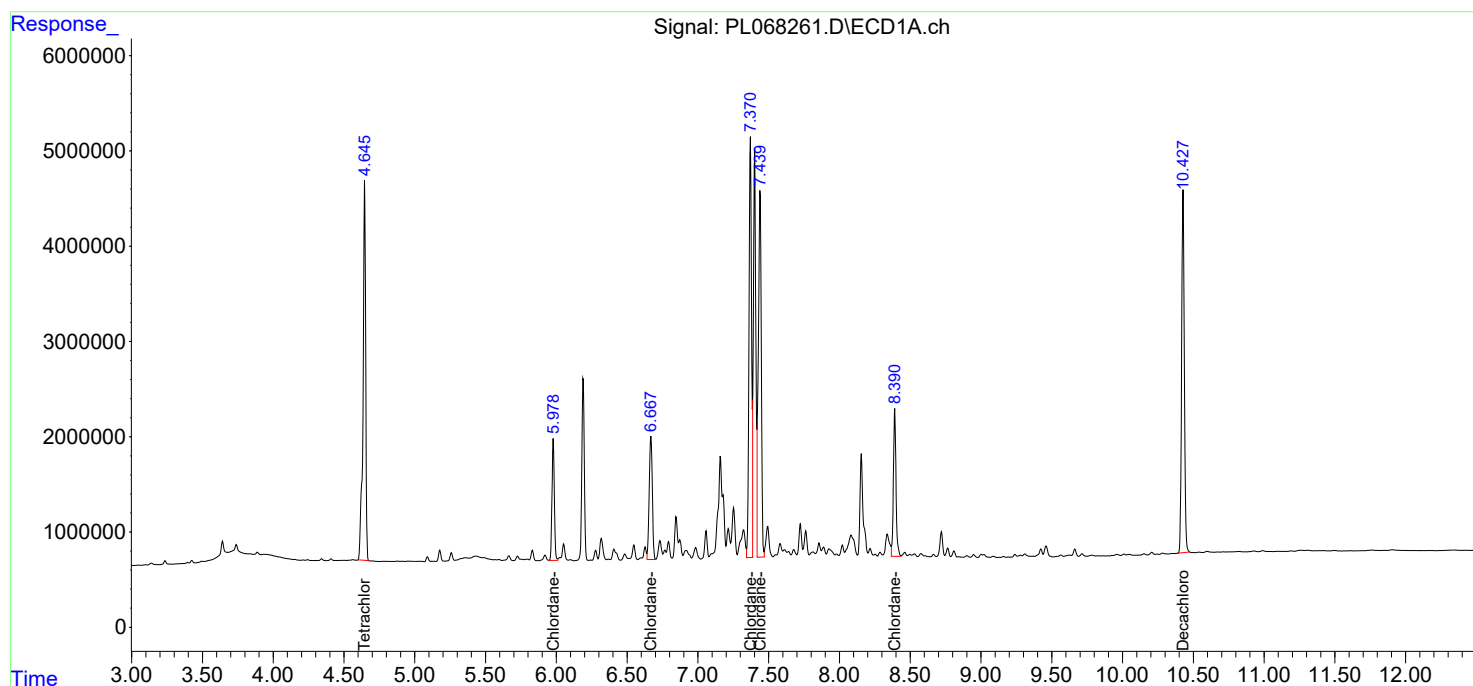


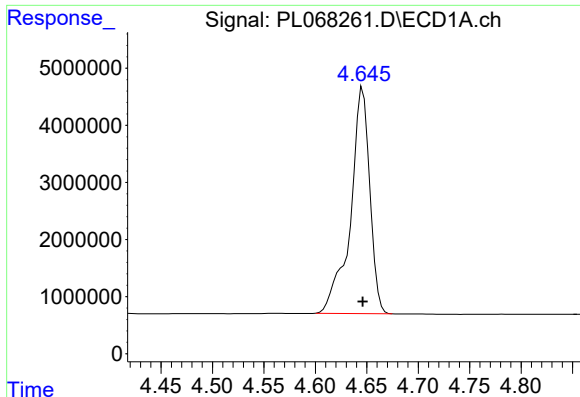

#1 Tetrachloro-m-xylene


R.T.: 4.646 min
Delta R.T.: 0.000 min
Response: 51838660
Conc: 97.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

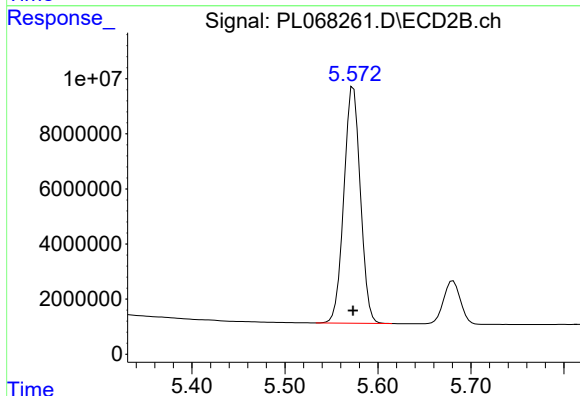


#1 Tetrachloro-m-xylene

R.T.: 5.574 min
Delta R.T.: 0.000 min
Response: 105938364
Conc: 97.51 ng/ml

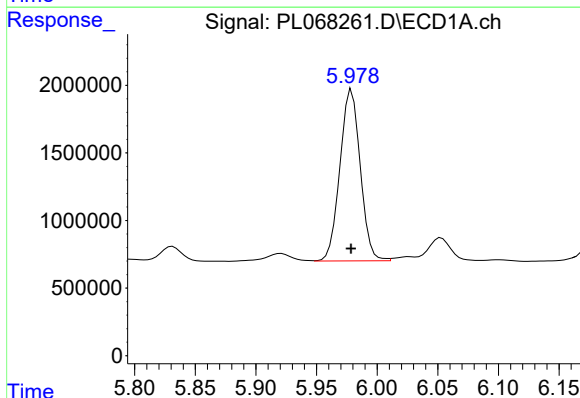


#23 Chlordane-1

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 14788365
Conc: 971.91 ng/ml

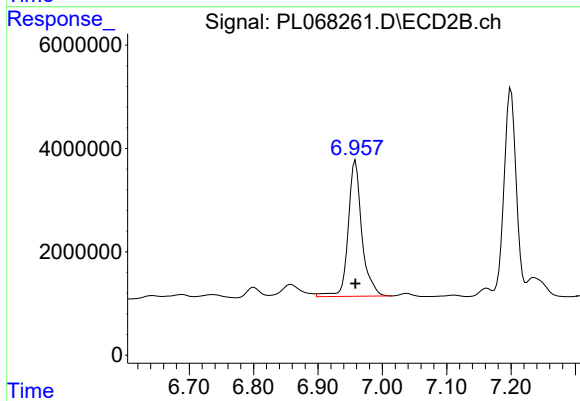

#23 Chlordane-1


R.T.: 6.958 min
Delta R.T.: 0.000 min
Response: 38900822
Conc: 978.22 ng/ml

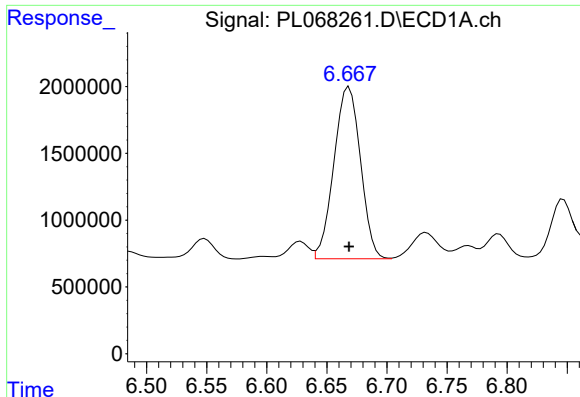

#24 Chlordane-2


R.T.: 6.668 min
Delta R.T.: 0.000 min
Response: 19819130
Conc: 931.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

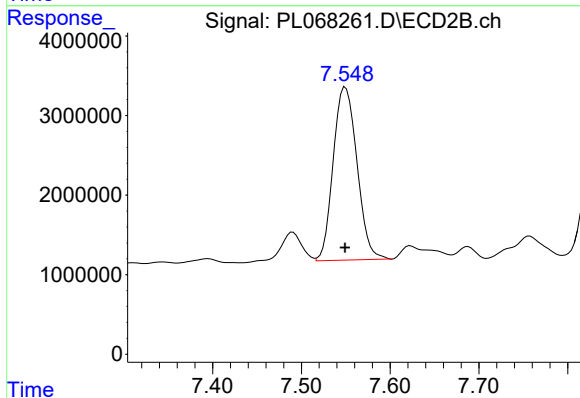


#24 Chlordane-2

R.T.: 7.550 min
Delta R.T.: 0.000 min
Response: 40510482
Conc: 937.48 ng/ml

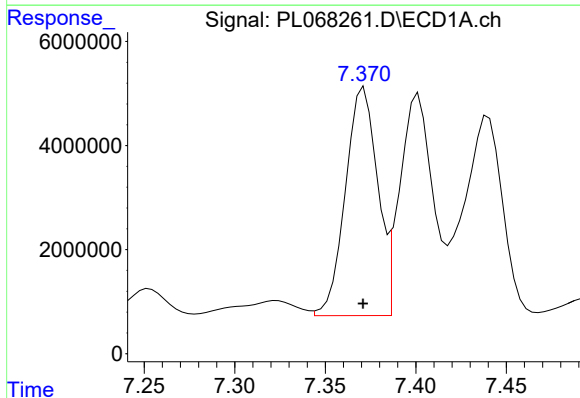


#25 Chlordane-3

R.T.: 7.372 min
Delta R.T.: 0.000 min
Response: 54089194
Conc: 992.50 ng/ml

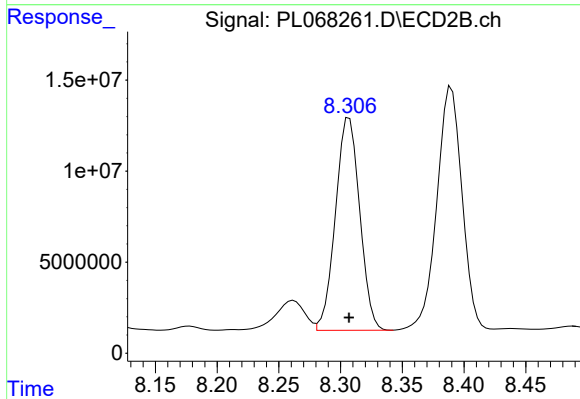

#25 Chlordane-3


R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 159687583
Conc: 992.66 ng/ml

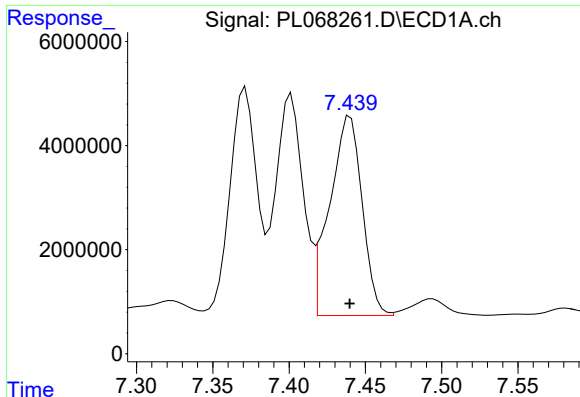

#26 Chlordane-4


R.T.: 7.440 min
Delta R.T.: 0.000 min
Response: 56667486
Conc: 990.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

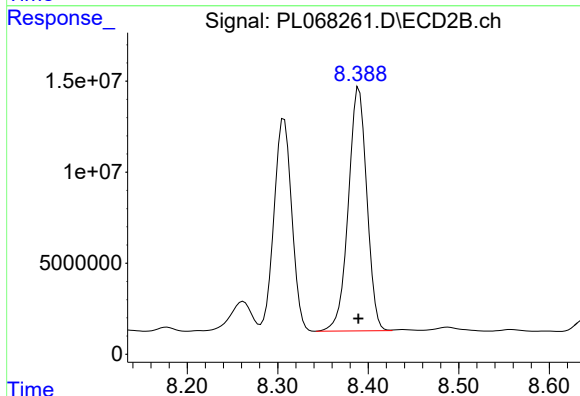


#26 Chlordane-4

R.T.: 8.390 min
Delta R.T.: 0.000 min
Response: 189523328
Conc: 975.50 ng/ml

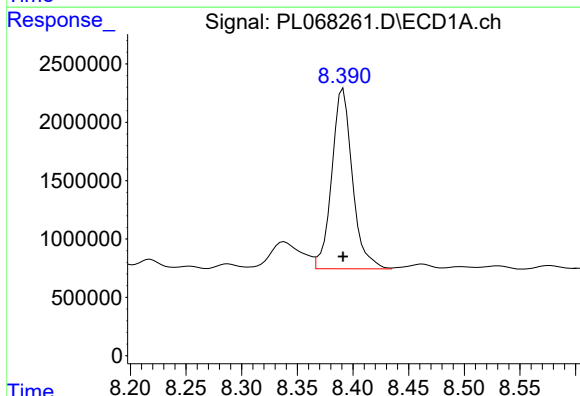


#27 Chlordane-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 19933122
Conc: 984.60 ng/ml

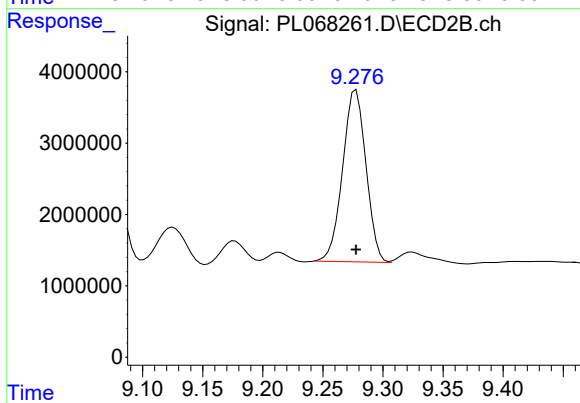

#27 Chlordane-5


R.T.: 9.278 min
Delta R.T.: 0.000 min
Response: 32625729
Conc: 970.07 ng/ml

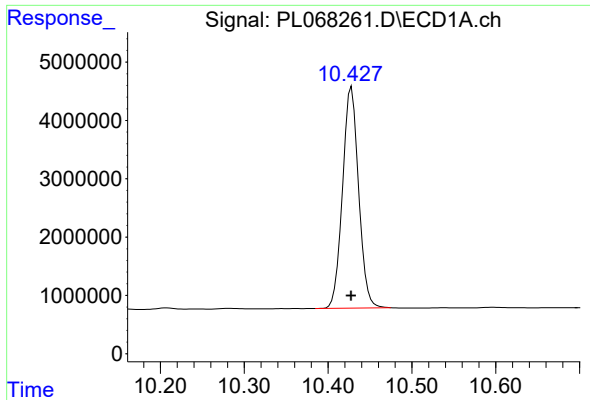

#28 Decachlorobiphenyl

R.T.: 10.428 min
Delta R.T.: 0.000 min
Response: 50565715
Conc: 90.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

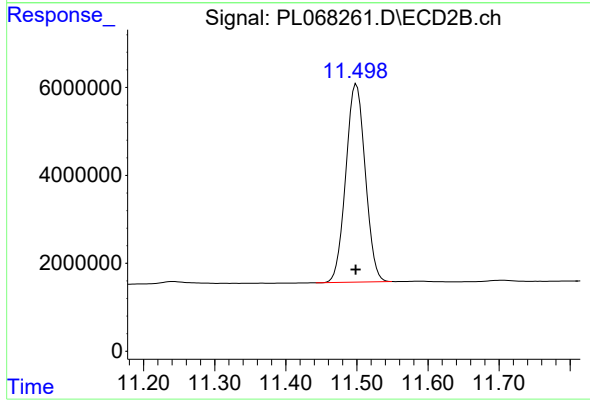

#28 Decachlorobiphenyl

R.T.: 11.499 min
Delta R.T.: 0.001 min
Response: 85759968
Conc: 92.22 ng/ml