

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 10:04
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 11:04:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:03:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.647	5.574	39274634	80122565	73.566	73.745
28)	SA Decachlor...	10.427	11.500	39406949	65825746	70.759	70.787
Target Compounds							
23)	Chlordane-1	5.979	6.959	11226637	28627469	737.832	719.880
24)	Chlordane-2	6.669	7.550	15292869	31181439	718.518	721.590
25)	Chlordane-3	7.372	8.307	40763346	119.9E6	747.979	745.150
26)	Chlordane-4	7.440	8.390	42688801	143.4E6	746.207	738.052
27)	Chlordane-5	8.391	9.278	15005598	24465584	741.204	727.441



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 10:04
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 11:04:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:03:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

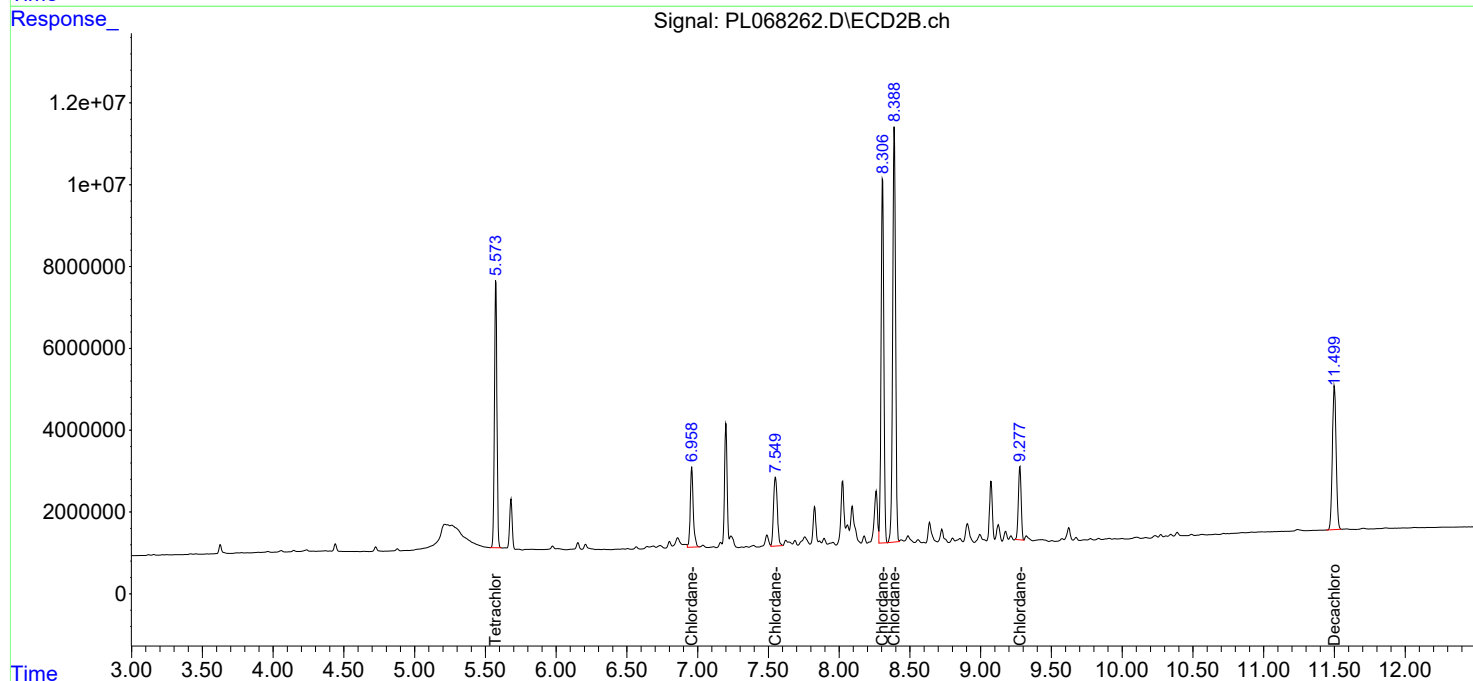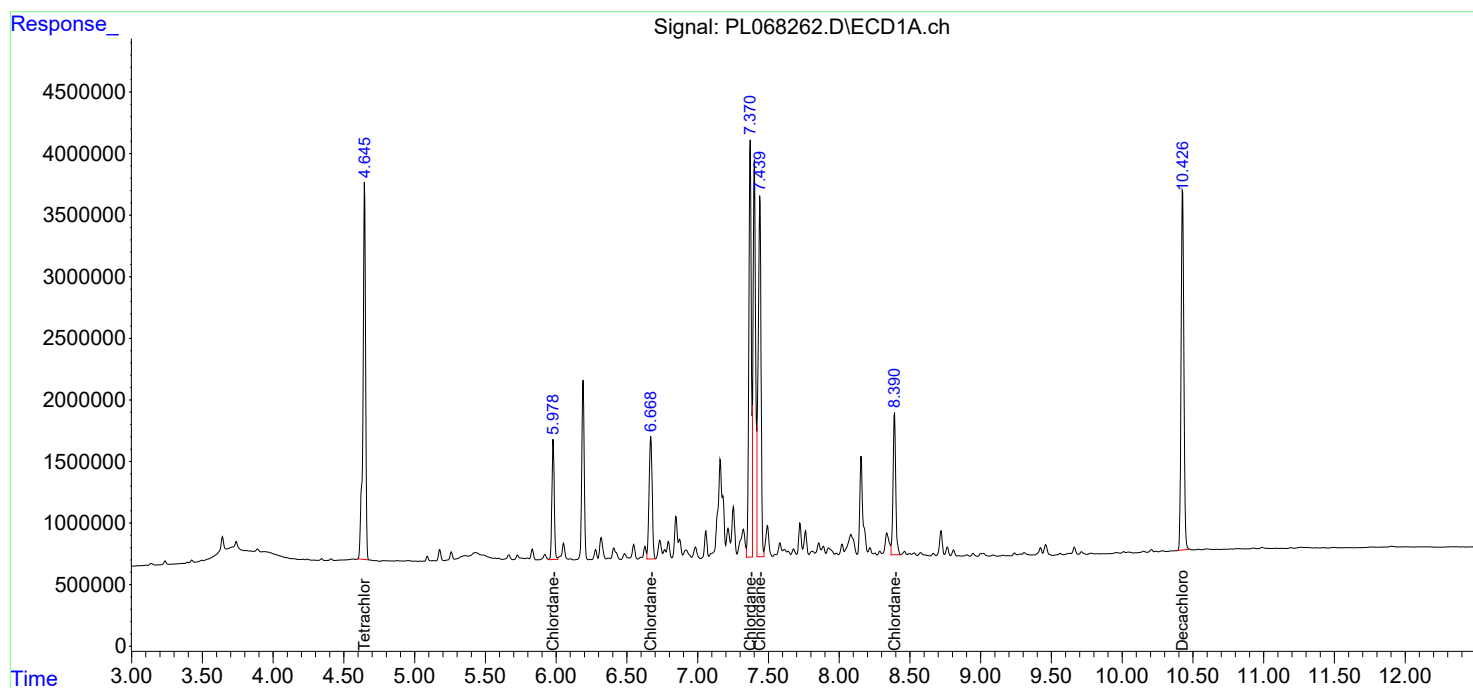


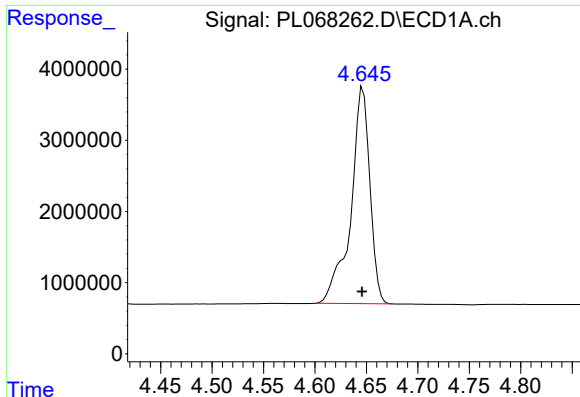

#1 Tetrachloro-m-xylene


R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 39274634
Conc: 73.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

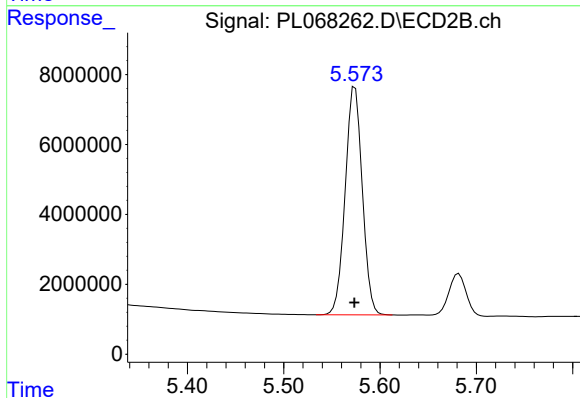


#1 Tetrachloro-m-xylene

R.T.: 5.574 min
Delta R.T.: 0.000 min
Response: 80122565
Conc: 73.75 ng/ml

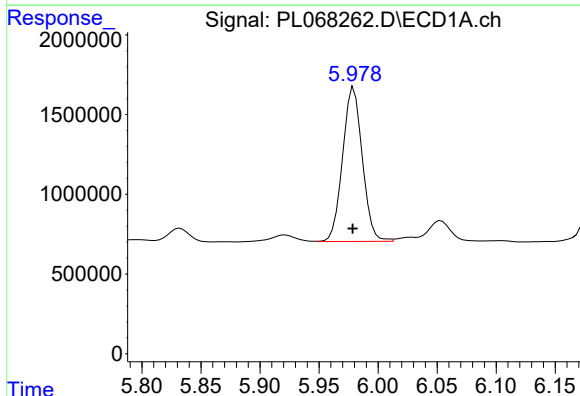


#23 Chlordane-1

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 11226637
Conc: 737.83 ng/ml

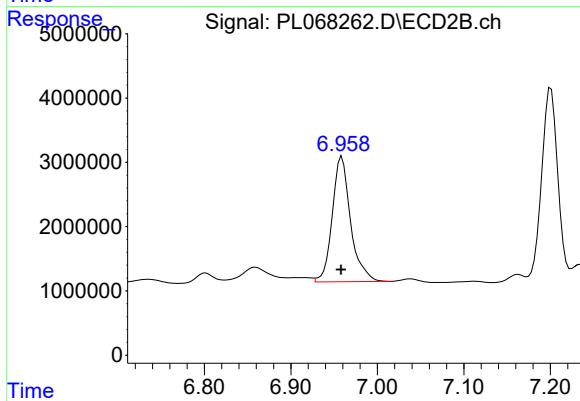

#23 Chlordane-1


R.T.: 6.959 min
Delta R.T.: 0.000 min
Response: 28627469
Conc: 719.88 ng/ml

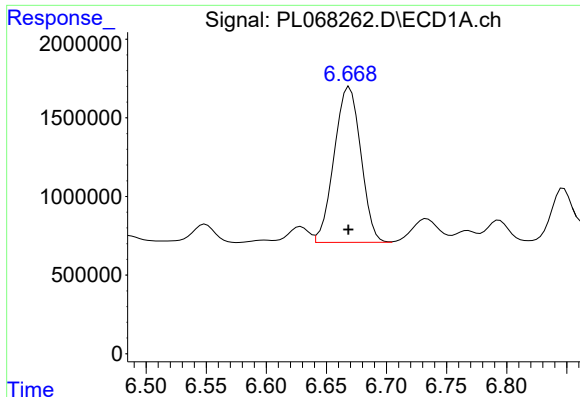

#24 Chlordane-2


R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 15292869
Conc: 718.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

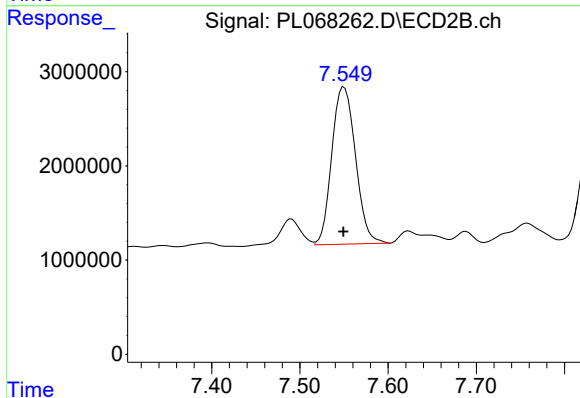


#24 Chlordane-2

R.T.: 7.550 min
Delta R.T.: 0.000 min
Response: 31181439
Conc: 721.59 ng/ml

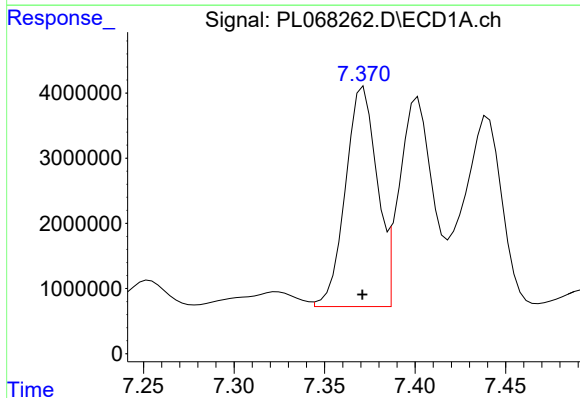


#25 Chlordane-3

R.T.: 7.372 min
Delta R.T.: 0.000 min
Response: 40763346
Conc: 747.98 ng/ml

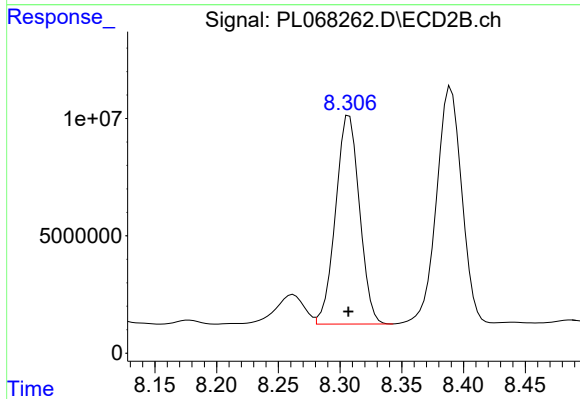

#25 Chlordane-3


R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 119871073
Conc: 745.15 ng/ml

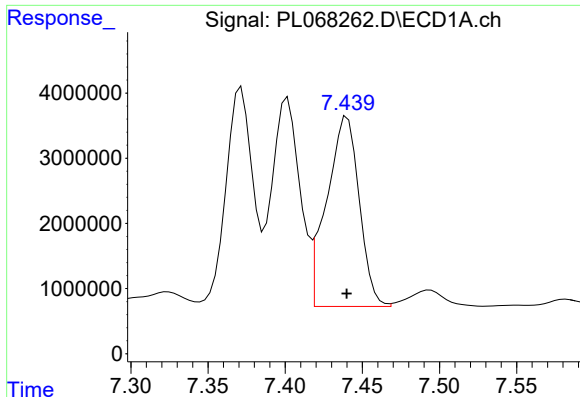

#26 Chlordane-4


R.T.: 7.440 min
Delta R.T.: 0.000 min
Response: 42688801
Conc: 746.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

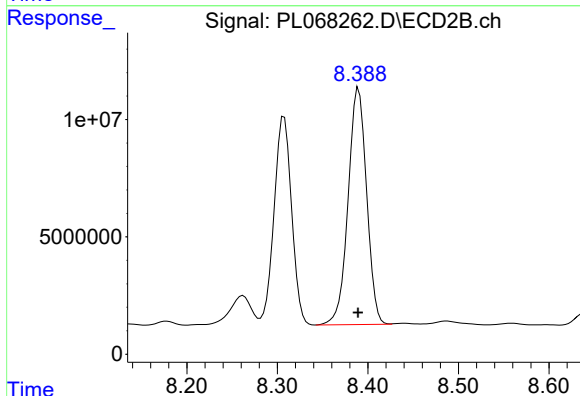


#26 Chlordane-4

R.T.: 8.390 min
Delta R.T.: 0.000 min
Response: 143390516
Conc: 738.05 ng/ml

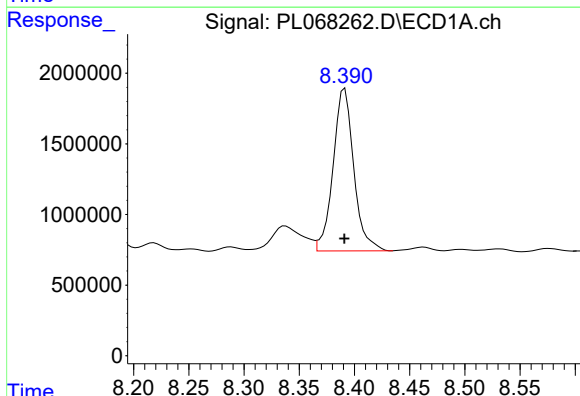


#27 Chlordane-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 15005598
Conc: 741.20 ng/ml

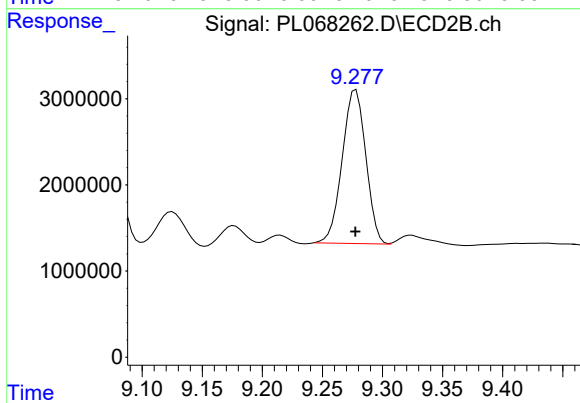

#27 Chlordane-5


R.T.: 9.278 min
Delta R.T.: 0.000 min
Response: 24465584
Conc: 727.44 ng/ml

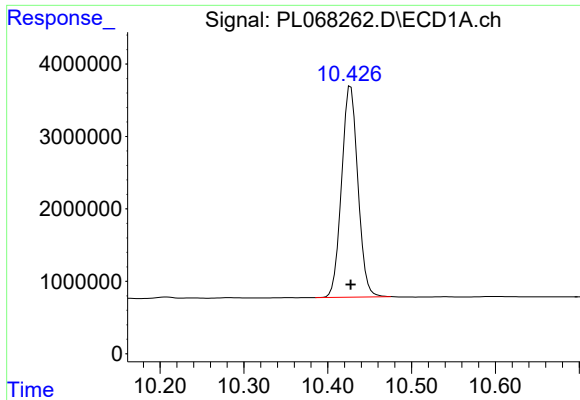

#28 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: 0.000 min
Response: 39406949
Conc: 70.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

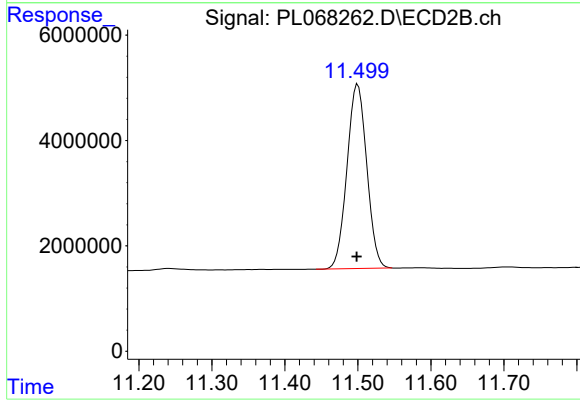

#28 Decachlorobiphenyl

R.T.: 11.500 min
Delta R.T.: 0.002 min
Response: 65825746
Conc: 70.79 ng/ml