

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 10:53
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 11:07:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:03:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.646	5.573	2715899	5021416	5.087	4.622
28)	SA Decachlor...	10.427	11.498	3164623	4926729	5.682	5.298
Target Compounds							
23)	Chlordane-1	5.978	6.958	748188	2333908	49.172	58.690
24)	Chlordane-2	6.668	7.548	1173969	2028542	55.158	46.944
25)	Chlordane-3	7.371	8.306	2678095	7203568	49.141	44.779
26)	Chlordane-4	7.440	8.389	2796656	8969990	48.886	46.170
27)	Chlordane-5	8.391	9.277	1026574	1475691	50.708	43.877



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 10:53
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 11:07:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:03:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

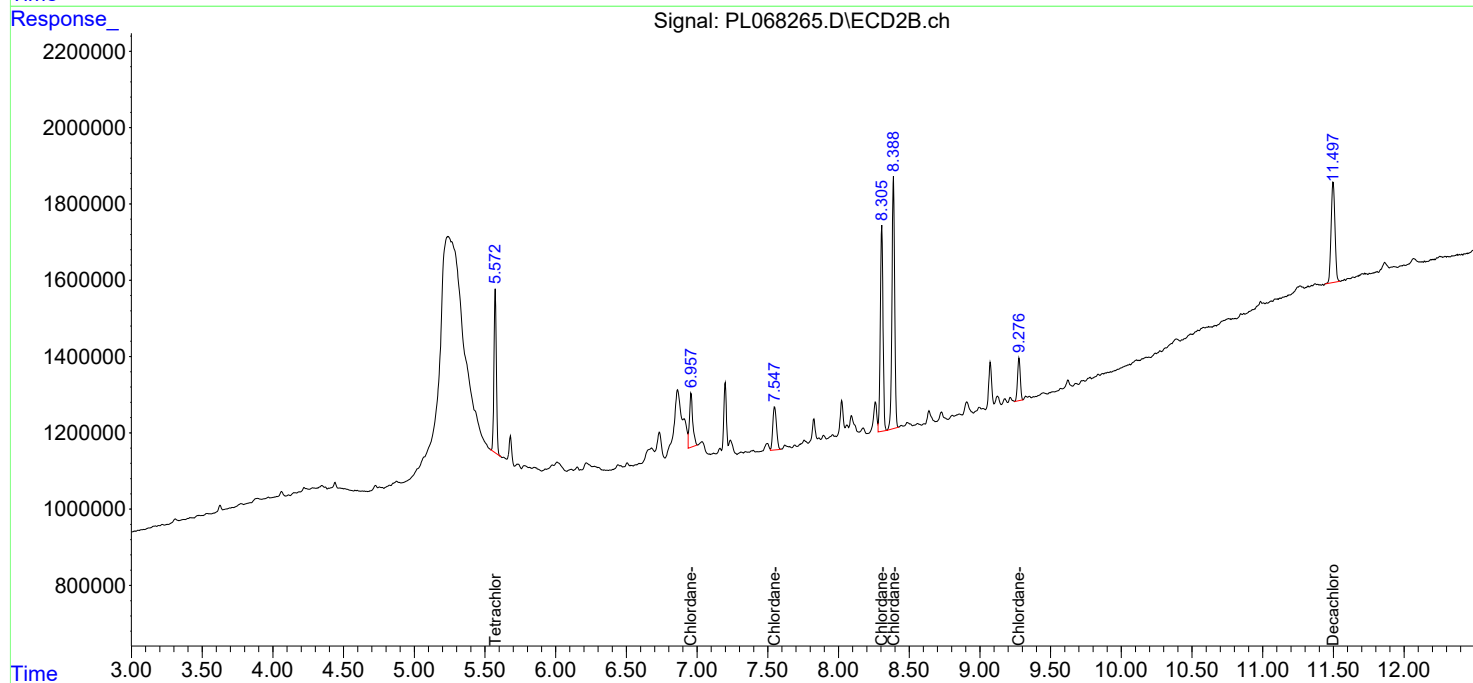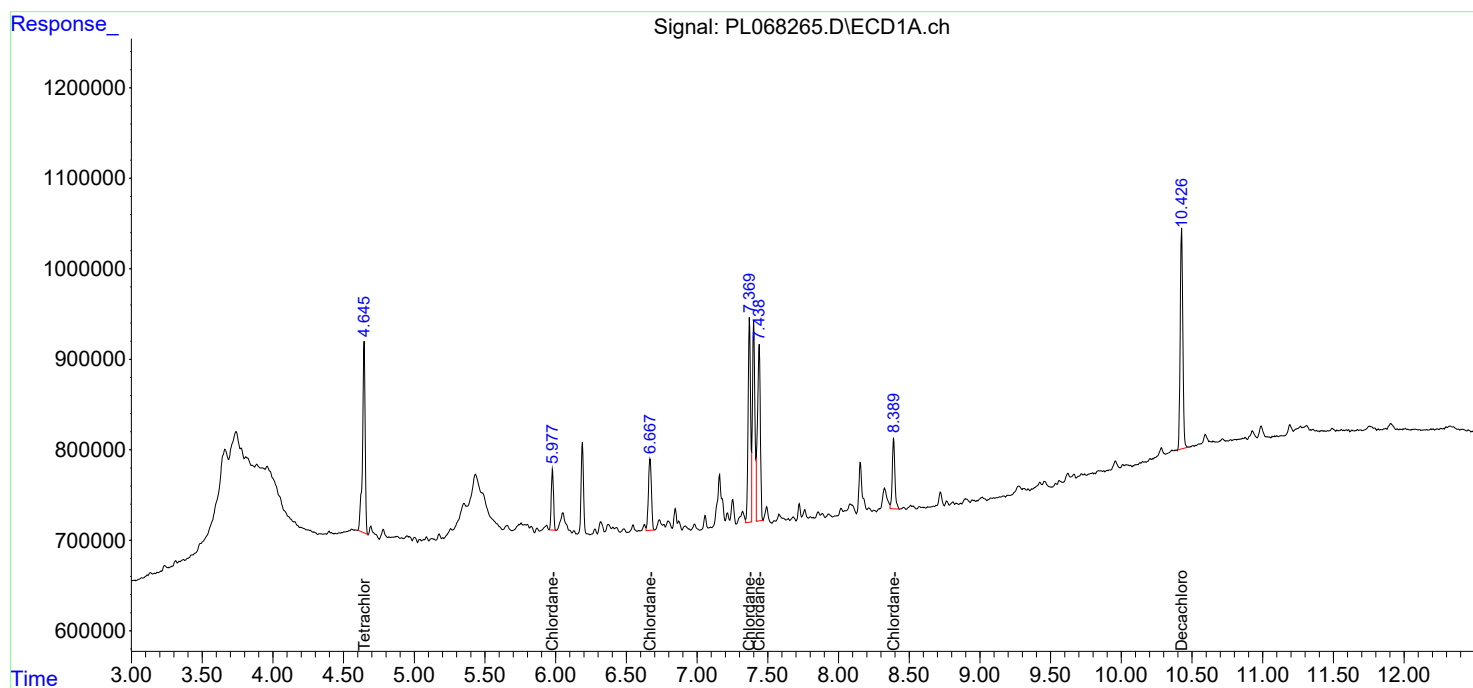


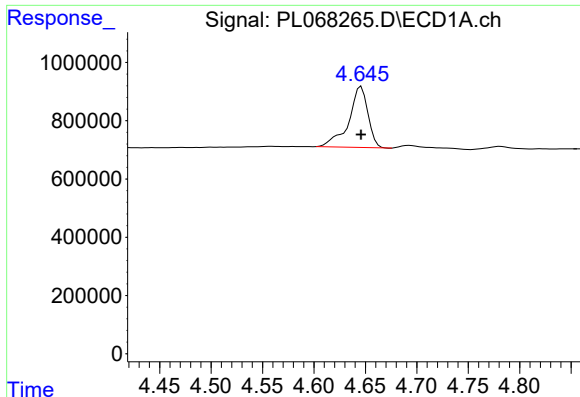

#1 Tetrachloro-m-xylene


R.T.: 4.646 min
Delta R.T.: 0.000 min
Response: 2715899
Conc: 5.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

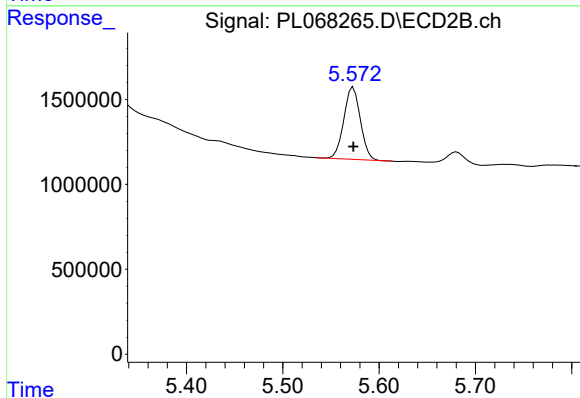


#1 Tetrachloro-m-xylene

R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 5021416
Conc: 4.62 ng/ml

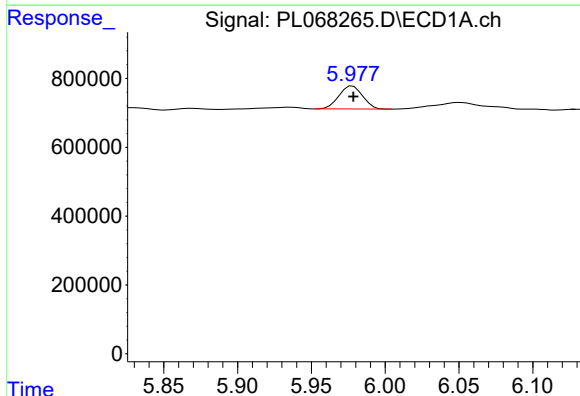


#23 Chlordane-1

R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 748188
Conc: 49.17 ng/ml

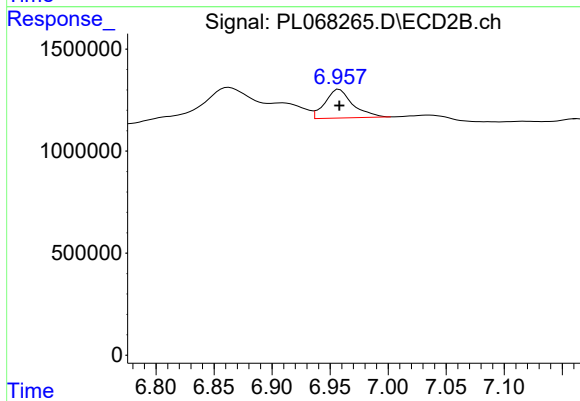

#23 Chlordane-1


R.T.: 6.958 min
Delta R.T.: 0.000 min
Response: 2333908
Conc: 58.69 ng/ml

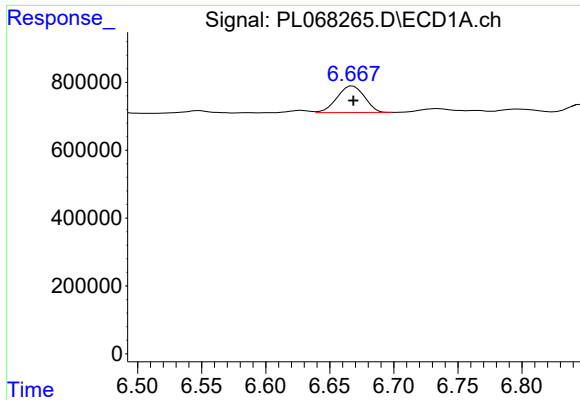

#24 Chlordane-2


R.T.: 6.668 min
Delta R.T.: 0.000 min
Response: 1173969
Conc: 55.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

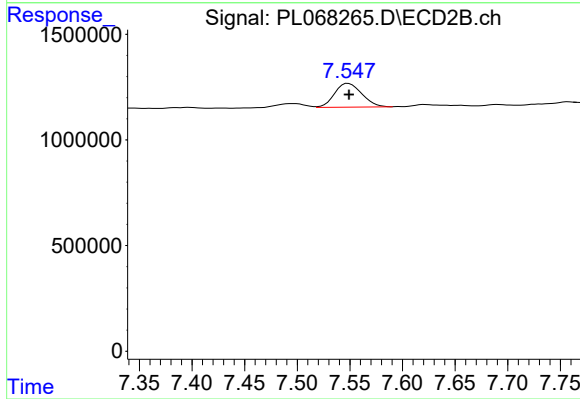


#24 Chlordane-2

R.T.: 7.548 min
Delta R.T.: 0.000 min
Response: 2028542
Conc: 46.94 ng/ml

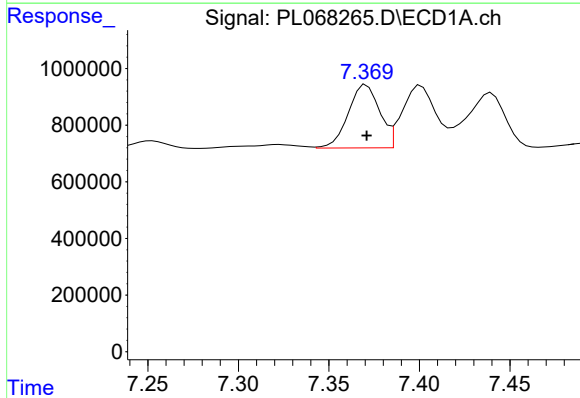


#25 Chlordane-3

R.T.: 7.371 min
Delta R.T.: 0.000 min
Response: 2678095
Conc: 49.14 ng/ml

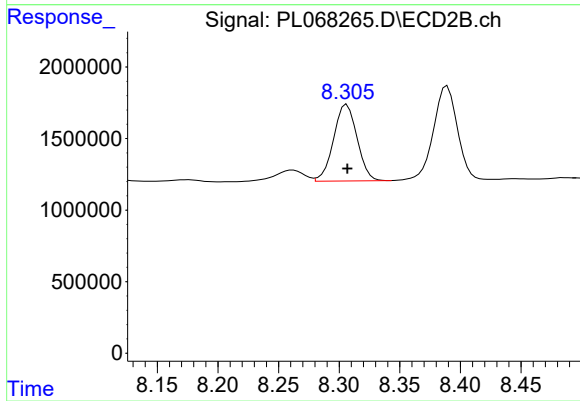

#25 Chlordane-3


R.T.: 8.306 min
Delta R.T.: 0.000 min
Response: 7203568
Conc: 44.78 ng/ml

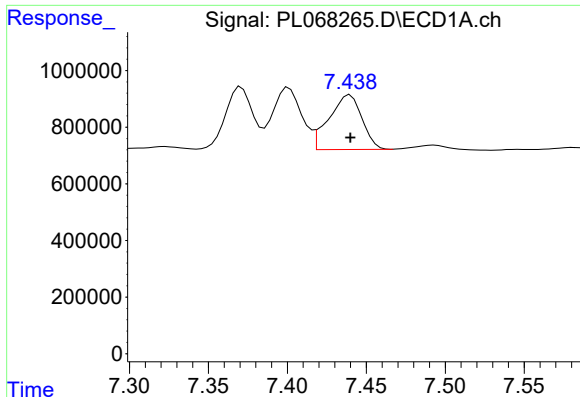

#26 Chlordane-4


R.T.: 7.440 min
Delta R.T.: 0.000 min
Response: 2796656
Conc: 48.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

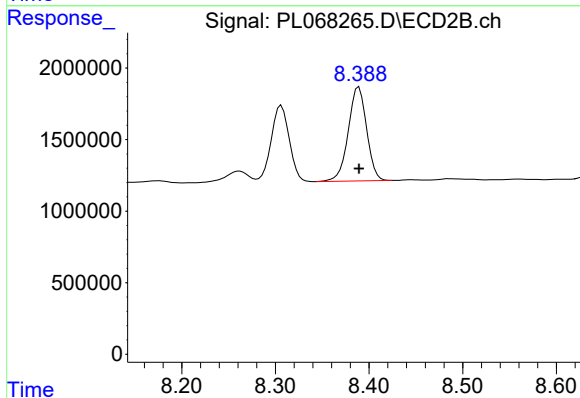


#26 Chlordane-4

R.T.: 8.389 min
Delta R.T.: 0.000 min
Response: 8969990
Conc: 46.17 ng/ml

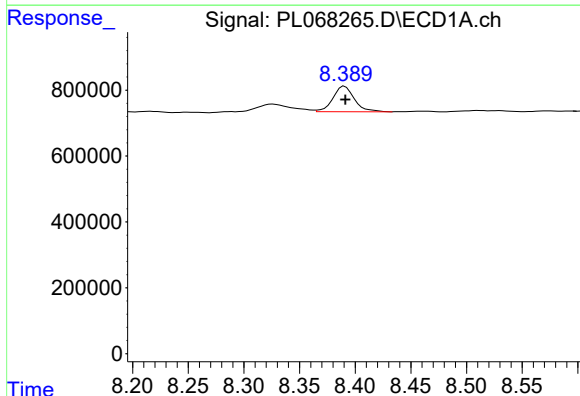


#27 Chlordane-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 1026574
Conc: 50.71 ng/ml

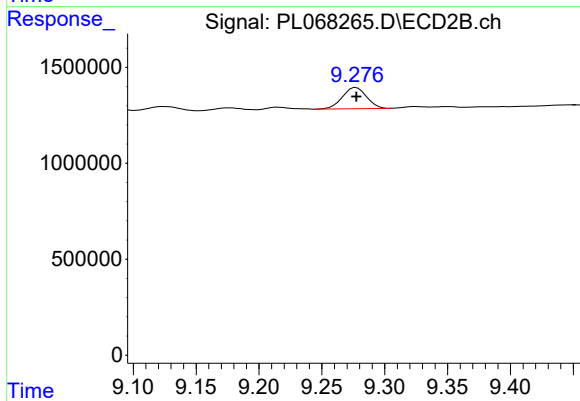

#27 Chlordane-5


R.T.: 9.277 min
Delta R.T.: 0.000 min
Response: 1475691
Conc: 43.88 ng/ml

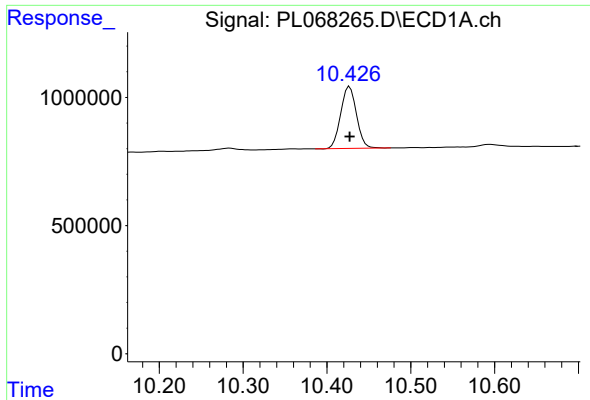

#28 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: 0.000 min
Response: 3164623
Conc: 5.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

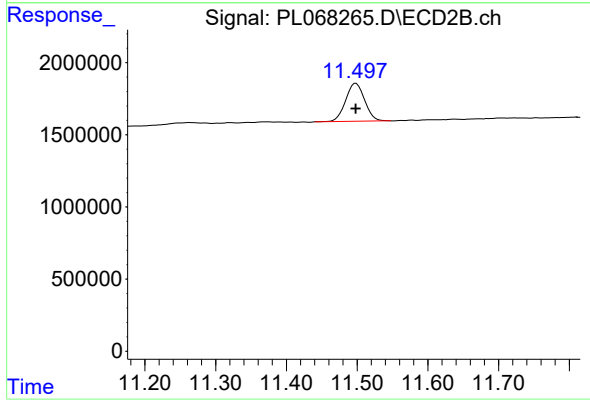

#28 Decachlorobiphenyl

R.T.: 11.498 min
Delta R.T.: 0.000 min
Response: 4926729
Conc: 5.30 ng/ml