

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 15:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 05:48:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.571	8879715	21869788	20.690	21.432
28)	SA Decachlor...	10.423	11.493	12373317	20308468	22.000	22.768
Target Compounds							
4)	MA Heptachlor	6.165f	0.000	387755	0	0.636	N.D. #
6)	B beta-BHC	6.165	0.000	387755	0	1.325	N.D. #
8)	B Heptachlo...	0.000	8.039	0	2226314	N.D.	1.969 #
14)	MA Endrin	8.093f	0.000	541624	0	1.083	N.D. #
15)	B Endosulfa...	0.000	9.217f	0	1675506	N.D.	1.849 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 15:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 05:48:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

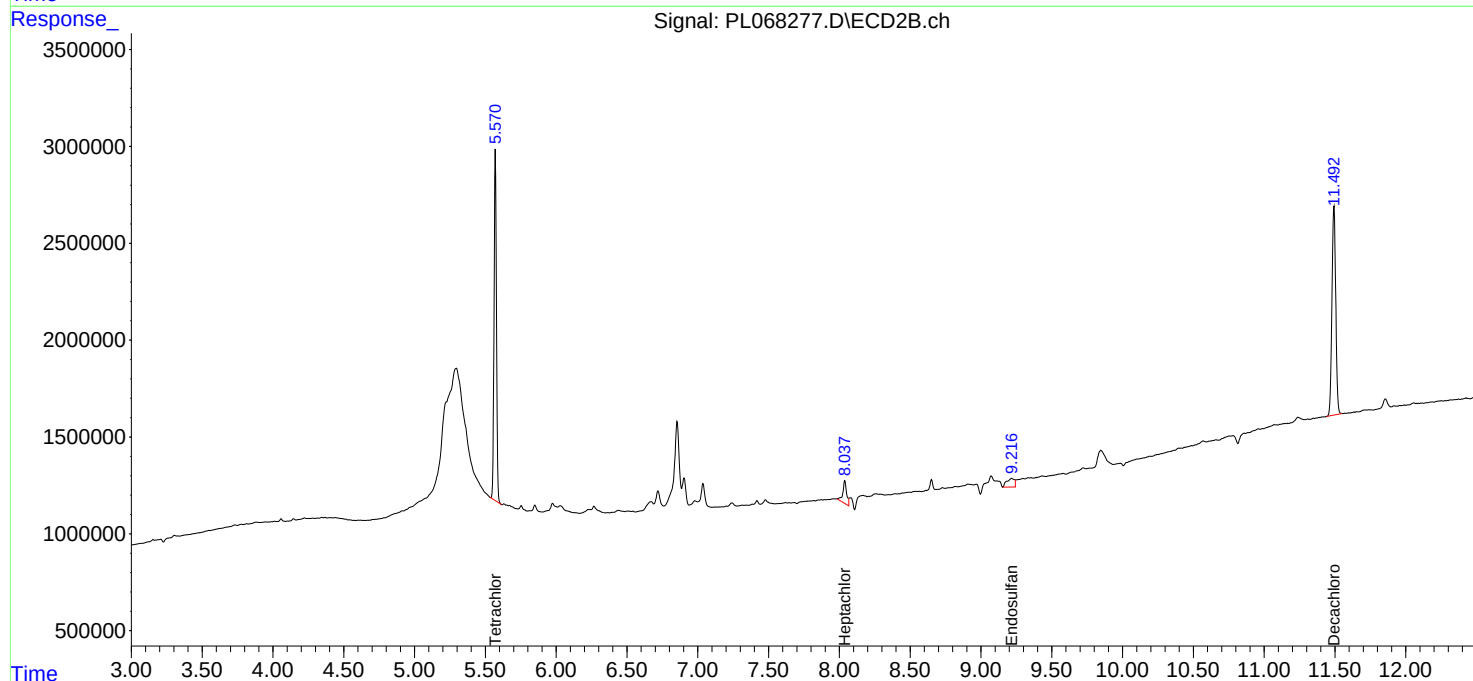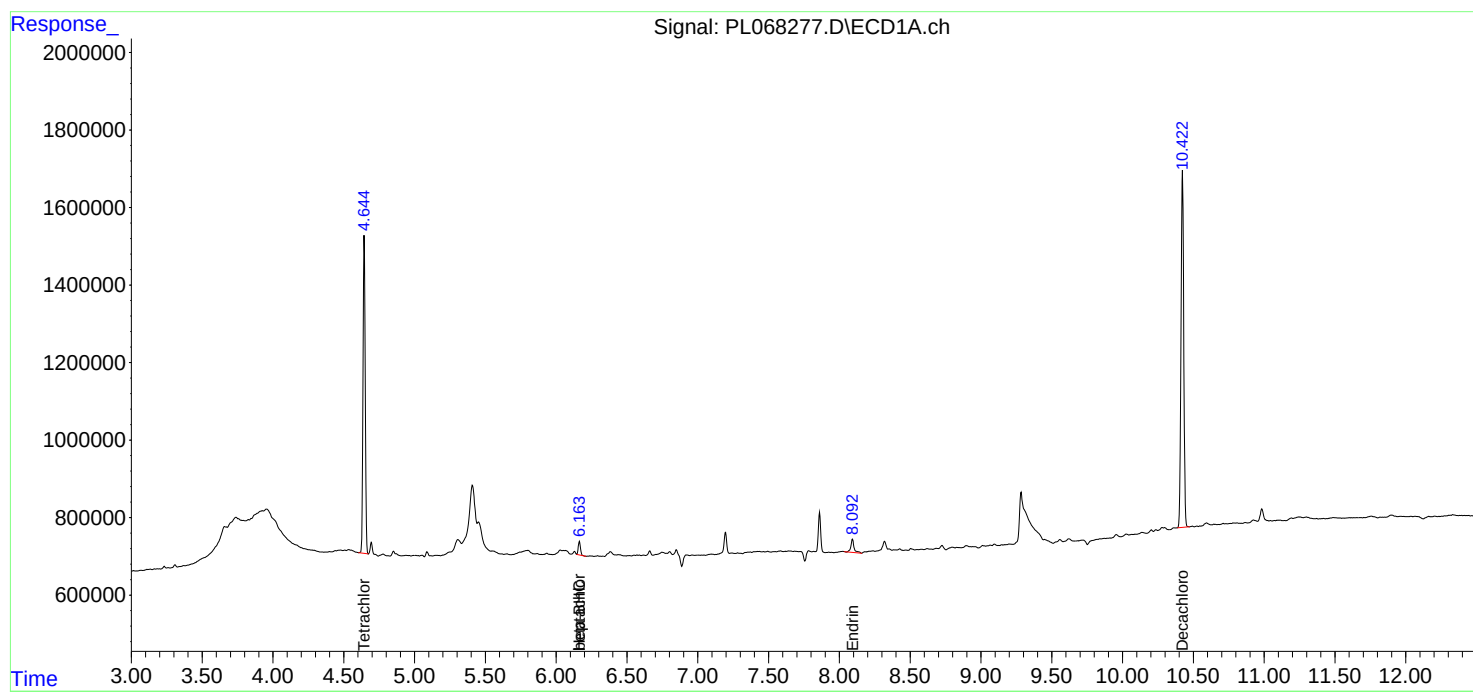


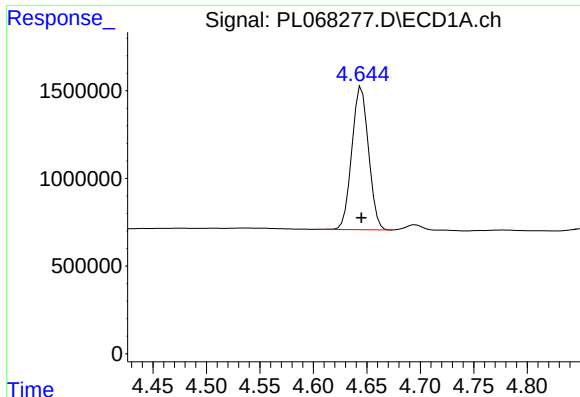

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 8879715
Conc: 20.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

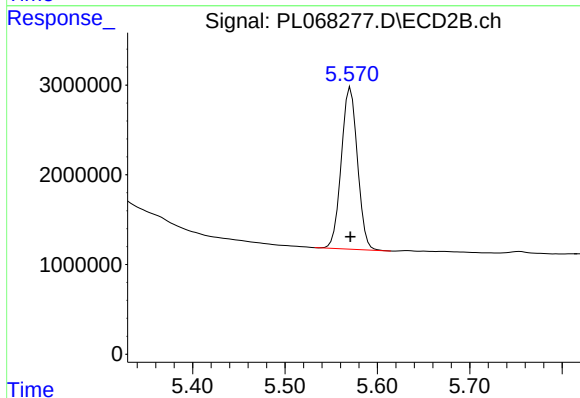


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 21869788
Conc: 21.43 ng/ml

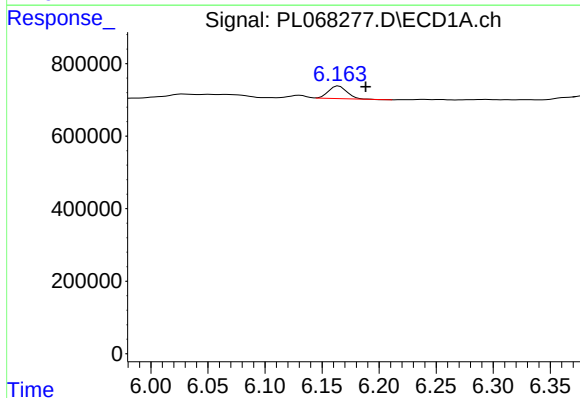


#4 Heptachlor

R.T.: 6.165 min
Delta R.T.: -0.024 min
Response: 387755
Conc: 0.64 ng/ml

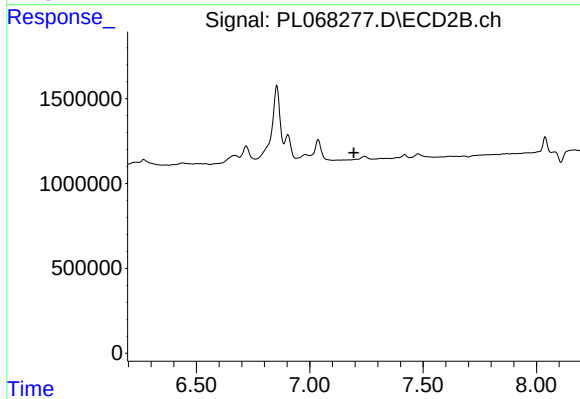

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

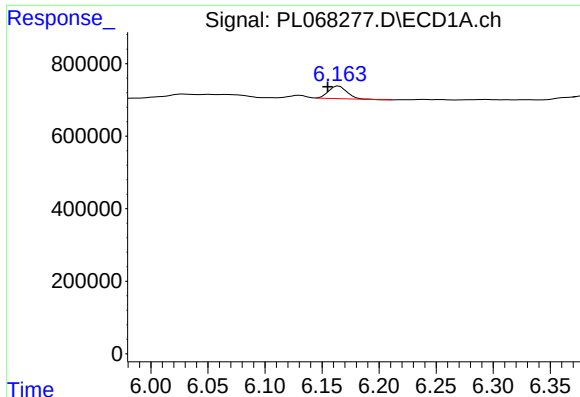

#6 beta-BHC


R.T.: 6.165 min
Delta R.T.: 0.010 min
Response: 387755
Conc: 1.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

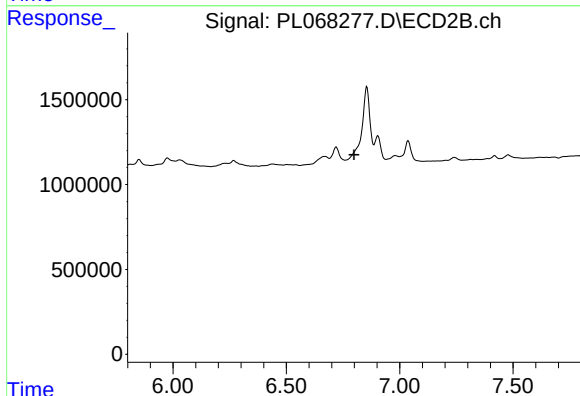


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

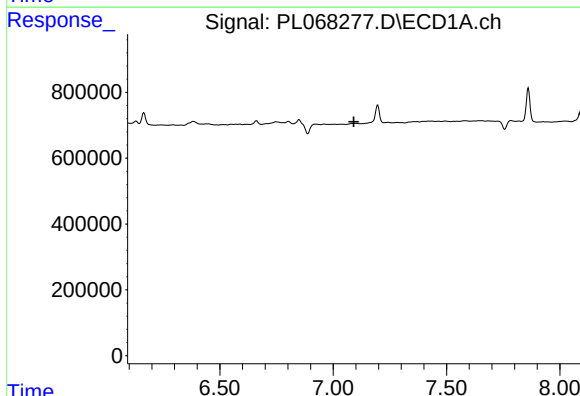


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

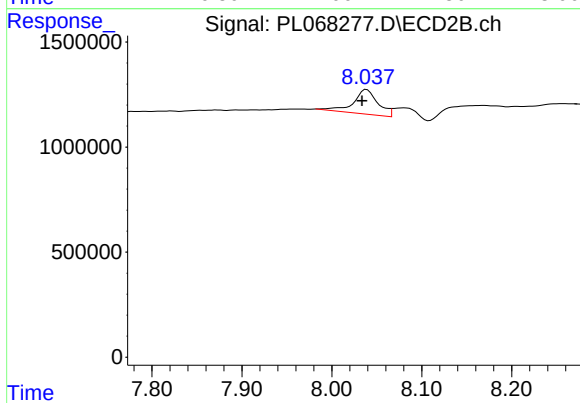

#8 Heptachlor epoxide


R.T.: 8.039 min
Delta R.T.: 0.005 min
Response: 2226314
Conc: 1.97 ng/ml

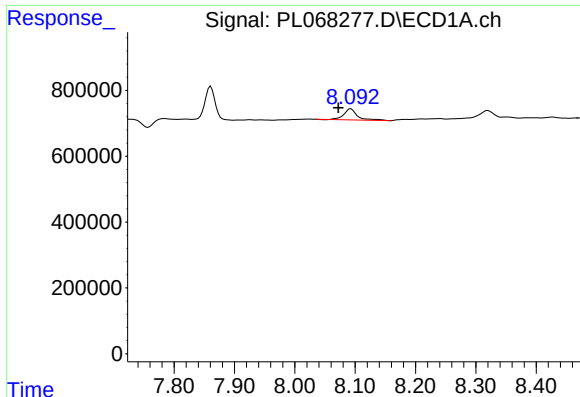

#14 Endrin


R.T.: 8.093 min
Delta R.T.: 0.021 min
Response: 541624
Conc: 1.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

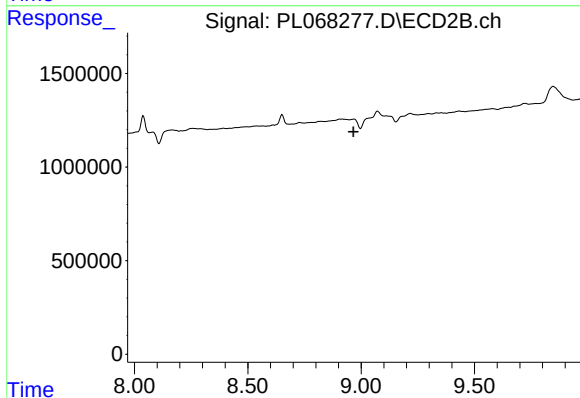


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.966 min
Response: 0
Conc: N.D.

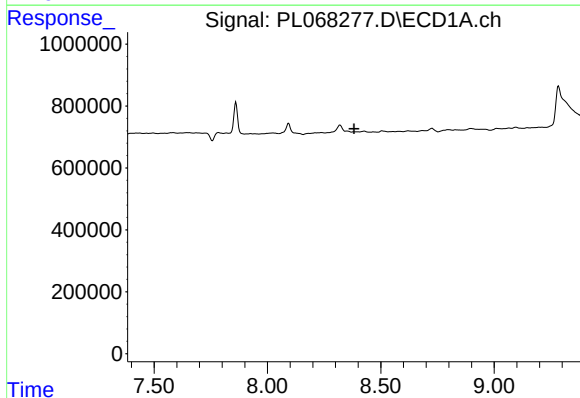


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

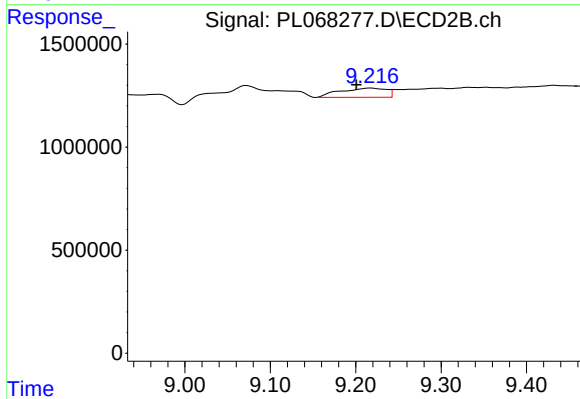

#15 Endosulfan II


R.T.: 9.217 min
Delta R.T.: 0.017 min
Response: 1675506
Conc: 1.85 ng/ml

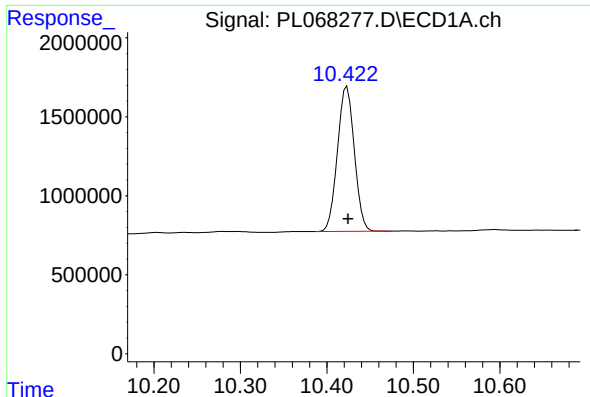

#28 Decachlorobiphenyl

R.T.: 10.423 min
Delta R.T.: -0.001 min
Response: 12373317
Conc: 22.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

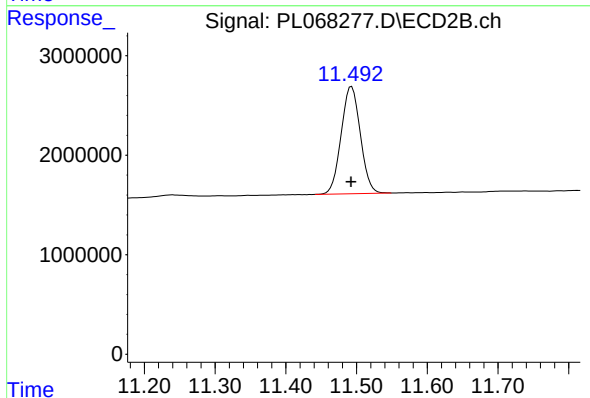

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 20308468
Conc: 22.77 ng/ml