

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 23:24
 Operator : AR\AJ
 Sample : M2076-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210587-AMENDED-COM-1-SPLP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 05:50:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.591f	8039077	18869977	18.731	18.492
28)	SA Decachlor...	10.421	11.512f	10847144	17208418	19.287	19.292
Target Compounds							
2)	A alpha-BHC	0.000	6.147	0	763298	N.D.	0.561 #
7)	B delta-BHC	0.000	7.062	0	720133	N.D.	0.588 #
15)	B Endosulfa...	0.000	9.193	0	229545	N.D.	0.253 #
16)	A 4,4'-DDD	0.000	9.092f	0	494364	N.D.	0.581 #
20)	A Methoxychlor	9.090	0.000	896993	0	2.868	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 23:24
Operator : AR\AJ
Sample : M2076-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20210587-AMENDED-COM-1-SPLP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 05:50:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

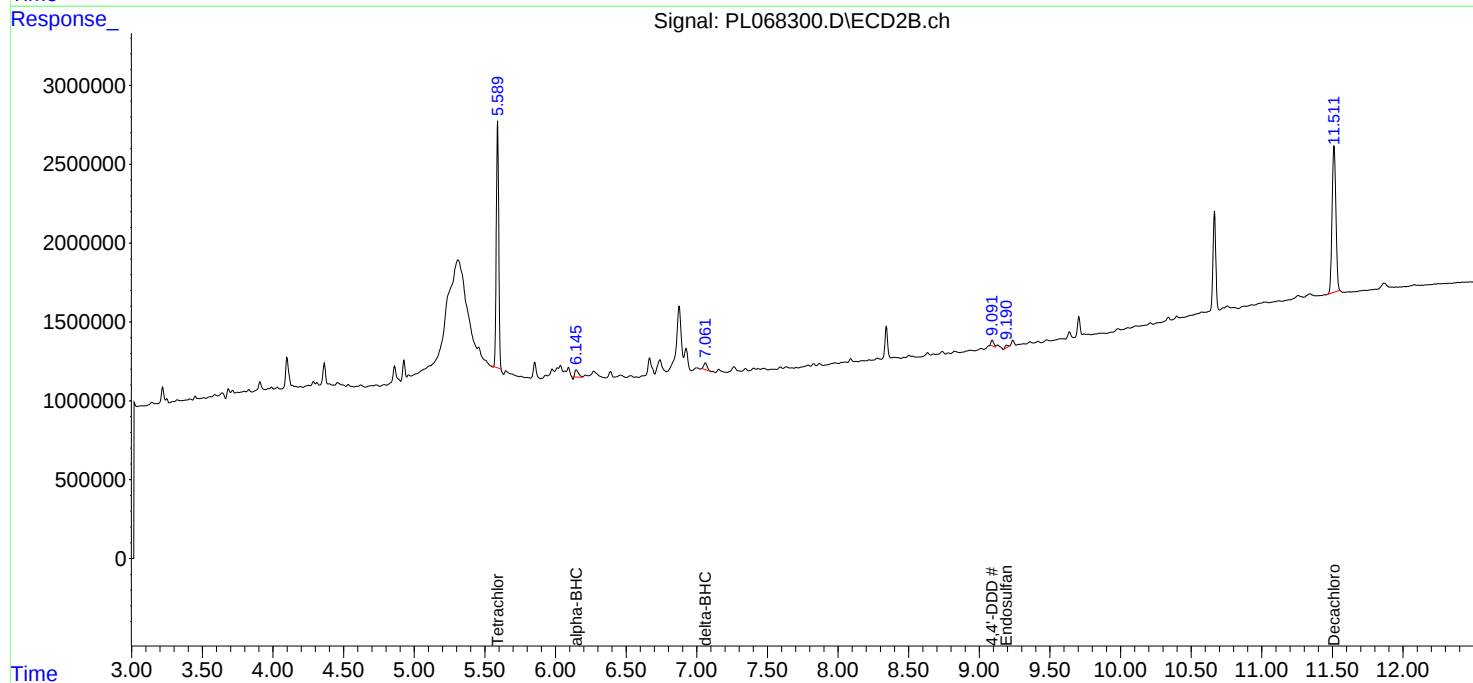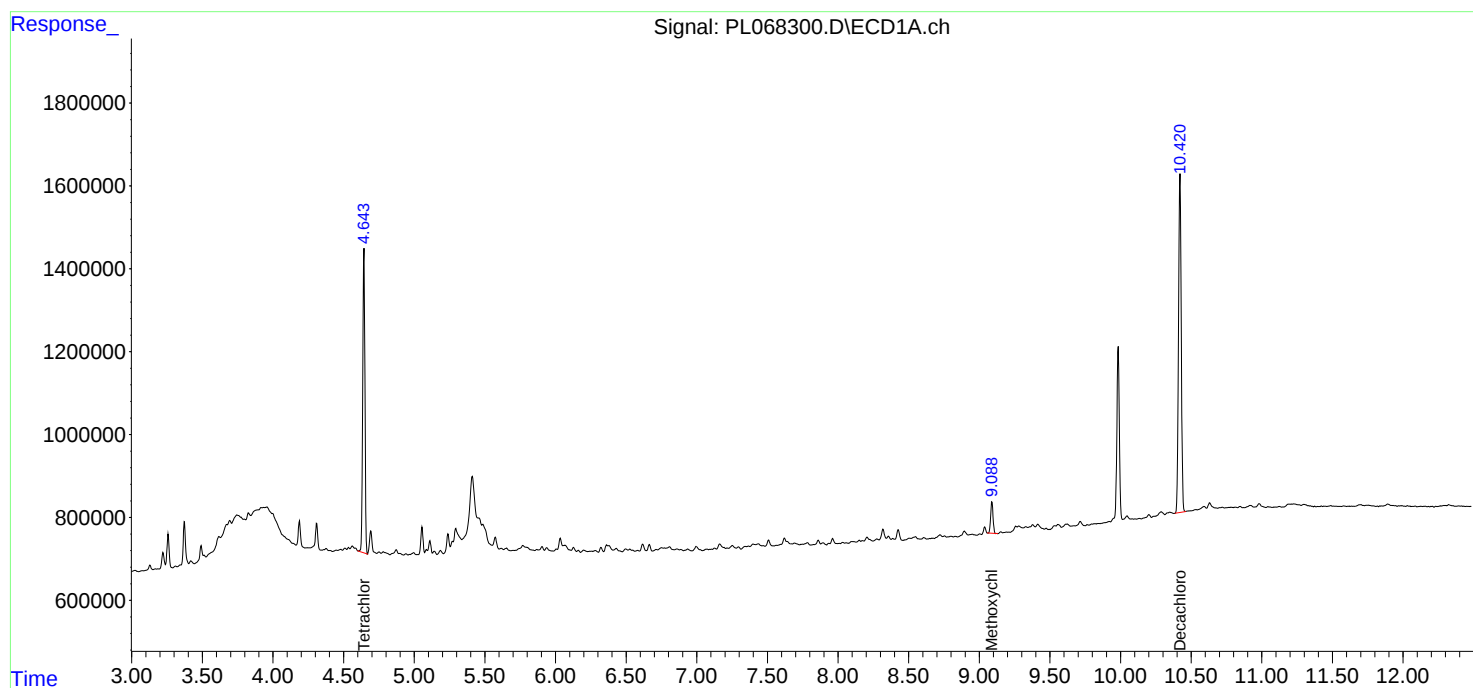


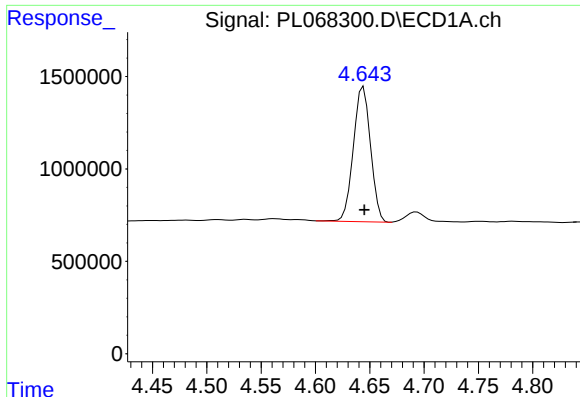

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 8039077
Conc: 18.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210587-AMENDED-COM-1-SPLP

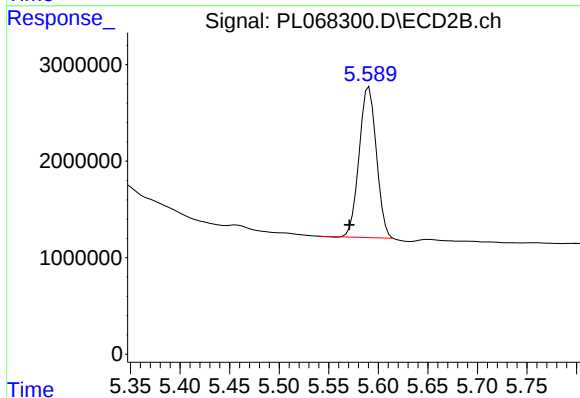


#1 Tetrachloro-m-xylene

R.T.: 5.591 min
Delta R.T.: 0.020 min
Response: 18869977
Conc: 18.49 ng/ml

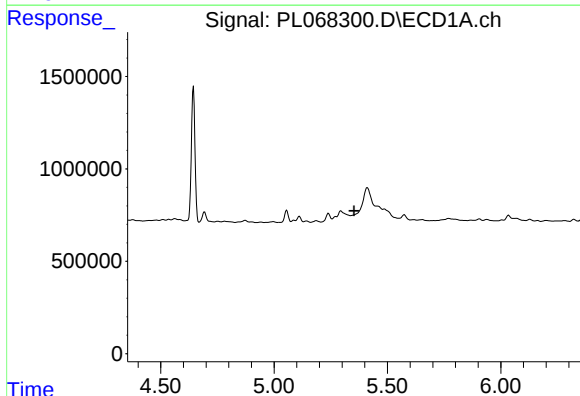


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.353 min
Response: 0
Conc: N.D.

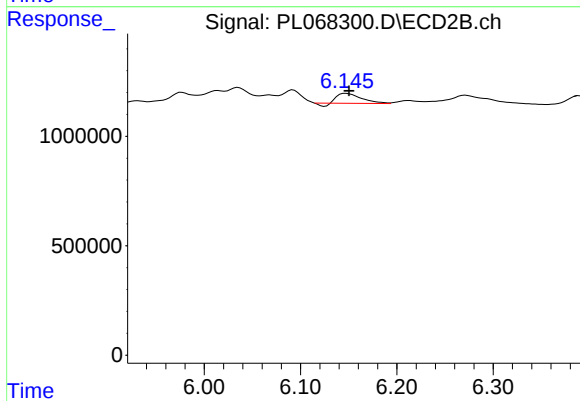

#2 alpha-BHC


R.T.: 6.147 min
Delta R.T.: -0.003 min
Response: 763298
Conc: 0.56 ng/ml

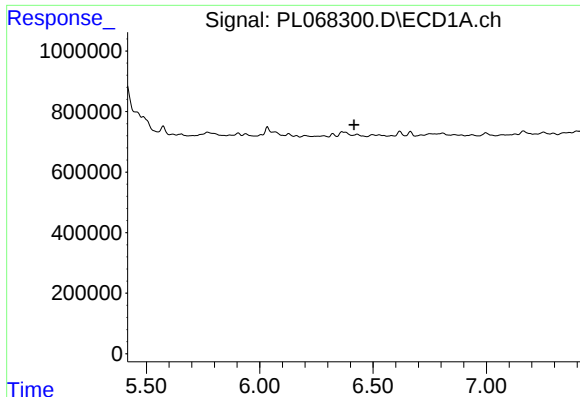

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.417 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210587-AMENDED-COM-1-SPLP

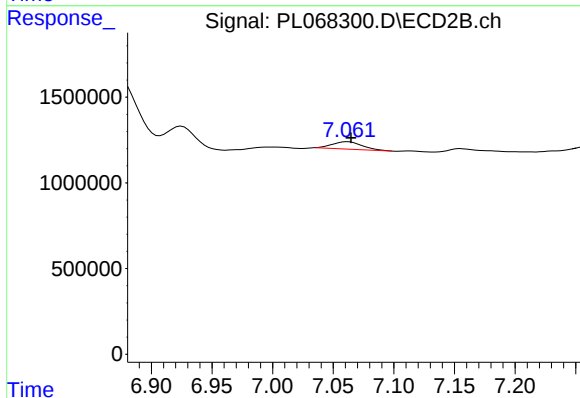


#7 delta-BHC

R.T.: 7.062 min
Delta R.T.: -0.003 min
Response: 720133
Conc: 0.59 ng/ml

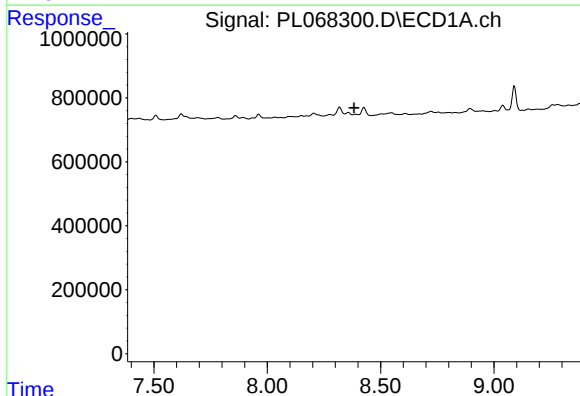


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

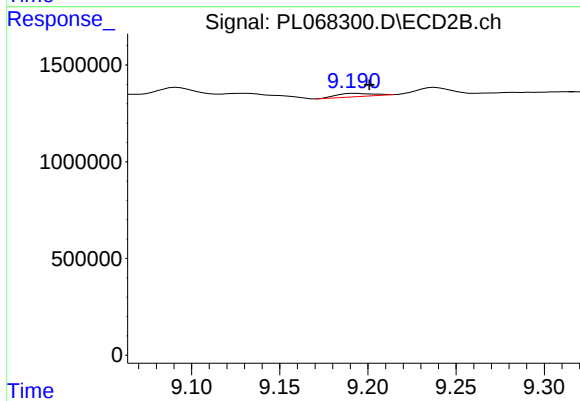

#15 Endosulfan II


R.T.: 9.193 min
Delta R.T.: -0.008 min
Response: 229545
Conc: 0.25 ng/ml

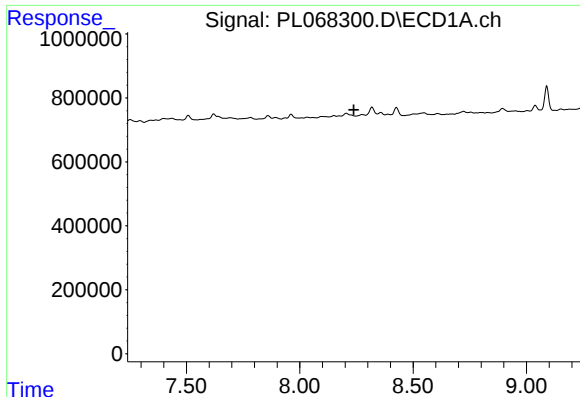

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210587-AMENDED-COM-1-SPLP

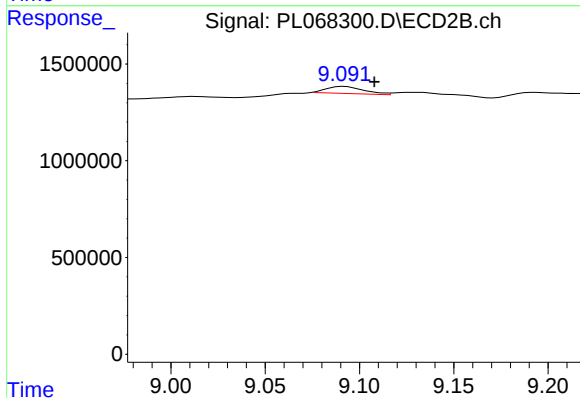


#16 4,4'-DDD

R.T.: 9.092 min
Delta R.T.: -0.016 min
Response: 494364
Conc: 0.58 ng/ml

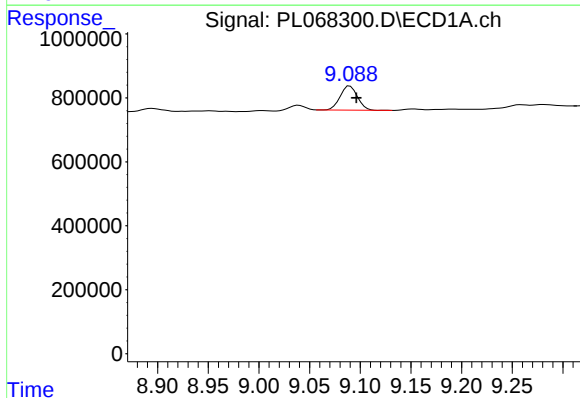


#20 Methoxychlor

R.T.: 9.090 min
Delta R.T.: -0.006 min
Response: 896993
Conc: 2.87 ng/ml

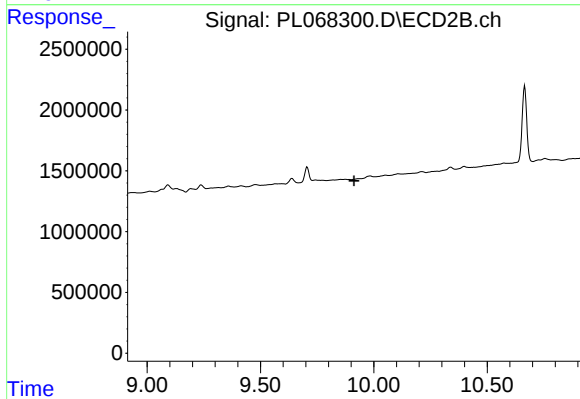

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.913 min
Response: 0
Conc: N.D.

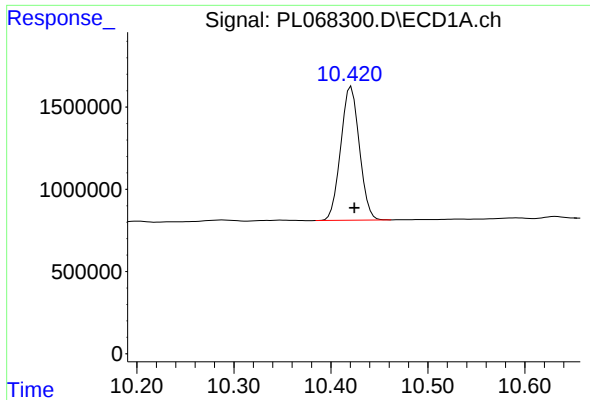

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: -0.003 min
Response: 10847144
Conc: 19.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210587-AMENDED-COM-1-SPLP

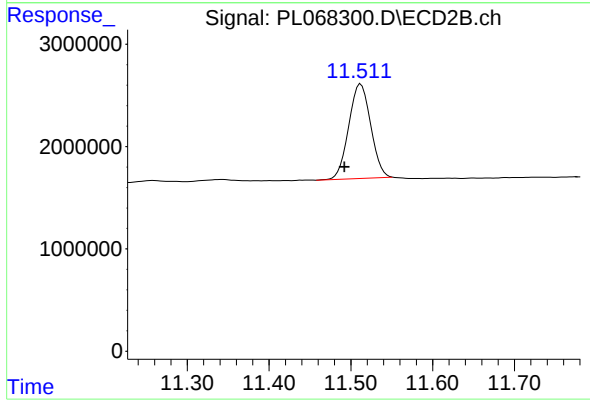

#28 Decachlorobiphenyl

R.T.: 11.512 min
Delta R.T.: 0.020 min
Response: 17208418
Conc: 19.29 ng/ml