

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2021 04:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 05:54:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.571	8845594	21604599	20.610	21.172
28)	SA Decachlor...	10.421	11.492	12417780	20585176	22.079	23.078
Target Compounds							
4)	MA Heptachlor	6.164f	0.000	391677	0	0.643	N.D. #
6)	B beta-BHC	6.164	0.000	391677	0	1.339	N.D. #
8)	B Heptachlo...	0.000	8.039	0	3945983	N.D.	3.490 #
10)	B gamma-Chl...	0.000	8.298	0	974521	N.D.	0.865 #
13)	MA Dieldrin	7.785	0.000	28249	0	0.052	N.D. #
14)	MA Endrin	8.091f	0.000	822689	0	1.645	N.D. #
15)	B Endosulfa...	0.000	9.216f	0	628857	N.D.	0.694 #
22)	Mirex	0.000	10.568f	0	151006	N.D.	0.195 #
25)	Chlordane-3	0.000	8.298	0	974521	N.D.	6.293 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2021 04:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 05:54:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

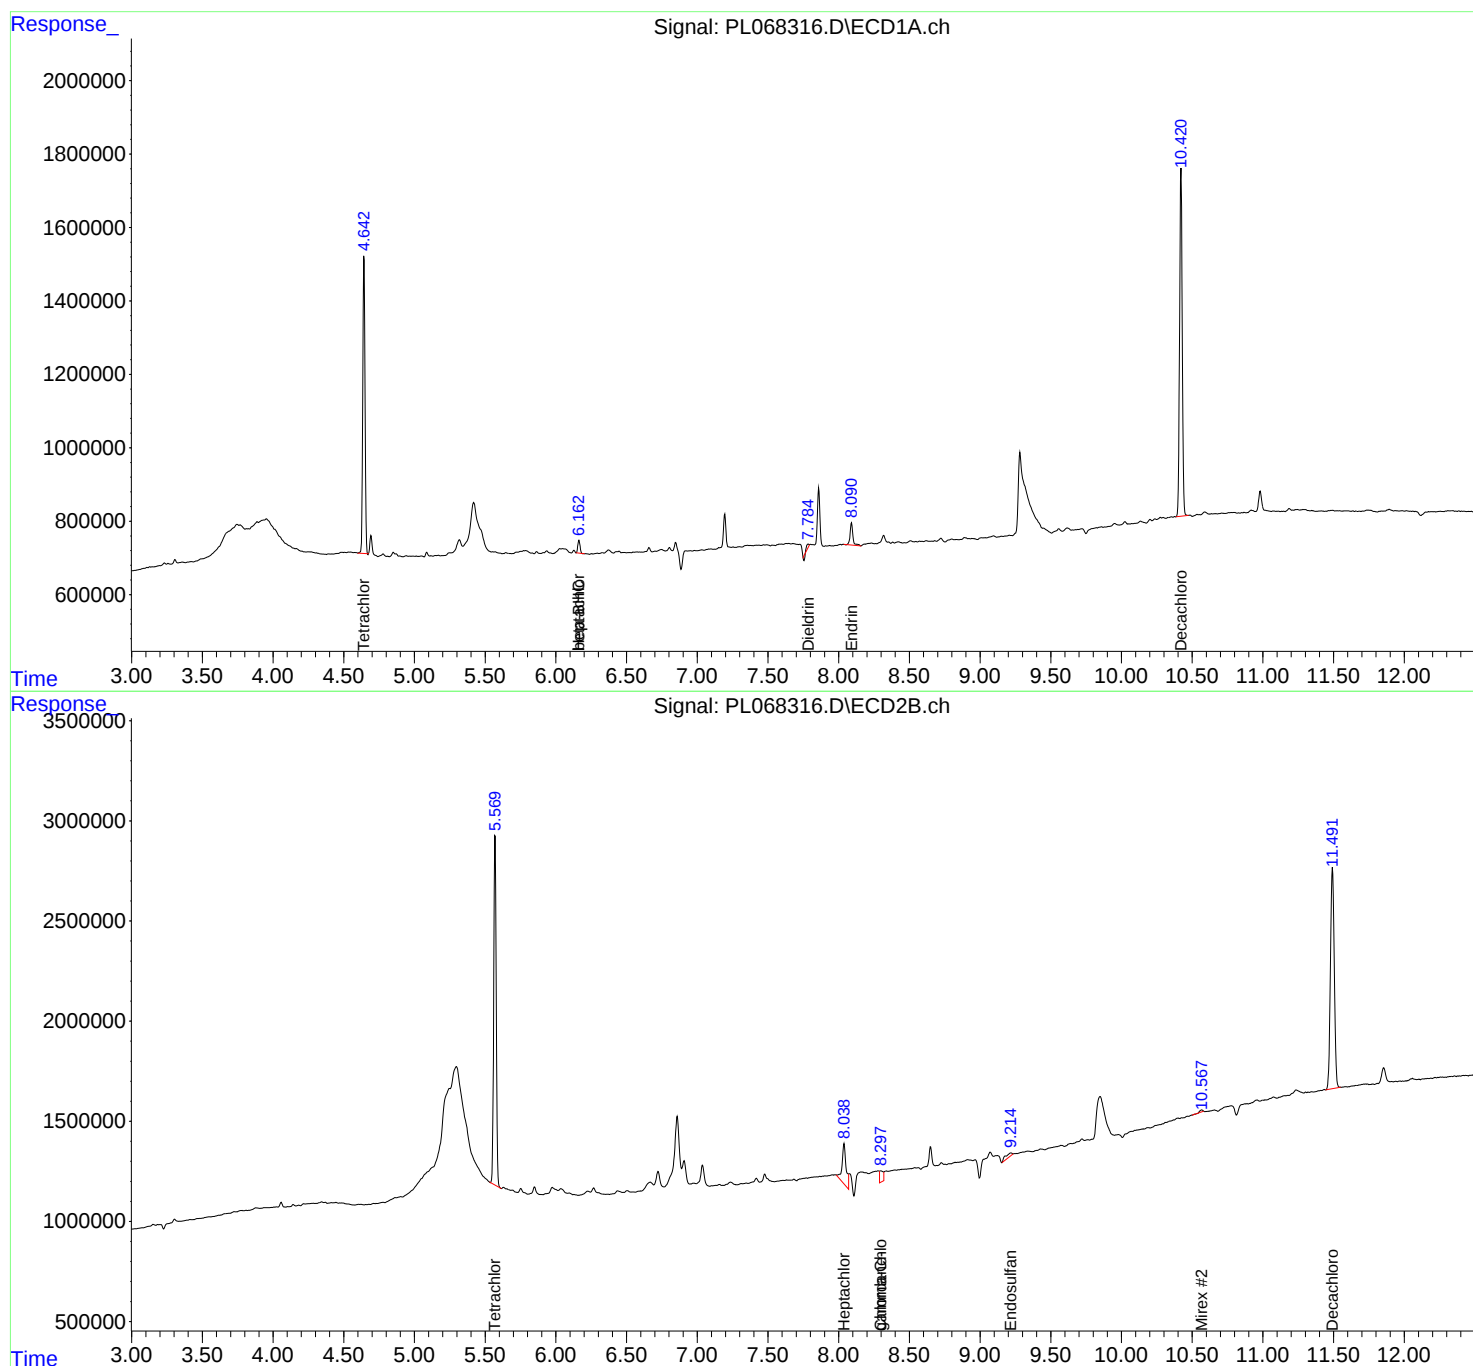


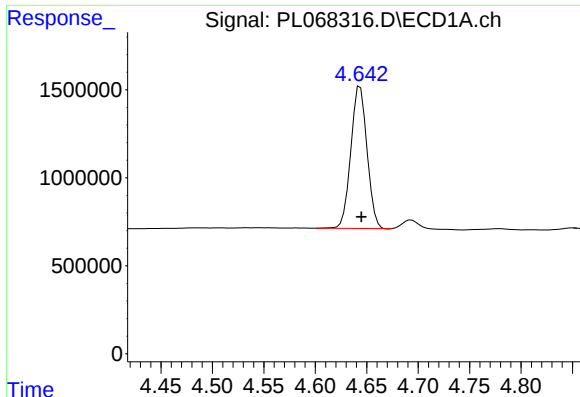

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: -0.001 min
Response: 8845594
Conc: 20.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

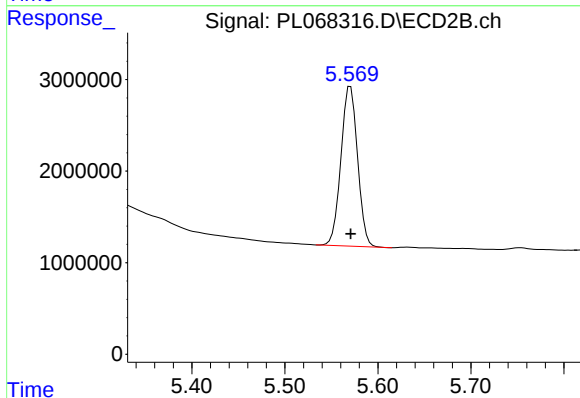


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 21604599
Conc: 21.17 ng/ml

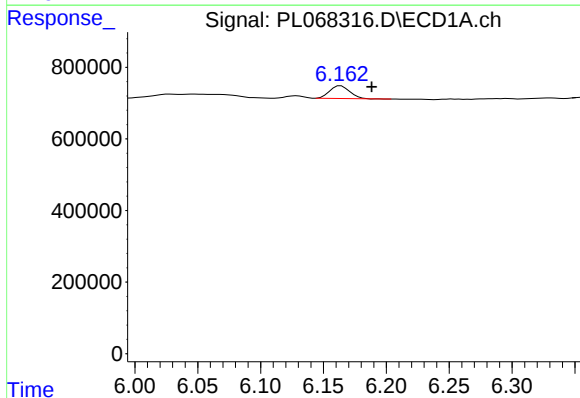


#4 Heptachlor

R.T.: 6.164 min
Delta R.T.: -0.025 min
Response: 391677
Conc: 0.64 ng/ml

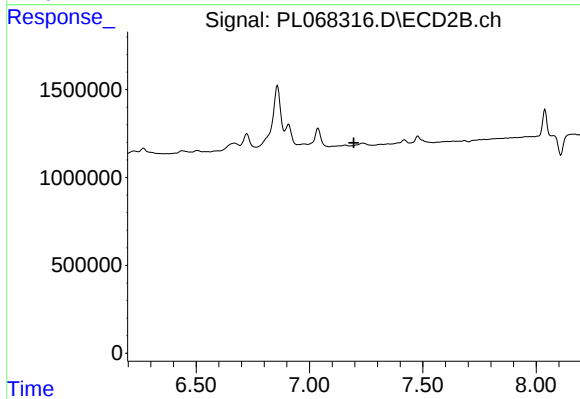

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

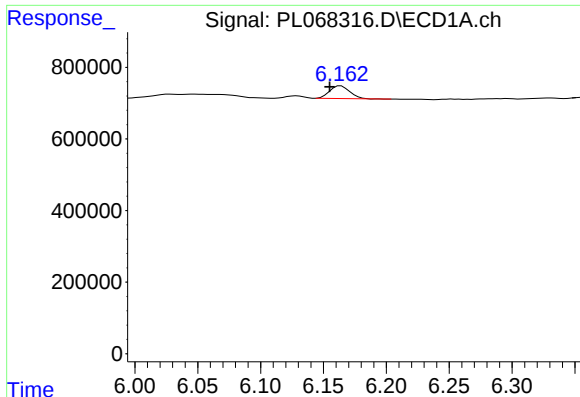

#6 beta-BHC


R.T.: 6.164 min
Delta R.T.: 0.009 min
Response: 391677
Conc: 1.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

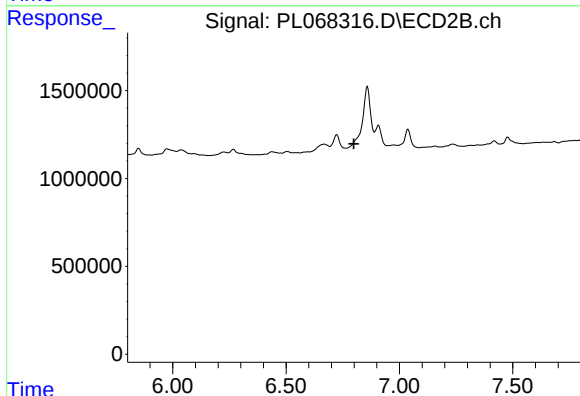


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

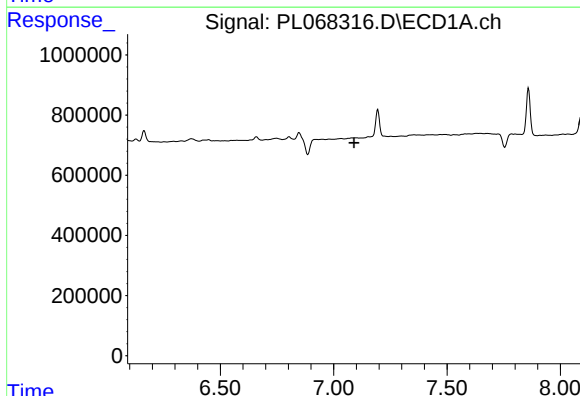


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

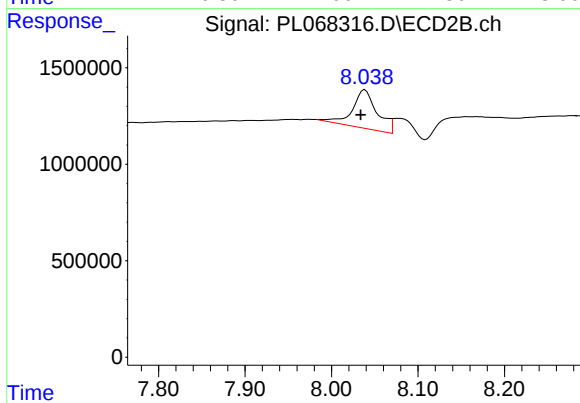

#8 Heptachlor epoxide


R.T.: 8.039 min
Delta R.T.: 0.005 min
Response: 3945983
Conc: 3.49 ng/ml

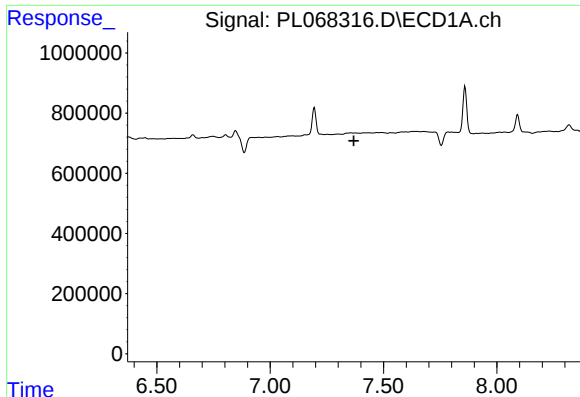

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

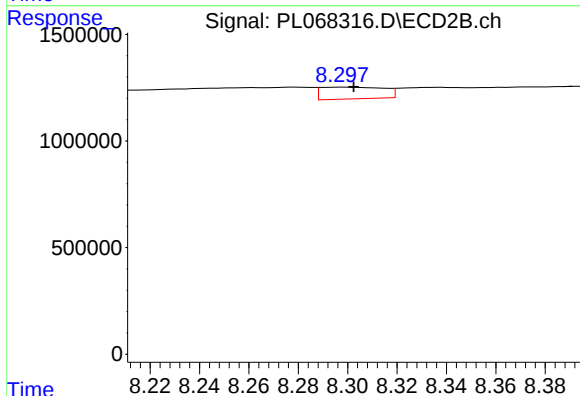


#10 gamma-Chlordane

R.T.: 8.298 min
Delta R.T.: -0.004 min
Response: 974521
Conc: 0.87 ng/ml

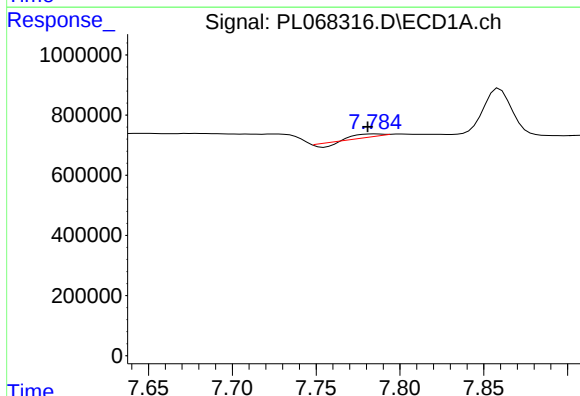


#13 Dieldrin

R.T.: 7.785 min
Delta R.T.: 0.004 min
Response: 28249
Conc: 0.05 ng/ml

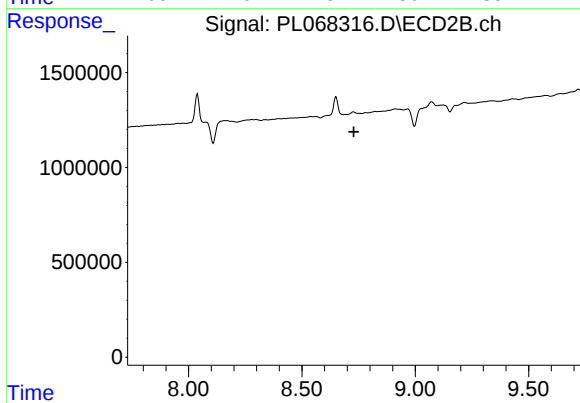

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.728 min
Response: 0
Conc: N.D.

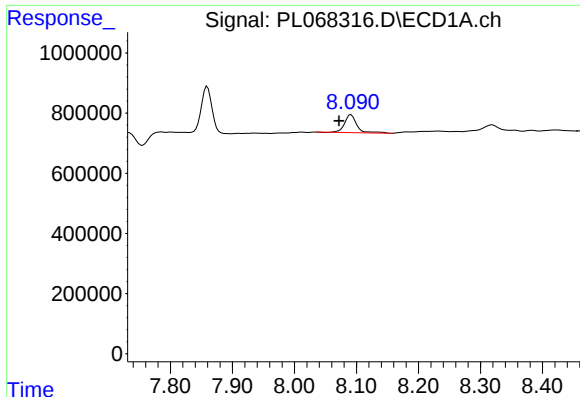

#14 Endrin


R.T.: 8.091 min
Delta R.T.: 0.019 min
Response: 822689
Conc: 1.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

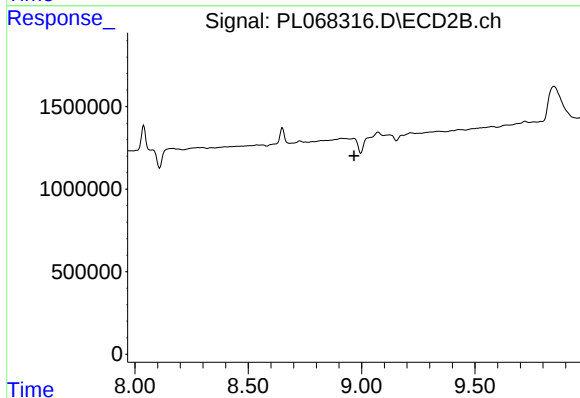


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.966 min
Response: 0
Conc: N.D.

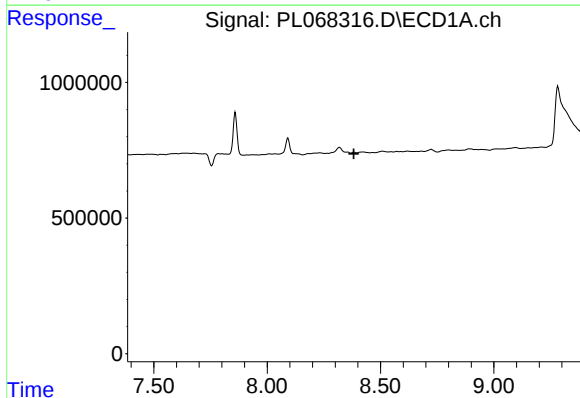


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

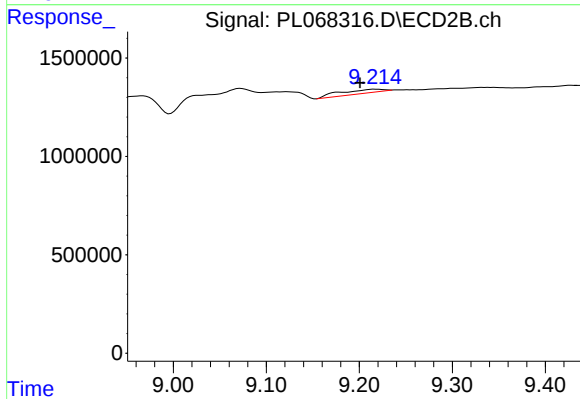

#15 Endosulfan II


R.T.: 9.216 min
Delta R.T.: 0.016 min
Response: 628857
Conc: 0.69 ng/ml

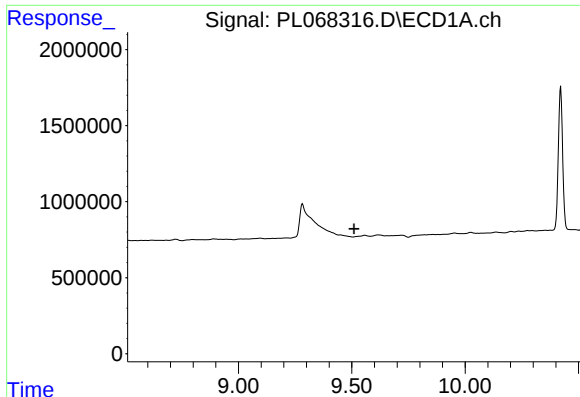

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

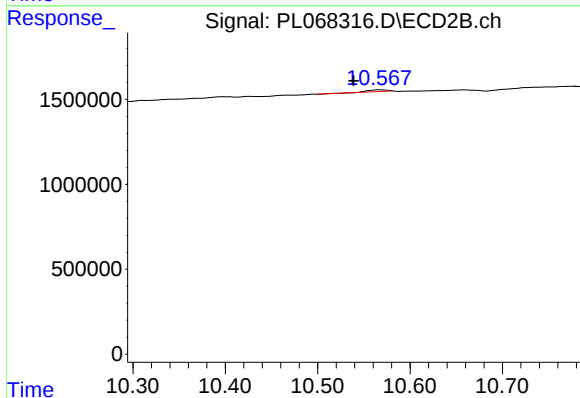


#22 Mirex

R.T.: 10.568 min
Delta R.T.: 0.029 min
Response: 151006
Conc: 0.20 ng/ml

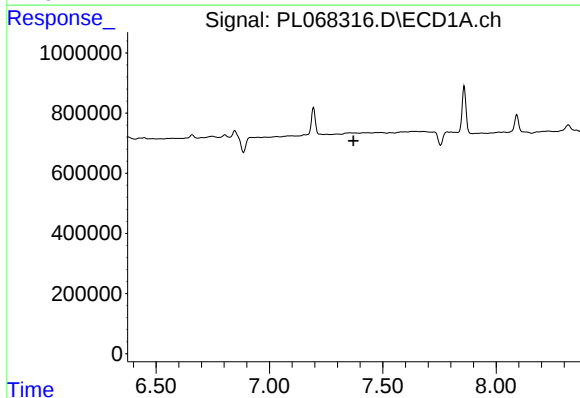


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.371 min
Response: 0
Conc: N.D.

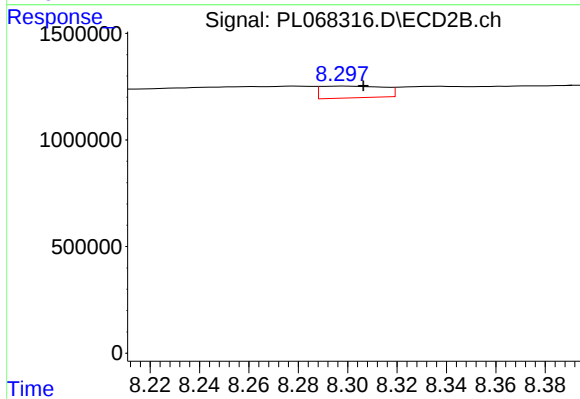

#25 Chlordane-3


R.T.: 8.298 min
Delta R.T.: -0.008 min
Response: 974521
Conc: 6.29 ng/ml

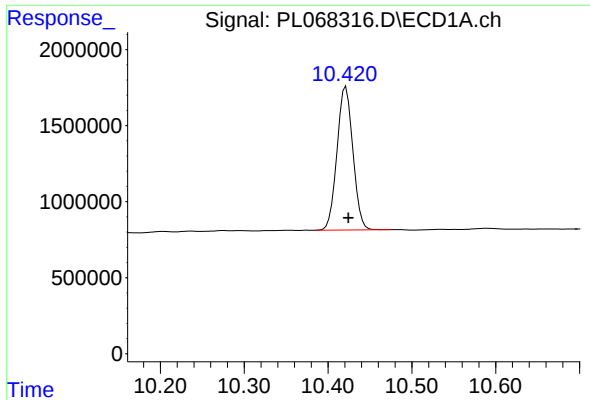

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: -0.003 min
Response: 12417780
Conc: 22.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

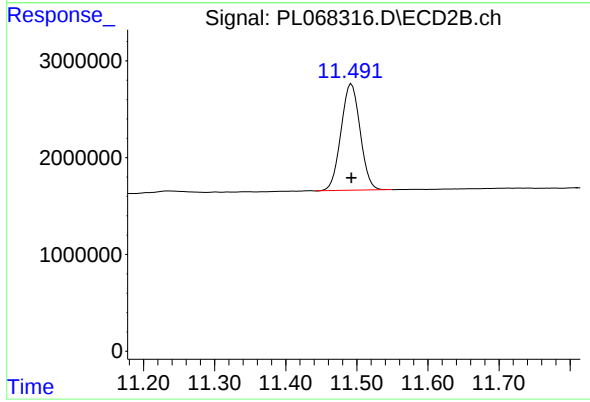

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: 0.000 min
Response: 20585176
Conc: 23.08 ng/ml