

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2021 07:42
 Operator : AR\AJ
 Sample : M3093-05
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210543-COM-16

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 08:50:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.571	8376642	20223924	19.518	19.819
28)	SA Decachlor...	10.421	11.493	7968602	13556954	14.168	15.199
Target Compounds							
10)	B gamma-Chl...	0.000	8.325f	0	842283	N.D.	0.748 #
15)	B Endosulfa...	0.000	9.219f	0	699837	N.D.	0.772 #
25)	Chlordane-3	0.000	8.325f	0	842283	N.D.	5.439 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2021 07:42
Operator : AR\AJ
Sample : M3093-05
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20210543-COM-16

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 08:50:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

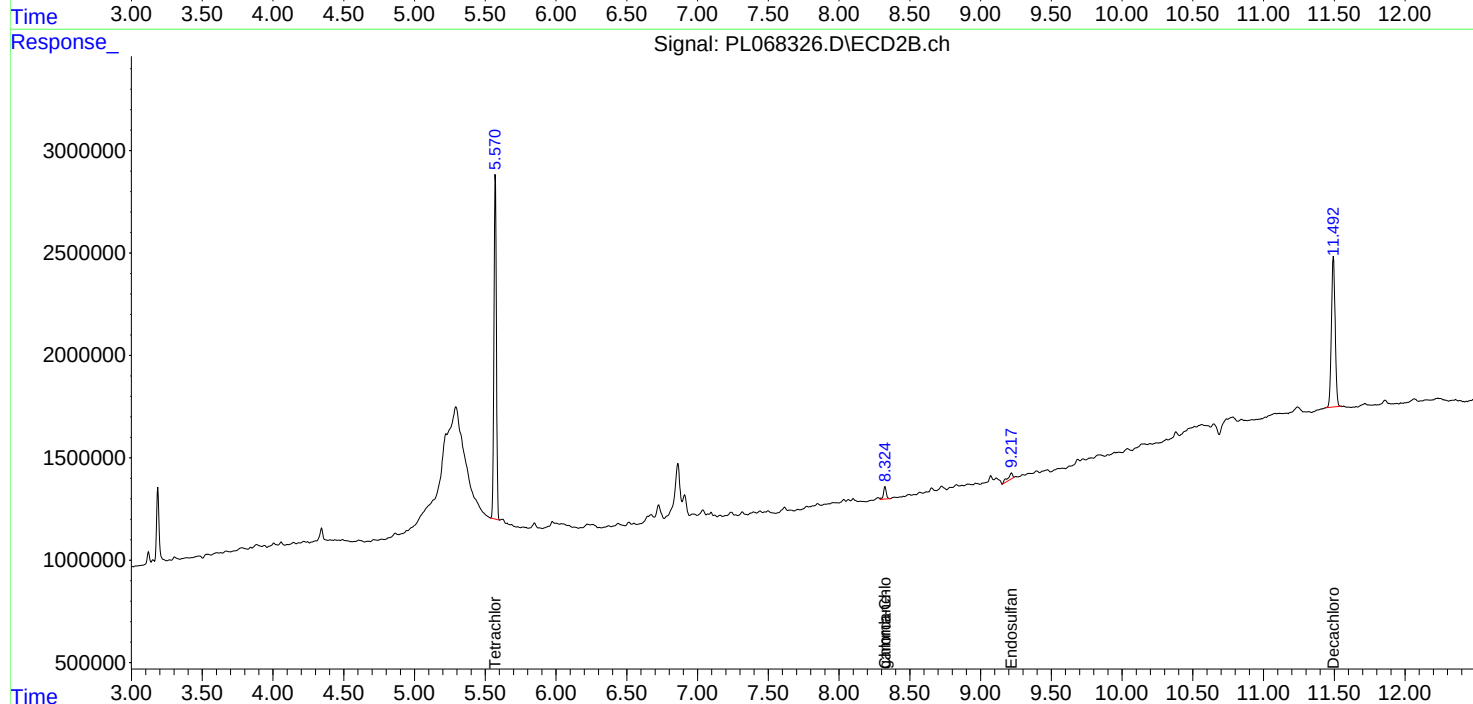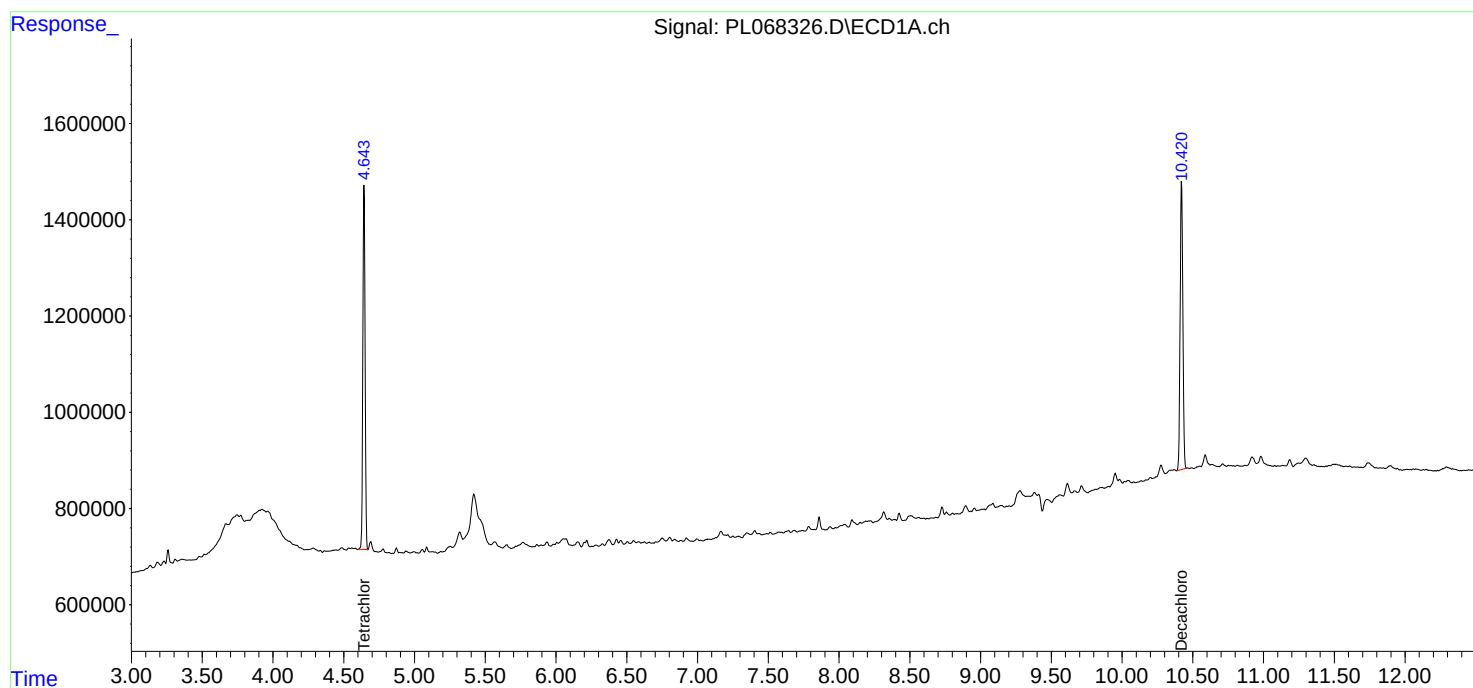


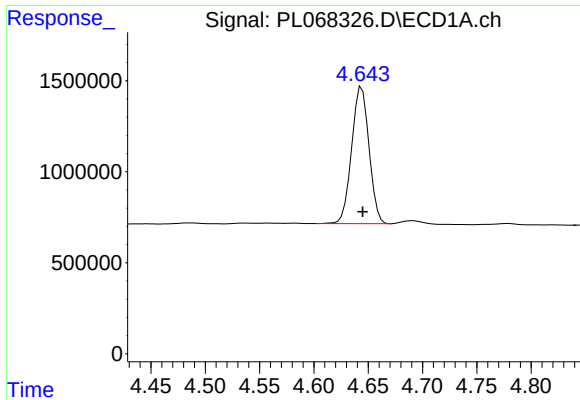

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 8376642
Conc: 19.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210543-COM-16

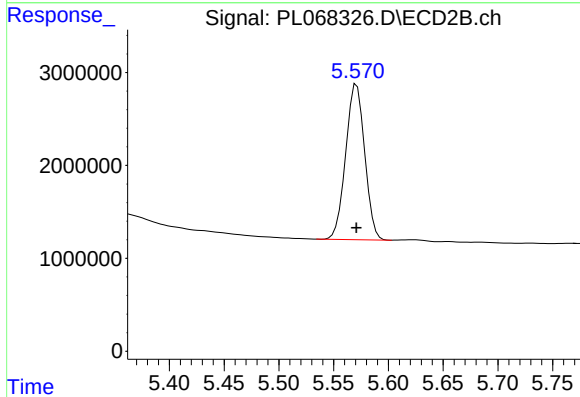


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 20223924
Conc: 19.82 ng/ml

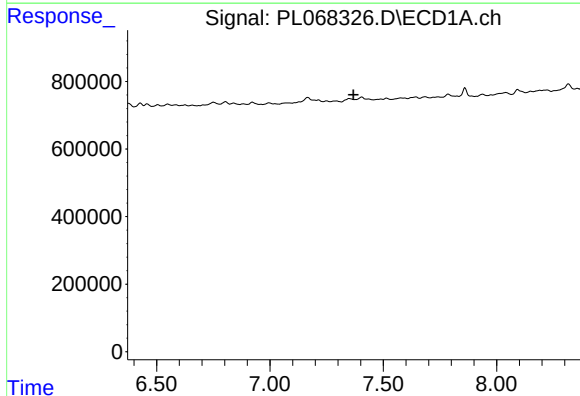


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.369 min
Response: 0
Conc: N.D.

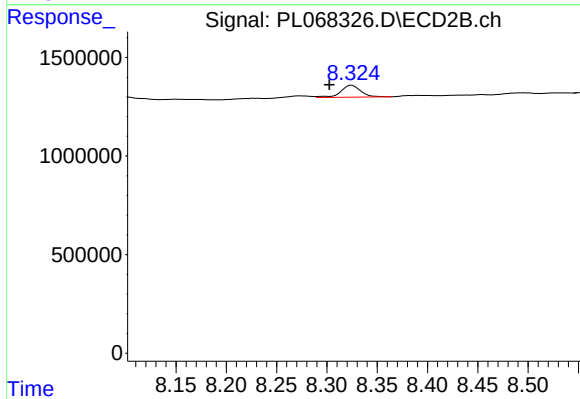

#10 gamma-Chlordane


R.T.: 8.325 min
Delta R.T.: 0.022 min
Response: 842283
Conc: 0.75 ng/ml

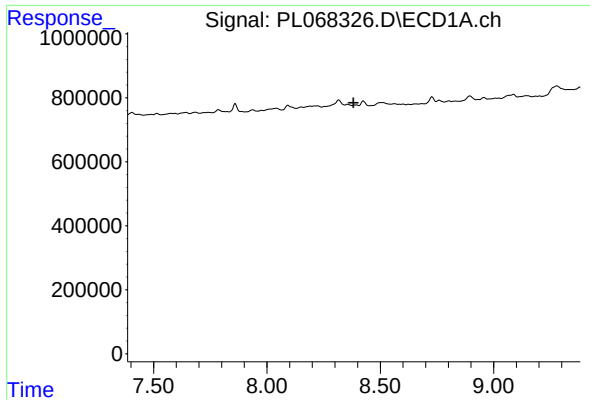

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210543-COM-16

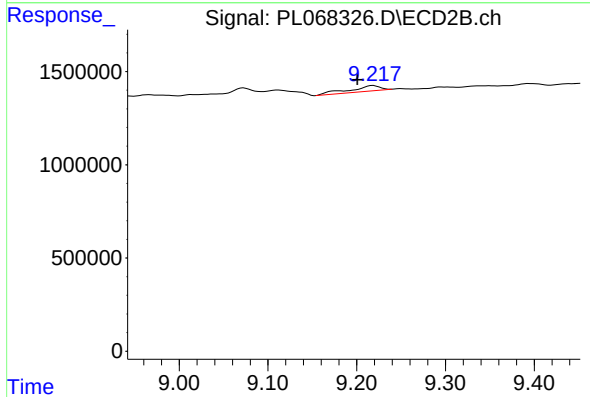


#15 Endosulfan II

R.T.: 9.219 min
Delta R.T.: 0.018 min
Response: 699837
Conc: 0.77 ng/ml

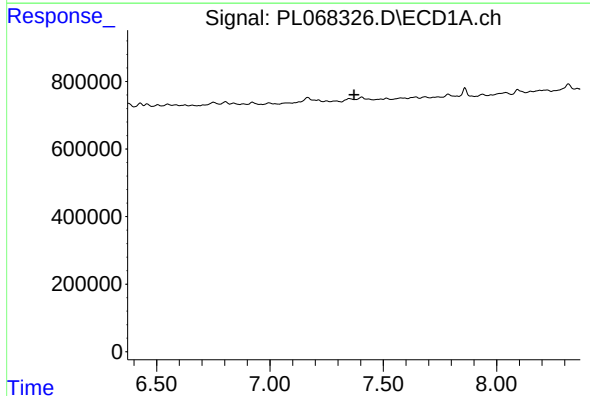


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.371 min
Response: 0
Conc: N.D.

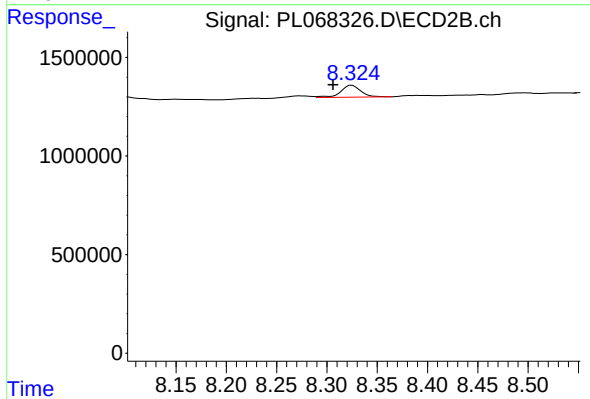

#25 Chlordane-3


R.T.: 8.325 min
Delta R.T.: 0.019 min
Response: 842283
Conc: 5.44 ng/ml

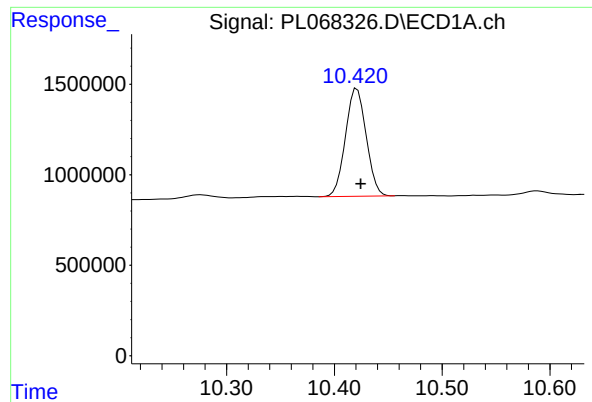

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: -0.003 min
Response: 7968602
Conc: 14.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210543-COM-16

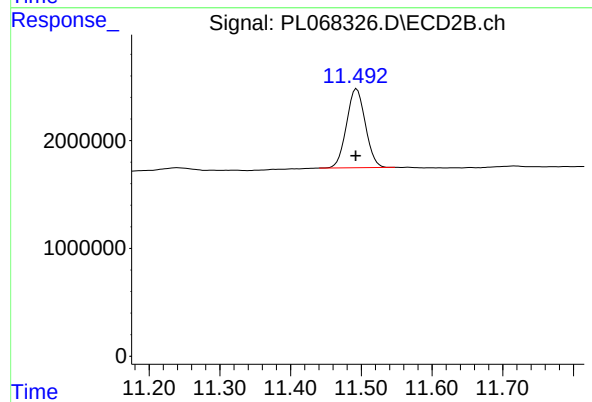

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.001 min
Response: 13556954
Conc: 15.20 ng/ml