

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 10:20
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 11:03:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:03:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.646	5.573	26693540	54324003	50.000	50.000
28)	SA Decachlor...	10.427	11.498	27846087	46495847	50.000	50.000
Target Compounds							
23)	Chlordane-1	5.979	6.958	7607854	19883505	500.000	500.000
24)	Chlordane-2	6.668	7.549	10641957	21606057	500.000	500.000
25)	Chlordane-3	7.371	8.307	27249009	80434157	500.000	500.000
26)	Chlordane-4	7.440	8.389	28603852	97141200	500.000	500.000
27)	Chlordane-5	8.391	9.278	10122452	16816202	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 10:20
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 11:03:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:03:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

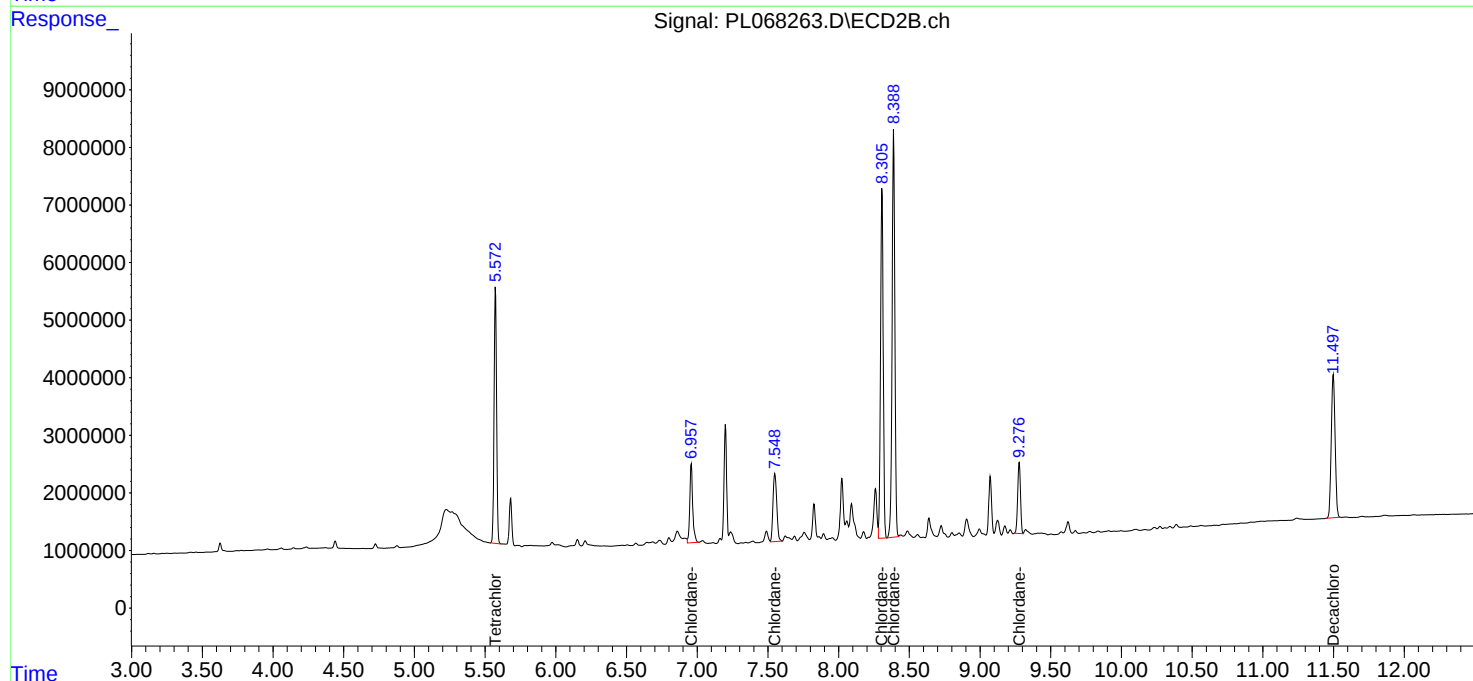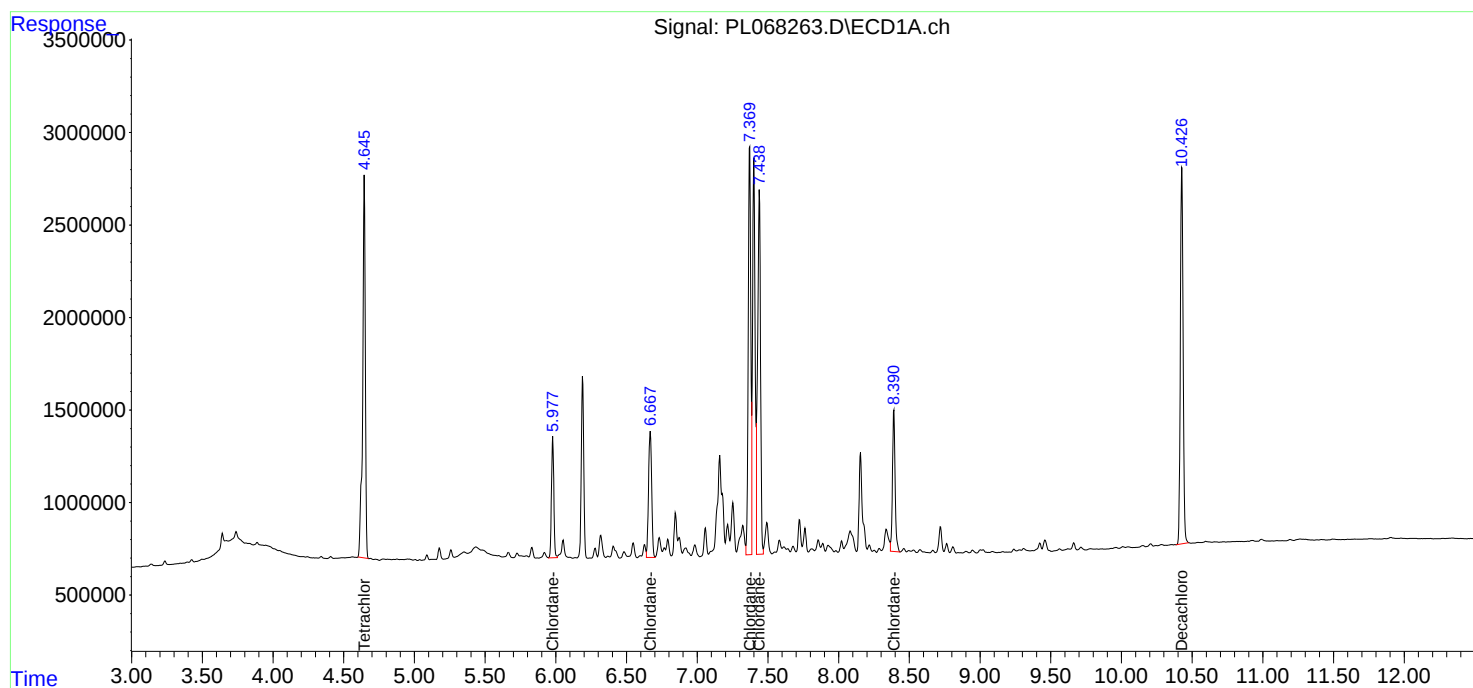


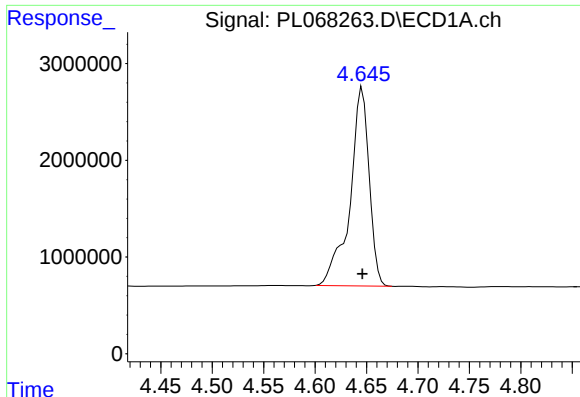

#1 Tetrachloro-m-xylene


R.T.: 4.646 min
Delta R.T.: 0.000 min
Response: 26693540
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

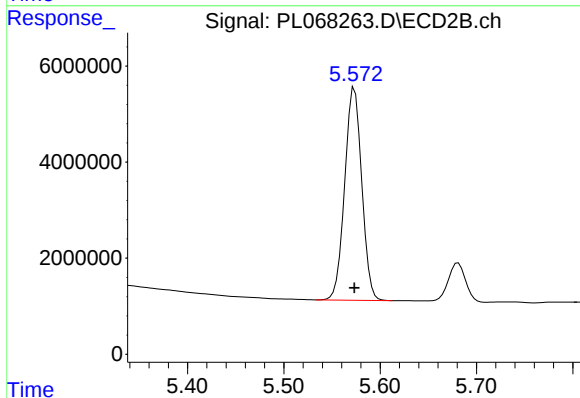


#1 Tetrachloro-m-xylene

R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 54324003
Conc: 50.00 ng/ml

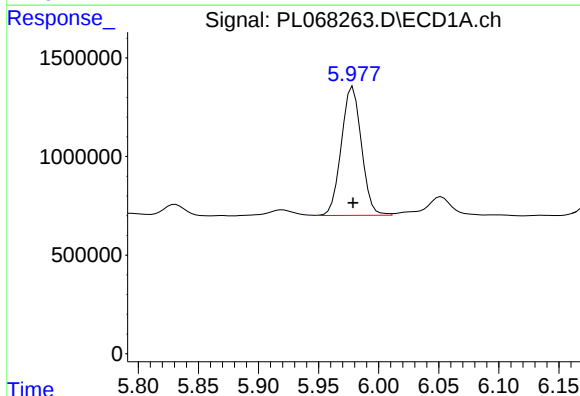


#23 Chlordane-1

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 7607854
Conc: 500.00 ng/ml

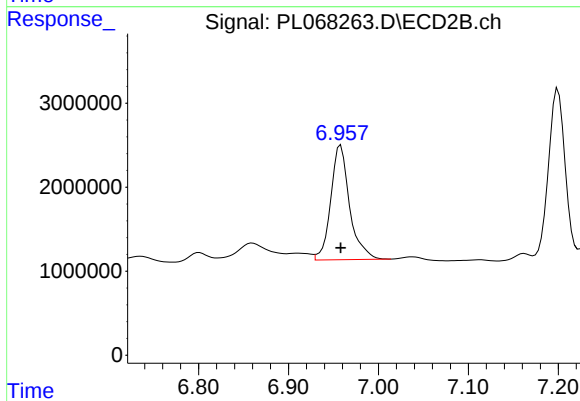

#23 Chlordane-1


R.T.: 6.958 min
Delta R.T.: 0.000 min
Response: 19883505
Conc: 500.00 ng/ml

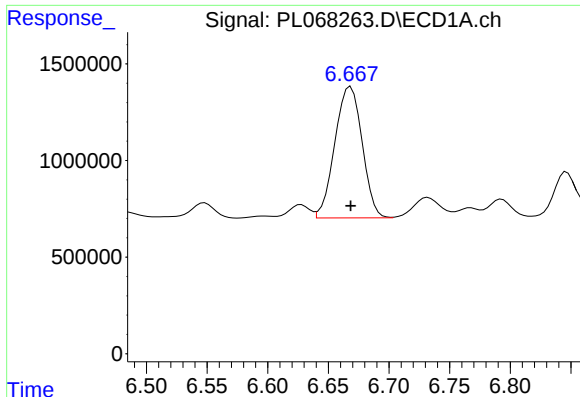

#24 Chlordane-2


R.T.: 6.668 min
Delta R.T.: 0.000 min
Response: 10641957
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

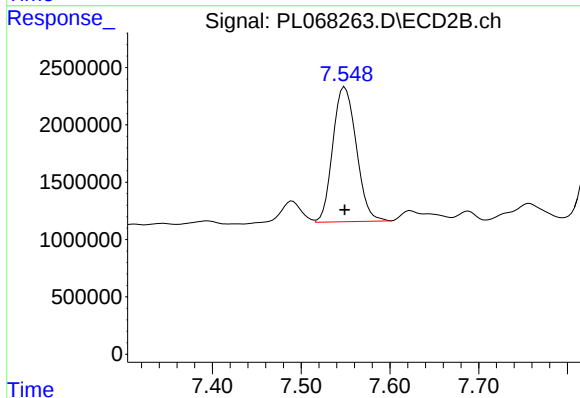


#24 Chlordane-2

R.T.: 7.549 min
Delta R.T.: 0.000 min
Response: 21606057
Conc: 500.00 ng/ml

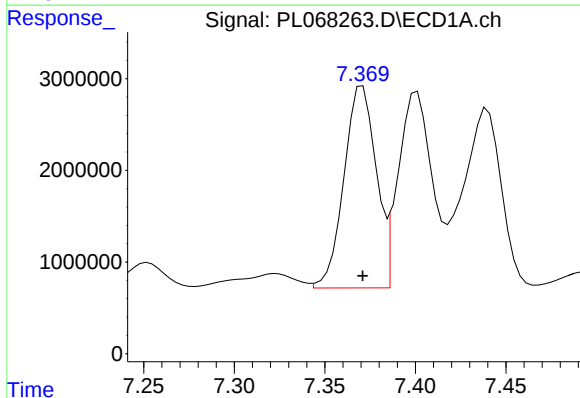


#25 Chlordane-3

R.T.: 7.371 min
Delta R.T.: 0.000 min
Response: 27249009
Conc: 500.00 ng/ml

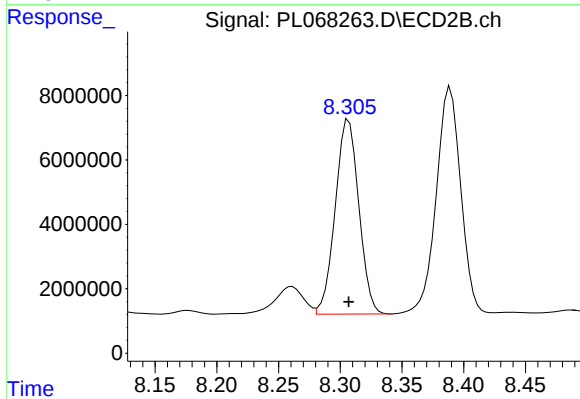

#25 Chlordane-3


R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 80434157
Conc: 500.00 ng/ml

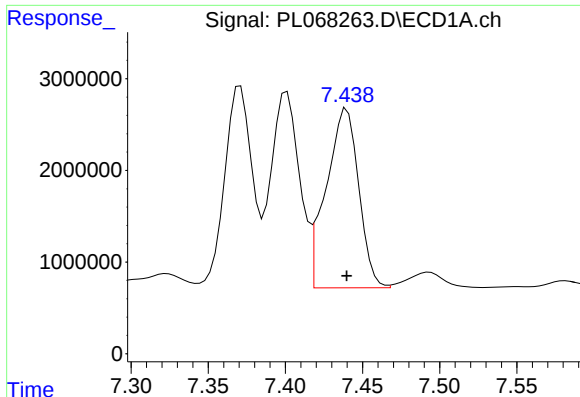

#26 Chlordane-4


R.T.: 7.440 min
Delta R.T.: 0.000 min
Response: 28603852
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

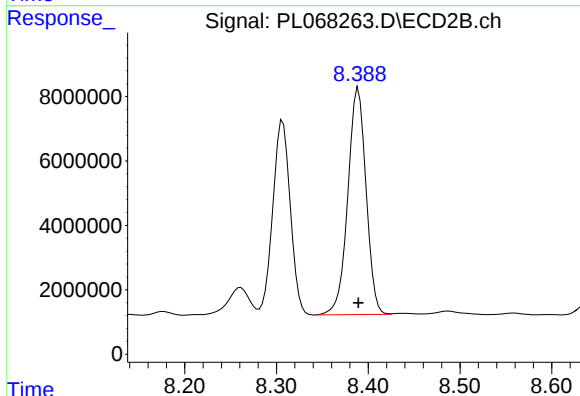


#26 Chlordane-4

R.T.: 8.389 min
Delta R.T.: 0.000 min
Response: 97141200
Conc: 500.00 ng/ml

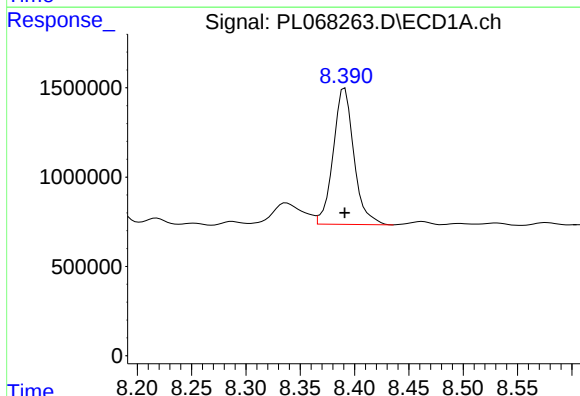


#27 Chlordane-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 10122452
Conc: 500.00 ng/ml

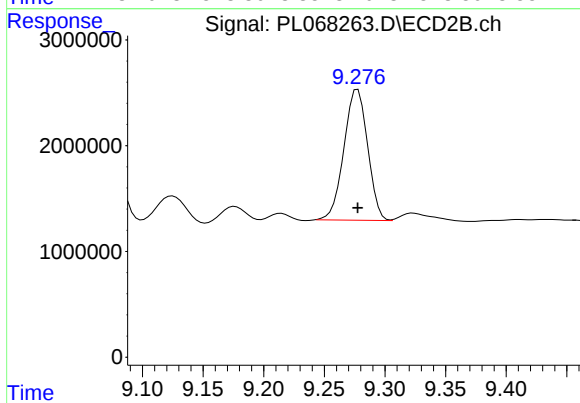

#27 Chlordane-5


R.T.: 9.278 min
Delta R.T.: 0.000 min
Response: 16816202
Conc: 500.00 ng/ml

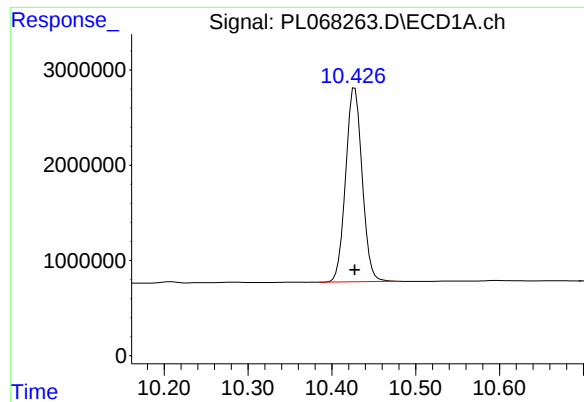

#28 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: 0.000 min
Response: 27846087
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

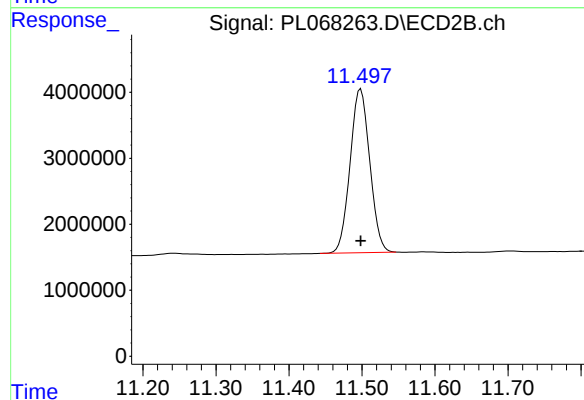

#28 Decachlorobiphenyl

R.T.: 11.498 min
Delta R.T.: 0.000 min
Response: 46495847
Conc: 50.00 ng/ml