

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 10:37
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 11:05:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:03:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.646	5.574	13101952	25968468	24.541	23.901
28)	SA Decachlor...	10.427	11.498	14345639	23437799	25.759	25.204
Target Compounds							
23)	Chlordane-1	5.979	6.958	3818637	9758289	250.967	245.387
24)	Chlordane-2	6.669	7.549	5565643	10539078	261.495	243.892
25)	Chlordane-3	7.371	8.307	13192226	37473309	242.068	232.944
26)	Chlordane-4	7.440	8.389	13893030	45752737	242.852	235.496
27)	Chlordane-5	8.391	9.278	4978571	7965219	245.917	236.832



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 10:37
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 11:05:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:03:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

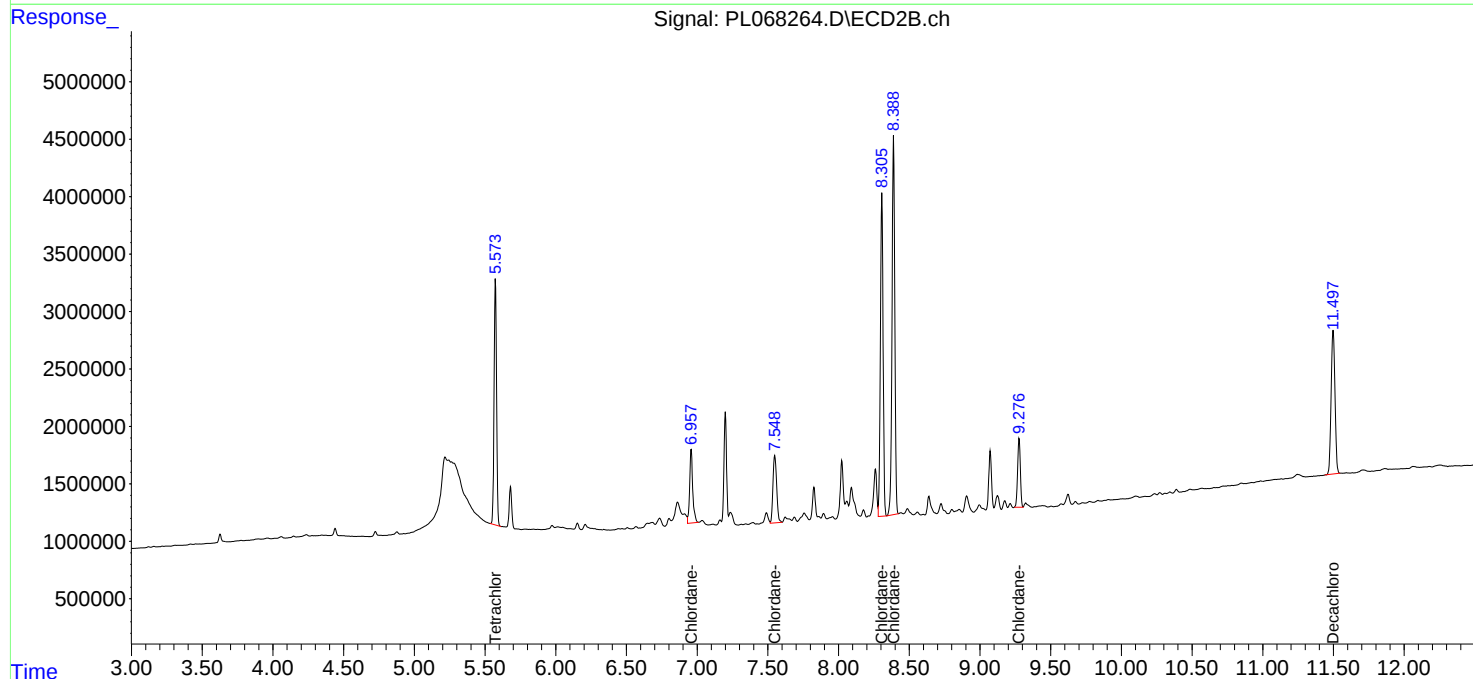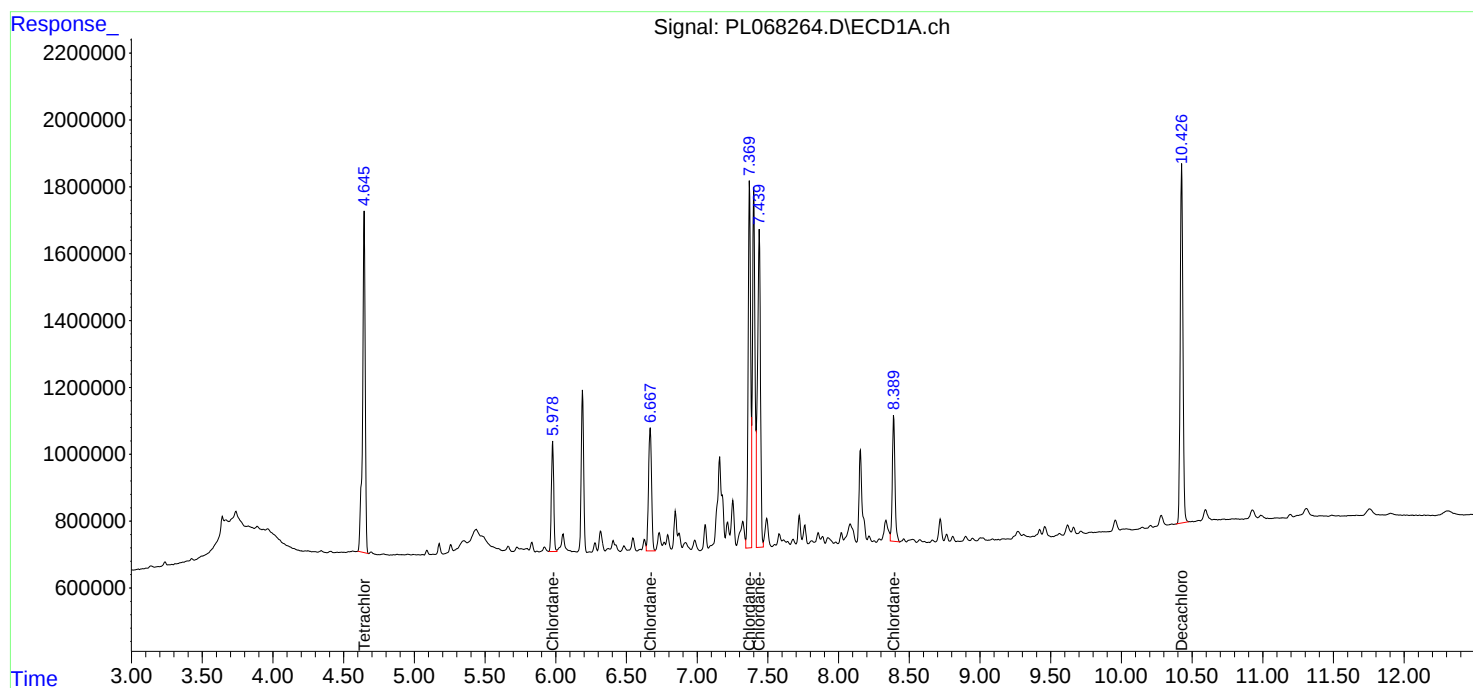


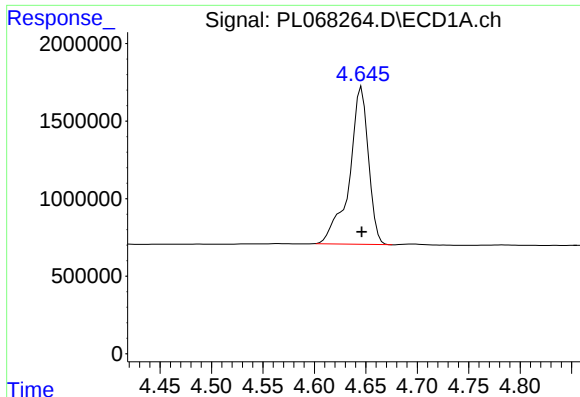

#1 Tetrachloro-m-xylene


R.T.: 4.646 min
Delta R.T.: 0.000 min
Response: 13101952
Conc: 24.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

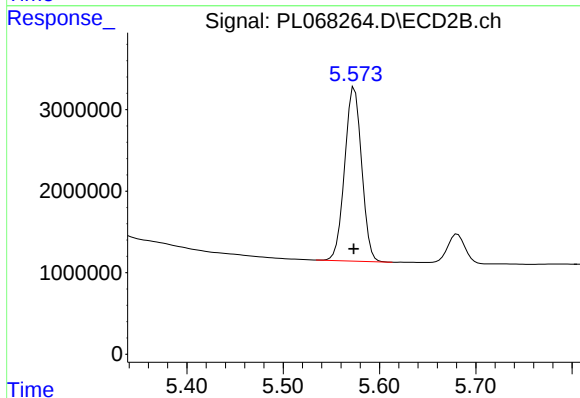


#1 Tetrachloro-m-xylene

R.T.: 5.574 min
Delta R.T.: 0.000 min
Response: 25968468
Conc: 23.90 ng/ml

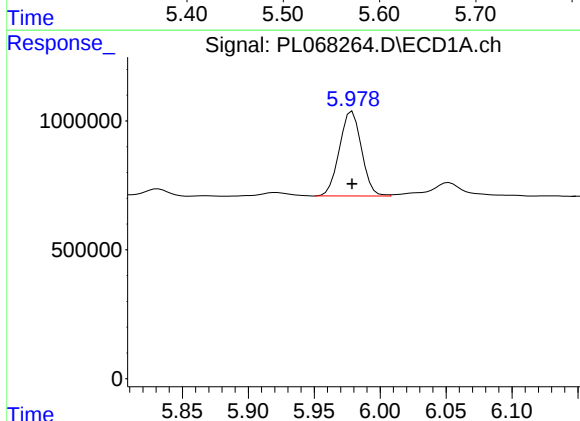


#23 Chlordane-1

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 3818637
Conc: 250.97 ng/ml

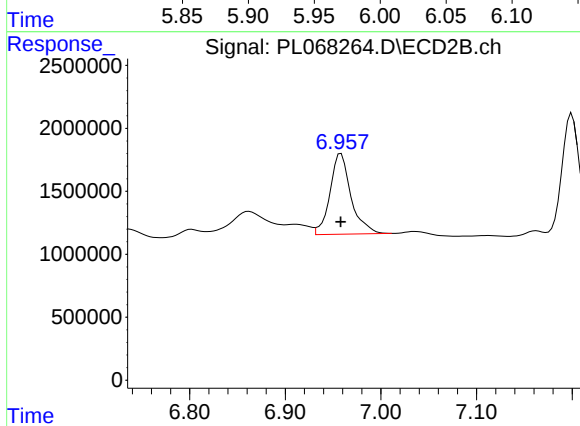

#23 Chlordane-1


R.T.: 6.958 min
Delta R.T.: 0.000 min
Response: 9758289
Conc: 245.39 ng/ml

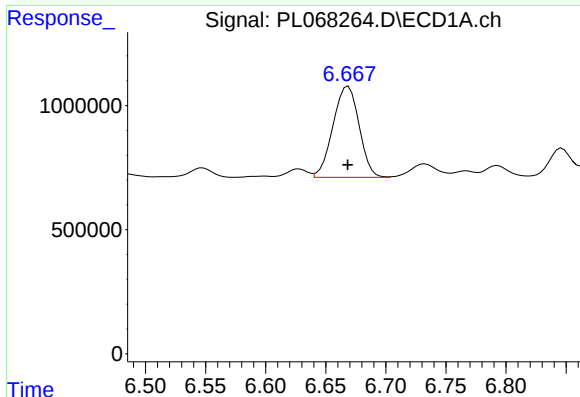

#24 Chlordane-2


R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 5565643
Conc: 261.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

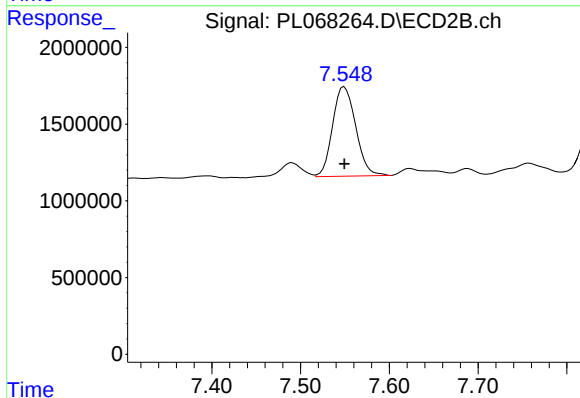


#24 Chlordane-2

R.T.: 7.549 min
Delta R.T.: 0.000 min
Response: 10539078
Conc: 243.89 ng/ml

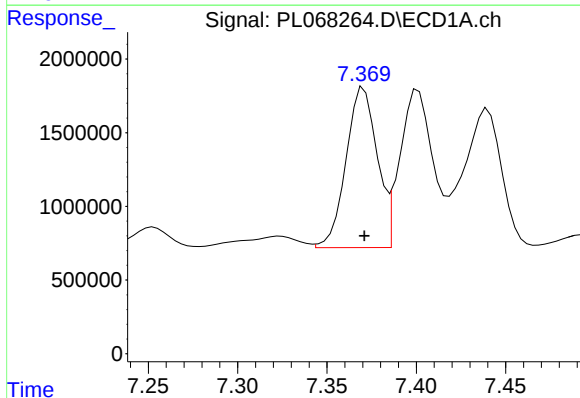


#25 Chlordane-3

R.T.: 7.371 min
Delta R.T.: 0.000 min
Response: 13192226
Conc: 242.07 ng/ml

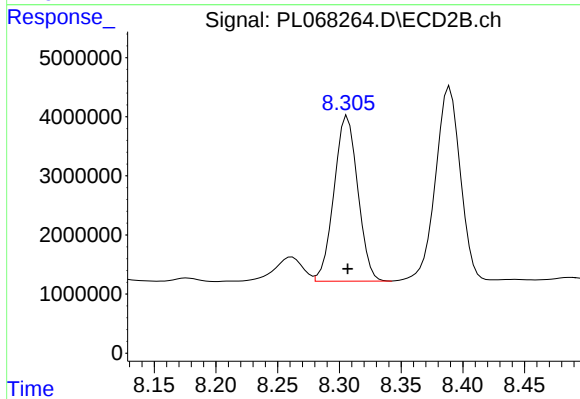

#25 Chlordane-3


R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 37473309
Conc: 232.94 ng/ml

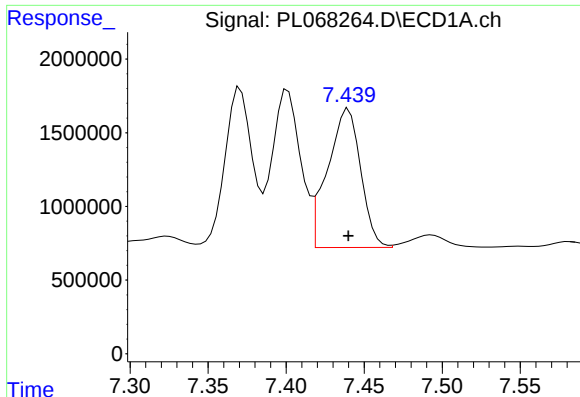

#26 Chlordane-4


R.T.: 7.440 min
Delta R.T.: 0.000 min
Response: 13893030
Conc: 242.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

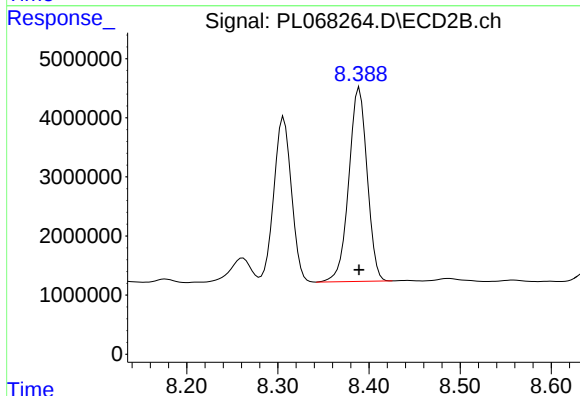


#26 Chlordane-4

R.T.: 8.389 min
Delta R.T.: 0.000 min
Response: 45752737
Conc: 235.50 ng/ml

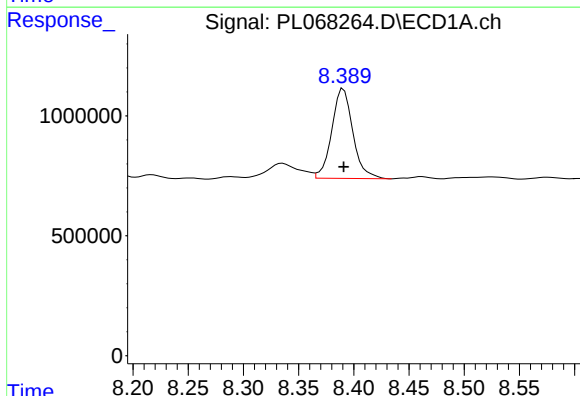


#27 Chlordane-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 4978571
Conc: 245.92 ng/ml

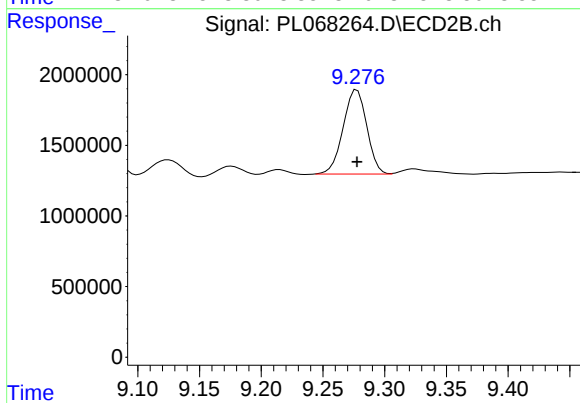

#27 Chlordane-5


R.T.: 9.278 min
Delta R.T.: 0.000 min
Response: 7965219
Conc: 236.83 ng/ml

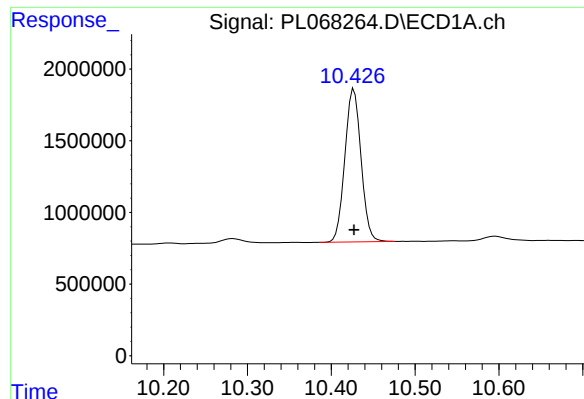

#28 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: 0.000 min
Response: 14345639
Conc: 25.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

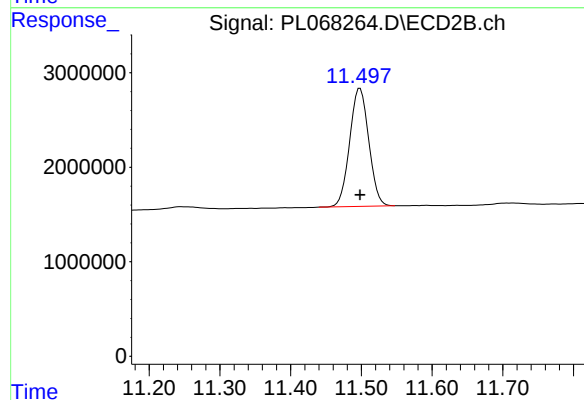

#28 Decachlorobiphenyl

R.T.: 11.498 min
Delta R.T.: 0.000 min
Response: 23437799
Conc: 25.20 ng/ml