

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 11:10
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL072021CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 11:25:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:09:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.647	5.574	26404727	53408932	49.949	50.796
28)	SA Decachlor...	10.428	11.499	27375017	45082249	48.976	49.130
Target Compounds							
23)	Chlordane-1	5.979	6.958	7532689	19398586	500.769	478.861
24)	Chlordane-2	6.669	7.550	10604659	21167141	494.457	508.764
25)	Chlordane-3	7.372	8.307	27154376	78529189	504.224	507.066
26)	Chlordane-4	7.440	8.390	28497778	94991924	504.745	506.676
27)	Chlordane-5	8.391	9.278	9948158	16479004	494.288	514.154



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 11:10
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL072021CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 11:25:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:09:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

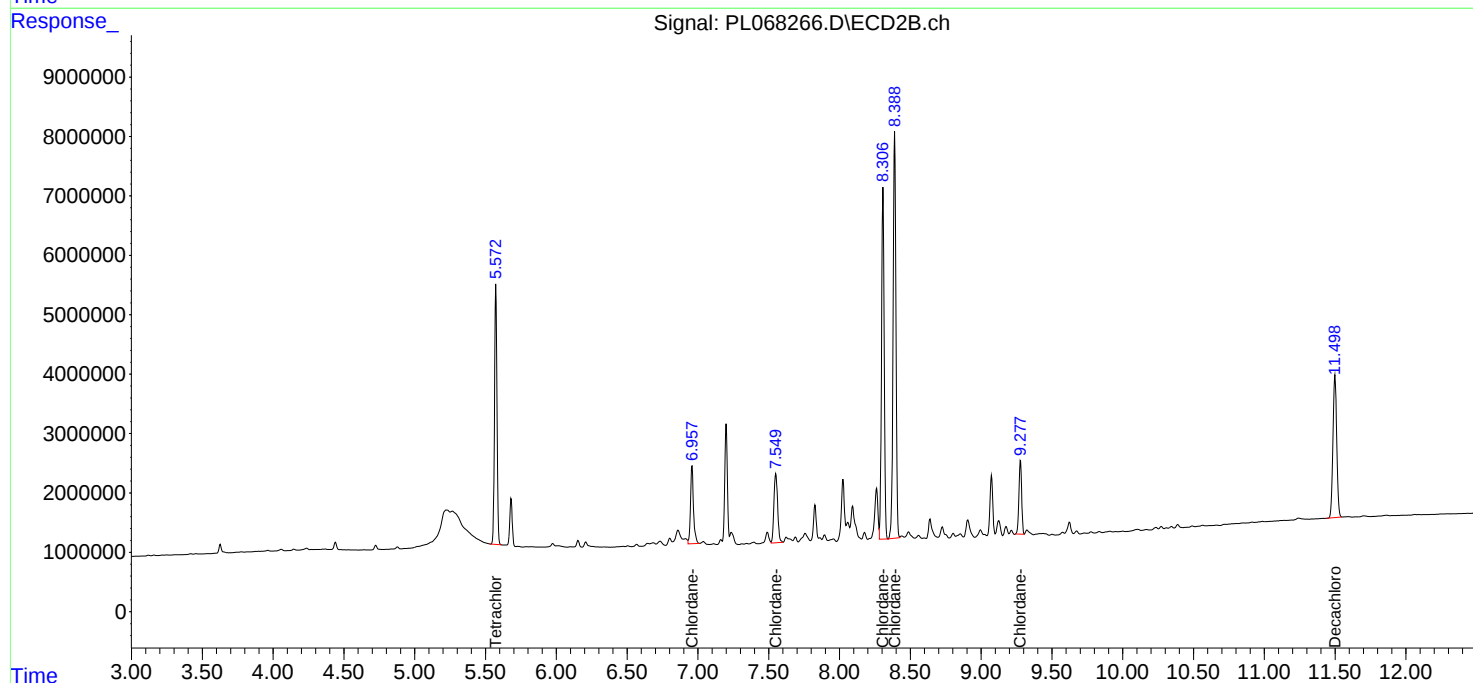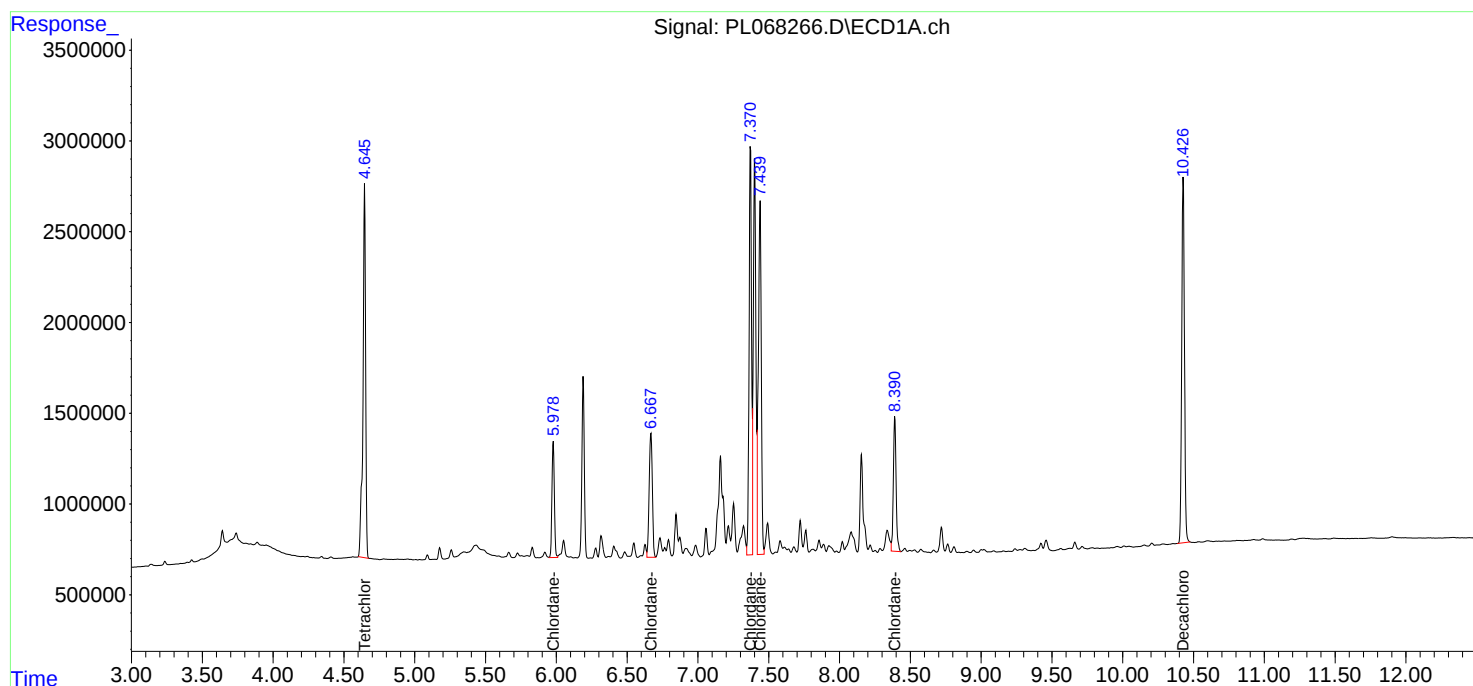


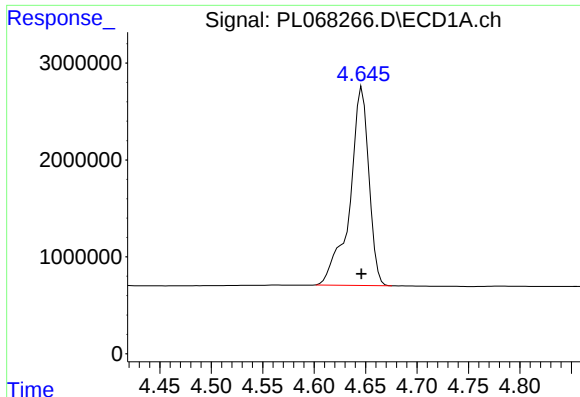

#1 Tetrachloro-m-xylene


R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 26404727
Conc: 49.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL072021CHLOR

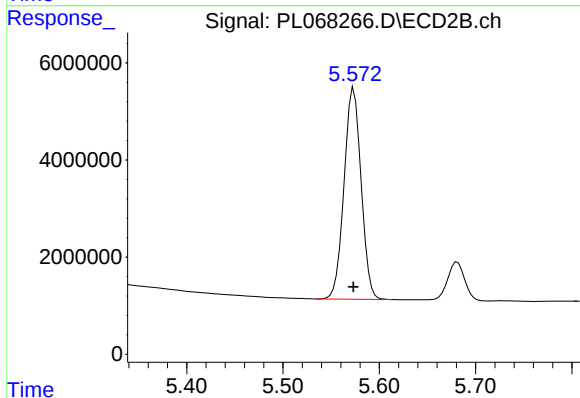


#1 Tetrachloro-m-xylene

R.T.: 5.574 min
Delta R.T.: 0.000 min
Response: 53408932
Conc: 50.80 ng/ml

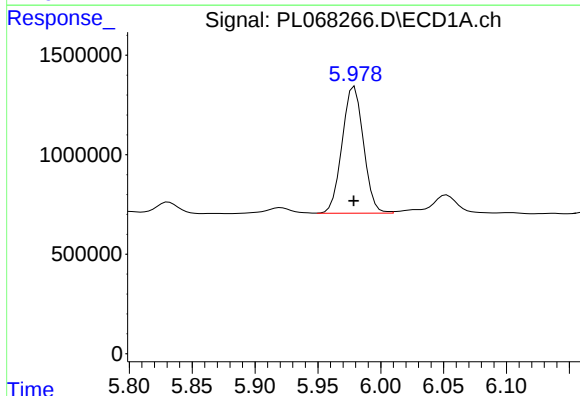


#23 Chlordane-1

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 7532689
Conc: 500.77 ng/ml

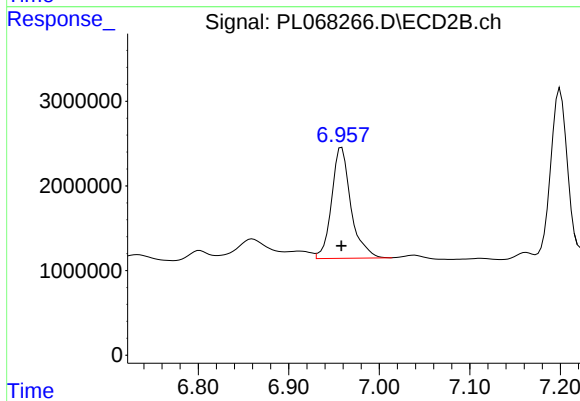

#23 Chlordane-1


R.T.: 6.958 min
Delta R.T.: 0.000 min
Response: 19398586
Conc: 478.86 ng/ml

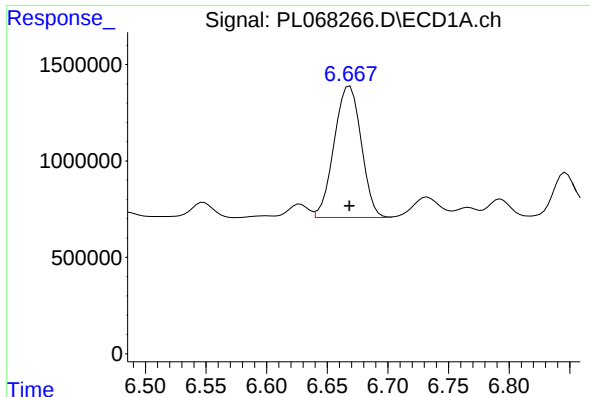

#24 Chlordane-2


R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 10604659
Conc: 494.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL072021CHLOR

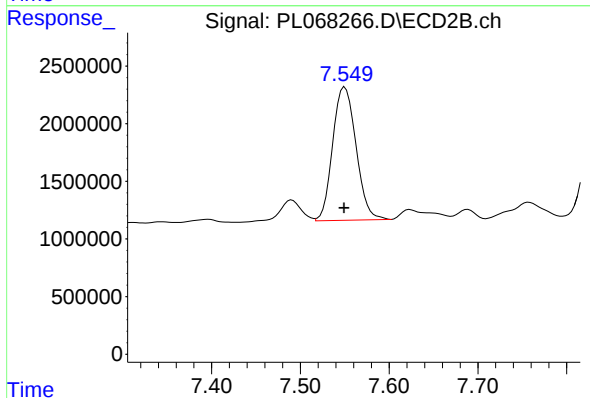


#24 Chlordane-2

R.T.: 7.550 min
Delta R.T.: 0.000 min
Response: 21167141
Conc: 508.76 ng/ml

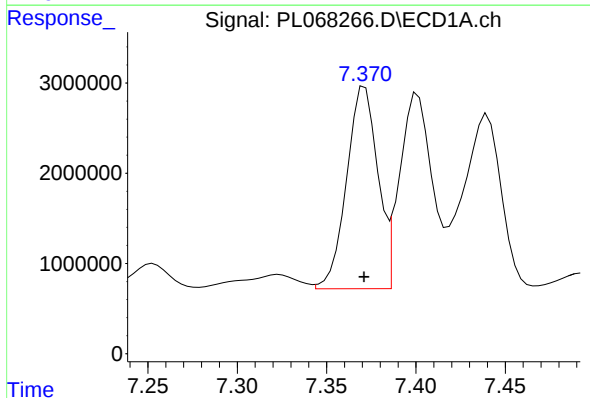


#25 Chlordane-3

R.T.: 7.372 min
Delta R.T.: 0.000 min
Response: 27154376
Conc: 504.22 ng/ml

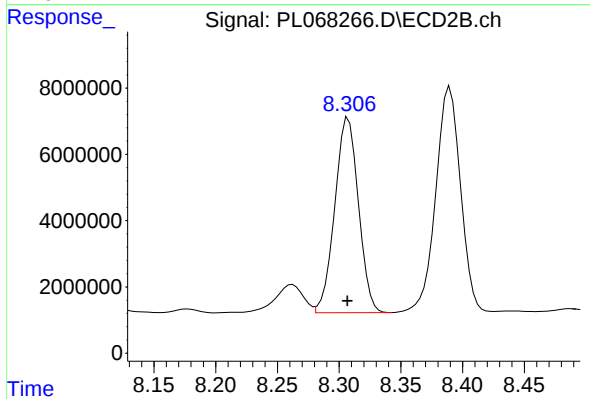

#25 Chlordane-3


R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 78529189
Conc: 507.07 ng/ml

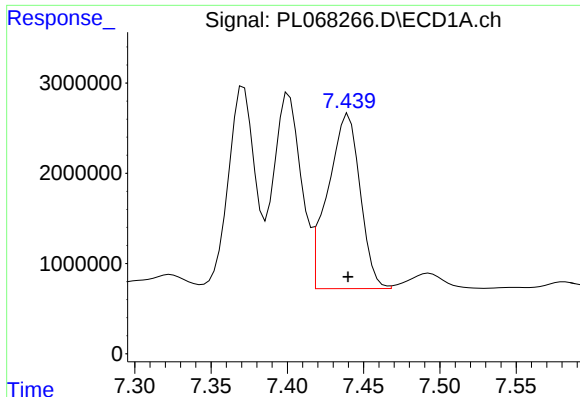

#26 Chlordane-4


R.T.: 7.440 min
Delta R.T.: 0.000 min
Response: 28497778
Conc: 504.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL072021CHLOR

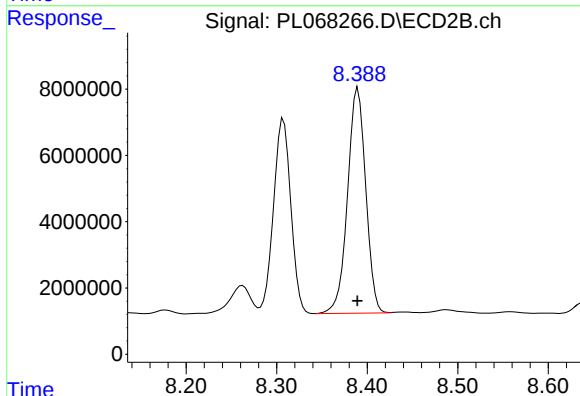


#26 Chlordane-4

R.T.: 8.390 min
Delta R.T.: 0.000 min
Response: 94991924
Conc: 506.68 ng/ml

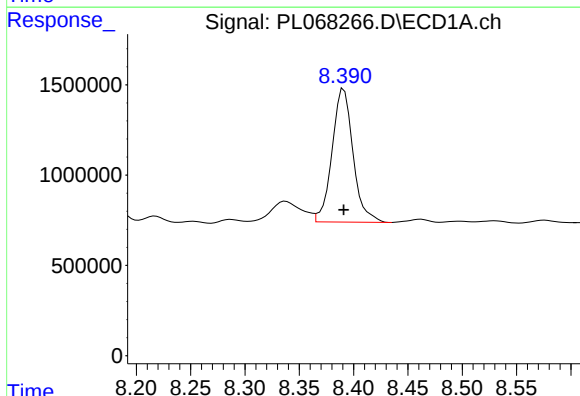


#27 Chlordane-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 9948158
Conc: 494.29 ng/ml

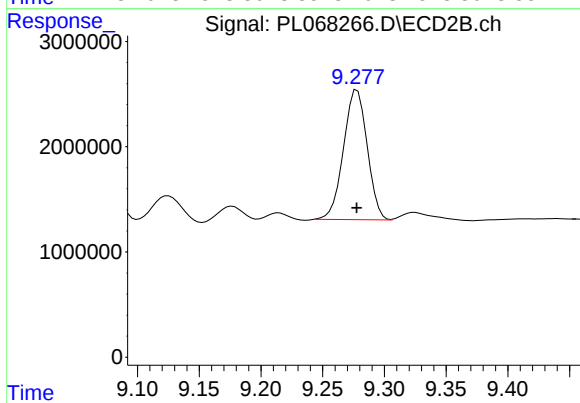

#27 Chlordane-5


R.T.: 9.278 min
Delta R.T.: 0.000 min
Response: 16479004
Conc: 514.15 ng/ml

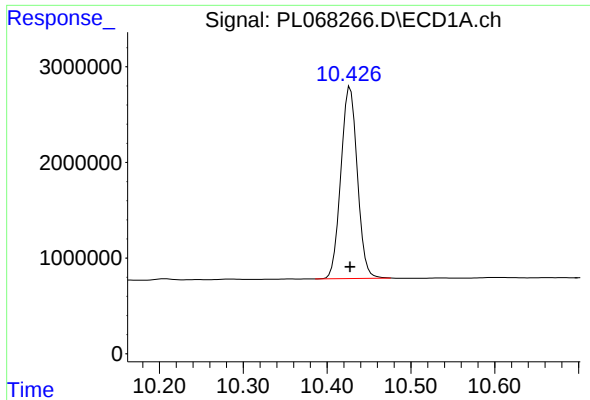

#28 Decachlorobiphenyl

R.T.: 10.428 min
Delta R.T.: 0.000 min
Response: 27375017
Conc: 48.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL072021CHLOR

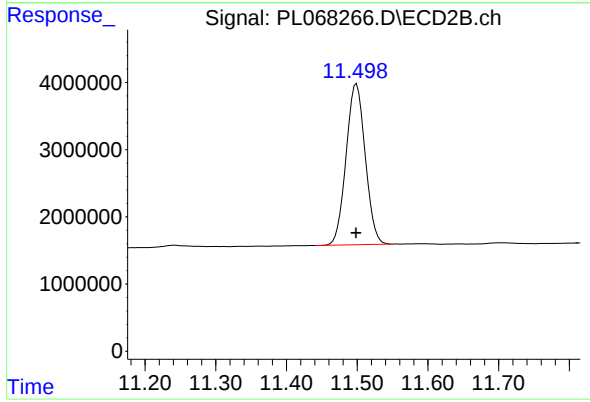

#28 Decachlorobiphenyl

R.T.: 11.499 min
Delta R.T.: 0.000 min
Response: 45082249
Conc: 49.13 ng/ml