

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 16:29
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 05:12:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.571	22914482	48177541	53.391	47.213
28)	SA Decachlor...	10.423	11.493	24984456	41191357	44.423	46.179
Target Compounds							
23)	Chlordane-1	5.976	6.955	6647003	17038377	441.889	420.599
24)	Chlordane-2	6.666	7.546	9415668	19328991	439.018	464.583
25)	Chlordane-3	7.368	8.304	23744543	71832443	440.907	463.825
26)	Chlordane-4	7.437	8.386	25083576	86868995	444.273	463.349
27)	Chlordane-5	8.388	9.273	8765070	14961369	435.504	466.803



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 16:29
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 05:12:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

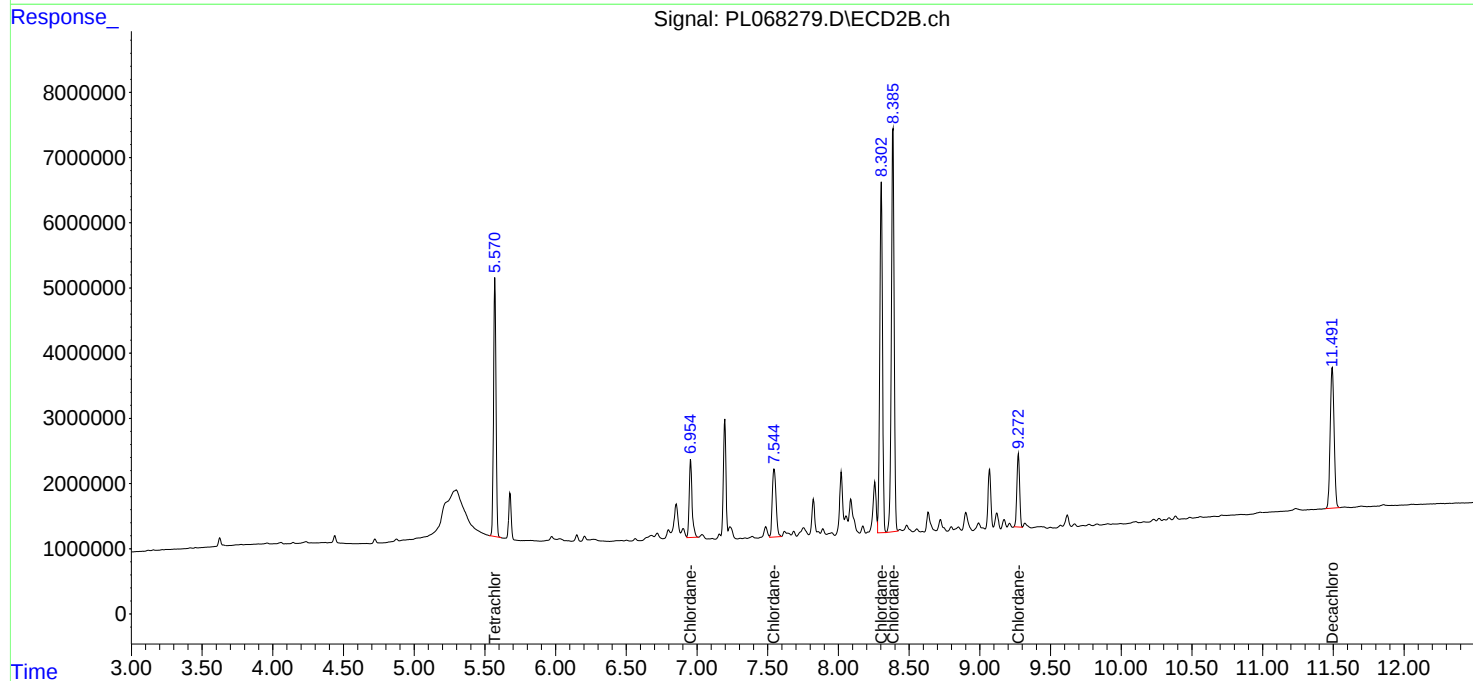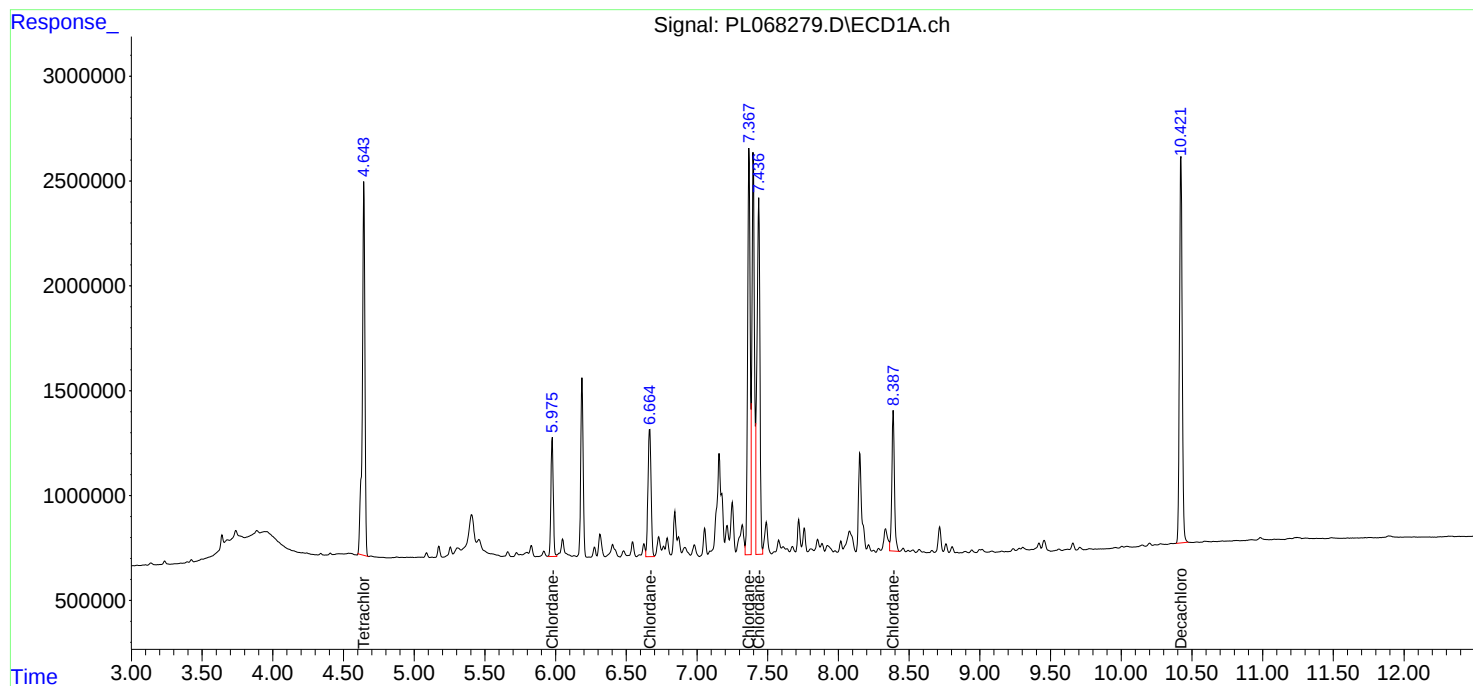


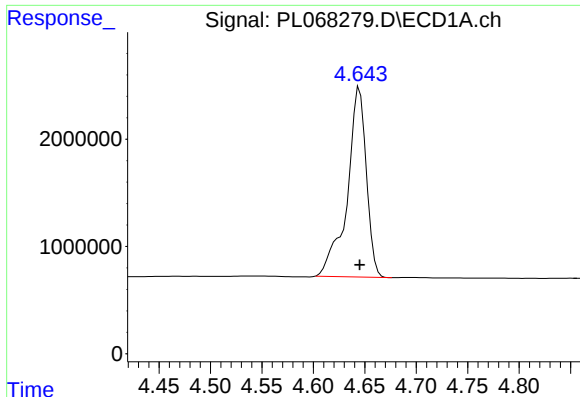

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 22914482
Conc: 53.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

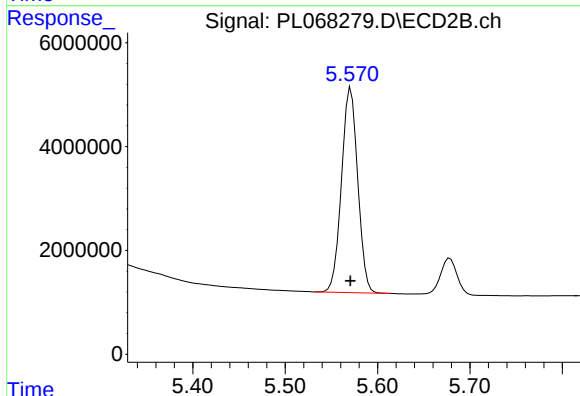


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 48177541
Conc: 47.21 ng/ml

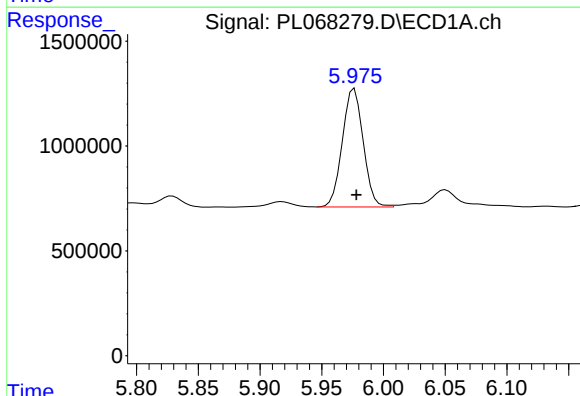


#23 Chlordane-1

R.T.: 5.976 min
Delta R.T.: -0.002 min
Response: 6647003
Conc: 441.89 ng/ml

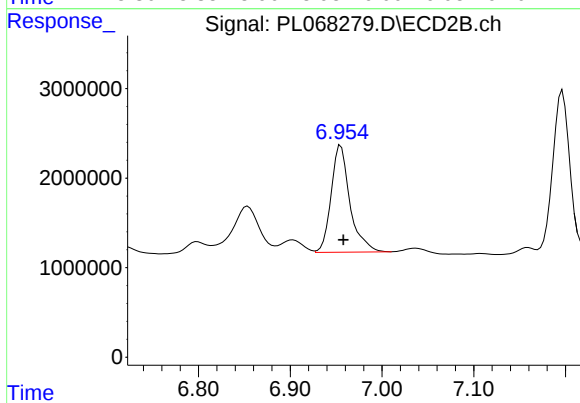

#23 Chlordane-1


R.T.: 6.955 min
Delta R.T.: -0.003 min
Response: 17038377
Conc: 420.60 ng/ml

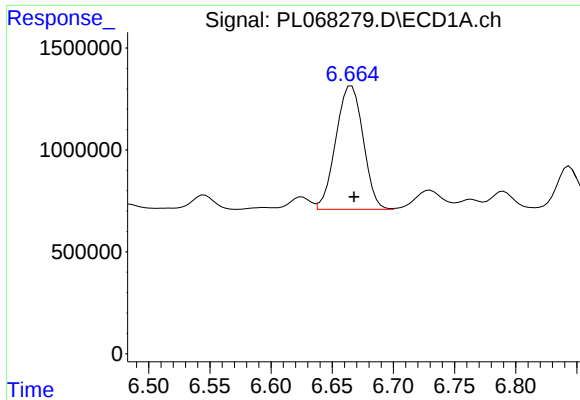

#24 Chlordane-2


R.T.: 6.666 min
Delta R.T.: -0.002 min
Response: 9415668
Conc: 439.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

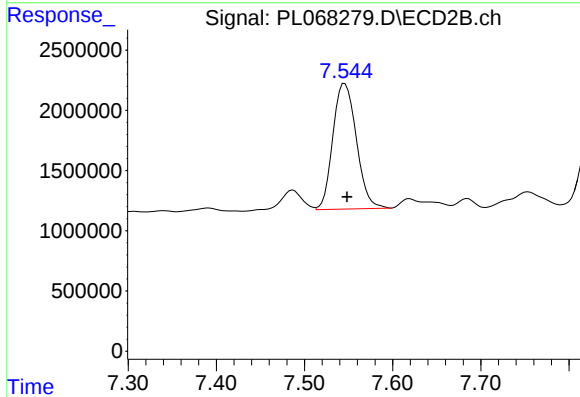


#24 Chlordane-2

R.T.: 7.546 min
Delta R.T.: -0.003 min
Response: 19328991
Conc: 464.58 ng/ml

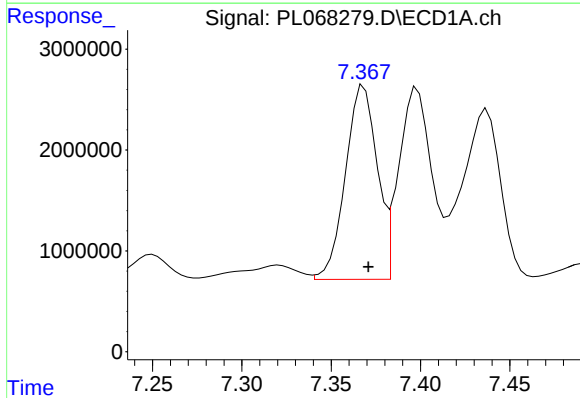


#25 Chlordane-3

R.T.: 7.368 min
Delta R.T.: -0.003 min
Response: 23744543
Conc: 440.91 ng/ml

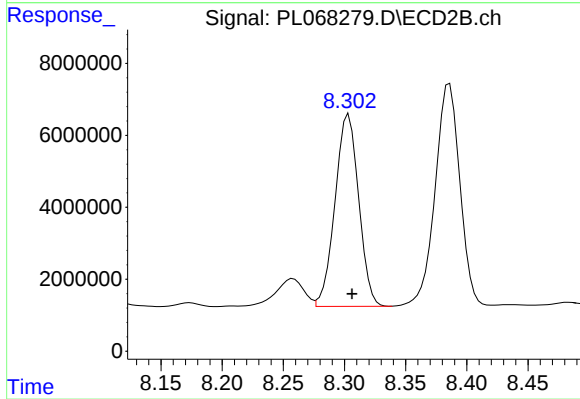

#25 Chlordane-3


R.T.: 8.304 min
Delta R.T.: -0.003 min
Response: 71832443
Conc: 463.82 ng/ml

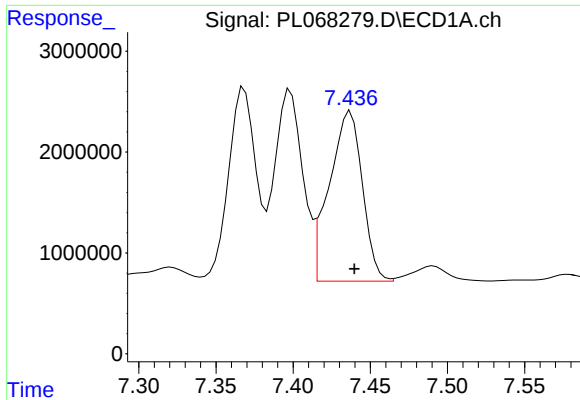

#26 Chlordane-4


R.T.: 7.437 min
Delta R.T.: -0.003 min
Response: 25083576
Conc: 444.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

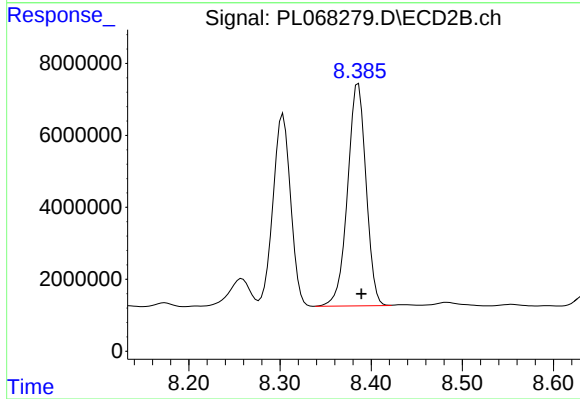


#26 Chlordane-4

R.T.: 8.386 min
Delta R.T.: -0.003 min
Response: 86868995
Conc: 463.35 ng/ml

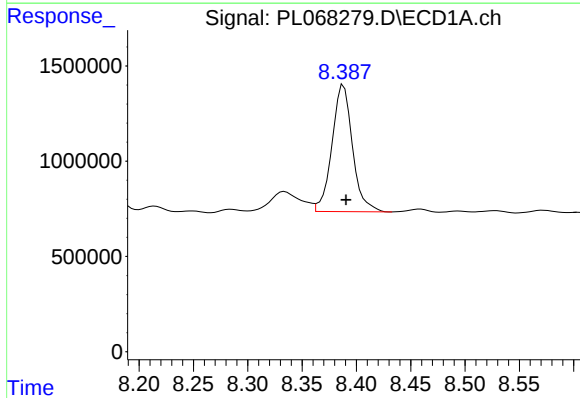


#27 Chlordane-5

R.T.: 8.388 min
Delta R.T.: -0.002 min
Response: 8765070
Conc: 435.50 ng/ml

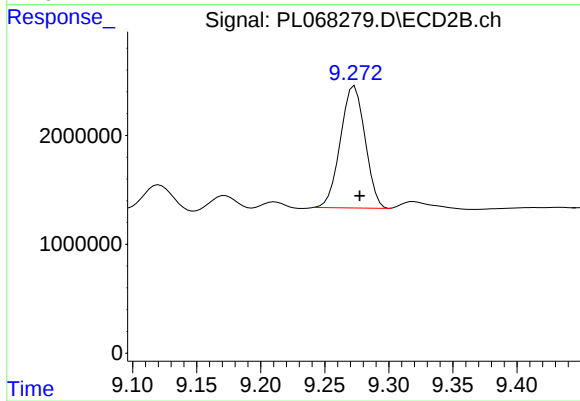

#27 Chlordane-5


R.T.: 9.273 min
Delta R.T.: -0.004 min
Response: 14961369
Conc: 466.80 ng/ml

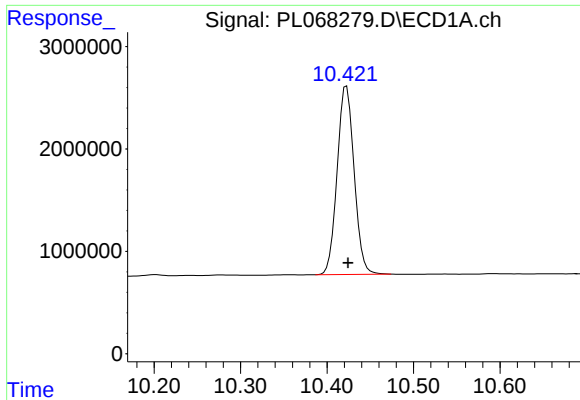

#28 Decachlorobiphenyl

R.T.: 10.423 min
Delta R.T.: -0.002 min
Response: 24984456
Conc: 44.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

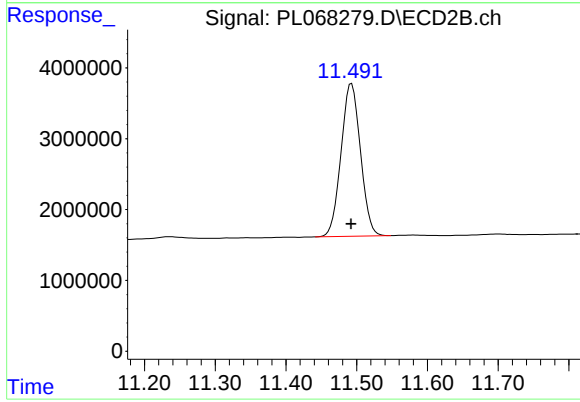

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 41191357
Conc: 46.18 ng/ml