

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
 Data File : PL068288.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 18:58
 Operator : AR\AJ
 Sample : M2940-08
 Misc : CHLOR LOQ 50 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LOQ-WATER-02-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 05:13:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.572	8211127	19425695	19.132	19.037
28)	SA Decachlor...	10.423	11.493	11106008	18046728	19.747	20.232
Target Compounds							
23)	Chlordane-1	5.977	6.956	712526	1708995	47.368	42.187
24)	Chlordane-2	6.665	7.546	1114014	1982267	51.942	47.645
25)	Chlordane-3	7.367	8.303	2534312	7195468	47.059	46.461
26)	Chlordane-4	7.437	8.386	2650458	8934112	46.944	47.653
27)	Chlordane-5	8.388	9.274	989342	1468125	49.157	45.806



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072021\
Data File : PL068288.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 18:58
Operator : AR\AJ
Sample : M2940-08
Misc : CHLOR LOQ 50 PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 05:13:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

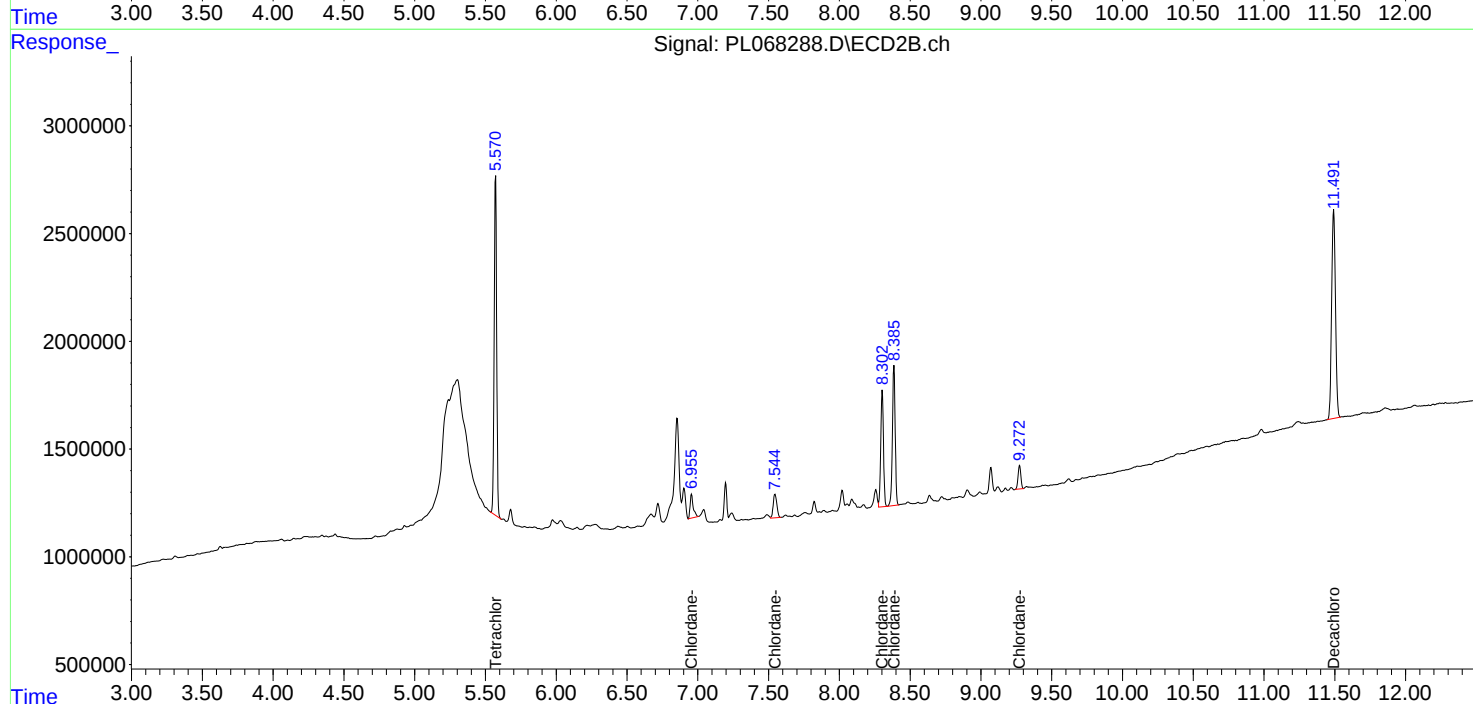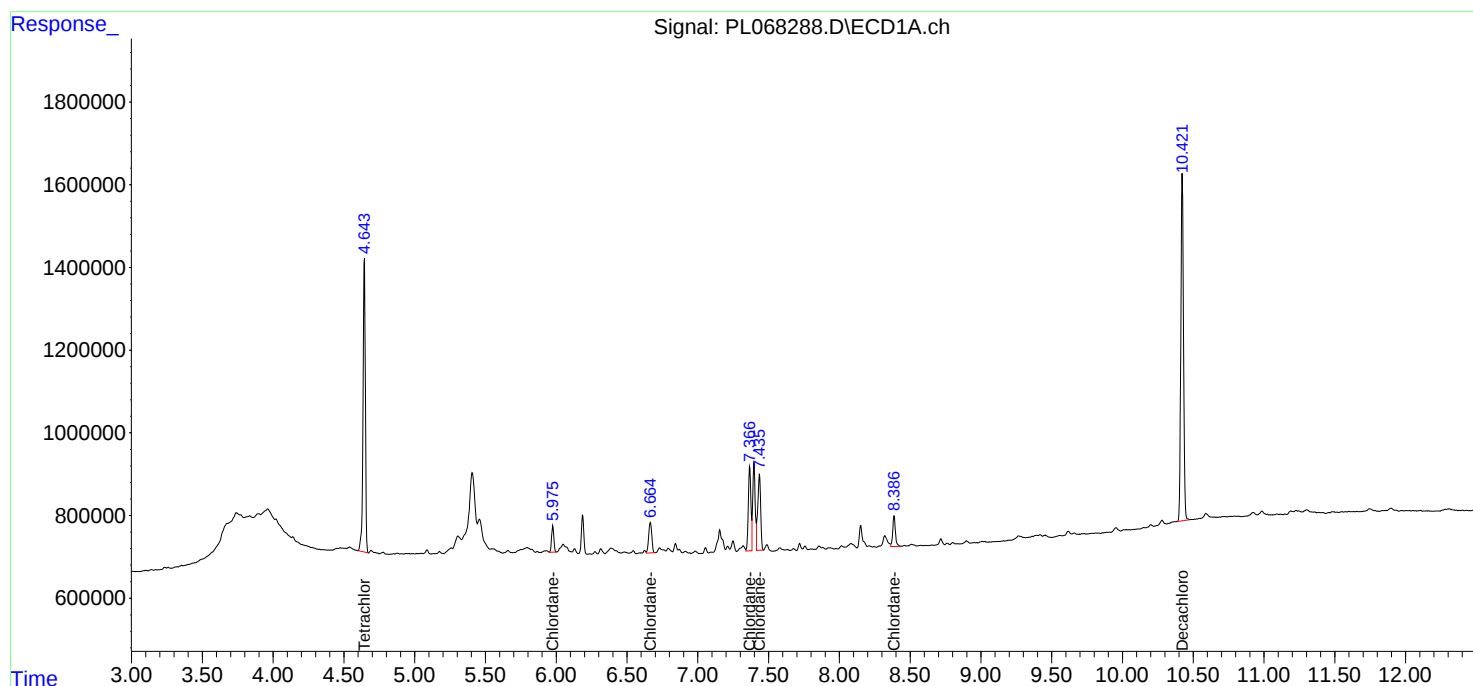


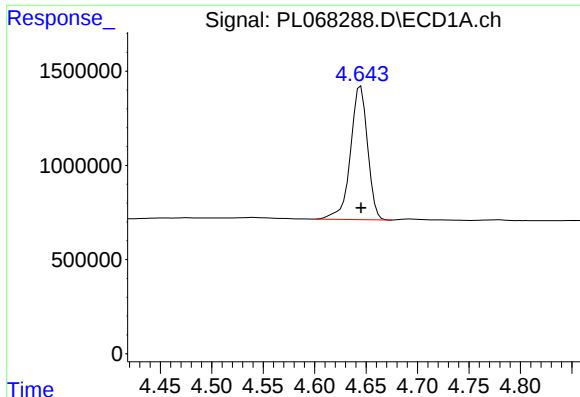

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 8211127
Conc: 19.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT3-2021

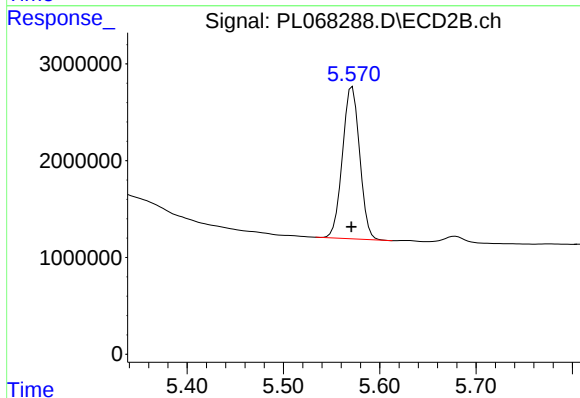


#1 Tetrachloro-m-xylene

R.T.: 5.572 min
Delta R.T.: 0.000 min
Response: 19425695
Conc: 19.04 ng/ml

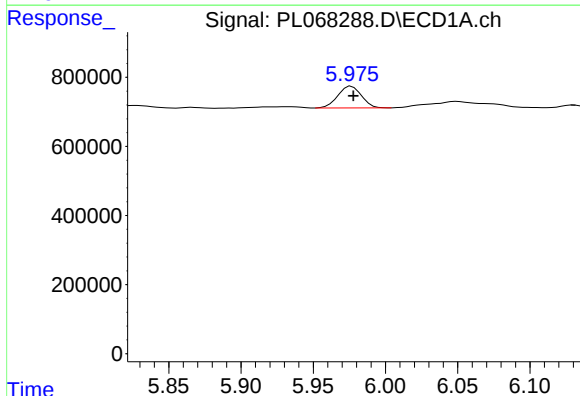


#23 Chlordane-1

R.T.: 5.977 min
Delta R.T.: -0.001 min
Response: 712526
Conc: 47.37 ng/ml

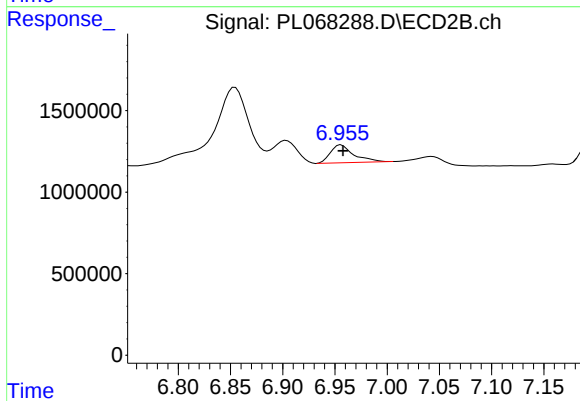

#23 Chlordane-1


R.T.: 6.956 min
Delta R.T.: -0.002 min
Response: 1708995
Conc: 42.19 ng/ml

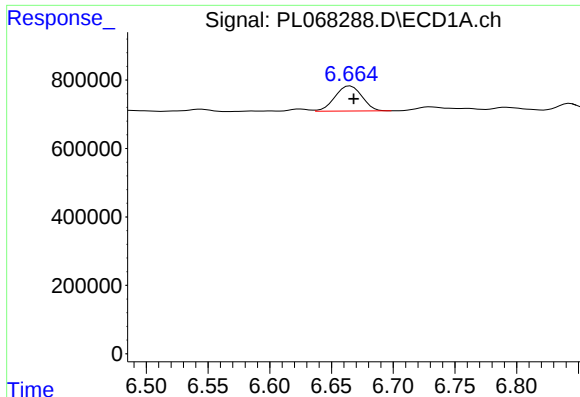

#24 Chlordane-2


R.T.: 6.665 min
Delta R.T.: -0.003 min
Response: 1114014
Conc: 51.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT3-2021

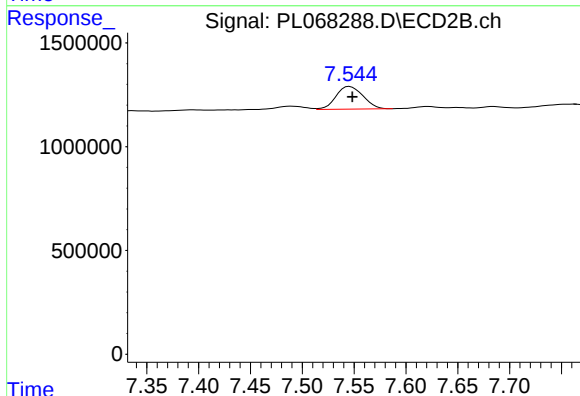


#24 Chlordane-2

R.T.: 7.546 min
Delta R.T.: -0.003 min
Response: 1982267
Conc: 47.64 ng/ml

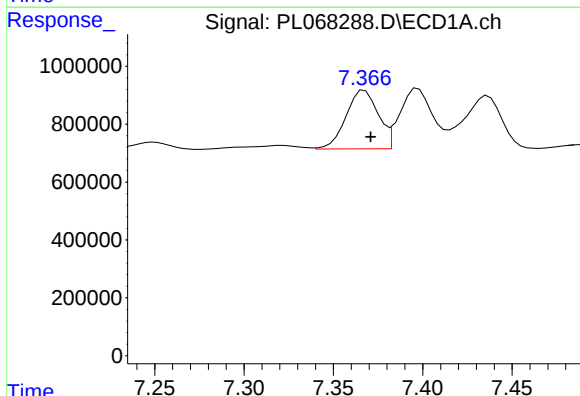


#25 Chlordane-3

R.T.: 7.367 min
Delta R.T.: -0.003 min
Response: 2534312
Conc: 47.06 ng/ml

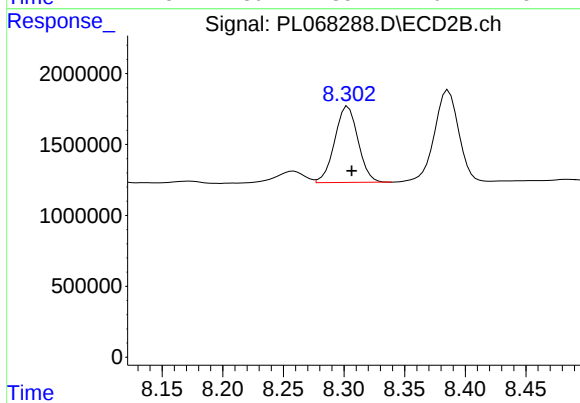

#25 Chlordane-3


R.T.: 8.303 min
Delta R.T.: -0.003 min
Response: 7195468
Conc: 46.46 ng/ml

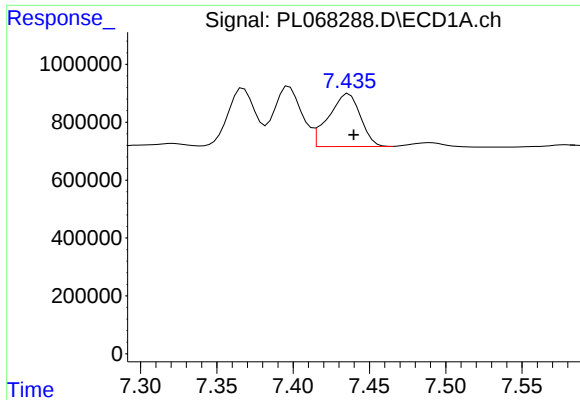

#26 Chlordane-4


R.T.: 7.437 min
Delta R.T.: -0.003 min
Response: 2650458
Conc: 46.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT3-2021

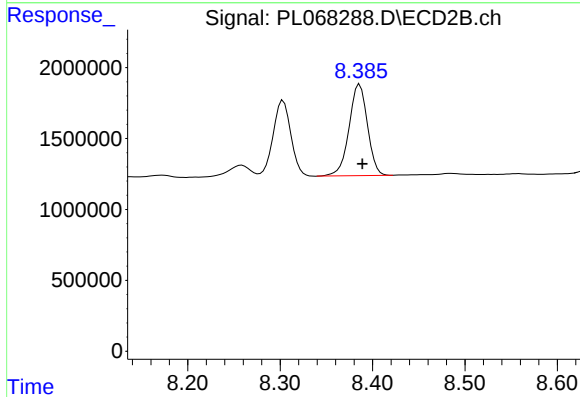


#26 Chlordane-4

R.T.: 8.386 min
Delta R.T.: -0.003 min
Response: 8934112
Conc: 47.65 ng/ml

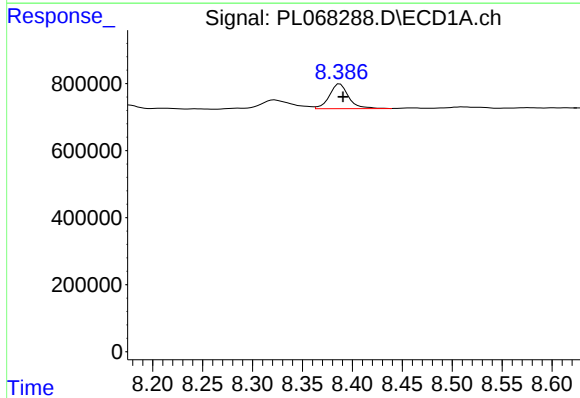


#27 Chlordane-5

R.T.: 8.388 min
Delta R.T.: -0.003 min
Response: 989342
Conc: 49.16 ng/ml

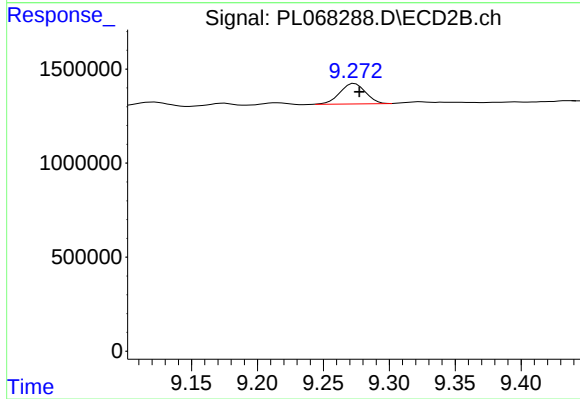

#27 Chlordane-5


R.T.: 9.274 min
Delta R.T.: -0.004 min
Response: 1468125
Conc: 45.81 ng/ml

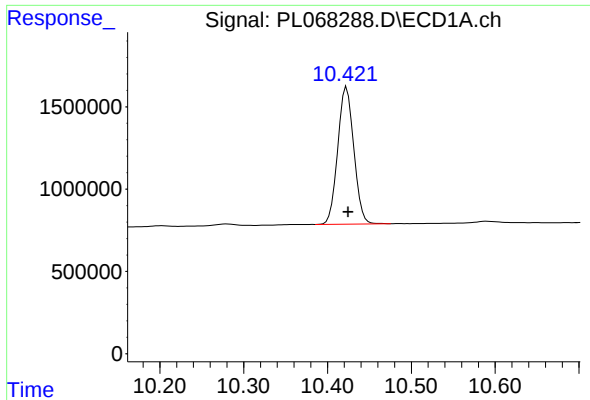

#28 Decachlorobiphenyl

R.T.: 10.423 min
Delta R.T.: -0.001 min
Response: 11106008
Conc: 19.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT3-2021

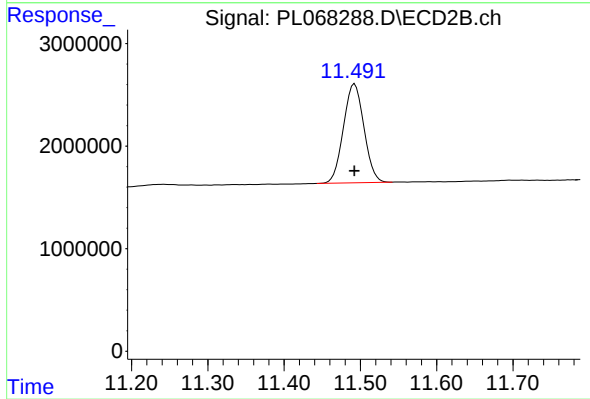

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 18046728
Conc: 20.23 ng/ml