

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072120\
 Data File : PL060048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2020 09:02
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 13:18:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	0.000	5.890	0	2996735	N.D.	1.113 #
9) A	Endosulfan I	5.502f	6.238	590863	21857925	0.351	8.195 #
10) B	gamma-Chl...	5.408	6.105f	5601360	96941019	3.088	33.853 #
11) B	alpha-Chl...	5.464	0.000	958320	0	0.531	N.D. #
12) B	4,4'-DDE	0.000	6.350	0	14169014	N.D.	5.294 #
17) MA	4,4'-DDT	6.404	0.000	6149159	0	4.729	N.D. #
18) B	Endrin al...	6.476	0.000	2698087	0	1.891	N.D. #
25)	Chlordane-3	5.408	6.105f	5601360	96941019	33.122	250.547 #
26)	Chlordane-4	5.464	0.000	958320	0	6.869	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072120\
Data File : PL060048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2020 09:02
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 13:18:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

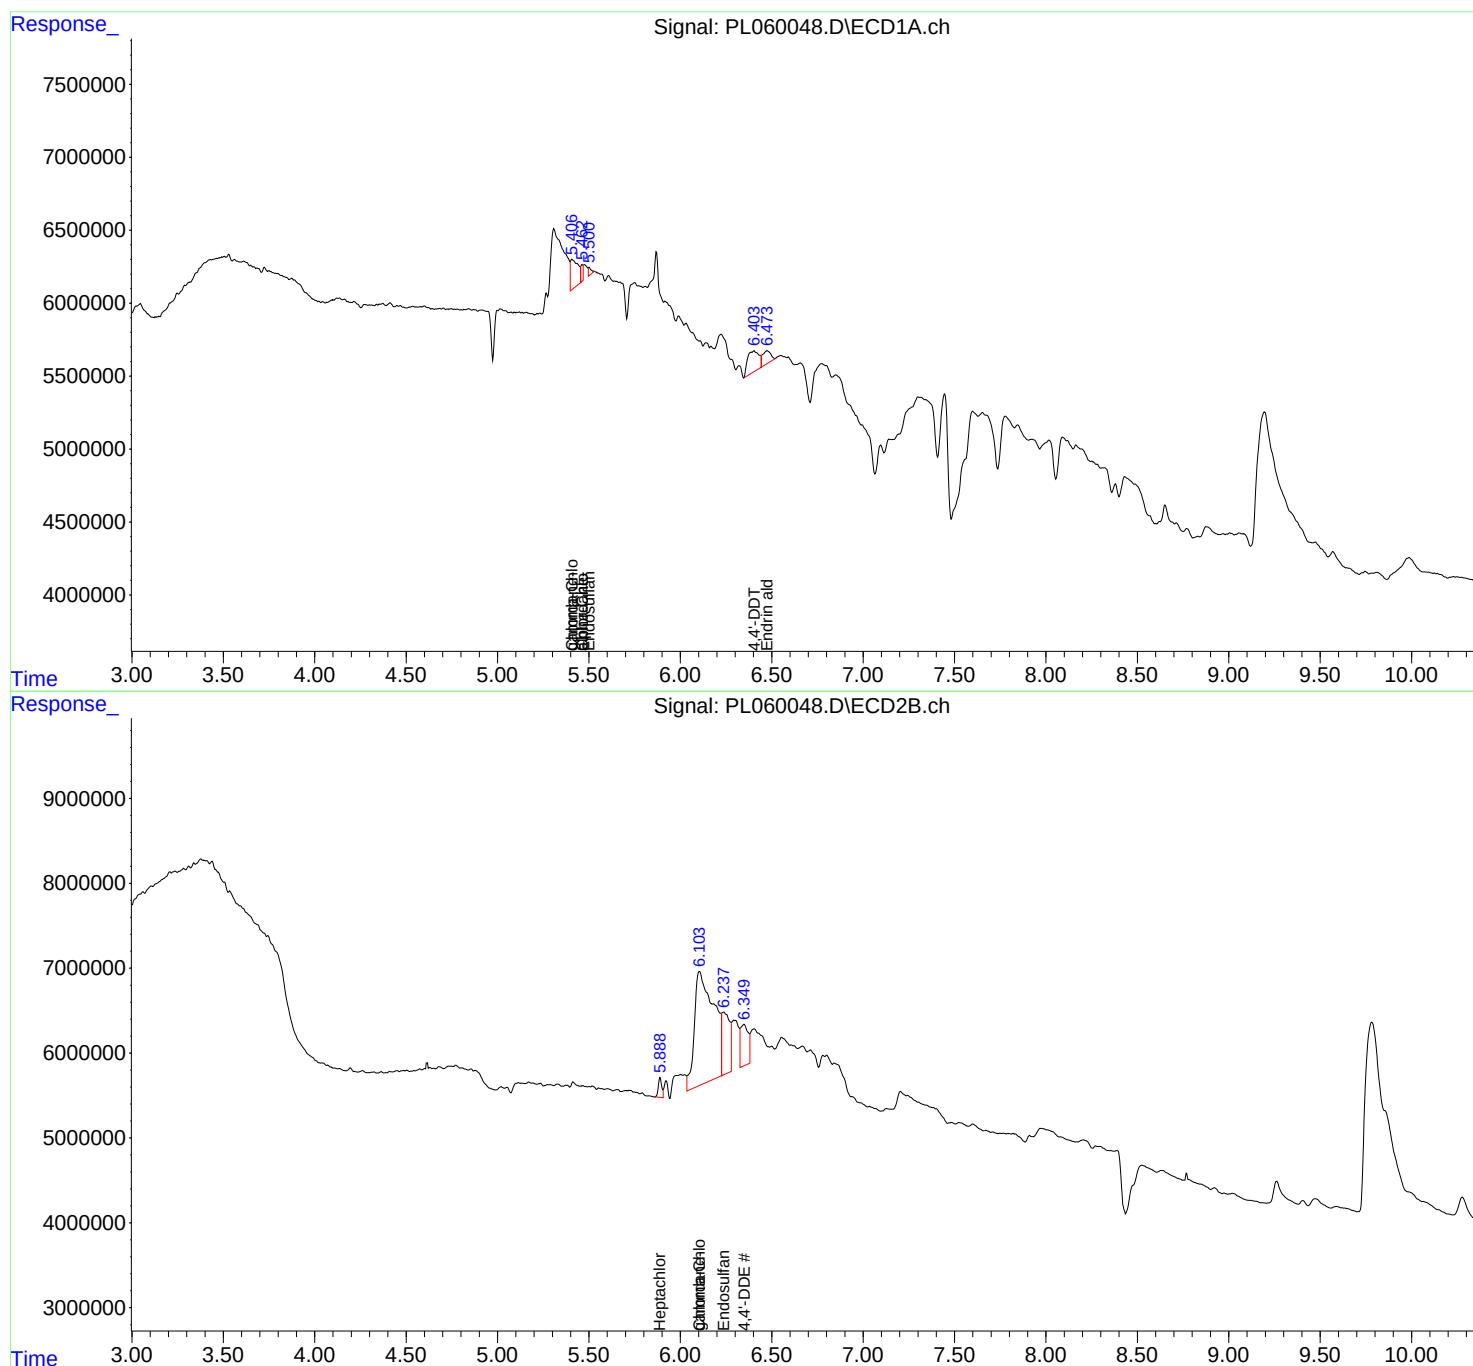


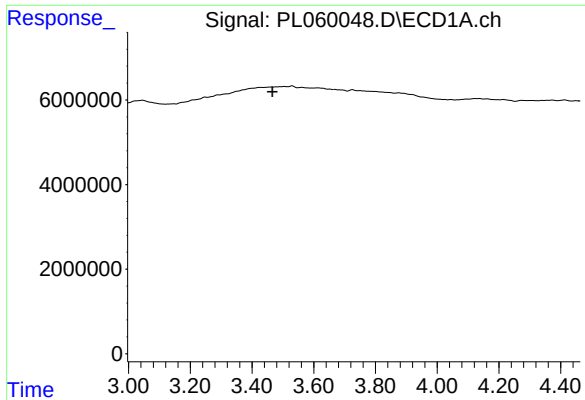

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.466 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

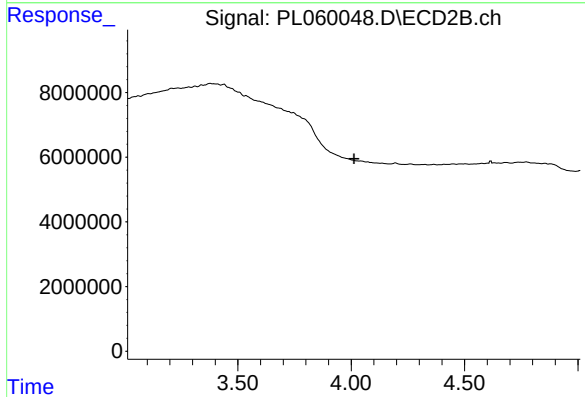


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.012 min
Response: 0
Conc: N.D.

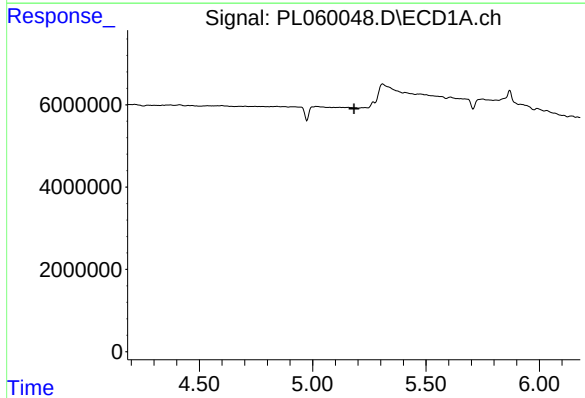


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.183 min
Response: 0
Conc: N.D.

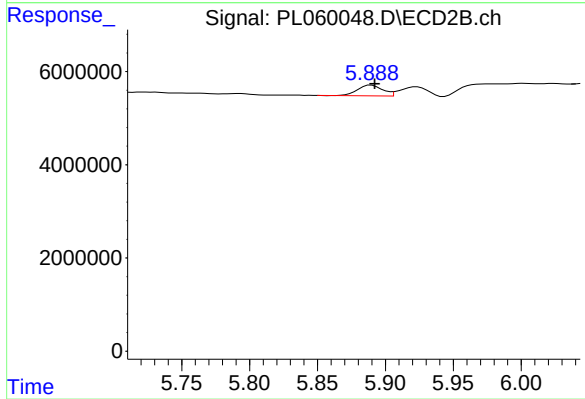

#8 Heptachlor epoxide


R.T.: 5.890 min
Delta R.T.: -0.003 min
Response: 2996735
Conc: 1.11 ng/ml

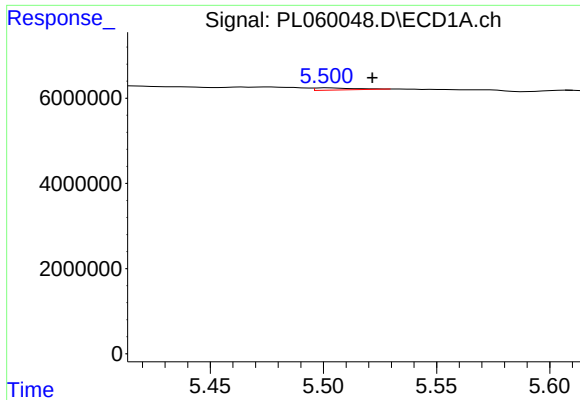

#9 Endosulfan I


R.T.: 5.502 min
Delta R.T.: -0.020 min
Response: 590863
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

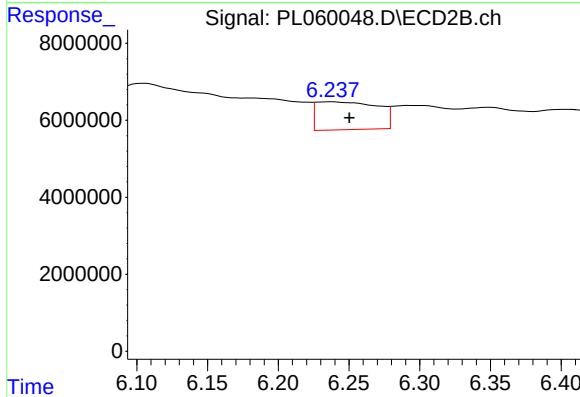


#9 Endosulfan I

R.T.: 6.238 min
Delta R.T.: -0.012 min
Response: 21857925
Conc: 8.19 ng/ml

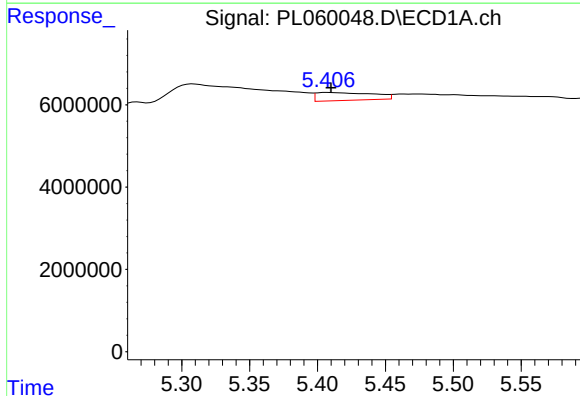


#10 gamma-Chlordane

R.T.: 5.408 min
Delta R.T.: -0.002 min
Response: 5601360
Conc: 3.09 ng/ml

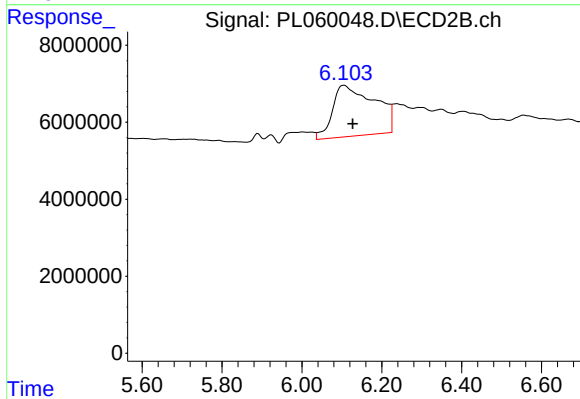

#10 gamma-Chlordane


R.T.: 6.105 min
Delta R.T.: -0.022 min
Response: 96941019
Conc: 33.85 ng/ml

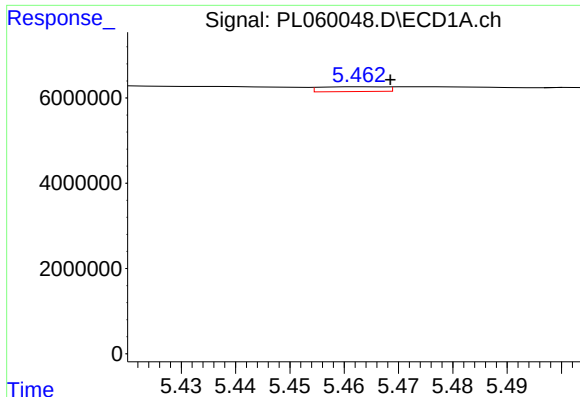

#11 alpha-Chlordane


R.T.: 5.464 min
Delta R.T.: -0.005 min
Response: 958320
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

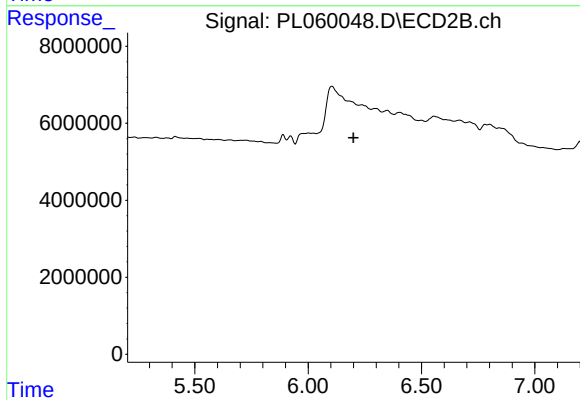


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.201 min
Response: 0
Conc: N.D.

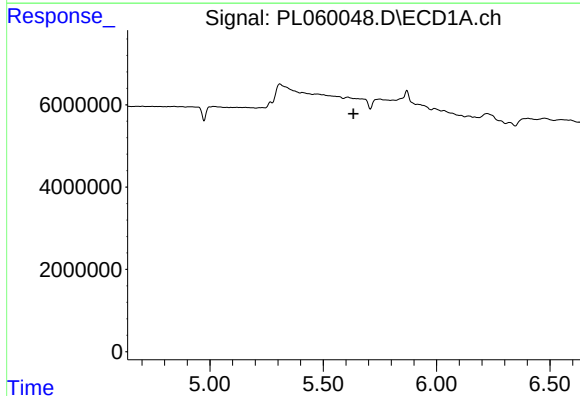


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.634 min
Response: 0
Conc: N.D.

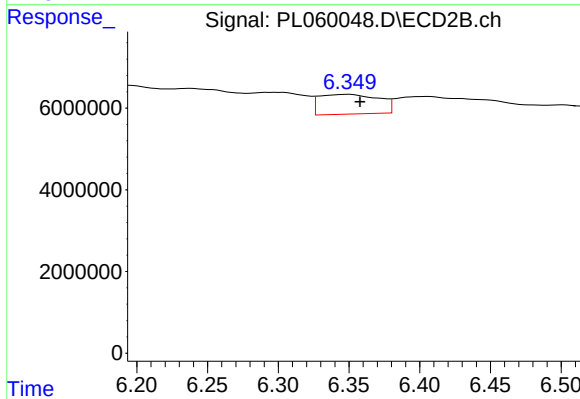

#12 4,4'-DDE


R.T.: 6.350 min
Delta R.T.: -0.008 min
Response: 14169014
Conc: 5.29 ng/ml

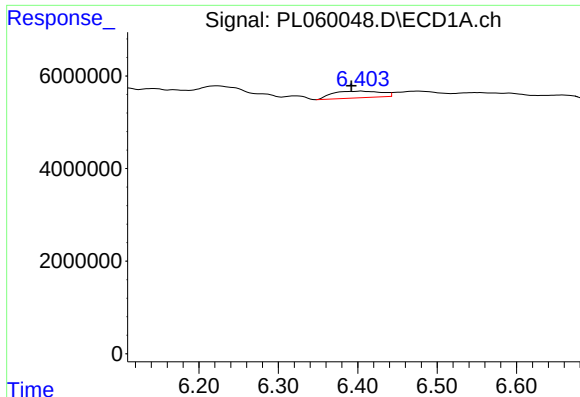

#17 4,4'-DDT


R.T.: 6.404 min
Delta R.T.: 0.012 min
Response: 6149159
Conc: 4.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

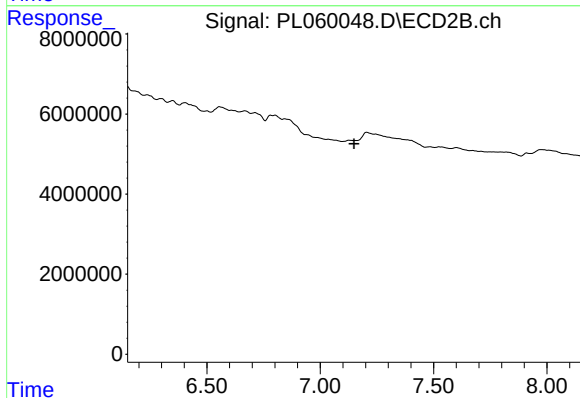


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

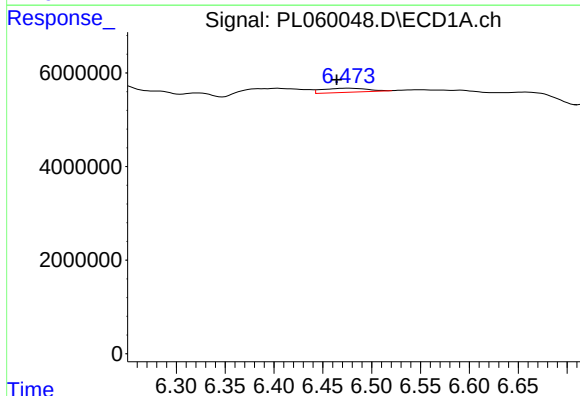


#18 Endrin aldehyde

R.T.: 6.476 min
Delta R.T.: 0.012 min
Response: 2698087
Conc: 1.89 ng/ml

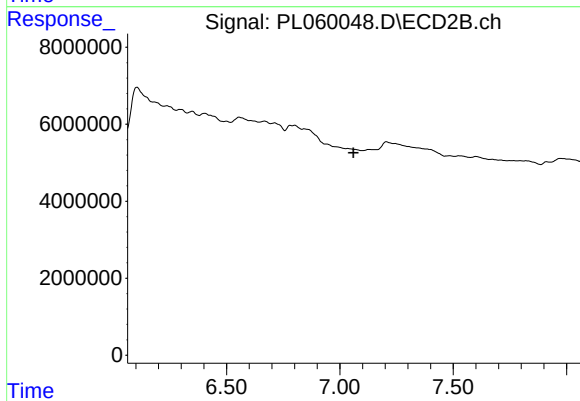

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

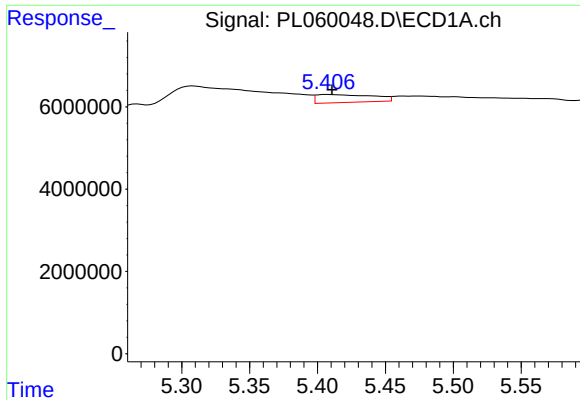

#25 Chlordane-3


R.T.: 5.408 min
Delta R.T.: -0.003 min
Response: 5601360
Conc: 33.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

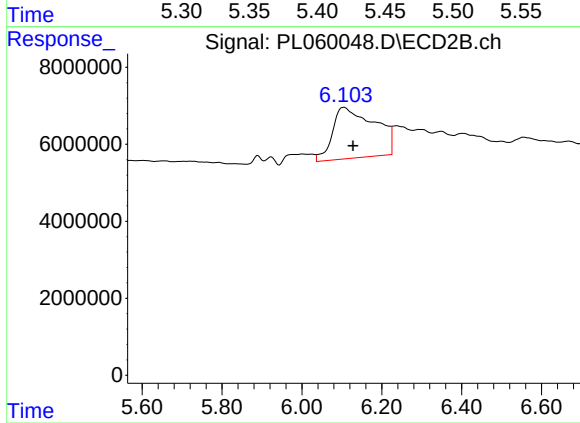


#25 Chlordane-3

R.T.: 6.105 min
Delta R.T.: -0.023 min
Response: 96941019
Conc: 250.55 ng/ml

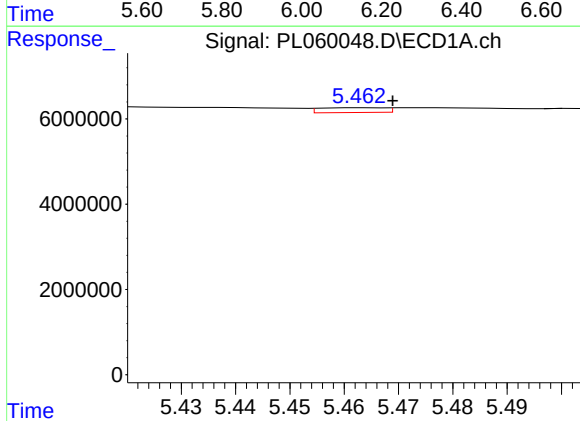


#26 Chlordane-4

R.T.: 5.464 min
Delta R.T.: -0.005 min
Response: 958320
Conc: 6.87 ng/ml

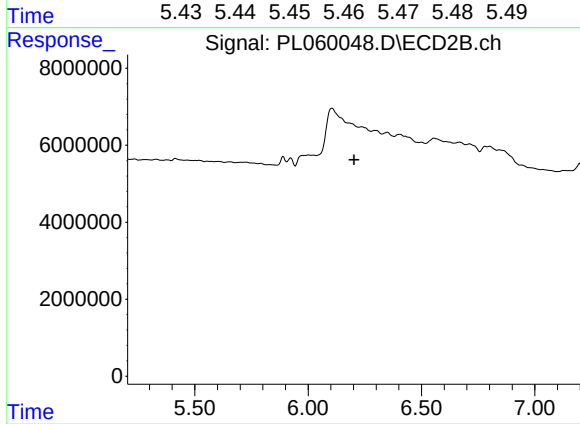

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.203 min
Response: 0
Conc: N.D.

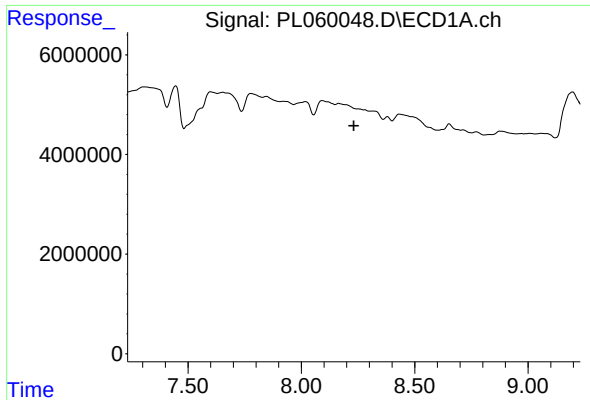

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

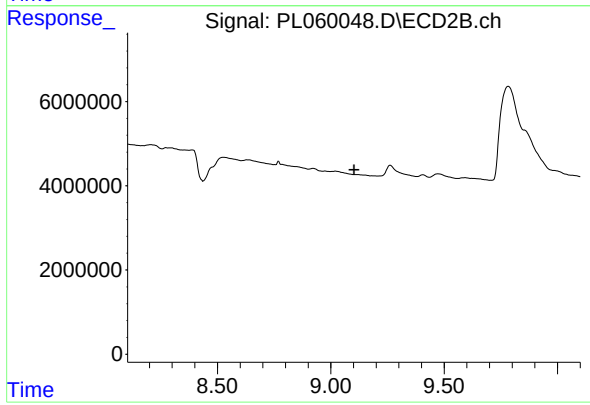

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.103 min
Response: 0
Conc: N.D.