

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072121\
 Data File : PL068355.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2021 18:21
 Operator : AR\AJ
 Sample : M3114-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:25:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.645	5.571	7746466	18928148	18.049	18.549
28) SA Decachlor...	10.422	11.493	7106183	11693140	12.635	13.109
Target Compounds						
14) MA Endrin	0.000	8.994f	0	74256	N.D.	0.083 #
15) B Endosulfa...	0.000	9.217f	0	421504	N.D.	0.465 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072121\
Data File : PL068355.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2021 18:21
Operator : AR\AJ
Sample : M3114-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:25:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

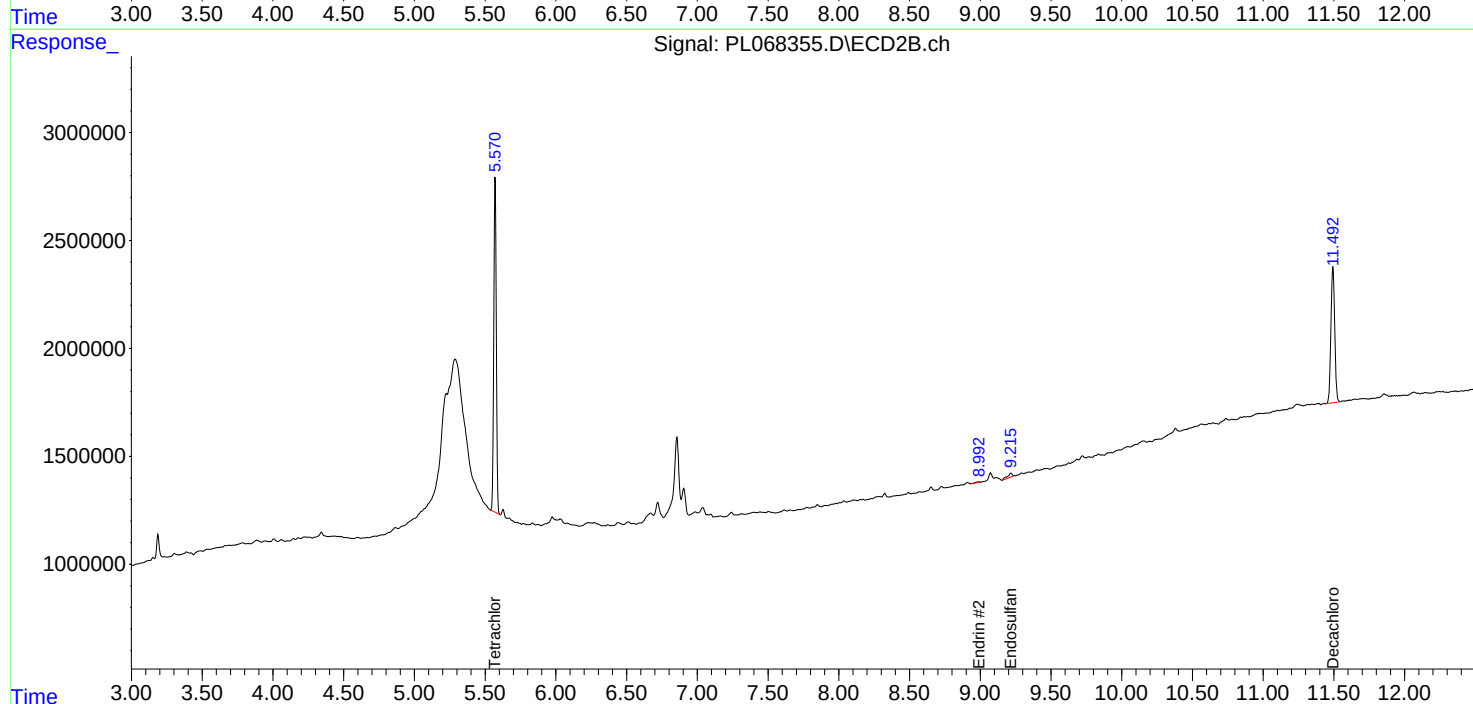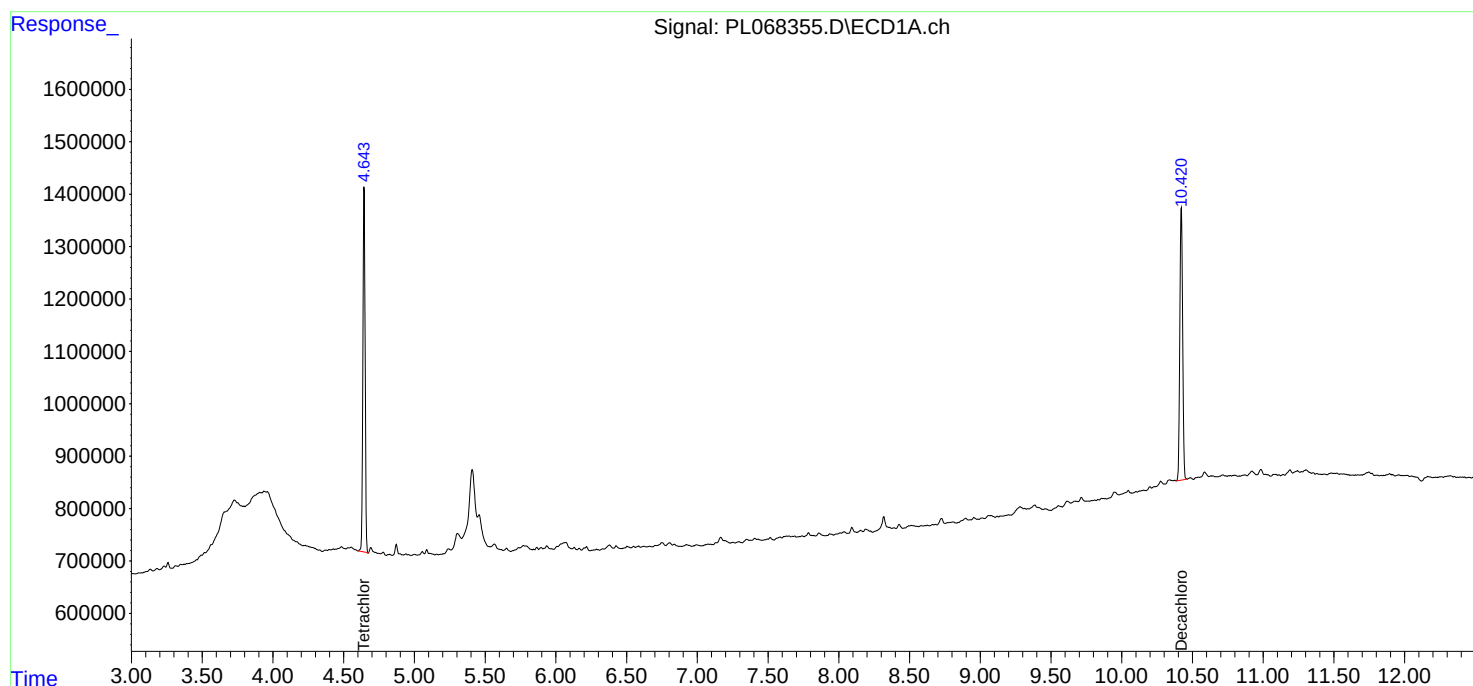


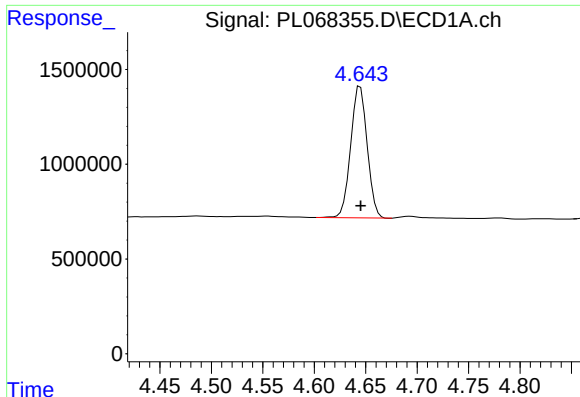

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 7746466
Conc: 18.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

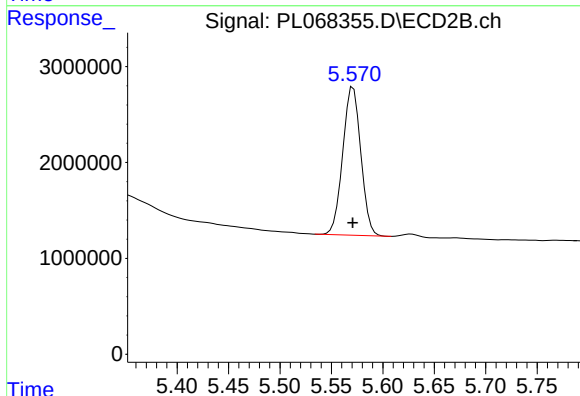


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 18928148
Conc: 18.55 ng/ml

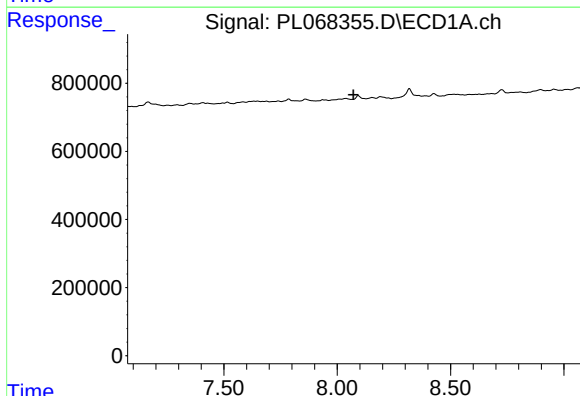


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.072 min
Response: 0
Conc: N.D.

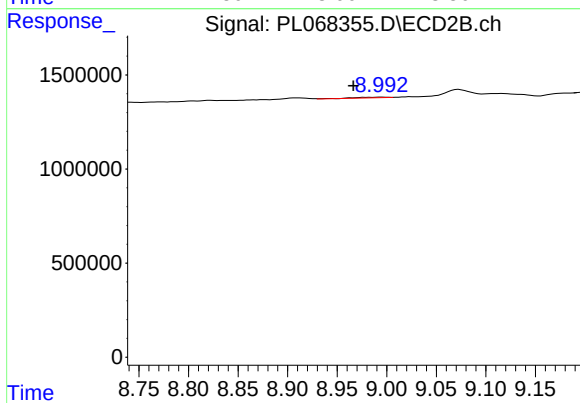

#14 Endrin


R.T.: 8.994 min
Delta R.T.: 0.027 min
Response: 74256
Conc: 0.08 ng/ml

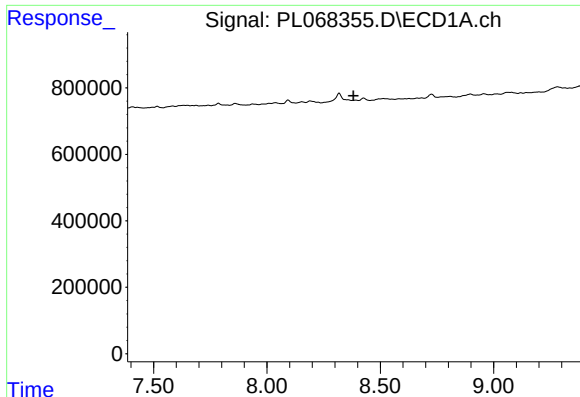

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

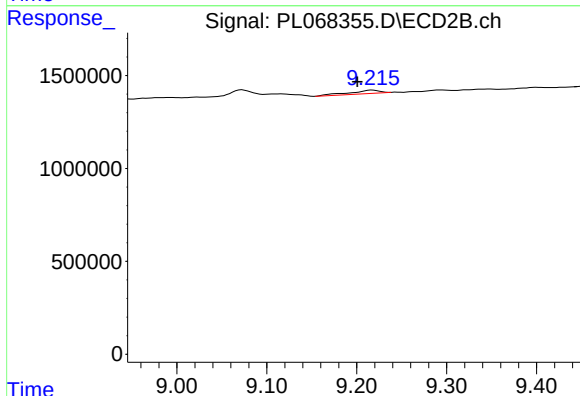


#15 Endosulfan II

R.T.: 9.217 min
Delta R.T.: 0.017 min
Response: 421504
Conc: 0.47 ng/ml

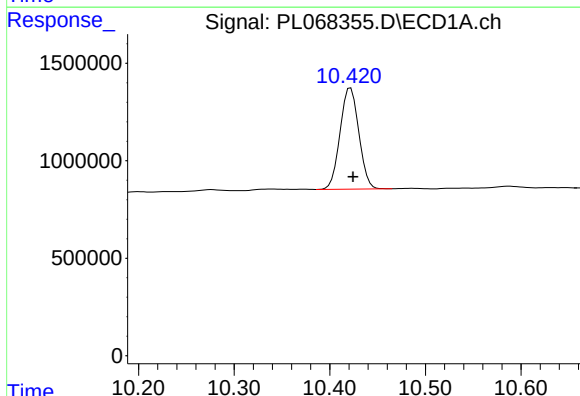

#28 Decachlorobiphenyl

R.T.: 10.422 min
Delta R.T.: -0.003 min
Response: 7106183
Conc: 12.64 ng/ml

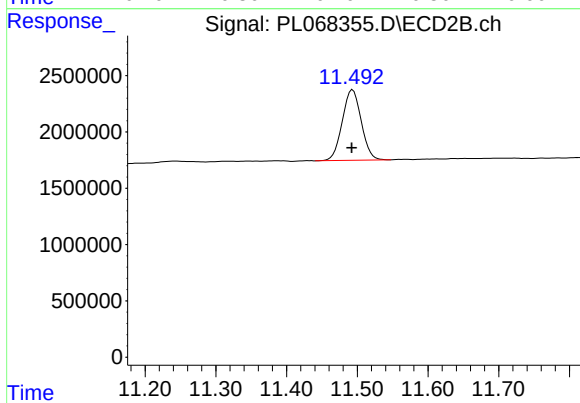

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.001 min
Response: 11693140
Conc: 13.11 ng/ml