

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072121\
 Data File : PL068358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2021 19:11
 Operator : AR\AJ
 Sample : M3114-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:26:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.571	8699716	21618318	20.270	21.186
28)	SA Decachlor...	10.422	11.495	8971310	14921257	15.951	16.728
Target Compounds							
15)	B Endosulfa...	0.000	9.219f	0	402510	N.D.	0.444 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072121\
Data File : PL068358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2021 19:11
Operator : AR\AJ
Sample : M3114-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:26:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

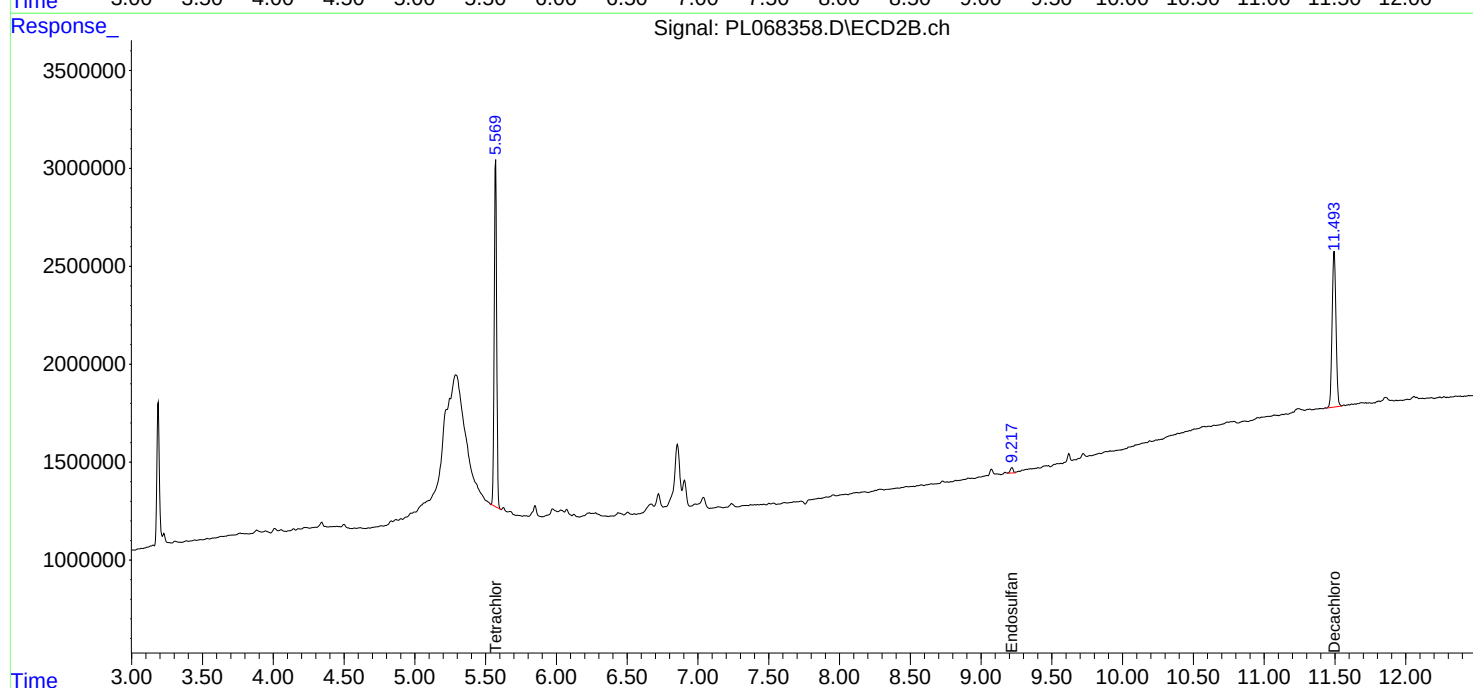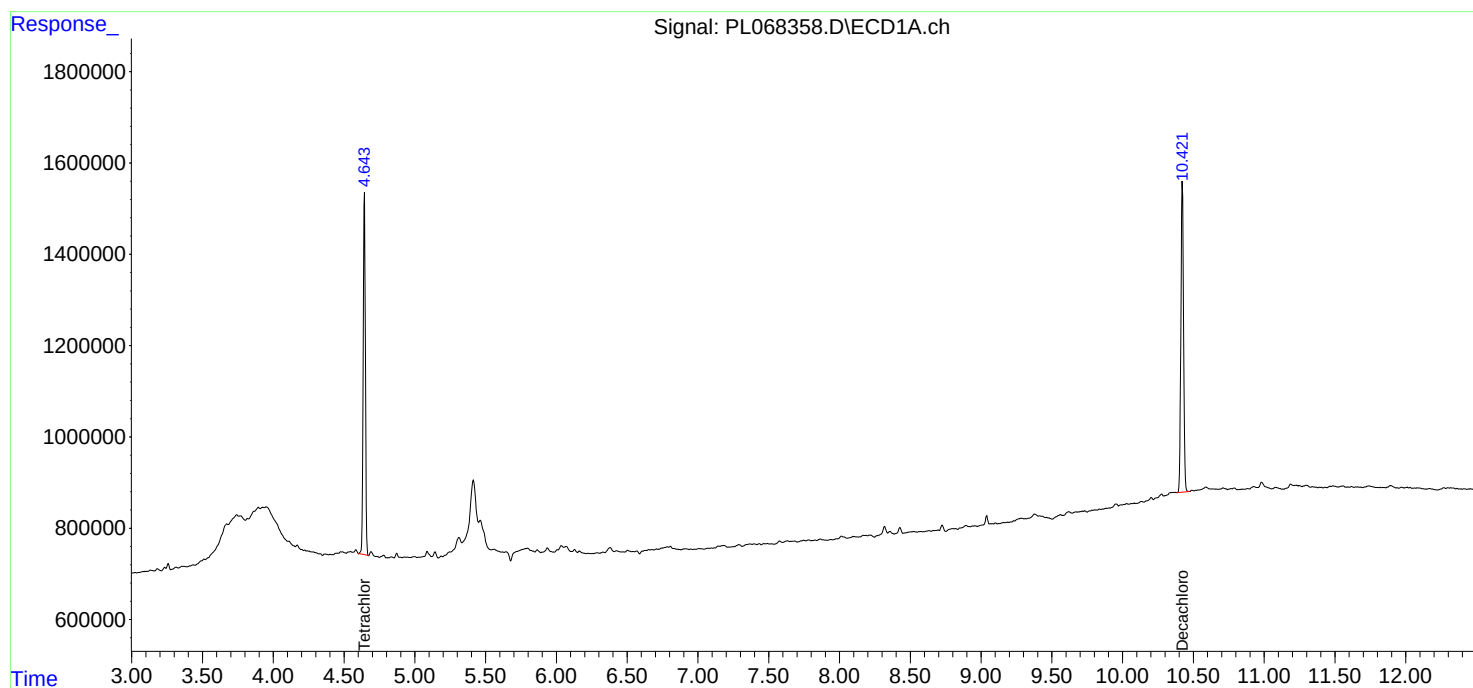


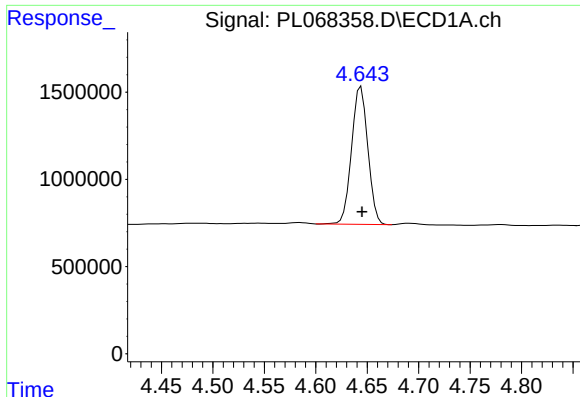

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: -0.001 min
Response: 8699716
Conc: 20.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

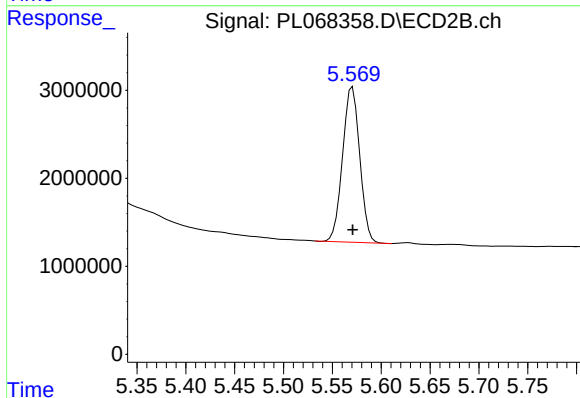


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 21618318
Conc: 21.19 ng/ml

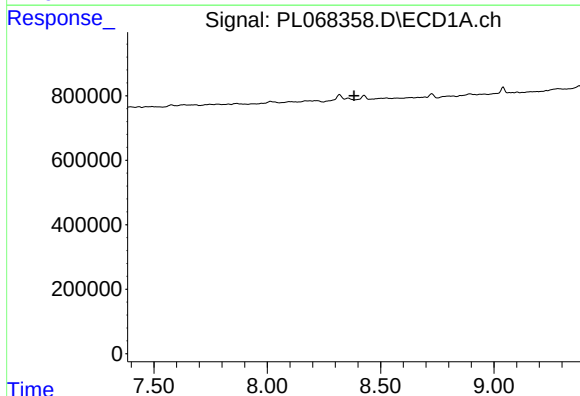


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

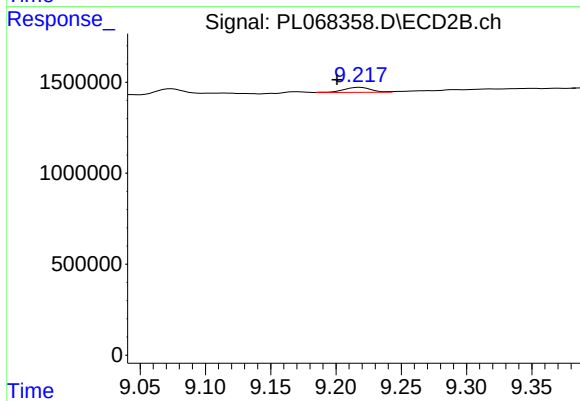

#15 Endosulfan II


R.T.: 9.219 min
Delta R.T.: 0.018 min
Response: 402510
Conc: 0.44 ng/ml

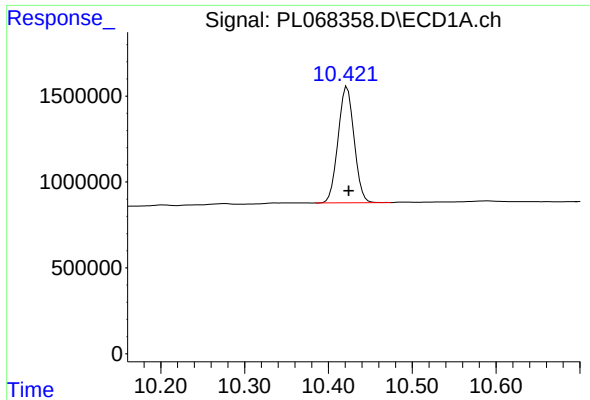

#28 Decachlorobiphenyl

R.T.: 10.422 min
Delta R.T.: -0.002 min
Response: 8971310
Conc: 15.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

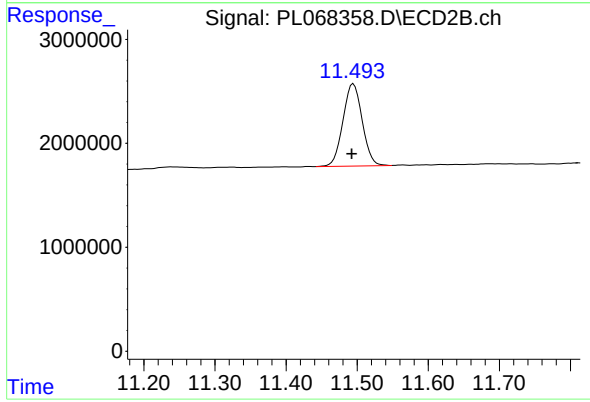

#28 Decachlorobiphenyl

R.T.: 11.495 min
Delta R.T.: 0.003 min
Response: 14921257
Conc: 16.73 ng/ml