

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072121\
 Data File : PL068342.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2021 12:53
 Operator : AR\AJ
 Sample : M2940-07
 Misc : TOX MDL 50 PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2021

Manual Integrations
 APPROVED

mohammad
 7/22/2021 10:55:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:22:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.645	5.573	7292079	17373473	16.991	17.026
28) SA Decachlor...	10.425	11.498	9865567	16320425	17.541	18.297
Target Compounds						
14) MA Endrin	0.000	8.985f	0	186959	N.D.	0.209 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072121\
Data File : PL068342.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2021 12:53
Operator : AR\AJ
Sample : M2940-07
Misc : TOX MDL 50 PPB
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021


Manual Integrations
APPROVED

mohammad
7/22/2021 10:55:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:22:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

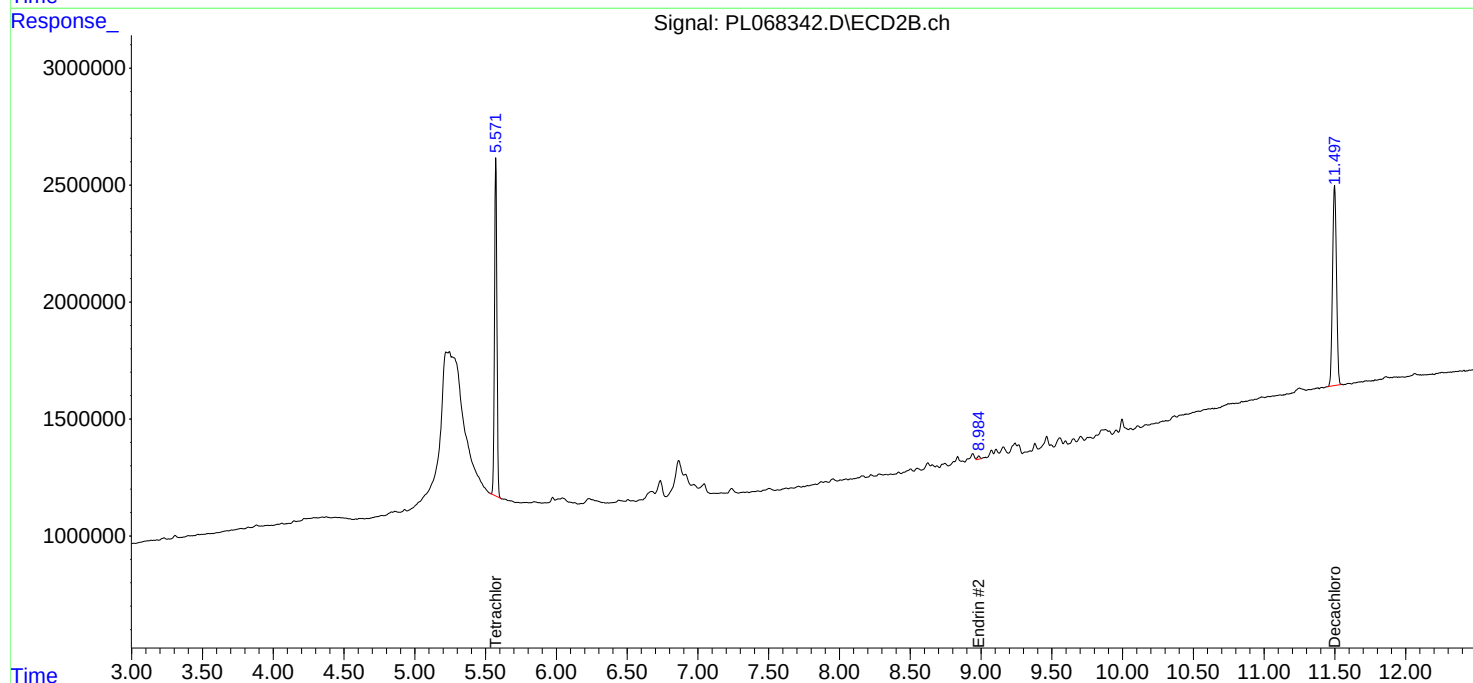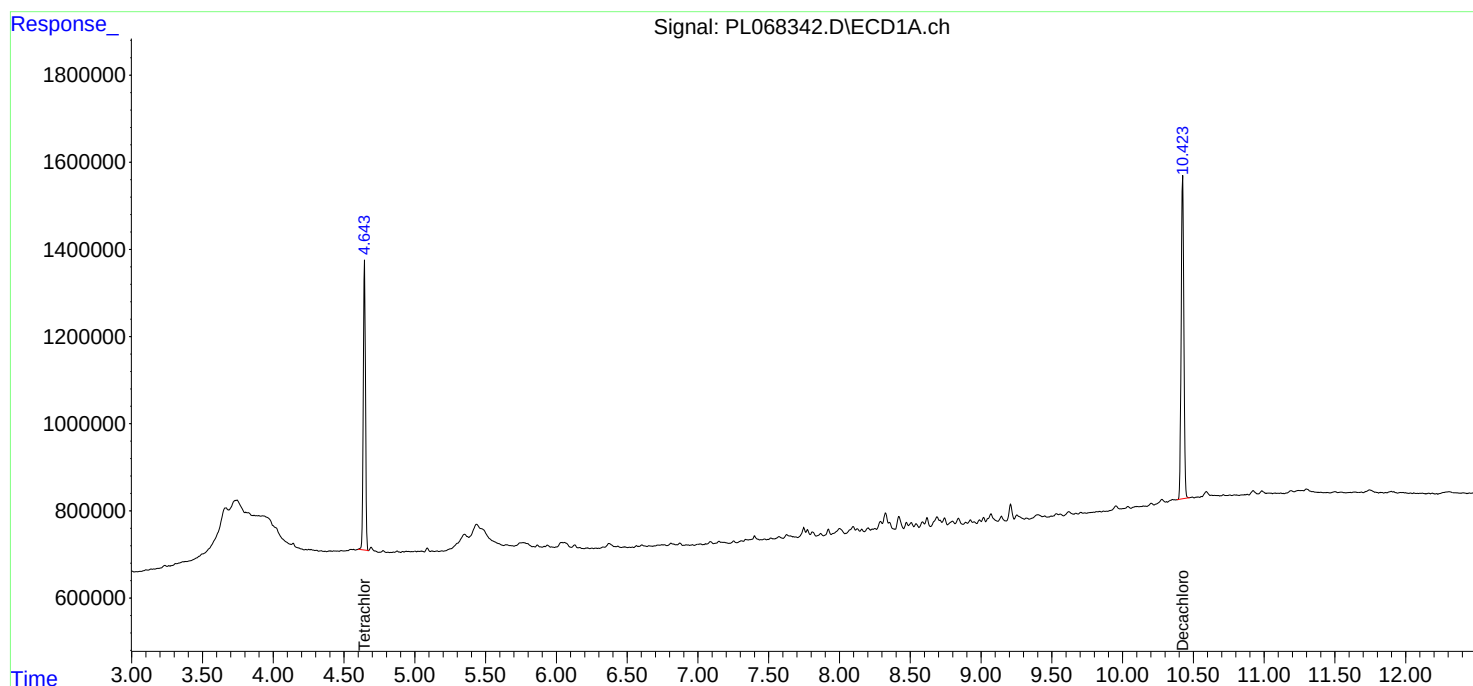

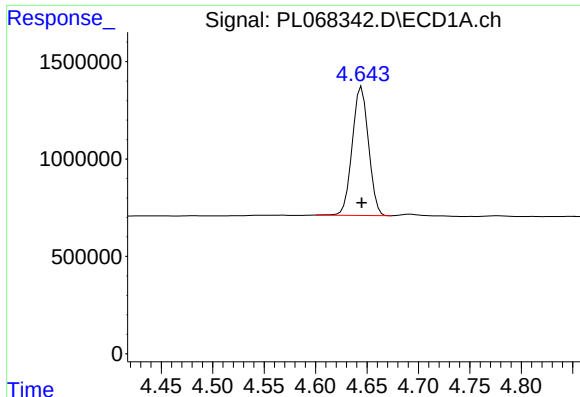


#1 Tetrachloro-m-xylene

R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 7292079
Conc: 16.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021


Manual Integrations
APPROVED

mohammad
7/22/2021 10:55:53 AM

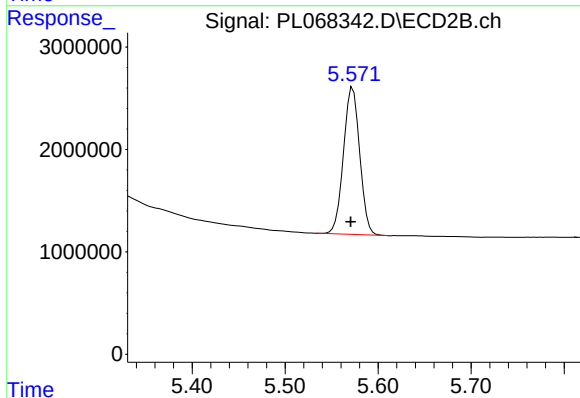


#1 Tetrachloro-m-xylene

R.T.: 5.573 min
Delta R.T.: 0.002 min
Response: 17373473
Conc: 17.03 ng/ml

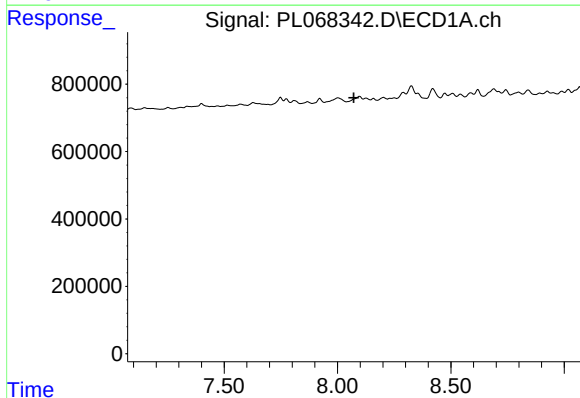


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.072 min
Response: 0
Conc: N.D.

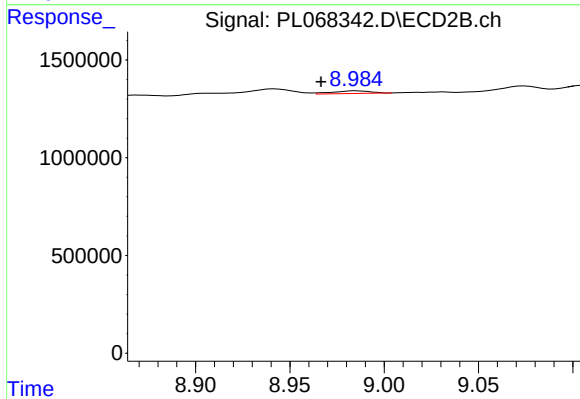

#14 Endrin

R.T.: 8.985 min
Delta R.T.: 0.019 min
Response: 186959
Conc: 0.21 ng/ml

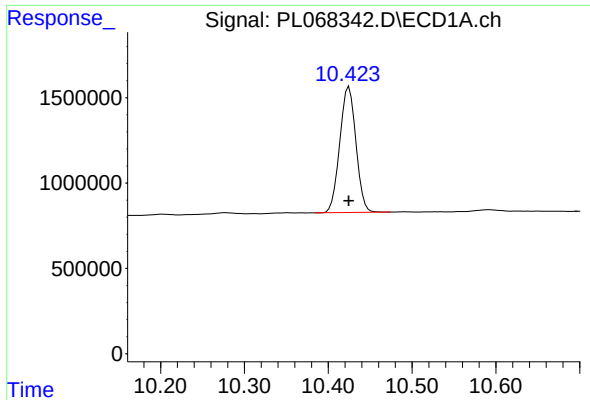


#28 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: 0.000 min
Response: 9865567
Conc: 17.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

Manual Integrations
APPROVED

mohammad
7/22/2021 10:55:53 AM

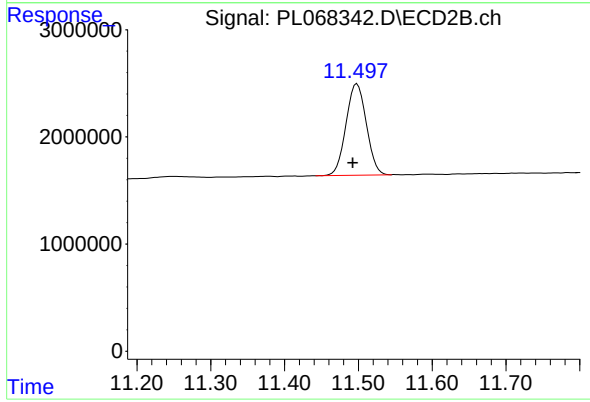

#28 Decachlorobiphenyl

R.T.: 11.498 min
Delta R.T.: 0.006 min
Response: 16320425
Conc: 18.30 ng/ml