

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072121\
 Data File : PL068343.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2021 13:10
 Operator : AR\AJ
 Sample : M2940-09
 Misc : TOX MDL 50 PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-03-QT3-2021

Manual Integrations
 APPROVED

mohammad
 7/22/2021 10:55:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:22:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.573	7086253	17011531	16.511	16.671
28)	SA Decachlor...	10.425	11.499	9609419	15923631	17.086	17.852
Target Compounds							
14)	MA Endrin	0.000	8.987f	0	214180	N.D.	0.240 #
19)	B Endosulfa...	0.000	9.556f	0	495731	N.D.	0.551 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072121\
Data File : PL068343.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2021 13:10
Operator : AR\AJ
Sample : M2940-09
Misc : TOX MDL 50 PPB
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-03-QT3-2021


Manual Integrations
APPROVED

mohammad
7/22/2021 10:55:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:22:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

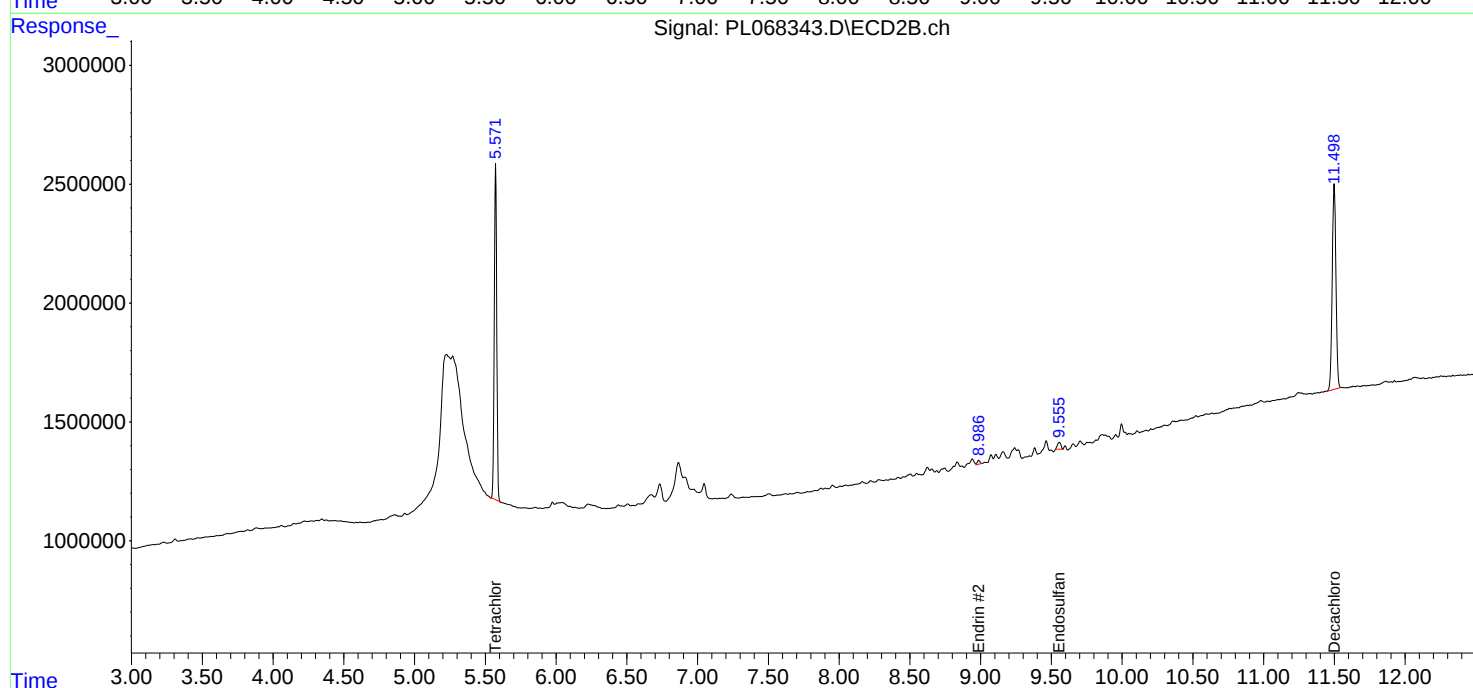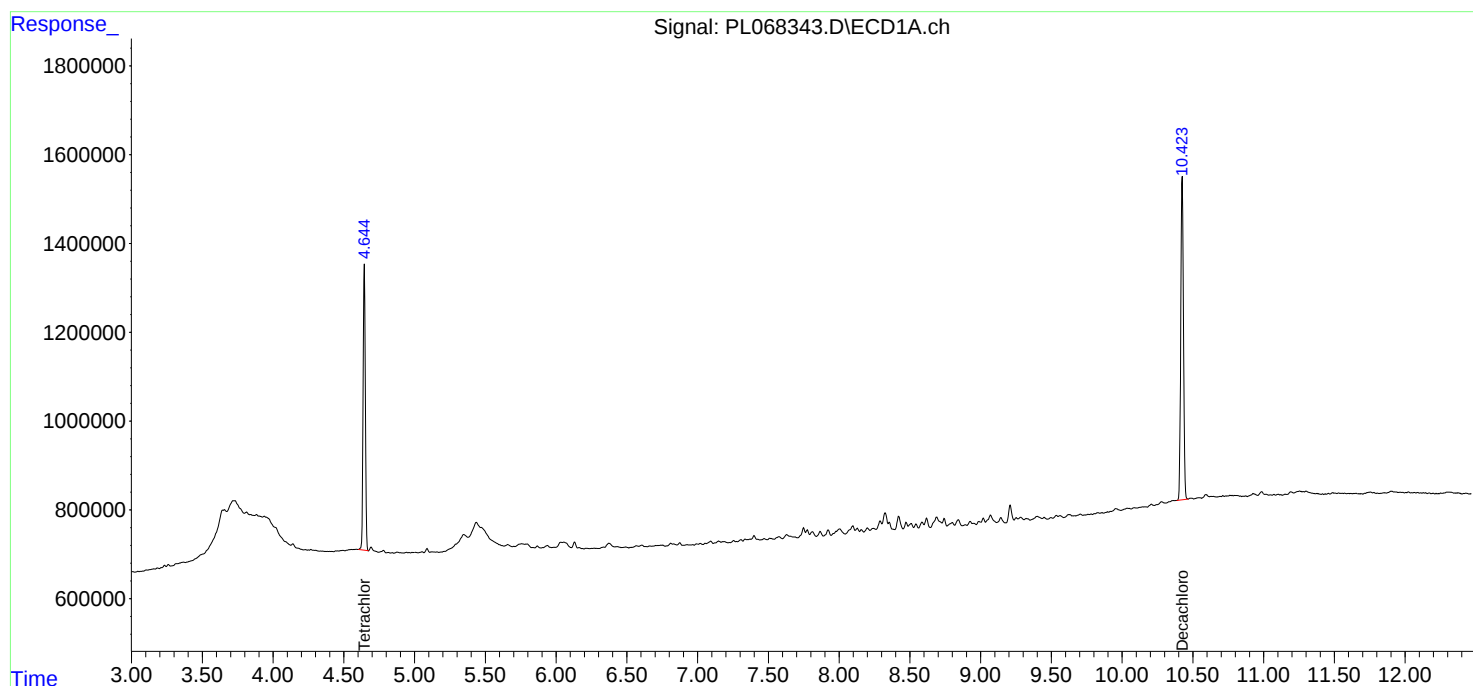

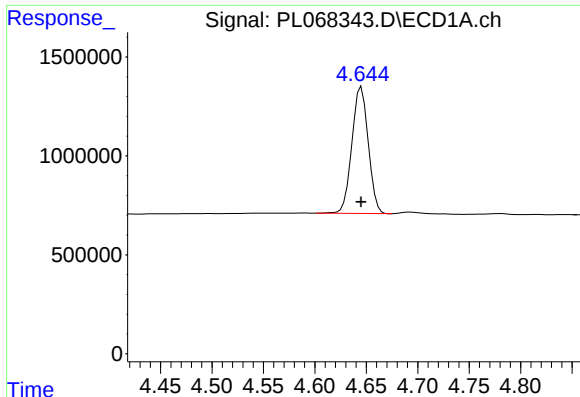


#1 Tetrachloro-m-xylene

R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 7086253
Conc: 16.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-WATER-03-QT3-2021


Manual Integrations
APPROVED

mohammad
7/22/2021 10:55:56 AM

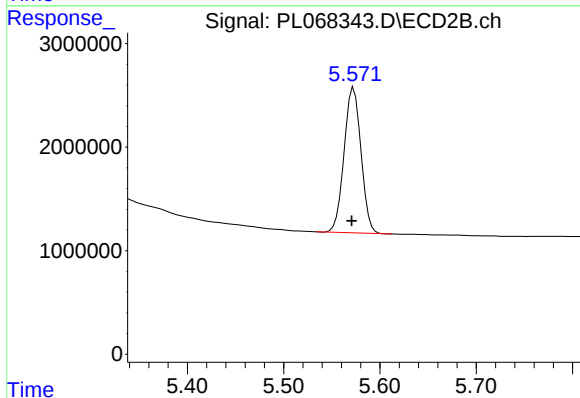


#1 Tetrachloro-m-xylene

R.T.: 5.573 min
Delta R.T.: 0.002 min
Response: 17011531
Conc: 16.67 ng/ml

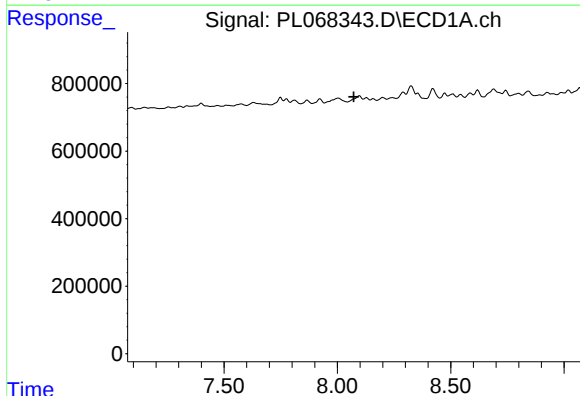


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.072 min
Response: 0
Conc: N.D.

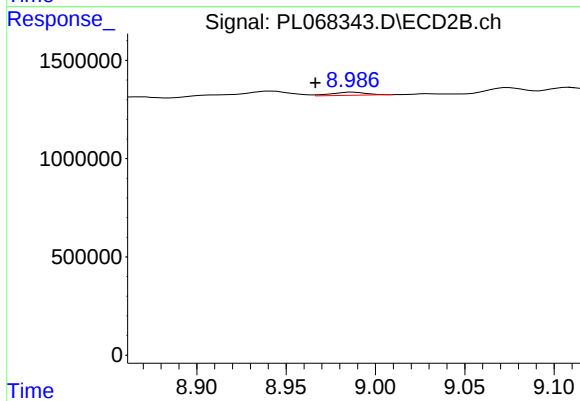

#14 Endrin

R.T.: 8.987 min
Delta R.T.: 0.021 min
Response: 214180
Conc: 0.24 ng/ml

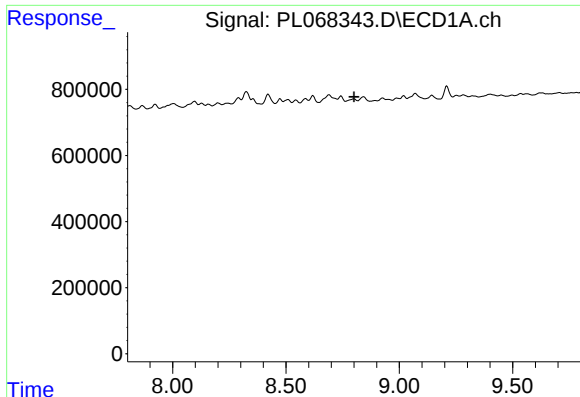


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MDL-WATER-03-QT3-2021


Manual Integrations
APPROVED

mohammad
7/22/2021 10:55:56 AM

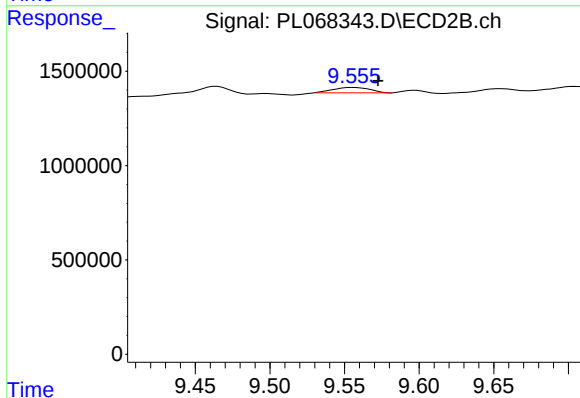


#19 Endosulfan Sulfate

R.T.: 9.556 min
Delta R.T.: -0.017 min
Response: 495731
Conc: 0.55 ng/ml

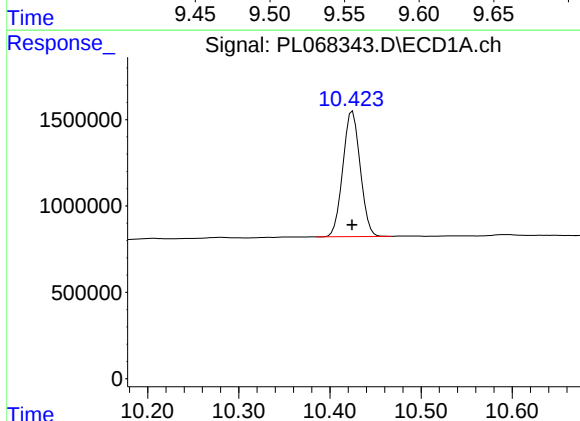

#28 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: 0.000 min
Response: 9609419
Conc: 17.09 ng/ml

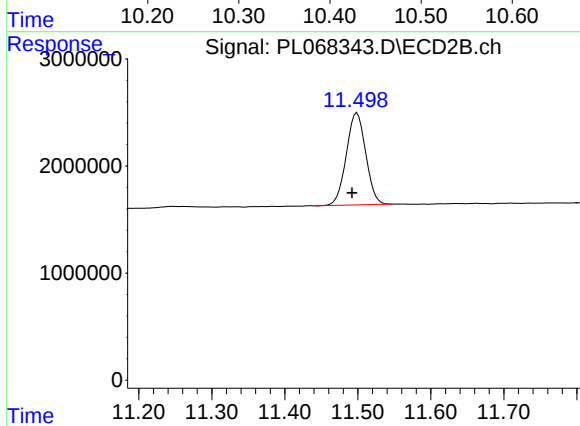

#28 Decachlorobiphenyl

R.T.: 11.499 min
Delta R.T.: 0.007 min
Response: 15923631
Conc: 17.85 ng/ml