

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
 Data File : PL076532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2022 11:48
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 12:58:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 21 12:57:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.642	4520832	12051168	4.934	5.074
27)	SA Decachlor...	8.910	7.752	8625002	21650855	10.822	10.702
Target Compounds							
2)	A alpha-BHC	3.885	3.136	5669891	16178181	4.630	4.792
3)	MA gamma-BHC...	4.220	3.460	5852072	15175601	4.885	4.730
4)	MA Heptachlor	4.797	3.795	6195154	15039801	5.118	5.007
9)	A Endosulfan I	5.956	4.935	4810855	11811369	5.001	5.084
13)	MA Dieldrin	6.233	5.199	9765721	24504448	9.640	9.803
14)	MA Endrin	6.465	5.472	7836918	19630391	9.421	9.580
16)	A 4,4'-DDD	6.605	5.629	7397121	18612899	9.489	9.743
17)	MA 4,4'-DDT	6.916	5.878	7984409	18275086	9.720	9.457
20)	A Methoxychlor	7.397	6.456	23558507	52557818	51.712	51.298


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
Data File : PL076532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 11:48
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 12:58:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 21 12:57:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

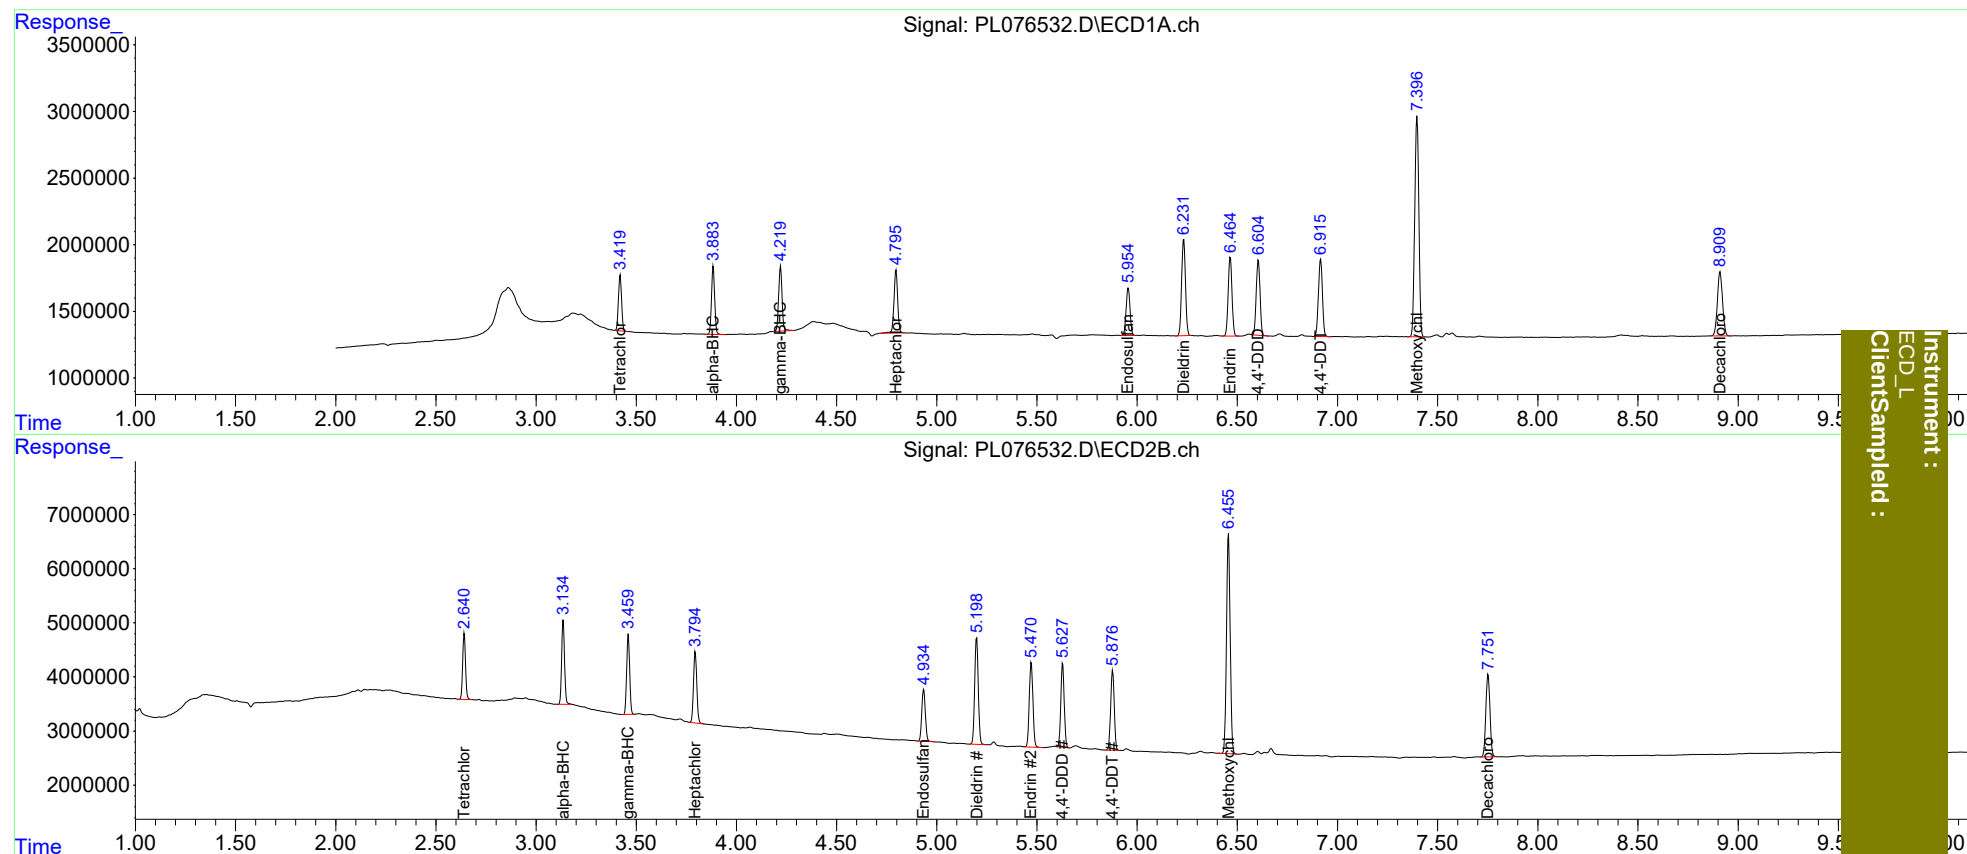


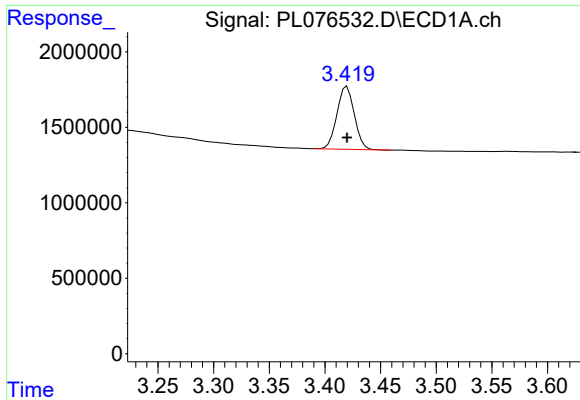

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 4520832
Conc: 4.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

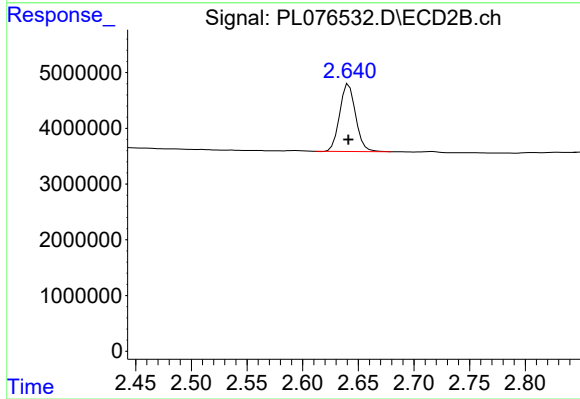


#1 Tetrachloro-m-xylene

R.T.: 2.642 min
Delta R.T.: 0.000 min
Response: 12051168
Conc: 5.07 ng/ml

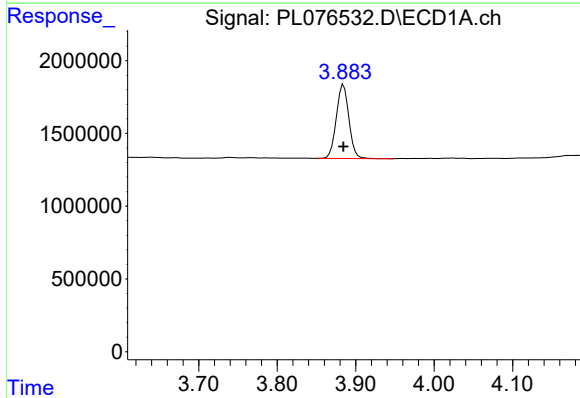


#2 alpha-BHC

R.T.: 3.885 min
Delta R.T.: 0.000 min
Response: 5669891
Conc: 4.63 ng/ml

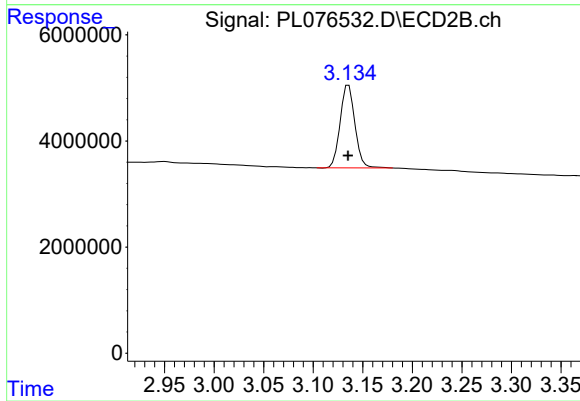

#2 alpha-BHC


R.T.: 3.136 min
Delta R.T.: 0.000 min
Response: 16178181
Conc: 4.79 ng/ml

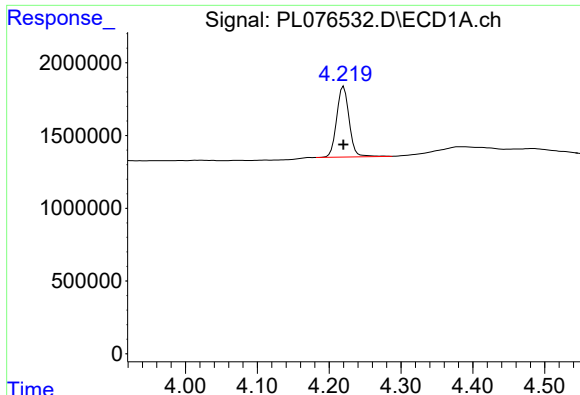

#3 gamma-BHC (Lindane)


R.T.: 4.220 min
Delta R.T.: 0.000 min
Response: 5852072
Conc: 4.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

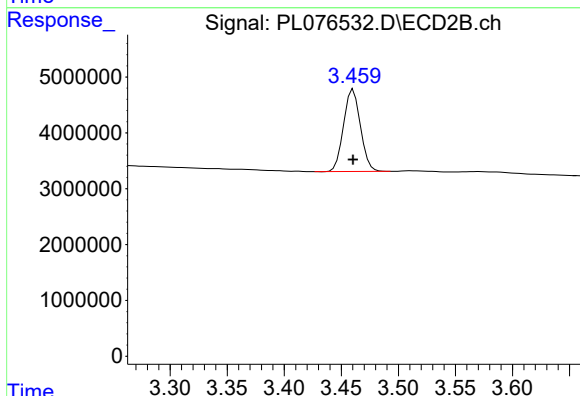


#3 gamma-BHC (Lindane)

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 15175601
Conc: 4.73 ng/ml

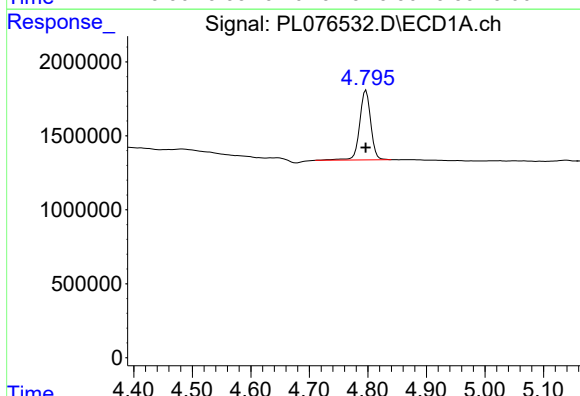


#4 Heptachlor

R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 6195154
Conc: 5.12 ng/ml

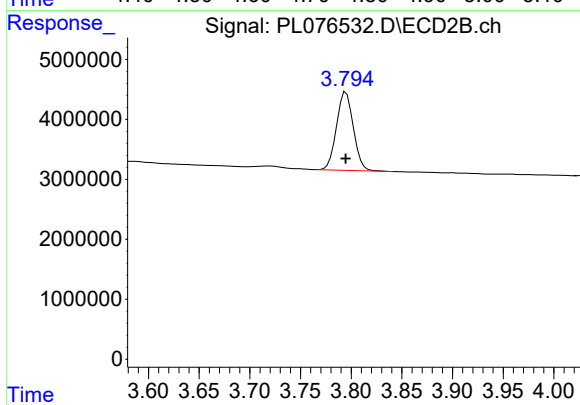

#4 Heptachlor


R.T.: 3.795 min
Delta R.T.: 0.000 min
Response: 15039801
Conc: 5.01 ng/ml

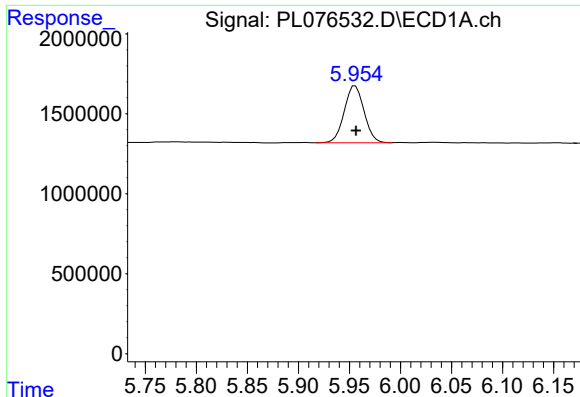

#9 Endosulfan I


R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 4810855
Conc: 5.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

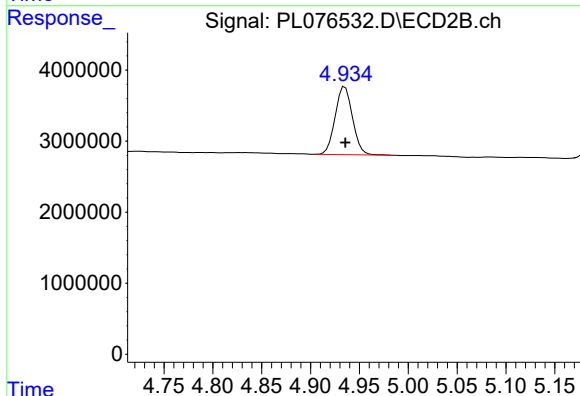


#9 Endosulfan I

R.T.: 4.935 min
Delta R.T.: 0.000 min
Response: 11811369
Conc: 5.08 ng/ml

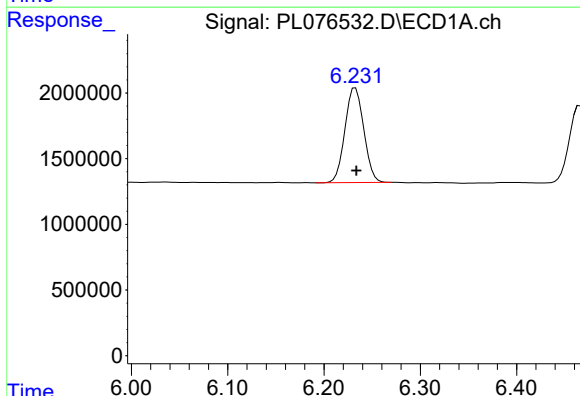


#13 Dieldrin

R.T.: 6.233 min
Delta R.T.: -0.001 min
Response: 9765721
Conc: 9.64 ng/ml

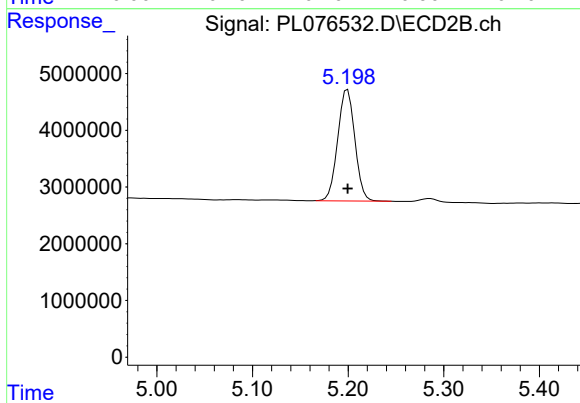

#13 Dieldrin


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 24504448
Conc: 9.80 ng/ml

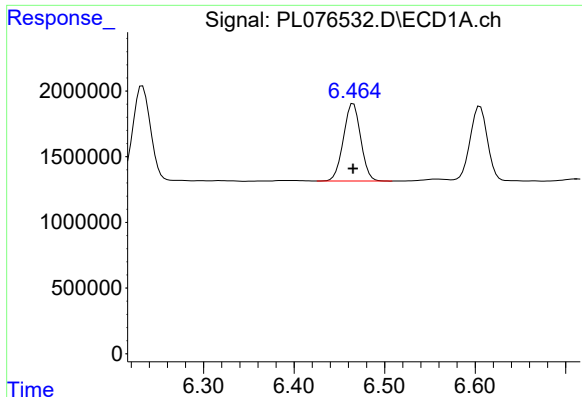

#14 Endrin


R.T.: 6.465 min
Delta R.T.: 0.000 min
Response: 7836918
Conc: 9.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

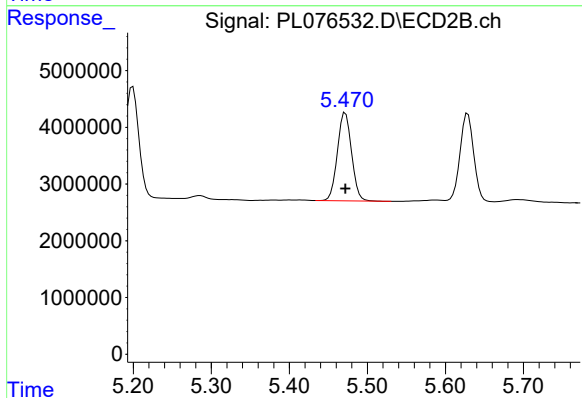


#14 Endrin

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 19630391
Conc: 9.58 ng/ml

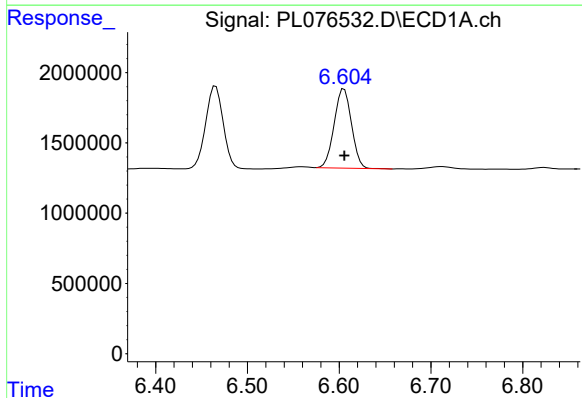


#16 4,4'-DDD

R.T.: 6.605 min
Delta R.T.: 0.000 min
Response: 7397121
Conc: 9.49 ng/ml

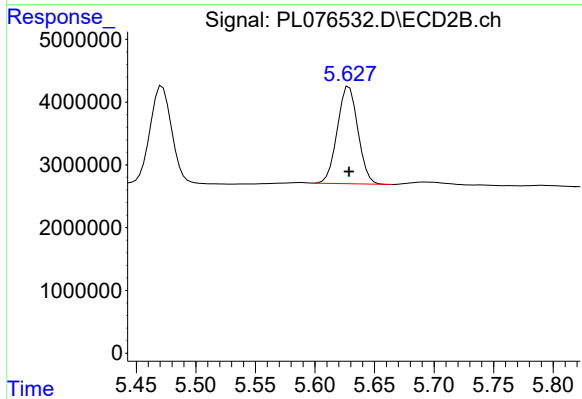

#16 4,4'-DDD


R.T.: 5.629 min
Delta R.T.: 0.000 min
Response: 18612899
Conc: 9.74 ng/ml

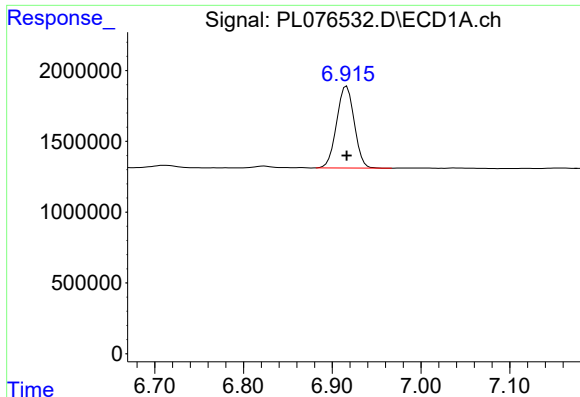

#17 4,4'-DDT


R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 7984409
Conc: 9.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

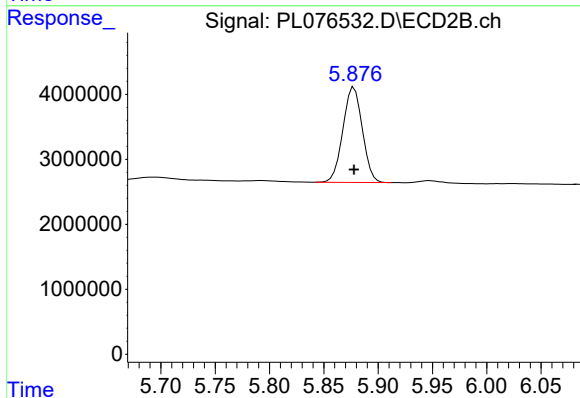


#17 4,4'-DDT

R.T.: 5.878 min
Delta R.T.: 0.000 min
Response: 18275086
Conc: 9.46 ng/ml

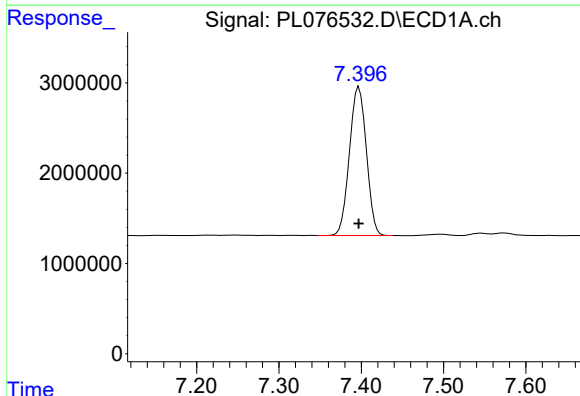


#20 Methoxychlor

R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 23558507
Conc: 51.71 ng/ml

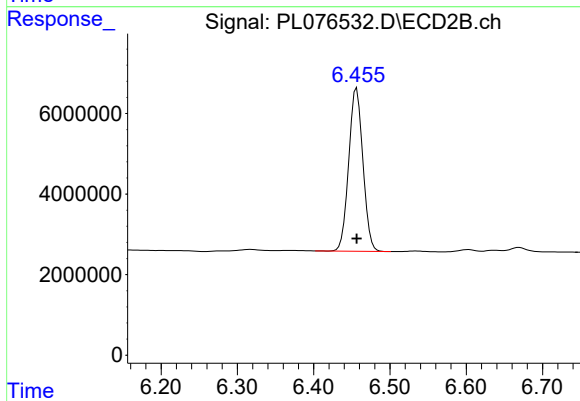

#20 Methoxychlor


R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 52557818
Conc: 51.30 ng/ml

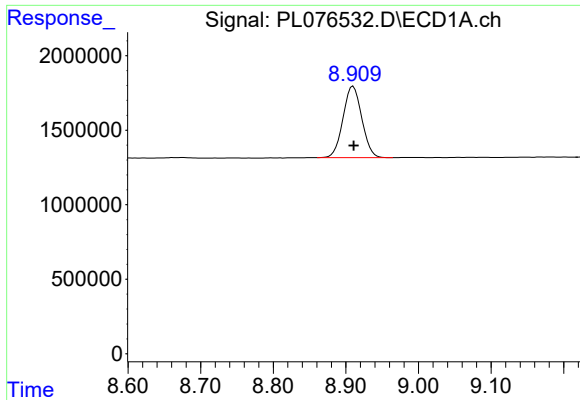

#27 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: -0.001 min
Response: 8625002
Conc: 10.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

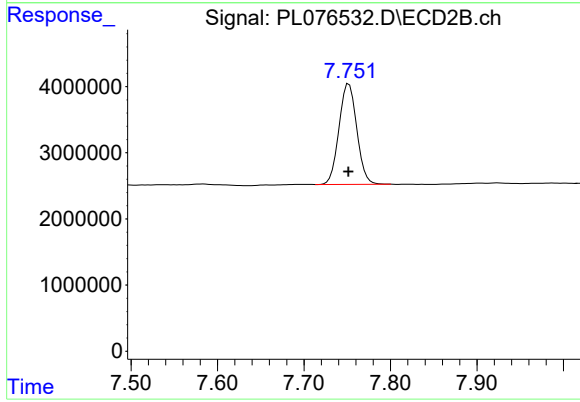

#27 Decachlorobiphenyl

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 21650855
Conc: 10.70 ng/ml