

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
 Data File : PL076534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2022 12:16
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 12:59:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 21 12:57:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.641	9360044	24154534	10.216	10.170
27)	SA Decachlor...	8.912	7.751	16867787	42434507	21.165	20.975
Target Compounds							
2)	A alpha-BHC	3.884	3.136	11962140	33321908	9.769	9.870
3)	MA gamma-BHC...	4.220	3.460	11853784	31807003	9.895	9.914
4)	MA Heptachlor	4.797	3.795	12360030	30356681	10.210	10.106
9)	A Endosulfan I	5.956	4.936	9711460	23702415	10.095	10.202
13)	MA Dieldrin	6.234	5.199	19986268	49939457	19.729	19.978
14)	MA Endrin	6.465	5.472	16377728	40593439	19.688	19.811
16)	A 4,4'-DDD	6.606	5.629	15275814	37847548	19.596	19.812
17)	MA 4,4'-DDT	6.917	5.878	16373709	38501926	19.933	19.925
20)	A Methoxychlor	7.397	6.457	46749855	105.5E6	102.618	102.965


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
Data File : PL076534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 12:16
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 12:59:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 21 12:57:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

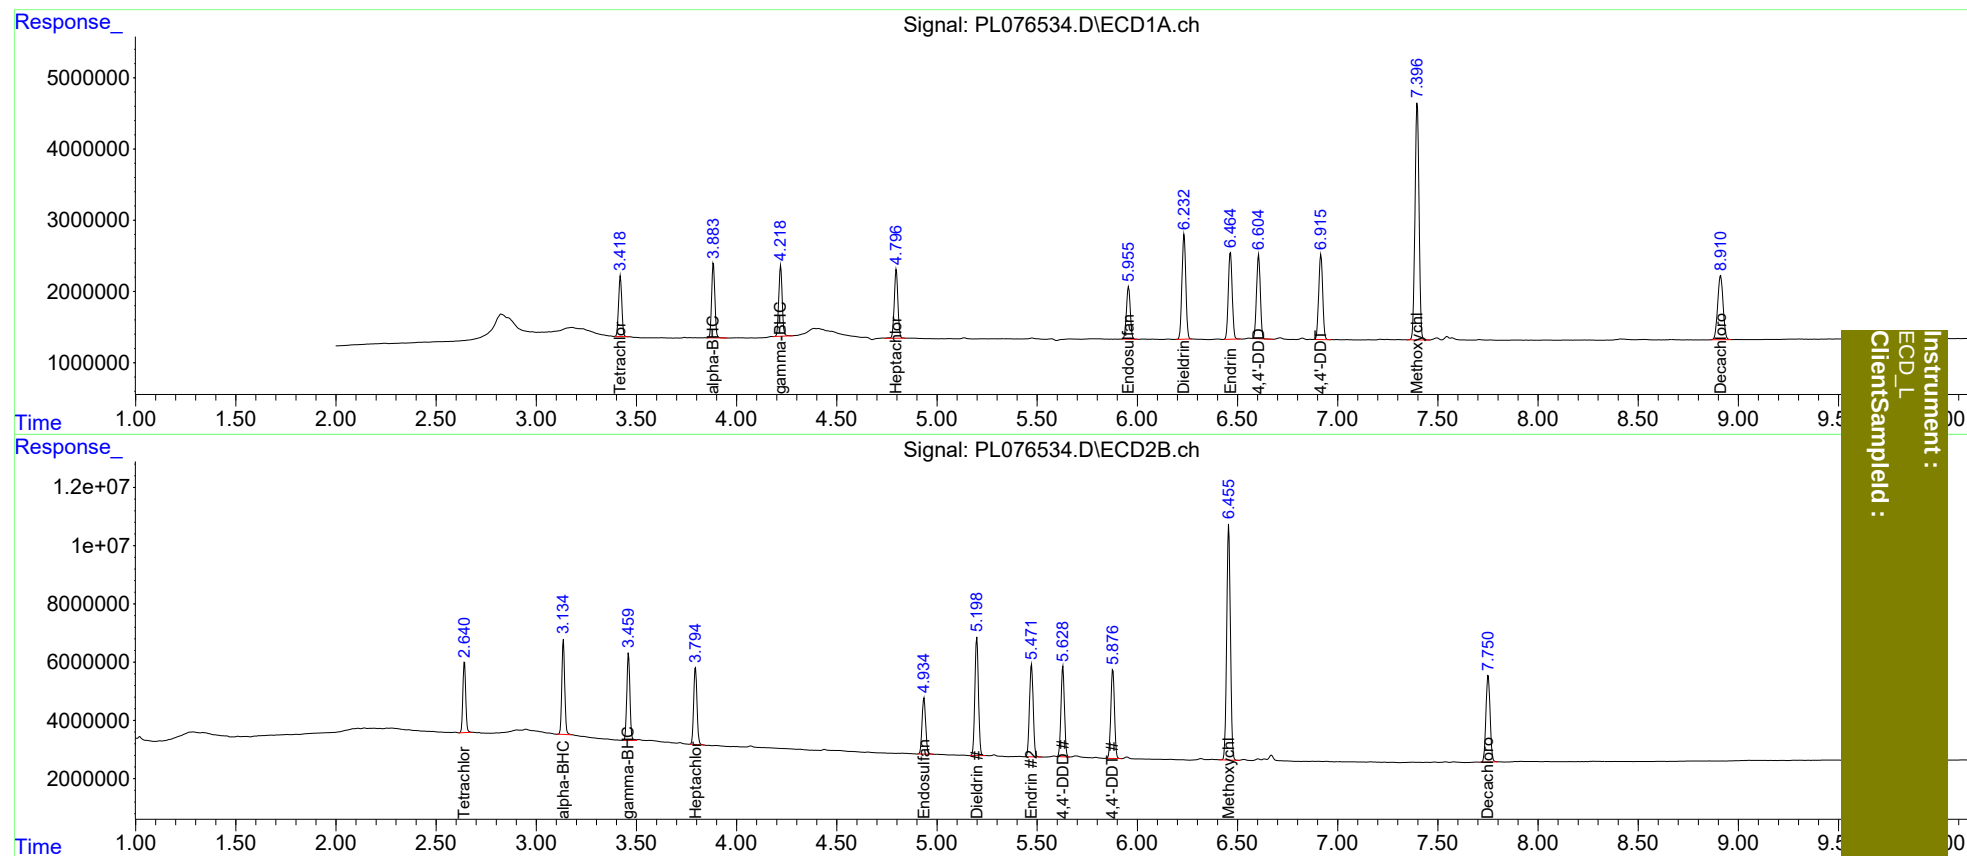


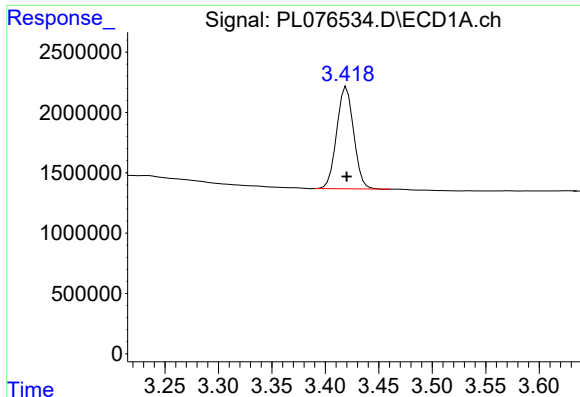

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 9360044
Conc: 10.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

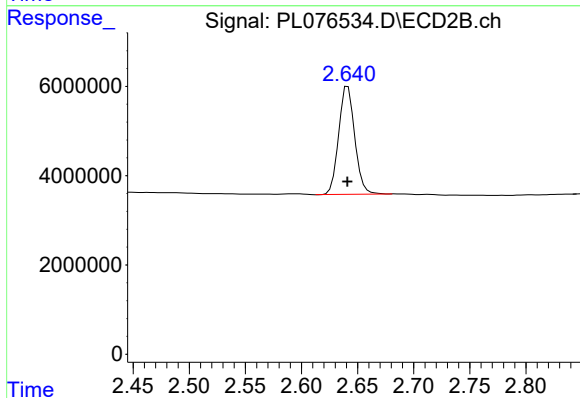


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: 0.000 min
Response: 24154534
Conc: 10.17 ng/ml

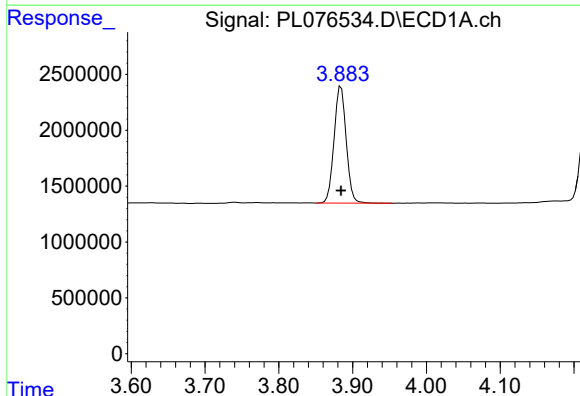


#2 alpha-BHC

R.T.: 3.884 min
Delta R.T.: 0.000 min
Response: 11962140
Conc: 9.77 ng/ml

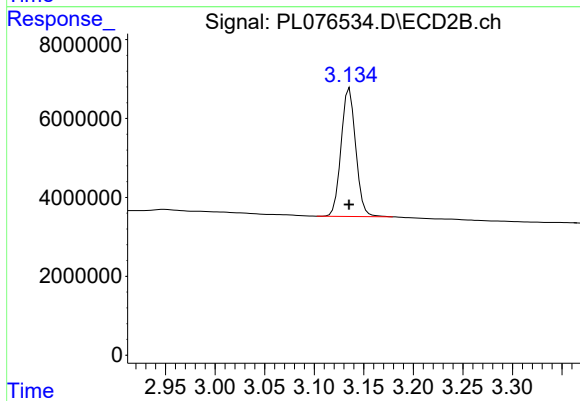

#2 alpha-BHC


R.T.: 3.136 min
Delta R.T.: 0.000 min
Response: 33321908
Conc: 9.87 ng/ml

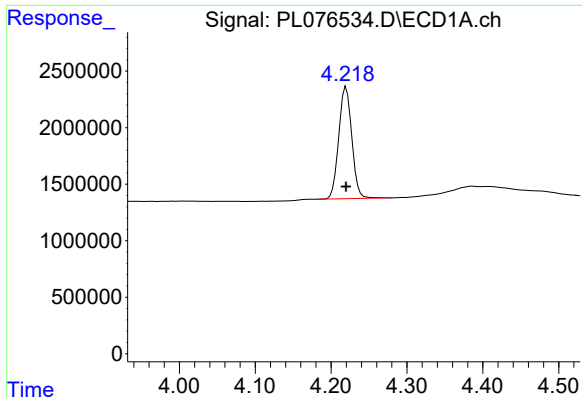

#3 gamma-BHC (Lindane)


R.T.: 4.220 min
Delta R.T.: 0.000 min
Response: 11853784
Conc: 9.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

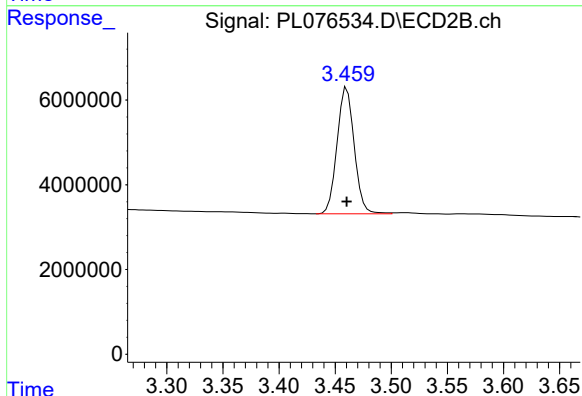


#3 gamma-BHC (Lindane)

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 31807003
Conc: 9.91 ng/ml

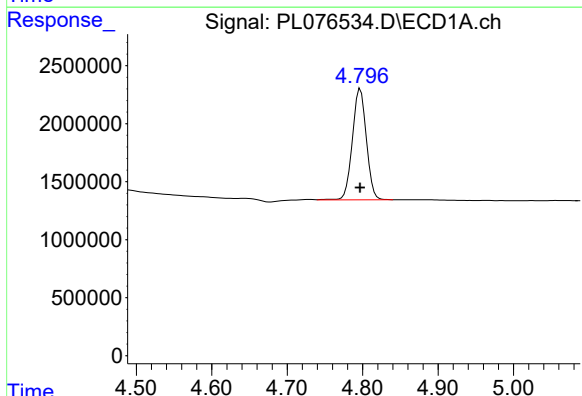


#4 Heptachlor

R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 12360030
Conc: 10.21 ng/ml

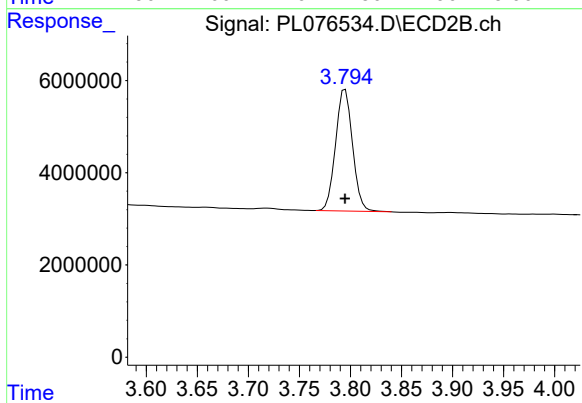

#4 Heptachlor


R.T.: 3.795 min
Delta R.T.: 0.000 min
Response: 30356681
Conc: 10.11 ng/ml

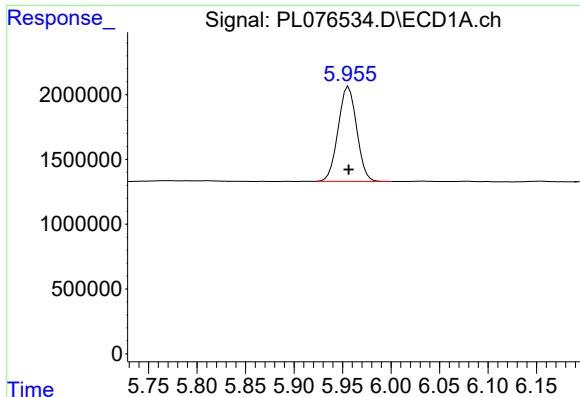

#9 Endosulfan I


R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 9711460
Conc: 10.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

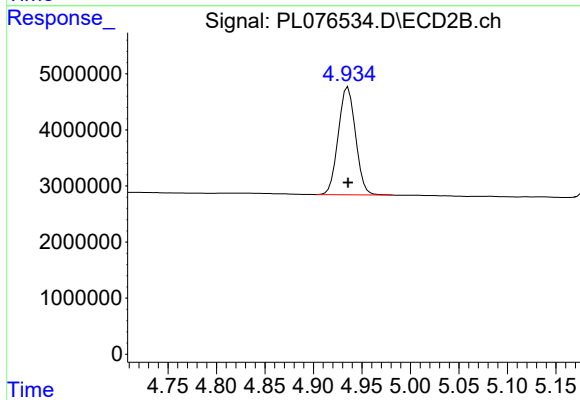


#9 Endosulfan I

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 23702415
Conc: 10.20 ng/ml

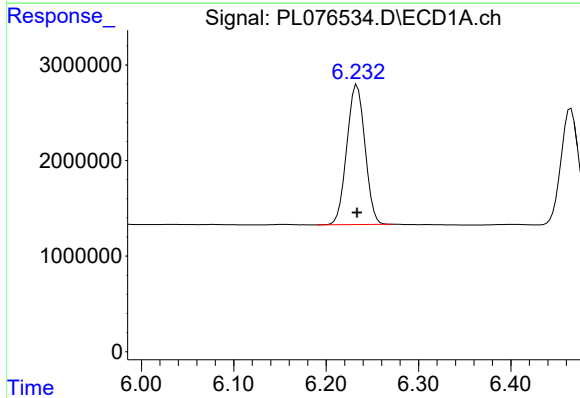


#13 Dieldrin

R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 19986268
Conc: 19.73 ng/ml

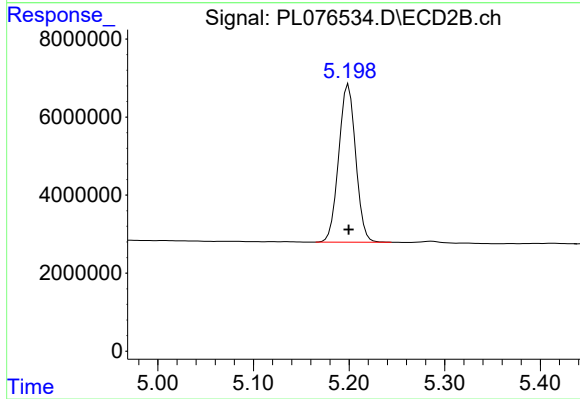

#13 Dieldrin


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 49939457
Conc: 19.98 ng/ml

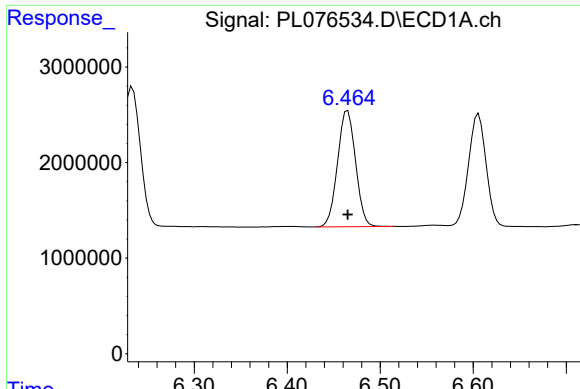

#14 Endrin


R.T.: 6.465 min
Delta R.T.: 0.000 min
Response: 16377728
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

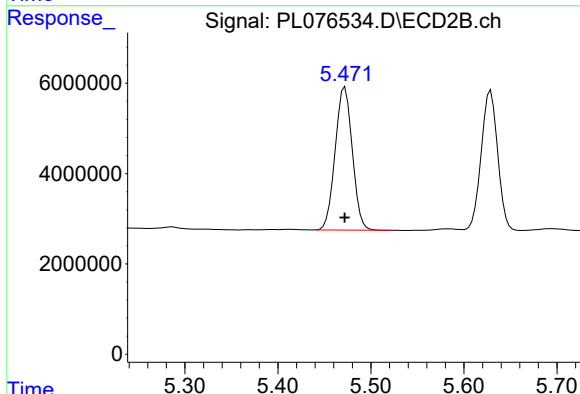


#14 Endrin

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 40593439
Conc: 19.81 ng/ml

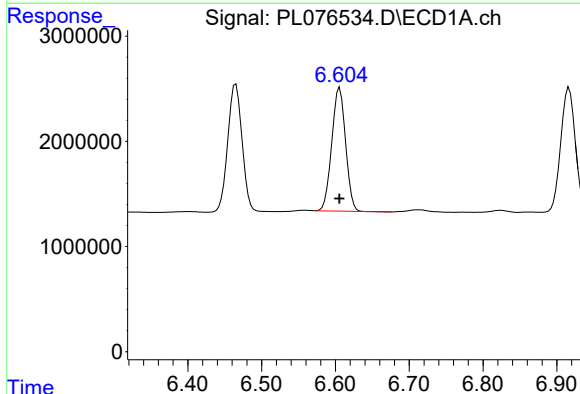


#16 4,4'-DDD

R.T.: 6.606 min
Delta R.T.: 0.000 min
Response: 15275814
Conc: 19.60 ng/ml

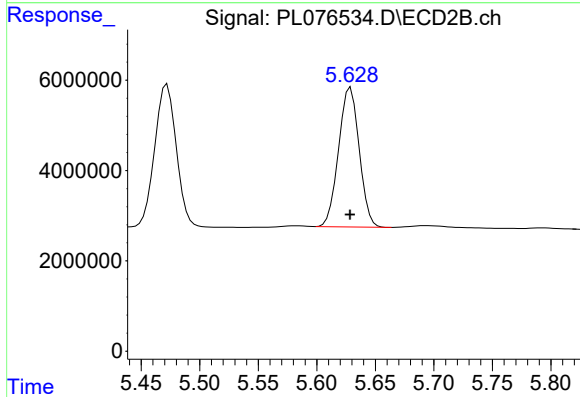

#16 4,4'-DDD


R.T.: 5.629 min
Delta R.T.: 0.000 min
Response: 37847548
Conc: 19.81 ng/ml

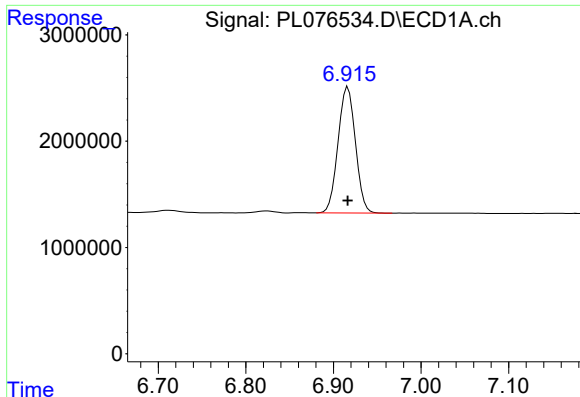

#17 4,4'-DDT


R.T.: 6.917 min
Delta R.T.: 0.000 min
Response: 16373709
Conc: 19.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

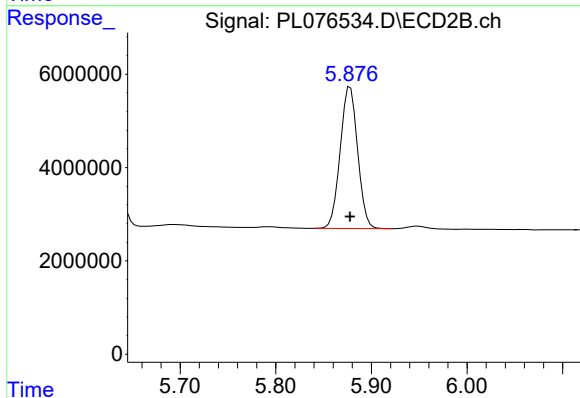


#17 4,4'-DDT

R.T.: 5.878 min
Delta R.T.: 0.000 min
Response: 38501926
Conc: 19.93 ng/ml

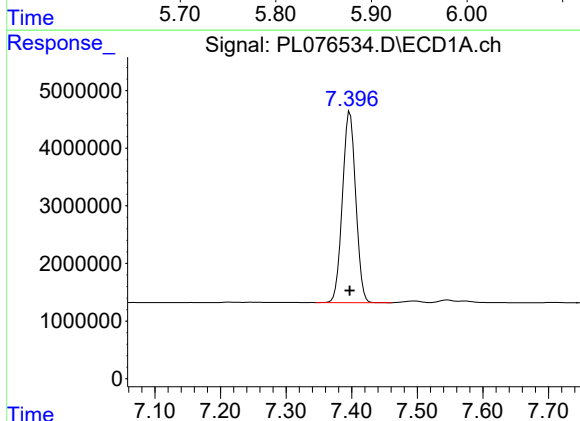


#20 Methoxychlor

R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 46749855
Conc: 102.62 ng/ml

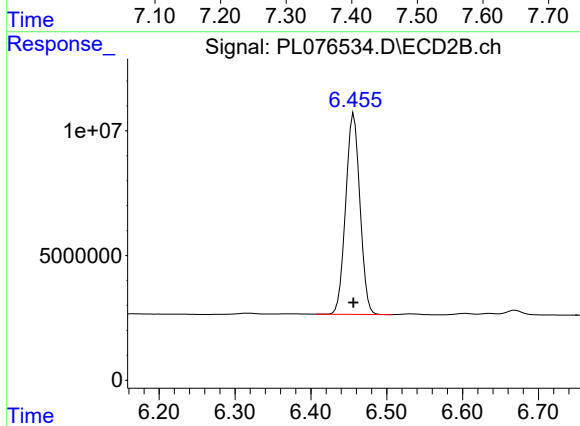

#20 Methoxychlor


R.T.: 6.457 min
Delta R.T.: 0.000 min
Response: 105493594
Conc: 102.96 ng/ml

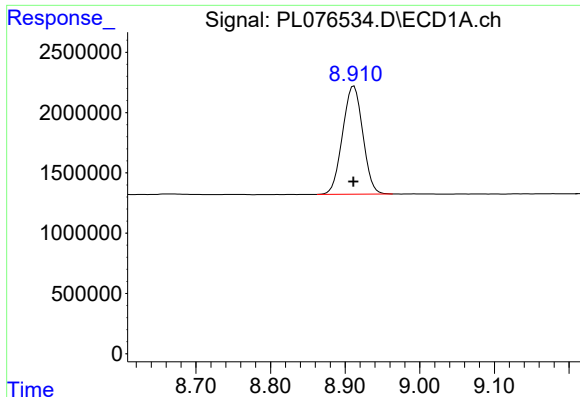

#27 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: 0.000 min
Response: 16867787
Conc: 21.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

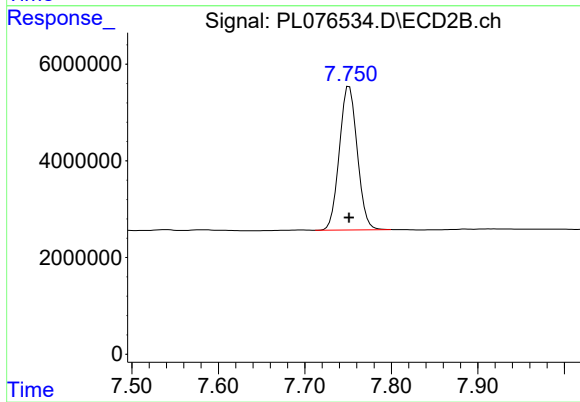

#27 Decachlorobiphenyl

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 42434507
Conc: 20.97 ng/ml