

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
 Data File : PL076536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2022 12:44
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 12:57:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 21 12:57:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.641	18324840	47502385	20.000	20.000
27)	SA Decachlor...	8.911	7.751	31879106	80925563	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.884	3.135	24489858	67520704	20.000	20.000
3)	MA gamma-BHC...	4.220	3.460	23960182	64166090	20.000	20.000
4)	MA Heptachlor	4.796	3.795	24210756	60079148	20.000	20.000
9)	A Endosulfan I	5.956	4.936	19239981	46464075	20.000	20.000
13)	MA Dieldrin	6.234	5.199	40521967	99990465	40.000	40.000
14)	MA Endrin	6.465	5.472	33274888	81961401	40.000	40.000
16)	A 4,4'-DDD	6.606	5.629	31181202	76411737	40.000	40.000
17)	MA 4,4'-DDT	6.916	5.878	32857874	77293685	40.000	40.000
20)	A Methoxychlor	7.397	6.456	91114517	204.9E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
Data File : PL076536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 12:44
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 12:57:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 21 12:57:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

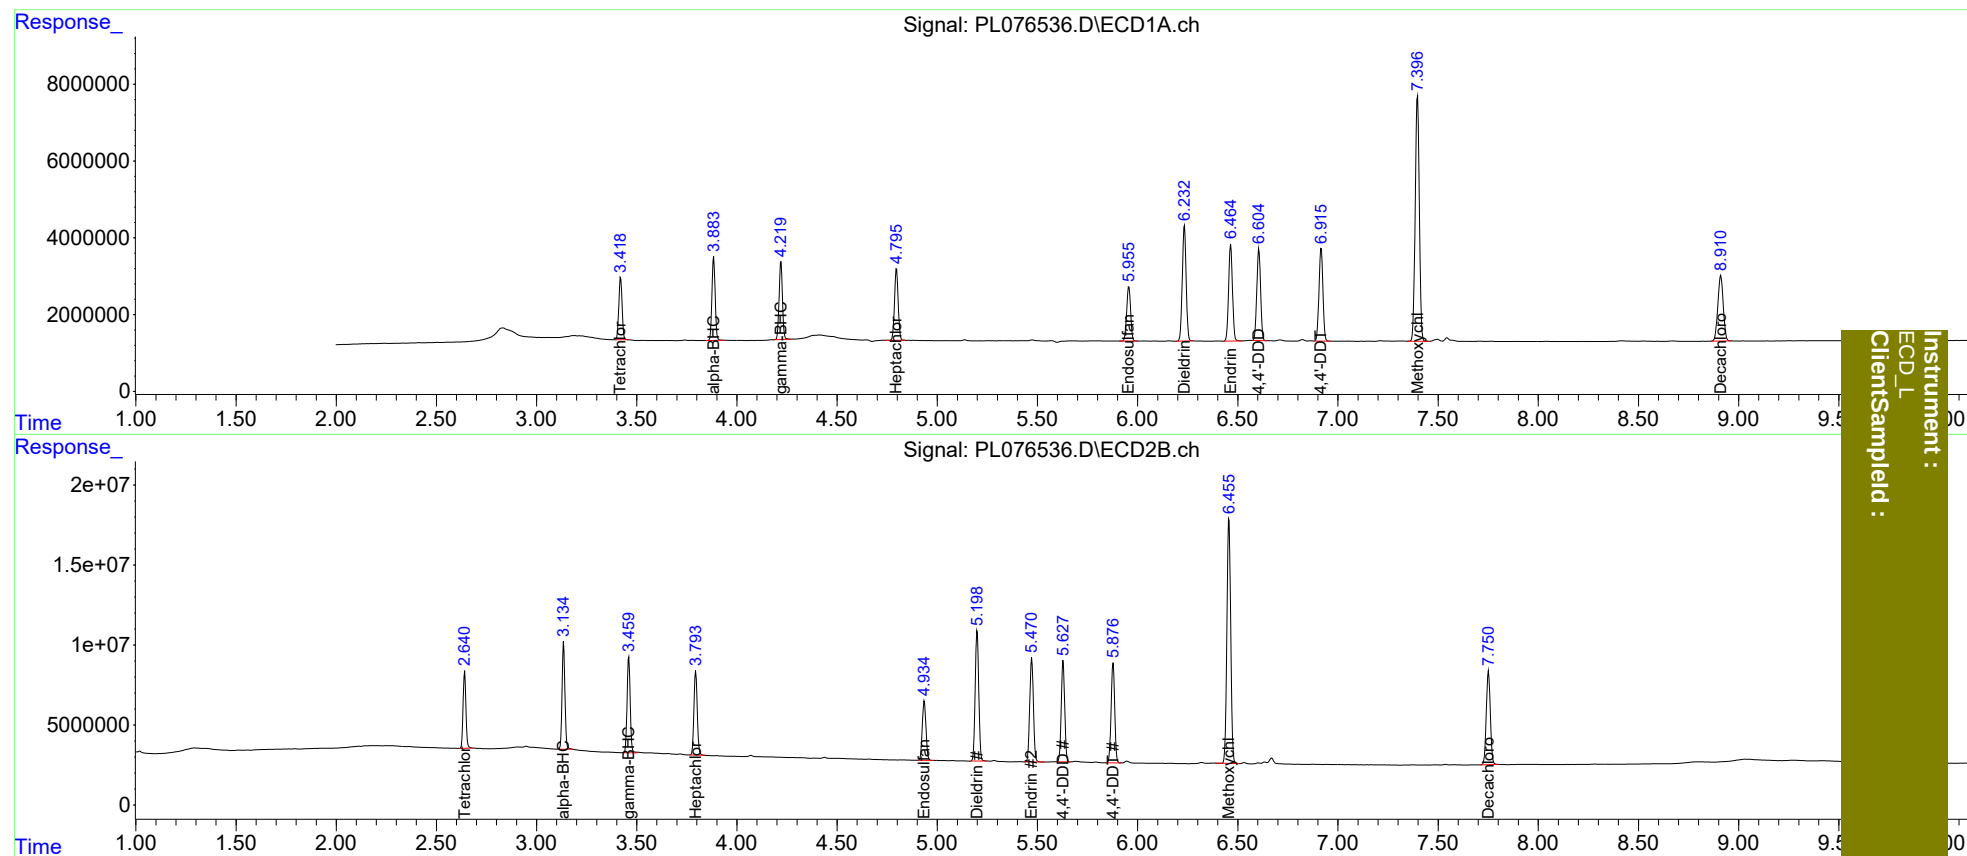


Instrument :
ECD_L
ClientSampled :
PL072122CLP.M Thu Jul 21 12:58:05 2022

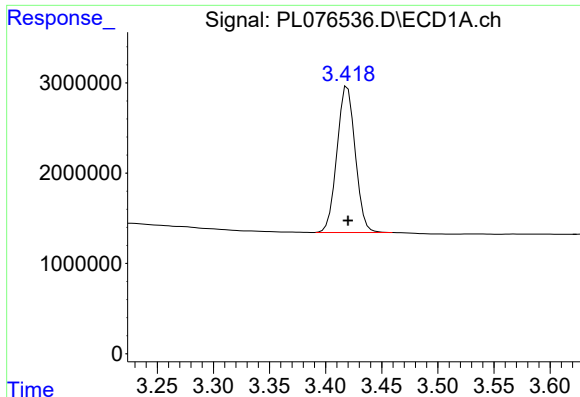

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 18324840
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

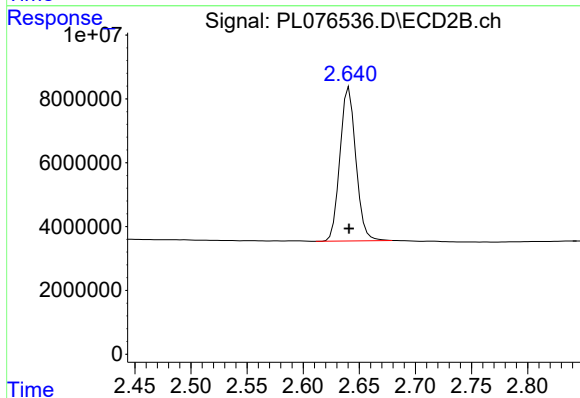


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: 0.000 min
Response: 47502385
Conc: 20.00 ng/ml

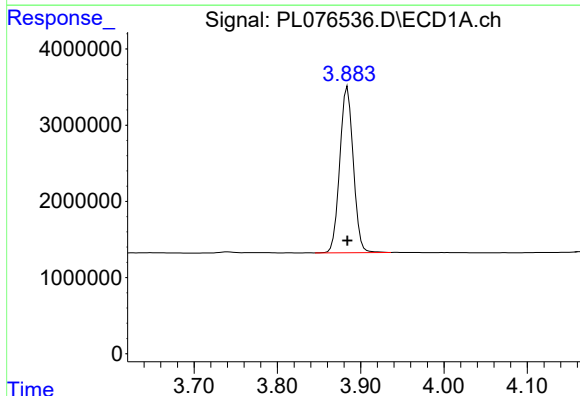


#2 alpha-BHC

R.T.: 3.884 min
Delta R.T.: 0.000 min
Response: 24489858
Conc: 20.00 ng/ml

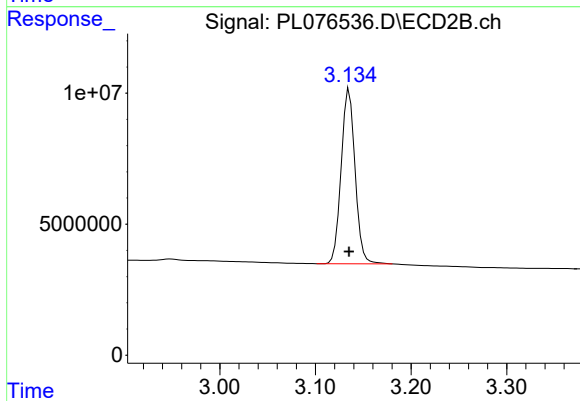

#2 alpha-BHC


R.T.: 3.135 min
Delta R.T.: 0.000 min
Response: 67520704
Conc: 20.00 ng/ml

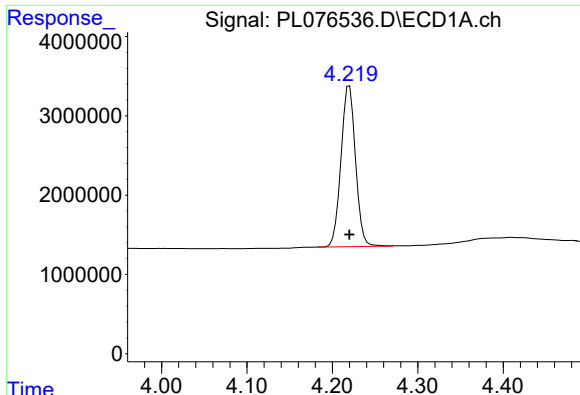

#3 gamma-BHC (Lindane)


R.T.: 4.220 min
Delta R.T.: 0.000 min
Response: 23960182
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

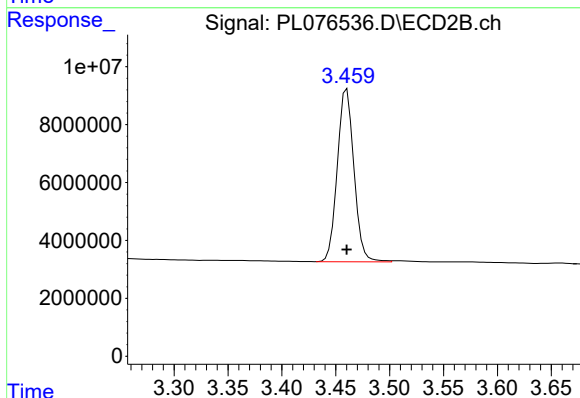


#3 gamma-BHC (Lindane)

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 64166090
Conc: 20.00 ng/ml

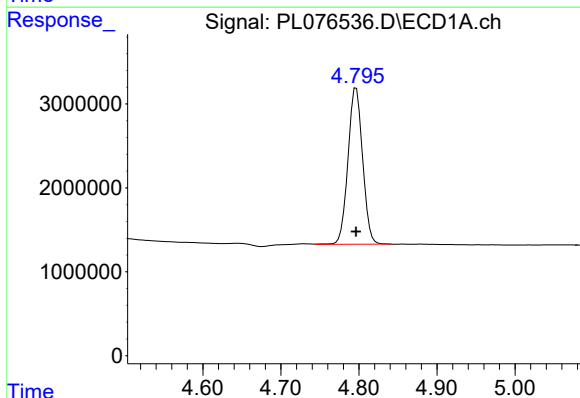


#4 Heptachlor

R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 24210756
Conc: 20.00 ng/ml

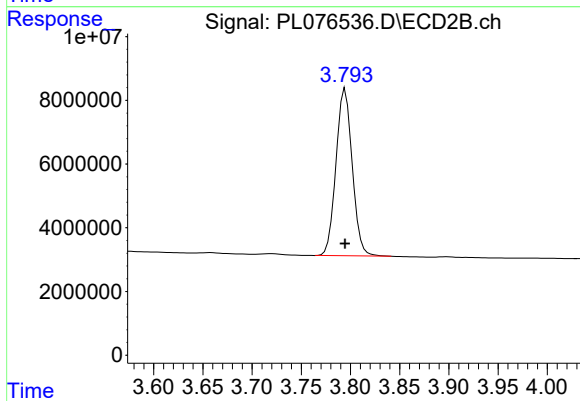

#4 Heptachlor


R.T.: 3.795 min
Delta R.T.: 0.000 min
Response: 60079148
Conc: 20.00 ng/ml

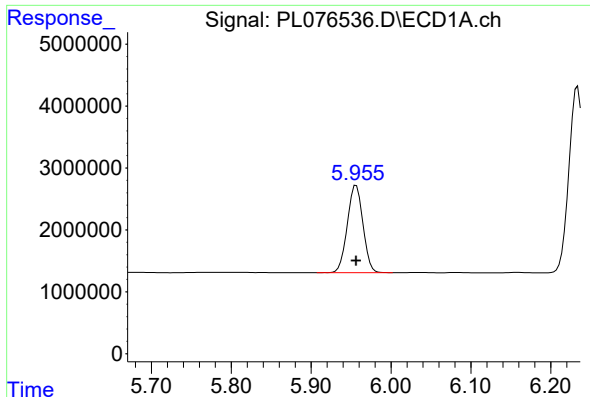

#9 Endosulfan I


R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 19239981
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

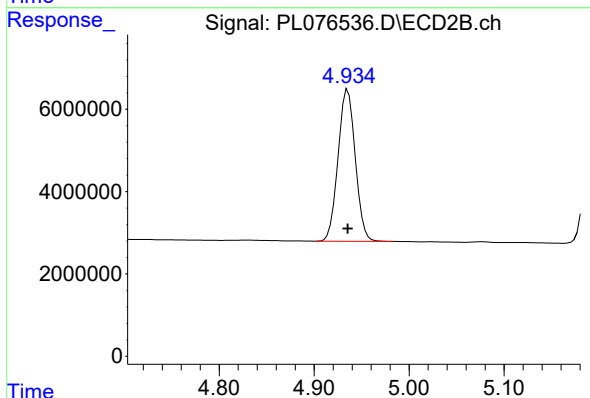


#9 Endosulfan I

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 46464075
Conc: 20.00 ng/ml

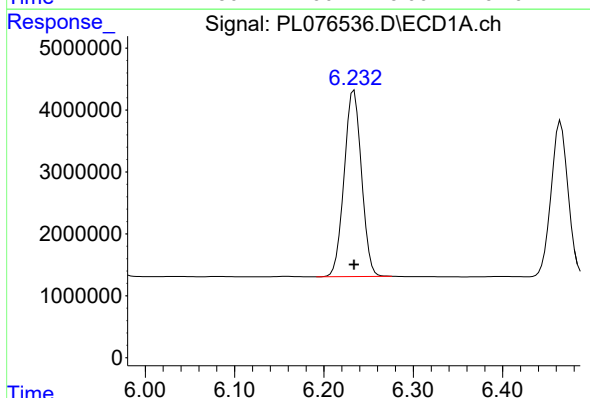


#13 Dieldrin

R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 40521967
Conc: 40.00 ng/ml

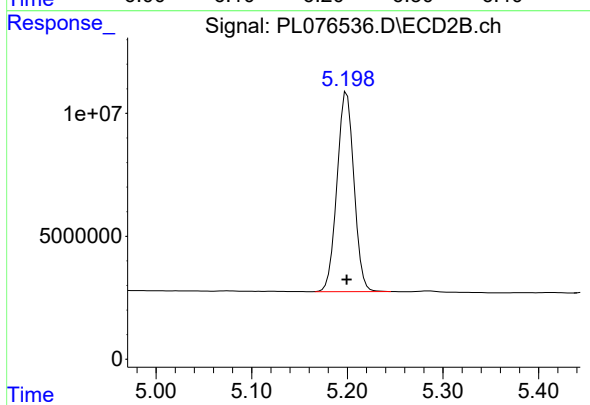

#13 Dieldrin


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 99990465
Conc: 40.00 ng/ml

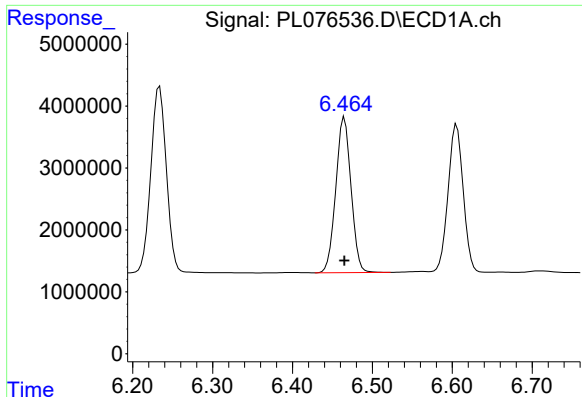

#14 Endrin


R.T.: 6.465 min
Delta R.T.: 0.000 min
Response: 33274888
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

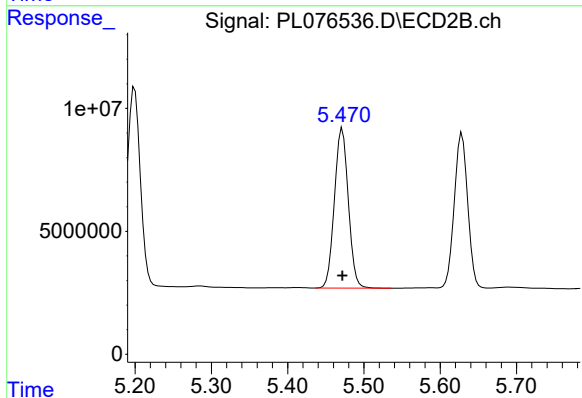


#14 Endrin

R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 81961401
Conc: 40.00 ng/ml

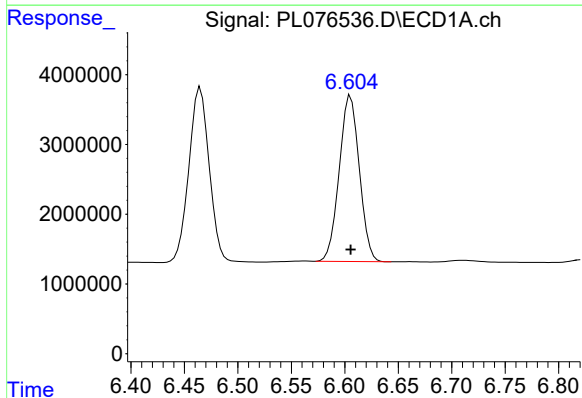


#16 4,4'-DDD

R.T.: 6.606 min
Delta R.T.: 0.000 min
Response: 31181202
Conc: 40.00 ng/ml

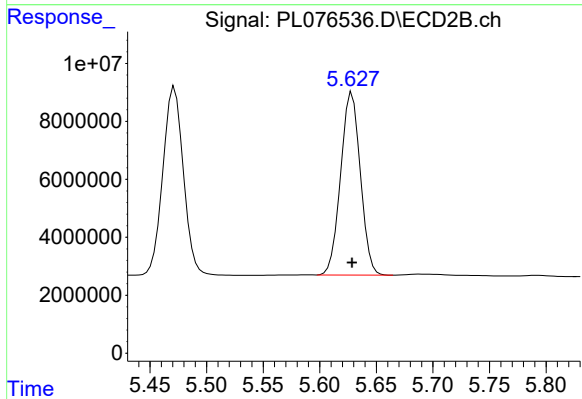

#16 4,4'-DDD


R.T.: 5.629 min
Delta R.T.: 0.000 min
Response: 76411737
Conc: 40.00 ng/ml

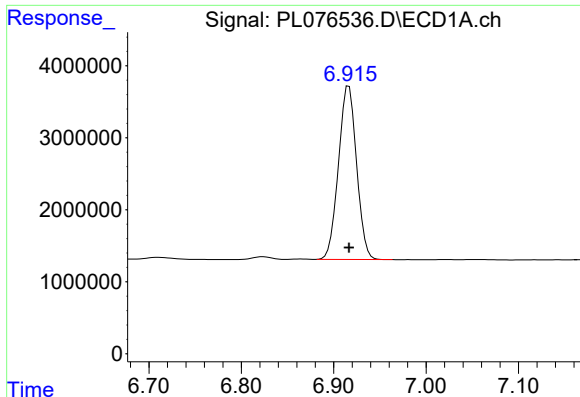

#17 4,4'-DDT


R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 32857874
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

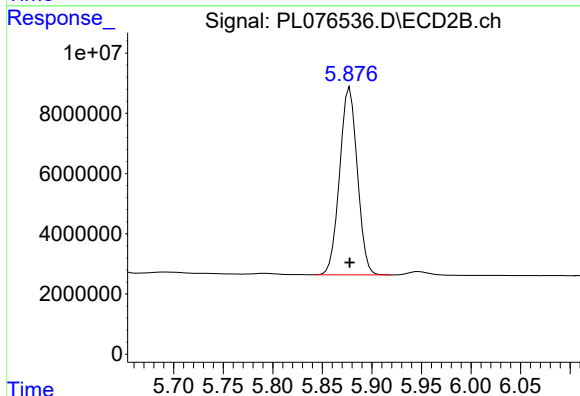


#17 4,4'-DDT

R.T.: 5.878 min
Delta R.T.: 0.000 min
Response: 77293685
Conc: 40.00 ng/ml

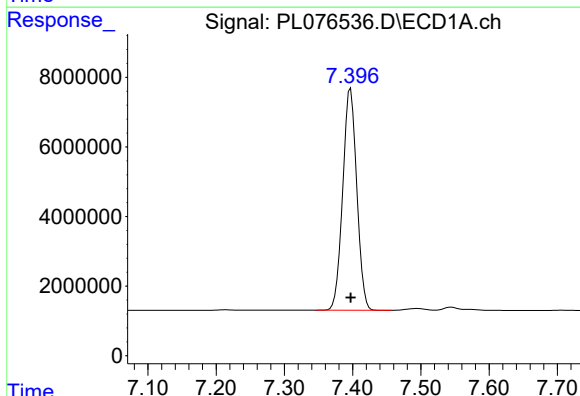


#20 Methoxychlor

R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 91114517
Conc: 200.00 ng/ml

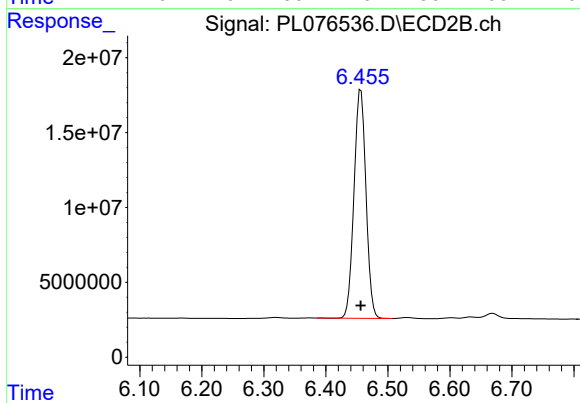

#20 Methoxychlor


R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 204911973
Conc: 200.00 ng/ml

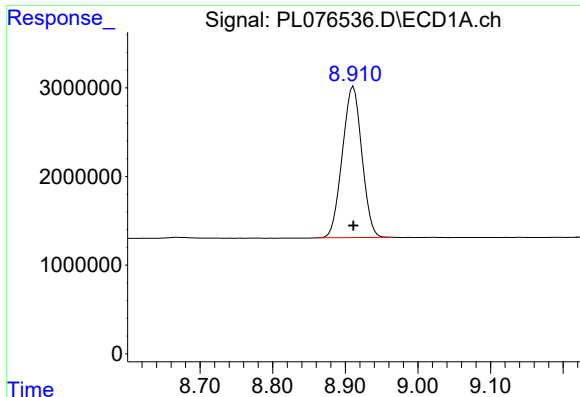

#27 Decachlorobiphenyl

R.T.: 8.911 min
Delta R.T.: 0.000 min
Response: 31879106
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

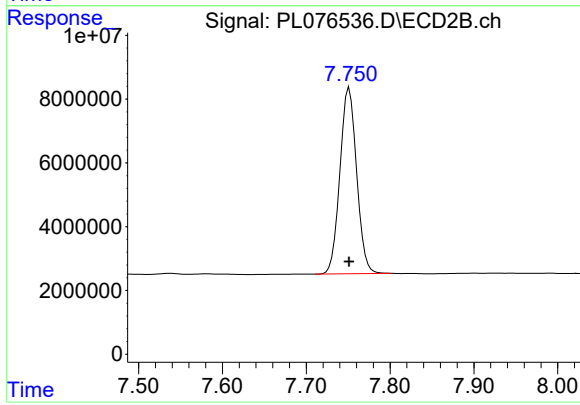

#27 Decachlorobiphenyl

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 80925563
Conc: 40.00 ng/ml