

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
 Data File : PL076525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2022 10:11
 Operator : AR\AJ
 Sample : RESC351
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESC206

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 14:15:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 21 14:14:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.424	2.646	17577858	42437349	19.399	18.099
2)	SA Decachlor...	8.920	7.758	30533509	71478796	38.994	35.596
Target Compounds							
2)	A alpha-BHC	3.888	3.140	11363655	29308589	9.257	8.767
3)	MA gamma-BHC...	4.224	3.465	10941584	27520048	9.110	8.738
4)	MA Heptachlor	4.801	3.800	11739569	26472097	9.672	8.887
5)	MB Aldrin	5.142	4.076	10692618	25036553	9.567	8.697
6)	B beta-BHC	4.436	3.763	5617506	12746855	9.448	8.869
7)	B delta-BHC	4.679	3.988	9530544	25972299	8.558	8.190
8)	B Heptachlo...	5.575	4.575	10381351	22791864	9.690	8.728
9)	A Endosulfan I	5.961	4.942	9241511	20632478	9.727	8.911
10)	B trans-Chl...	5.831	4.825	10176813	23089745	9.575	8.750
11)	B cis-Chlor...	5.908	4.888	10122684	22568885	9.623	8.750
12)	B 4,4'-DDE	6.087	5.082	17567398	41820079	18.316	17.244
13)	MA Dieldrin	6.239	5.205	18919291	42993390	18.832	17.313
14)	MA Endrin	6.471	5.478	15620366	35210140	19.152	17.511
15)	B Endosulfa...	6.698	5.774	16840429	35331032	19.206	17.197
16)	A 4,4'-DDD	6.612	5.635	14586536	32829025	18.937	17.283
17)	MA 4,4'-DDT	6.922	5.884	15389097	31959957	18.893	17.093
18)	B Endrin al...	6.830	5.953	14938073	31332753	19.361	17.702
19)	B Endosulfa...	7.063	6.176	16836866	35331858	18.952	16.943
20)	A Methoxychlor	7.404	6.463	44026676	89486940	98.323	89.093
21)	B Endrin ke...	7.551	6.677	19054515	41164616	19.507	18.083

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
Data File : PL076525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 10:11
Operator : AR\AJ
Sample : RESC351
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 14:15:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 21 14:14:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

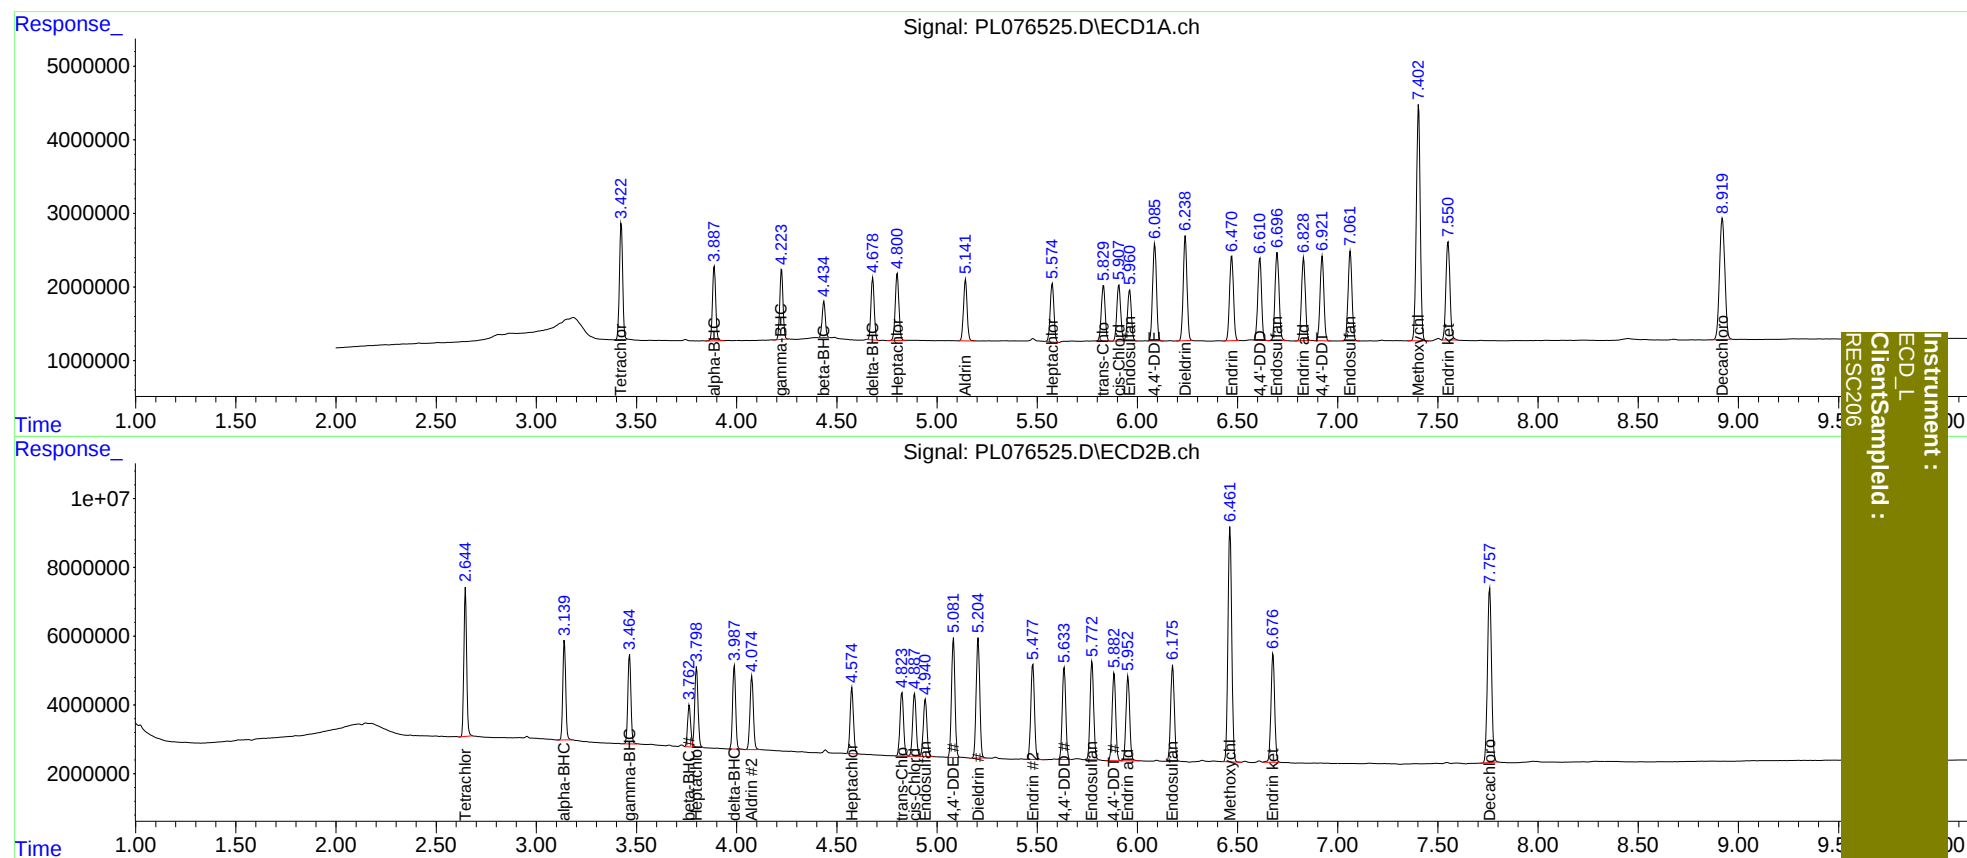

Instrument :
ECD_L
ClientSampled :
RESC206

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
Data File : PL076525.D
Acq On : 21 Jul 2022 10:11
Operator : AR\AJ
Sample : RESC351
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC206

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
Title : GC Extractables
Last Update : Thu Jul 21 14:14:01 2022
Integrator: ChemStation

RT#1	RT#2	Resolution
3.424	3.888	100.00%
3.888	4.224	100.00%
4.224	4.436	100.00%
4.436	4.679	100.00%
4.679	4.801	100.00%
4.801	5.142	100.00%
5.142	5.575	100.00%
5.575	5.831	100.00%
5.831	5.908	99.75%
5.908	5.961	97.92%
5.961	6.087	100.00%
6.087	6.239	100.00%
6.239	6.471	100.00%
6.471	6.612	100.00%
6.612	6.698	100.00%
6.698	6.830	100.00%
6.830	6.922	100.00%
6.922	7.063	100.00%
7.063	7.404	100.00%
7.404	7.551	100.00%
7.551	8.920	100.00%

Signal #2


2.646	3.140	100.00%
3.140	3.465	100.00%
3.465	3.763	100.00%
3.763	3.800	89.24%
3.800	3.988	100.00%
3.988	4.076	100.00%
4.076	4.575	100.00%
4.575	4.825	100.00%
4.825	4.888	99.12%
4.888	4.942	98.76%
4.942	5.082	100.00%
5.082	5.205	100.00%
5.205	5.478	100.00%
5.478	5.635	100.00%
5.635	5.774	100.00%
5.774	5.884	100.00%
5.884	5.953	100.00%
5.953	6.176	100.00%
6.176	6.463	100.00%
6.463	6.677	100.00%
6.677	7.758	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
Data File : PL076525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 10:11
Operator : AR\AJ
Sample : RESC351
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC206

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 14:15:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 21 14:14:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

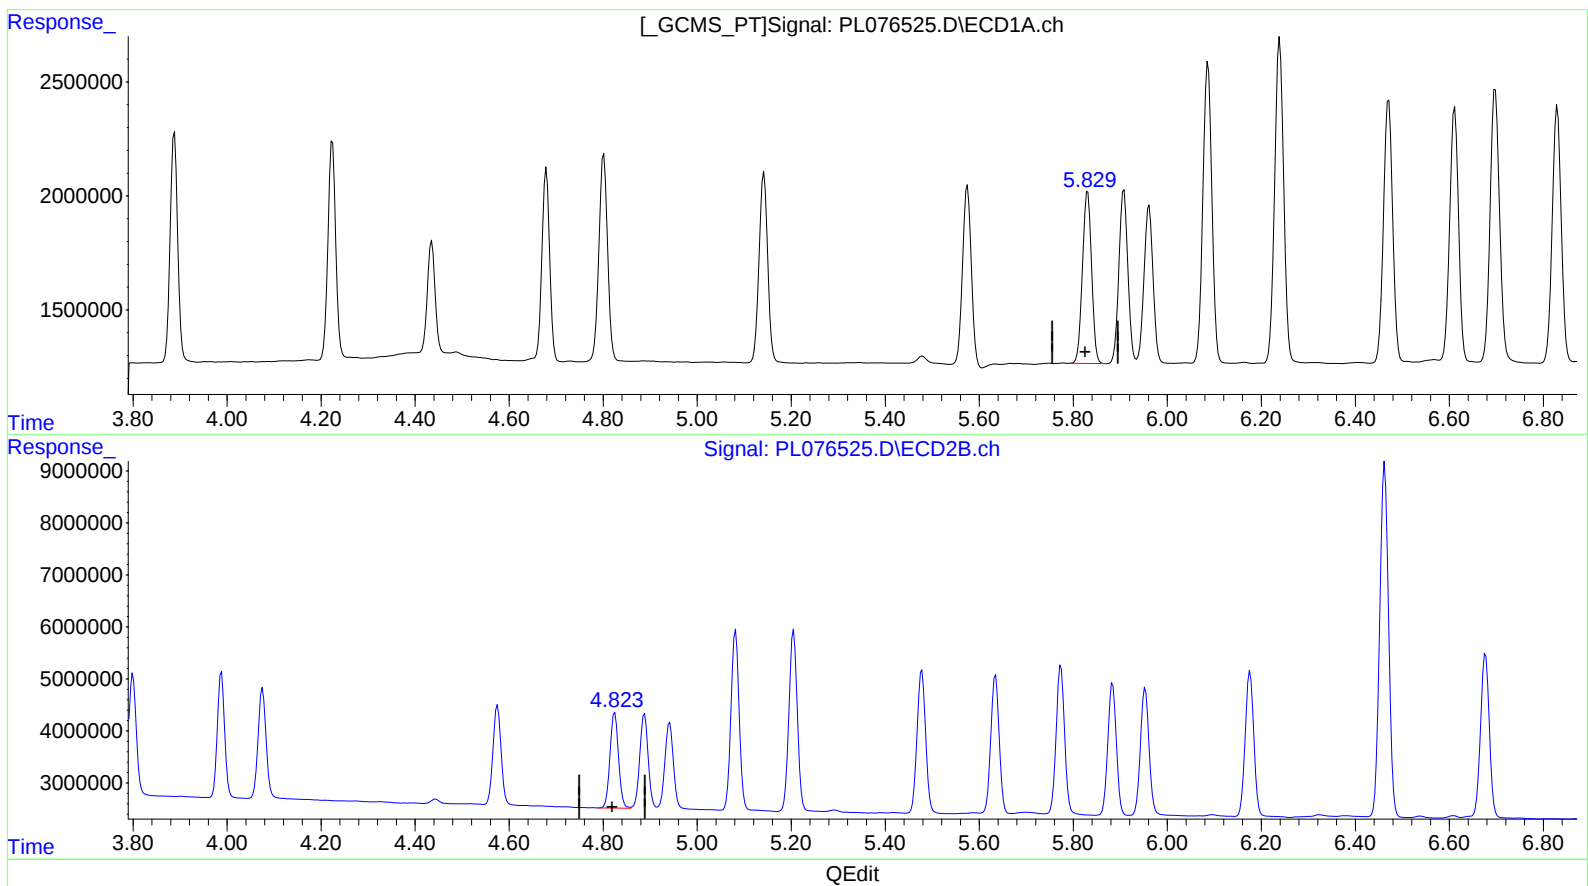

(10) trans-Chlordane (B)

5.831min 9.575 ng/ml

response 10176813

(10) trans-Chlordane #2 (B)

4.825min 8.750 ng/ml


response 23089745

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
Data File : PL076525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 10:11
Operator : AR\AJ
Sample : RESC351
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC206

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 14:15:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 21 14:14:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

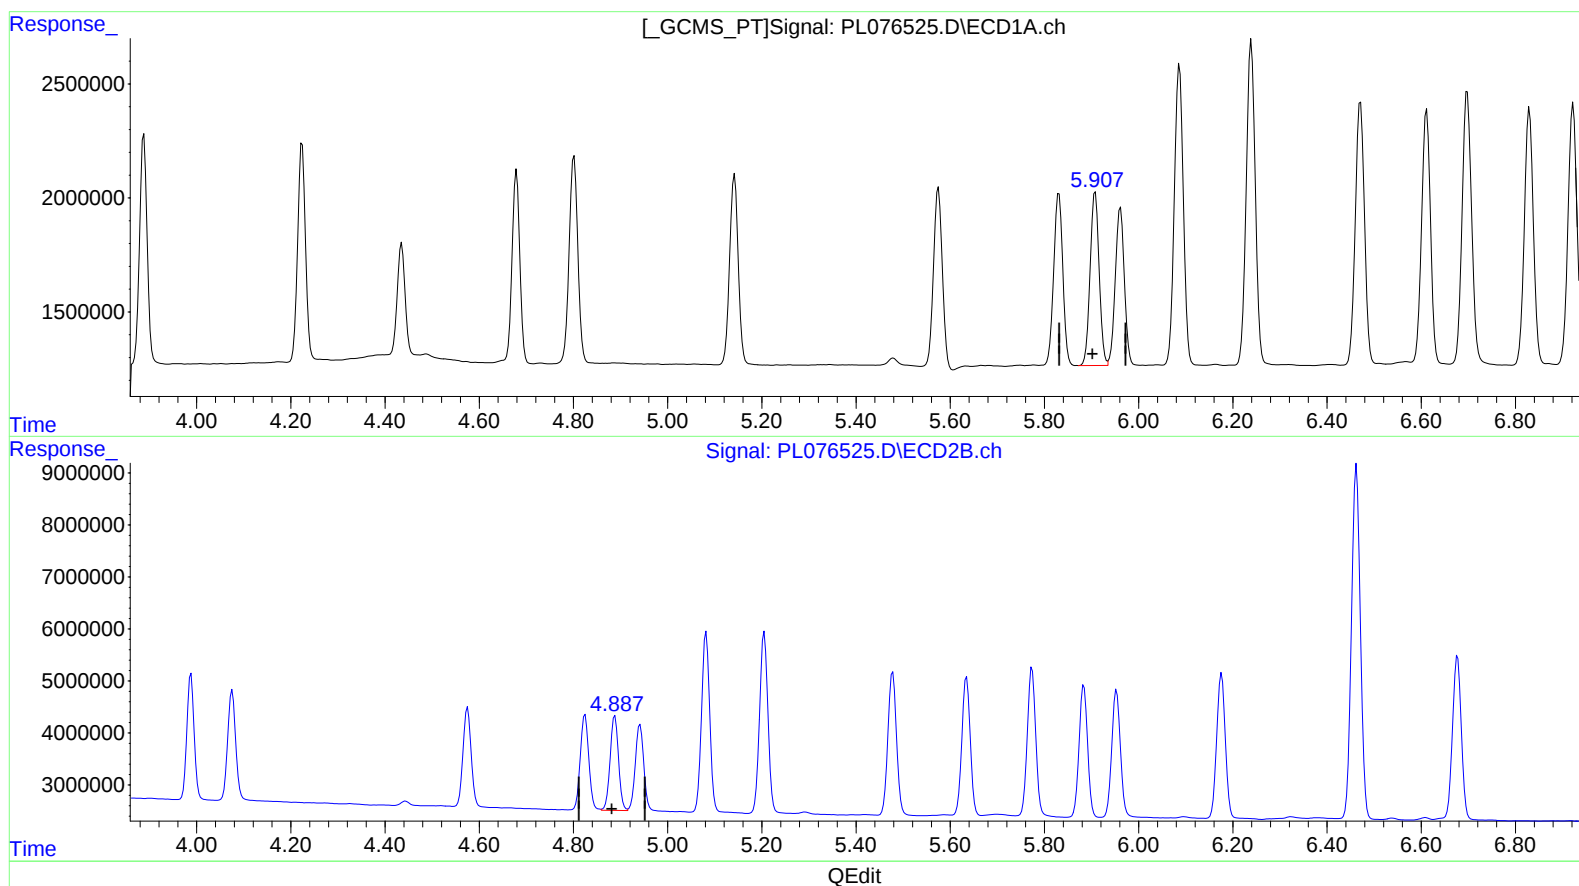

(11) cis-Chlordane (B)

5.908min 9.623 ng/ml

response 10122684

(11) cis-Chlordane #2 (B)

4.888min 8.750 ng/ml


response 22568885

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072122\
Data File : PL076525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 10:11
Operator : AR\AJ
Sample : RESC351
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC206

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 14:15:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 21 14:14:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

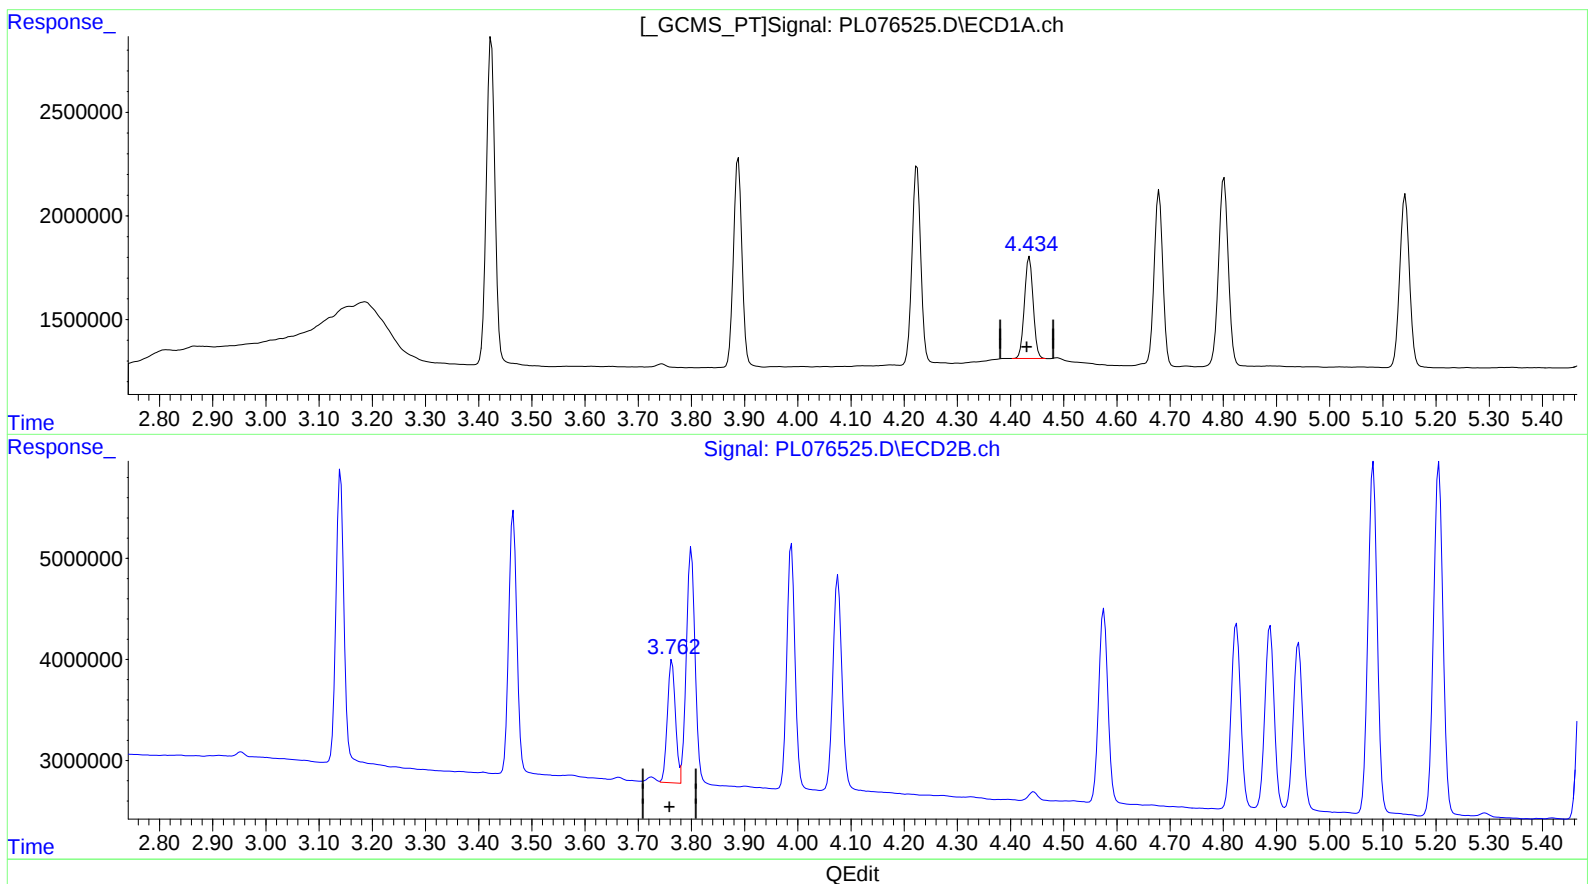

(6) beta-BHC (B)
4.436min 9.448 ng/ml
response 5617506

(6) beta-BHC #2 (B)
3.763min 8.869 ng/ml
response 12746855