

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072125\
 Data File : PL096496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 17:20
 Operator : AR\AJ
 Sample : Q2638-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:48:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.829	40150448	65473561	11.003	11.345
28)	SA Decachlor...	9.020	7.994	20546560	33778485	7.304	6.774
Target Compounds							
10)	B gamma-Chl...	5.919	0.000	6417009	0	1.450	N.D. #
11)	B alpha-Chl...	6.001	5.116	9931050	9497197	2.268	1.263 #
12)	B 4,4'-DDE	6.168	5.305	5126975	7772994	1.383	1.203
23)	Chlordane-1	0.000	3.839	0	6272732	N.D.	26.539 #
25)	Chlordane-3	5.919	0.000	6417009	0	8.710	N.D. #
26)	Chlordane-4	6.001	5.116	9931050	9497197	11.069	12.639



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072125\
Data File : PL096496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2025 17:20
Operator : AR\AJ
Sample : Q2638-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:48:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

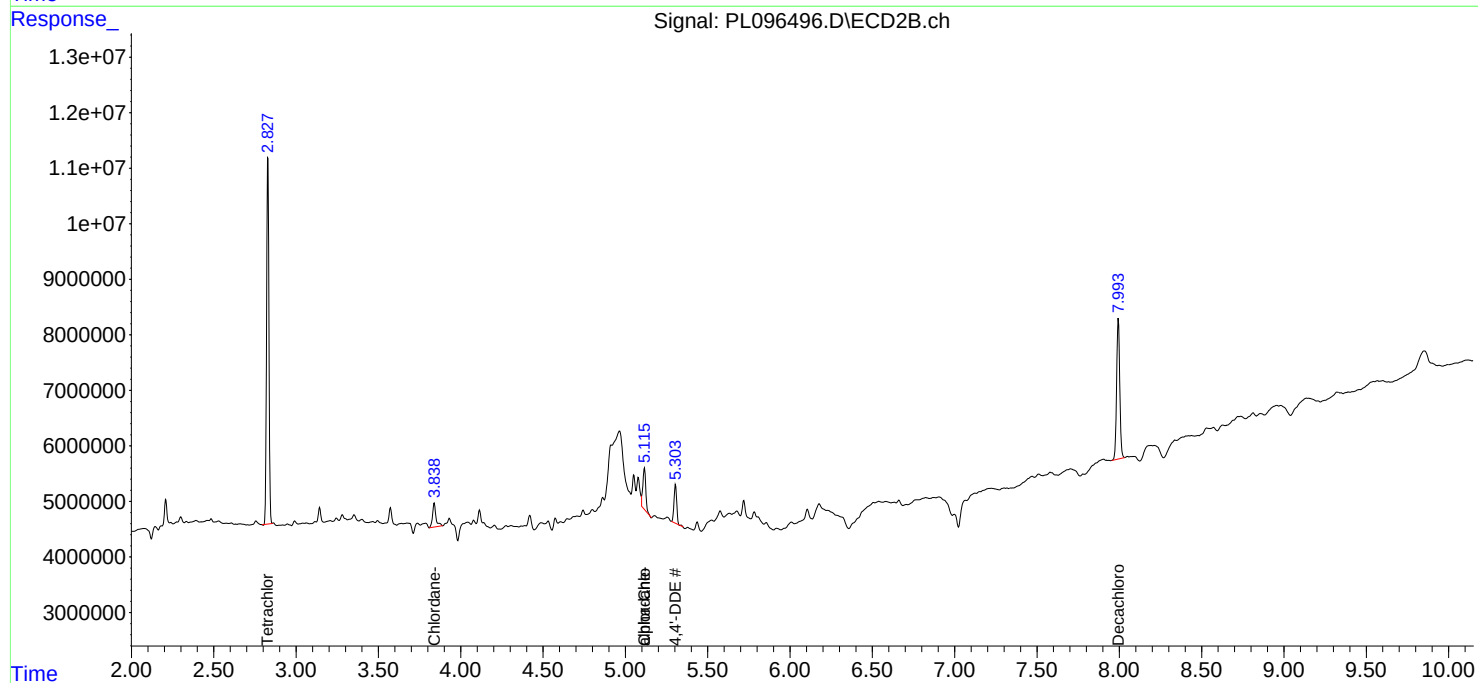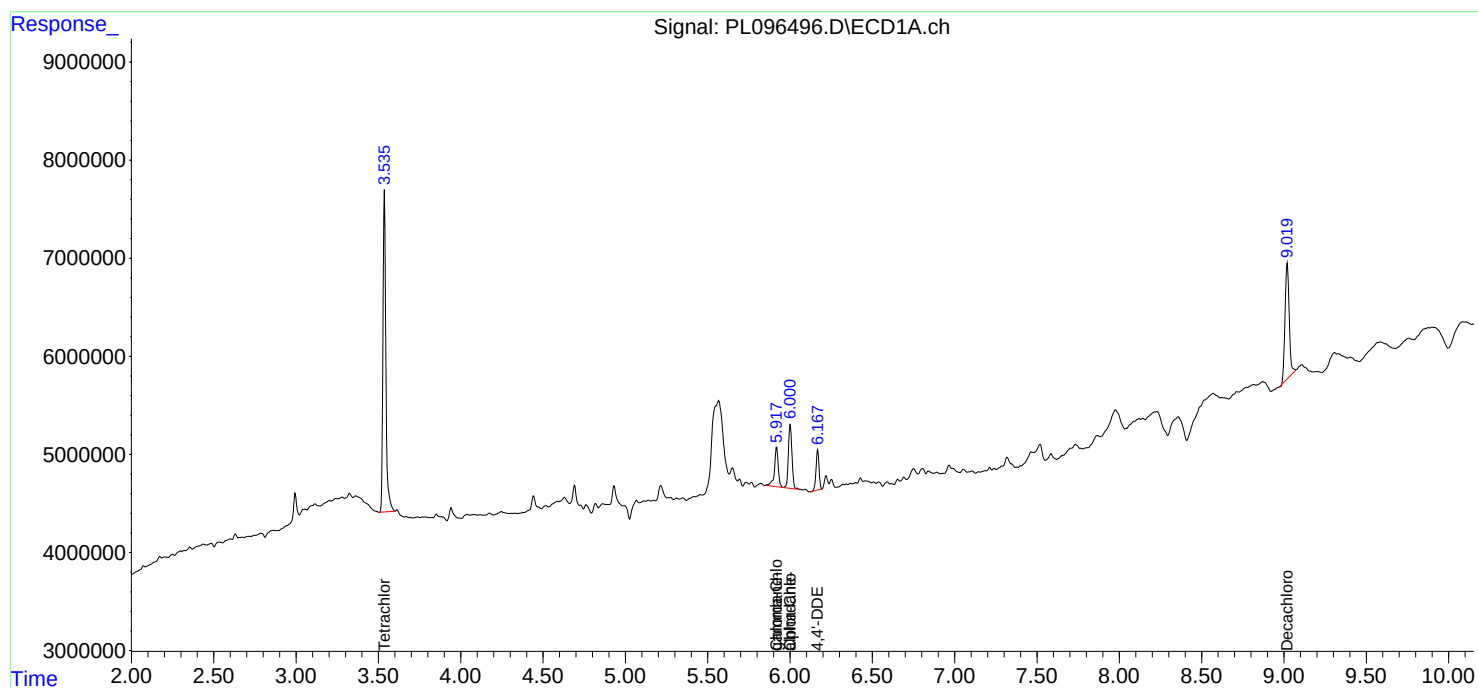


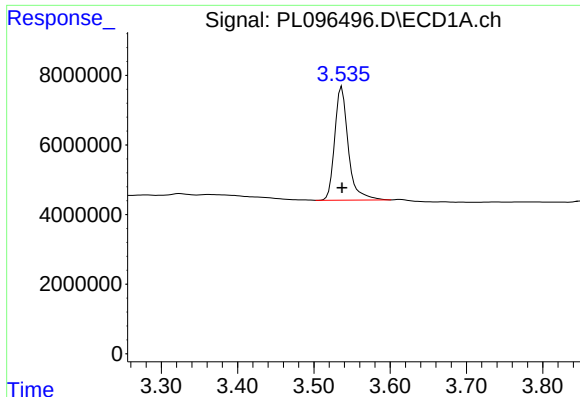

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 40150448
Conc: 11.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

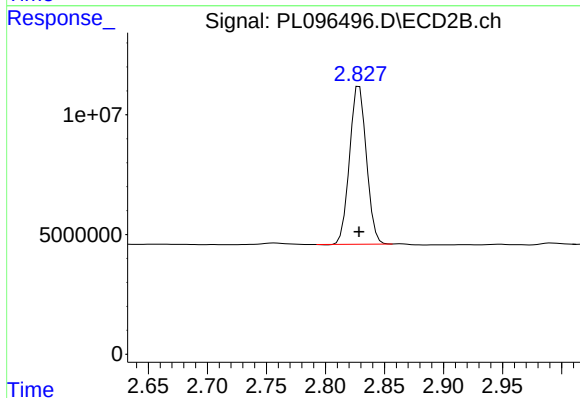


#1 Tetrachloro-m-xylene

R.T.: 2.829 min
Delta R.T.: 0.000 min
Response: 65473561
Conc: 11.34 ng/ml

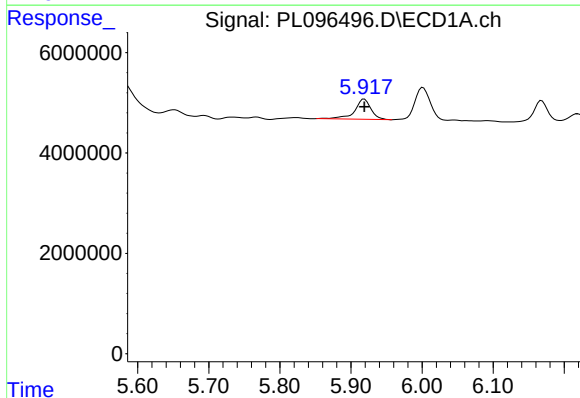


#10 gamma-Chlordane

R.T.: 5.919 min
Delta R.T.: 0.000 min
Response: 6417009
Conc: 1.45 ng/ml

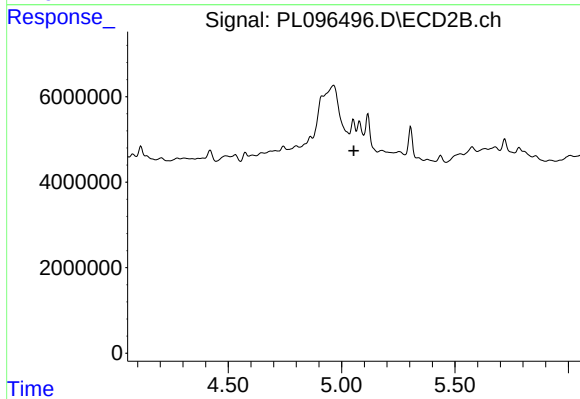

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.054 min
Response: 0
Conc: N.D.

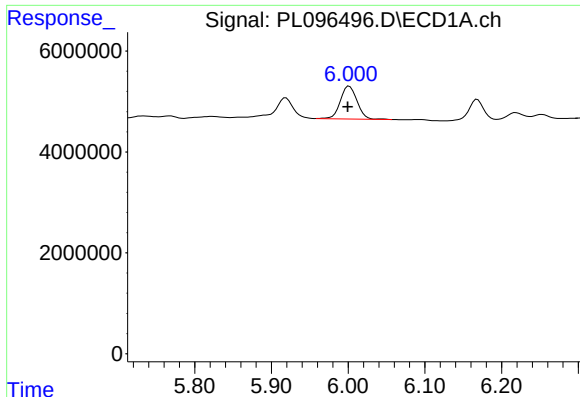

#11 alpha-Chlordane


R.T.: 6.001 min
Delta R.T.: 0.002 min
Response: 9931050
Conc: 2.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

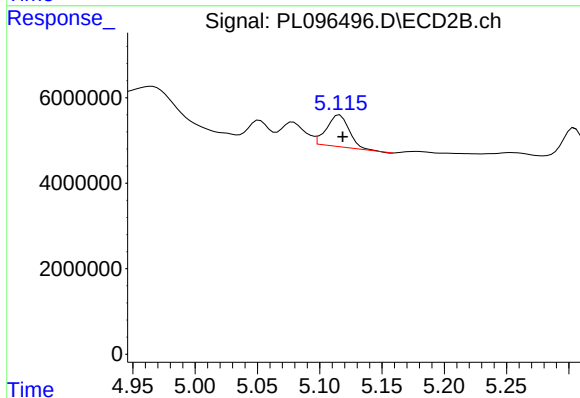


#11 alpha-Chlordane

R.T.: 5.116 min
Delta R.T.: -0.003 min
Response: 9497197
Conc: 1.26 ng/ml

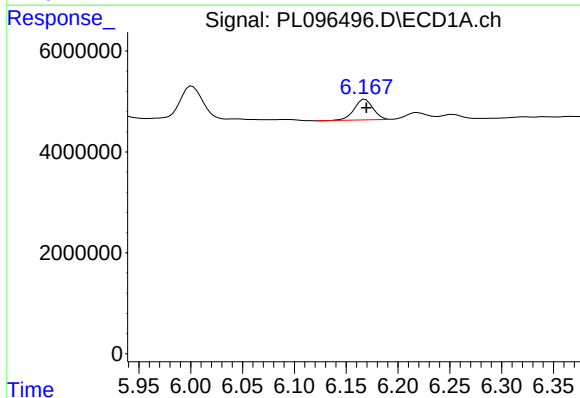


#12 4,4'-DDE

R.T.: 6.168 min
Delta R.T.: -0.001 min
Response: 5126975
Conc: 1.38 ng/ml

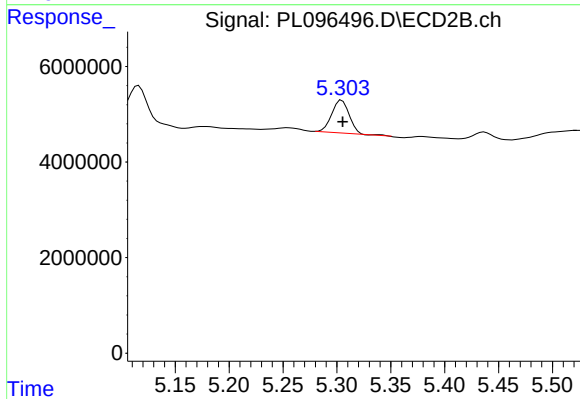

#12 4,4'-DDE


R.T.: 5.305 min
Delta R.T.: 0.000 min
Response: 7772994
Conc: 1.20 ng/ml

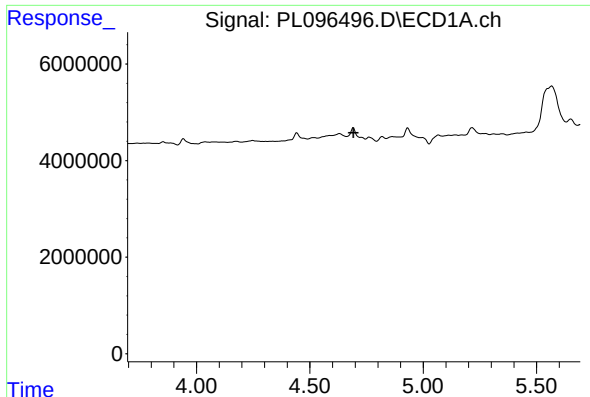

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

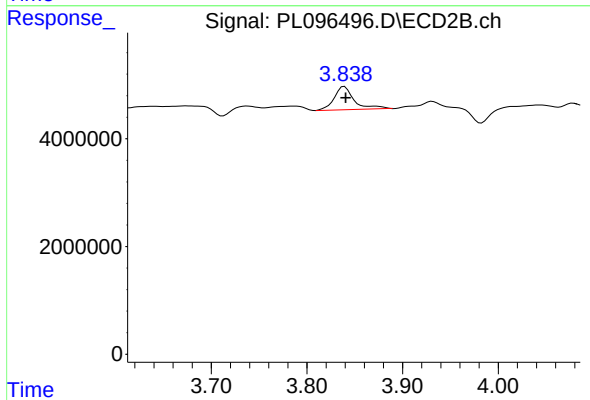


#23 Chlordane-1

R.T.: 3.839 min
Delta R.T.: -0.001 min
Response: 6272732
Conc: 26.54 ng/ml

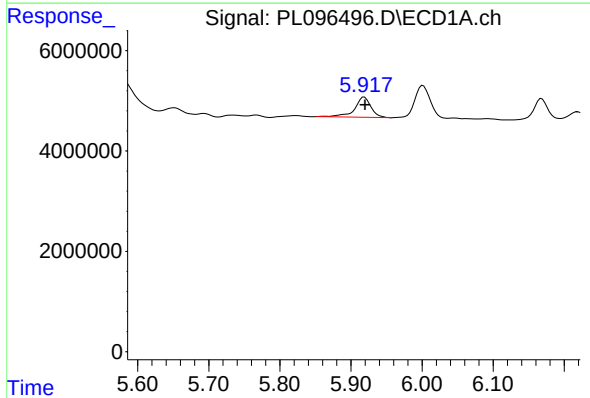


#25 Chlordane-3

R.T.: 5.919 min
Delta R.T.: -0.001 min
Response: 6417009
Conc: 8.71 ng/ml

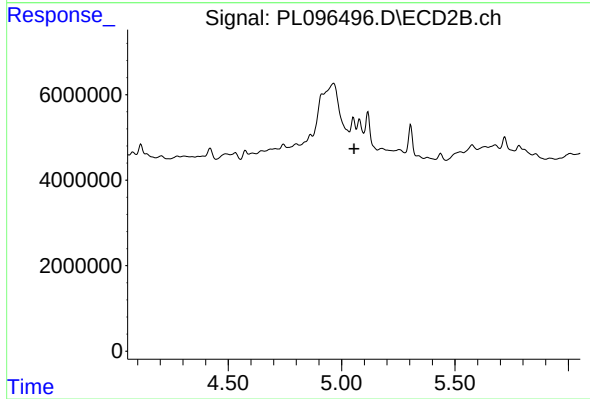

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.055 min
Response: 0
Conc: N.D.

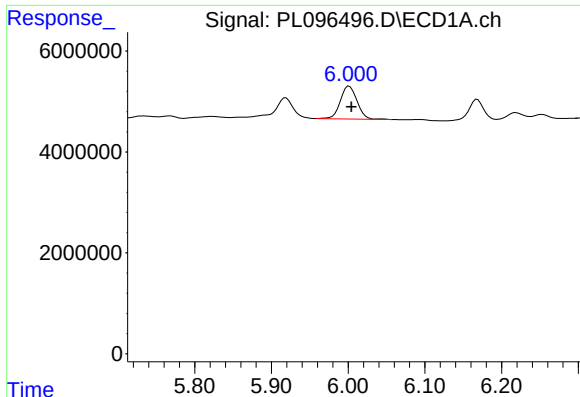

#26 Chlordane-4


R.T.: 6.001 min
Delta R.T.: -0.003 min
Response: 9931050
Conc: 11.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

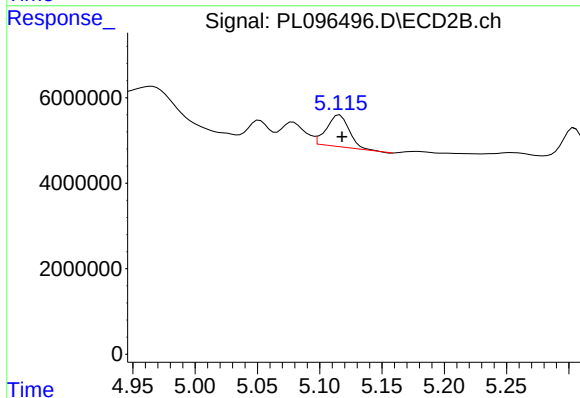


#26 Chlordane-4

R.T.: 5.116 min
Delta R.T.: -0.002 min
Response: 9497197
Conc: 12.64 ng/ml

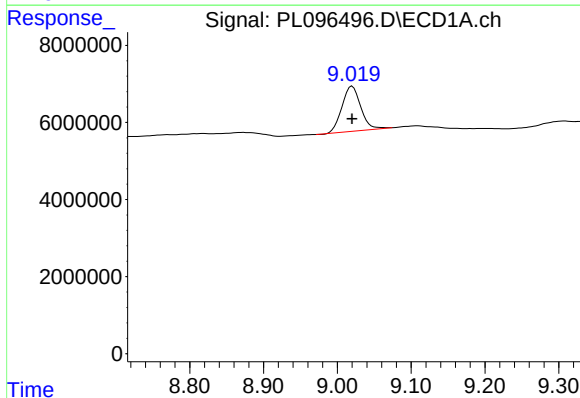

#28 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.000 min
Response: 20546560
Conc: 7.30 ng/ml

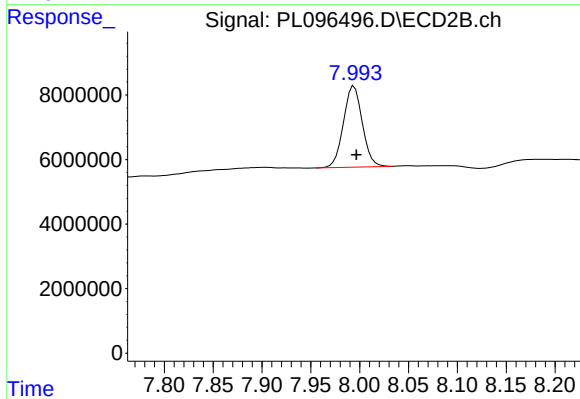

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: -0.002 min
Response: 33778485
Conc: 6.77 ng/ml