

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072219\
 Data File : PL050667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2019 08:43
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:14:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3) MA	gamma-BHC...	0.000	4.612	0	360199	N.D.	0.093 #
12) B	4,4'-DDE	5.436	0.000	4278902	0	0.286	N.D. #
16) A	4,4'-DDD	5.933	0.000	111.4E6	0	9.294	N.D. #
17) MA	4,4'-DDT	6.159	0.000	145.3E6	0	11.730	N.D. #
18) B	Endrin al...	6.234	0.000	50298384	0	4.360	N.D. #
20) A	Methoxychlor	6.724	0.000	28046602	0	4.495	N.D. #
21) B	Endrin ke...	6.936	0.000	85397951	0	6.244	N.D. #
23)	Chlordane-1	4.166	0.000	4449371	0	12.092	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072219\
Data File : PL050667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2019 08:43
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 01:14:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

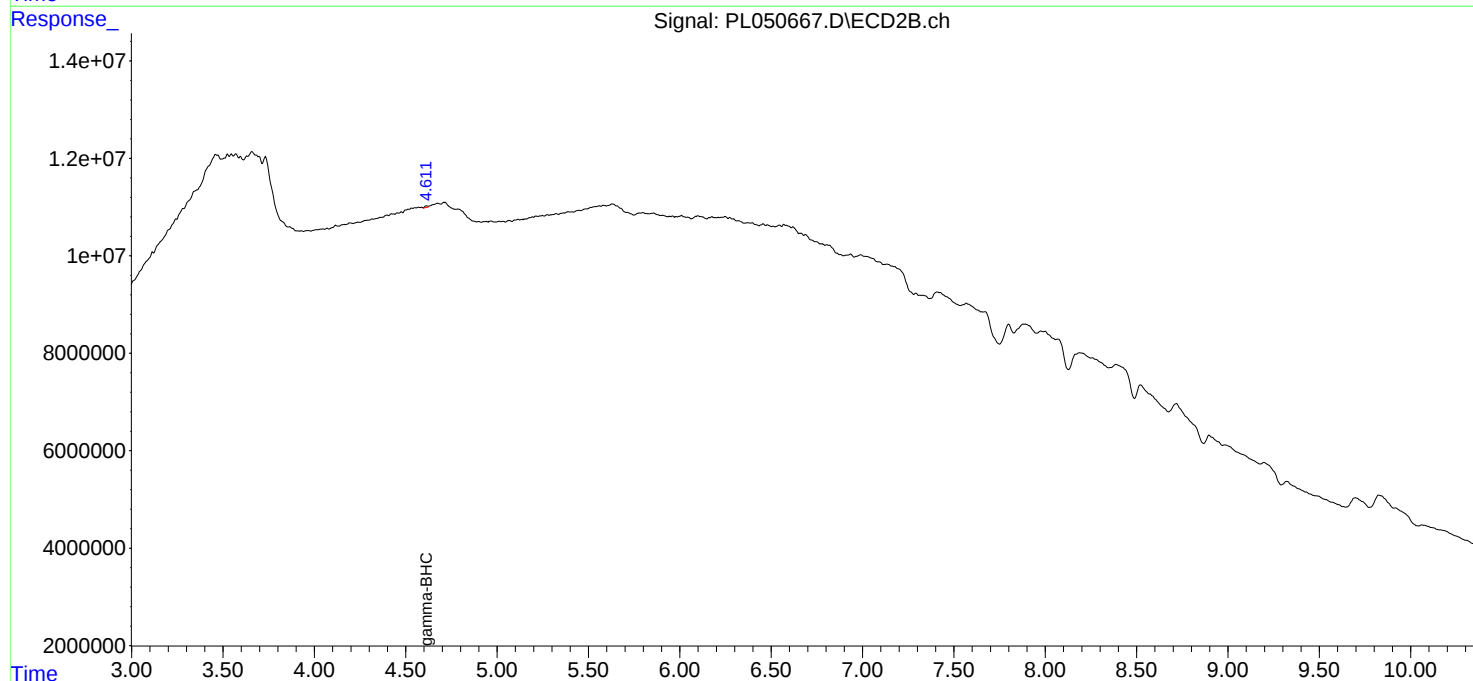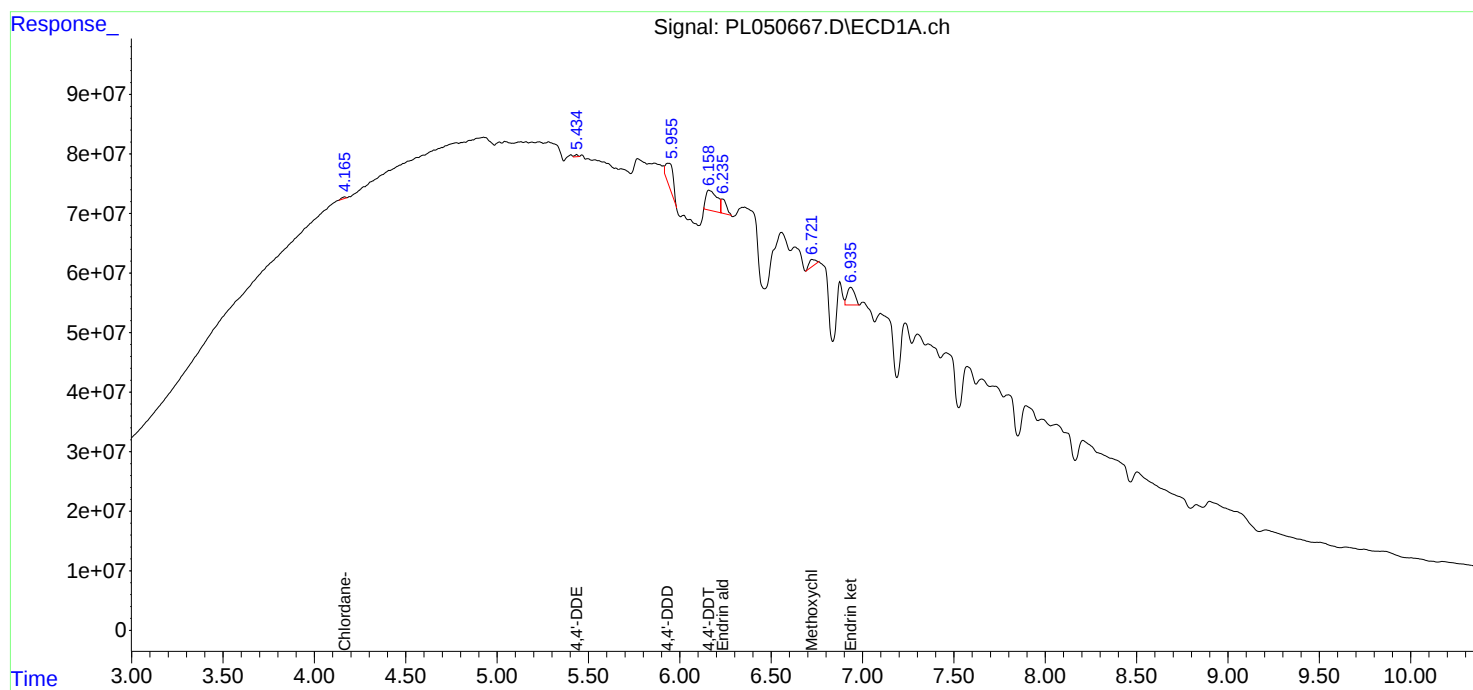


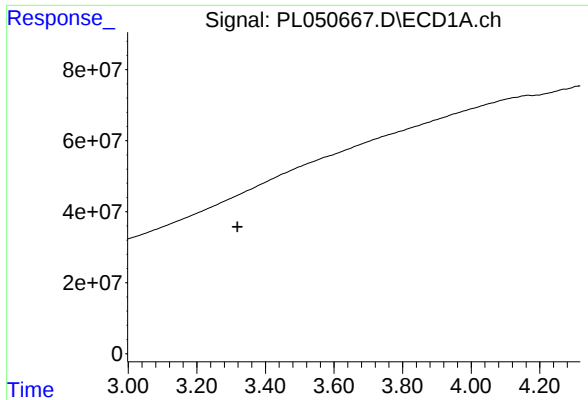

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

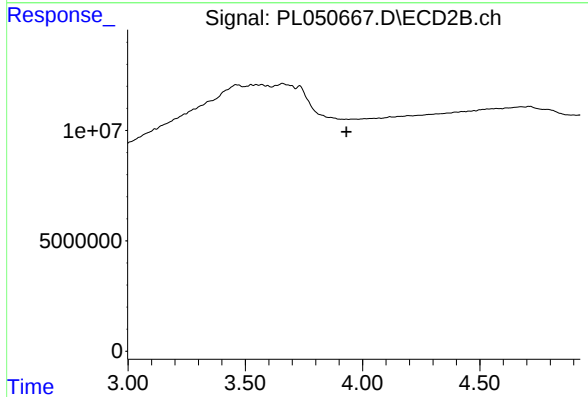


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.931 min
Response: 0
Conc: N.D.

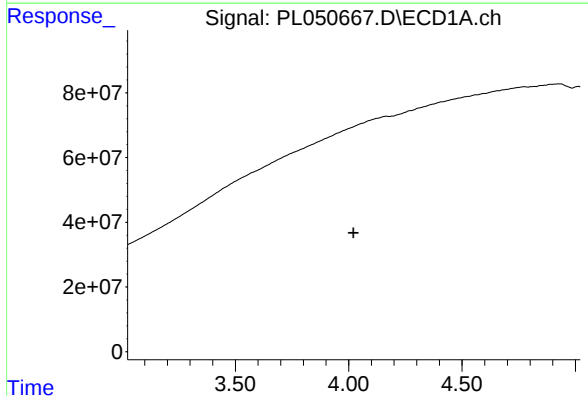


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.021 min
Response: 0
Conc: N.D.

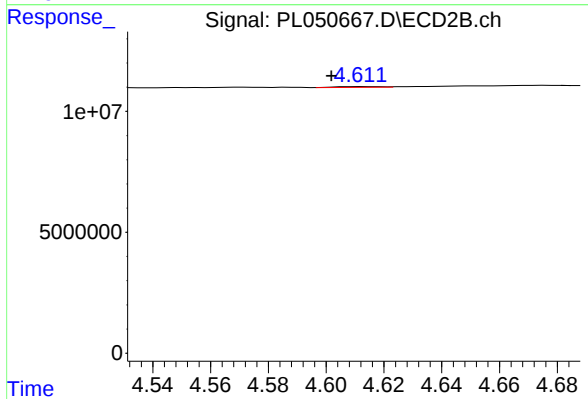

#3 gamma-BHC (Lindane)


R.T.: 4.612 min
Delta R.T.: 0.010 min
Response: 360199
Conc: 0.09 ng/ml

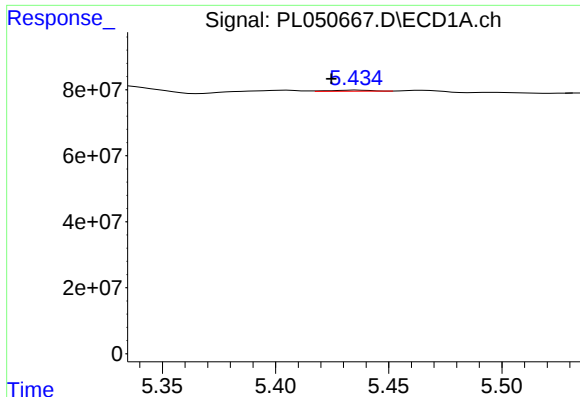

#12 4,4'-DDE


R.T.: 5.436 min
Delta R.T.: 0.011 min
Response: 4278902
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

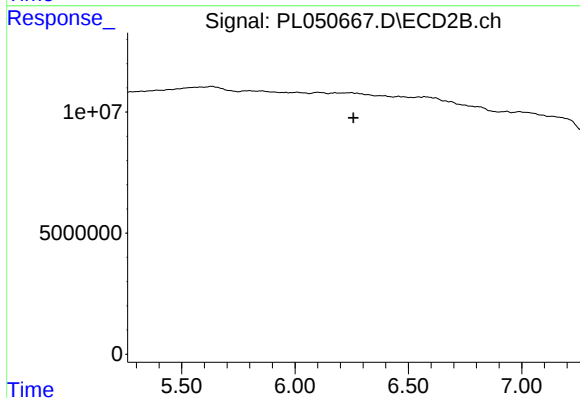


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.258 min
Response: 0
Conc: N.D.

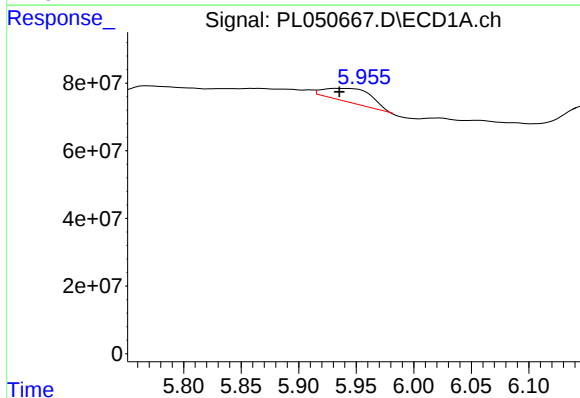


#16 4,4'-DDD

R.T.: 5.933 min
Delta R.T.: -0.002 min
Response: 111383485
Conc: 9.29 ng/ml

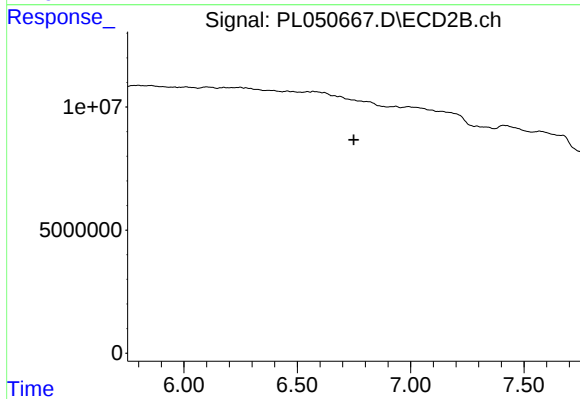

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

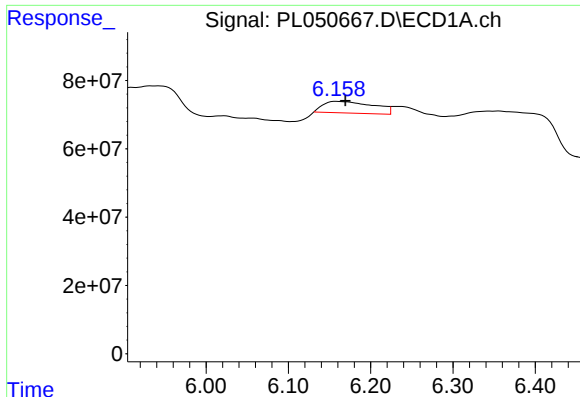

#17 4,4'-DDT


R.T.: 6.159 min
Delta R.T.: -0.011 min
Response: 145289655
Conc: 11.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

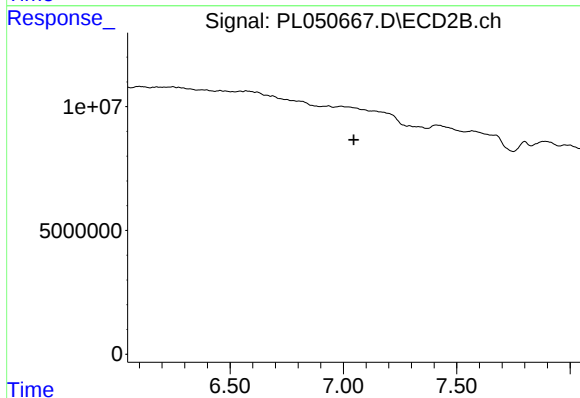


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

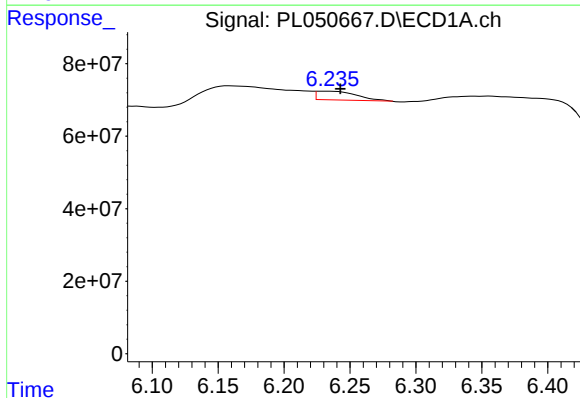


#18 Endrin aldehyde

R.T.: 6.234 min
Delta R.T.: -0.009 min
Response: 50298384
Conc: 4.36 ng/ml

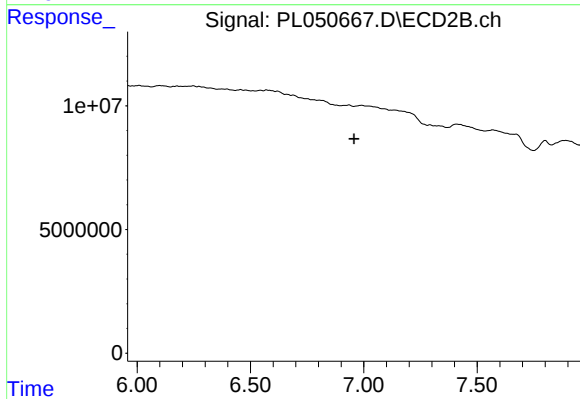

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.957 min
Response: 0
Conc: N.D.

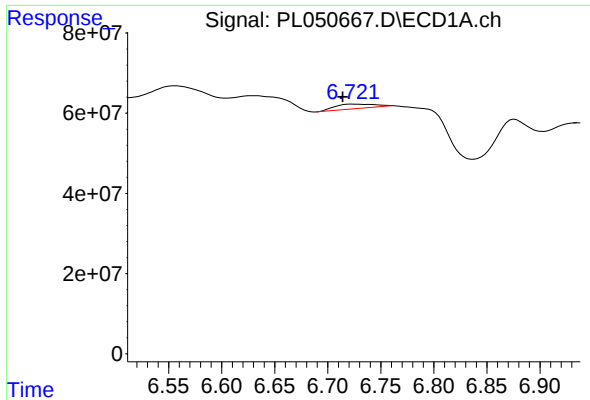

#20 Methoxychlor


R.T.: 6.724 min
Delta R.T.: 0.010 min
Response: 28046602
Conc: 4.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

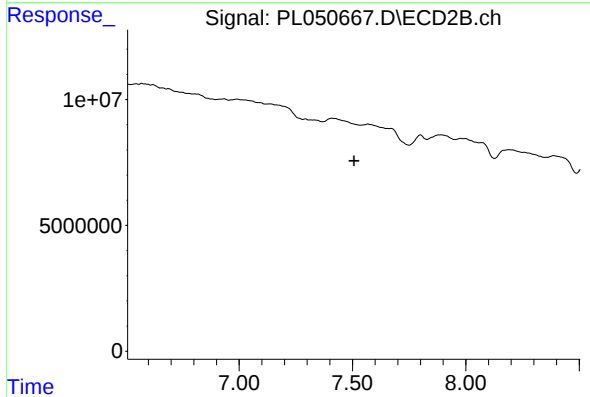


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.507 min
Response: 0
Conc: N.D.

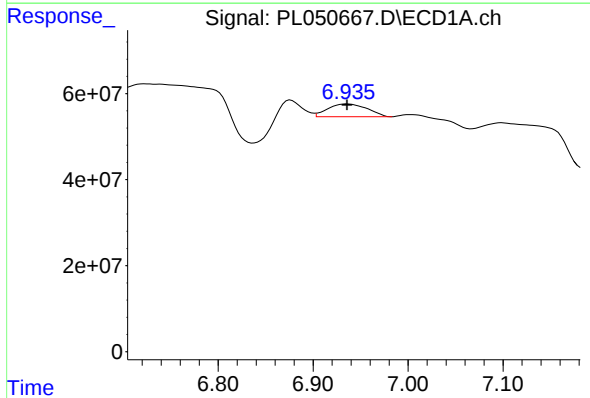


#21 Endrin ketone

R.T.: 6.936 min
Delta R.T.: 0.000 min
Response: 85397951
Conc: 6.24 ng/ml

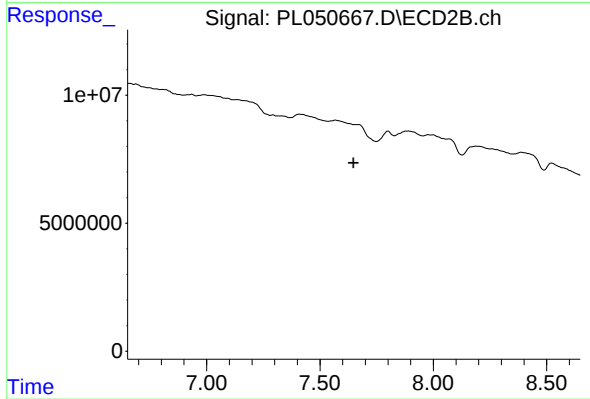

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.648 min
Response: 0
Conc: N.D.

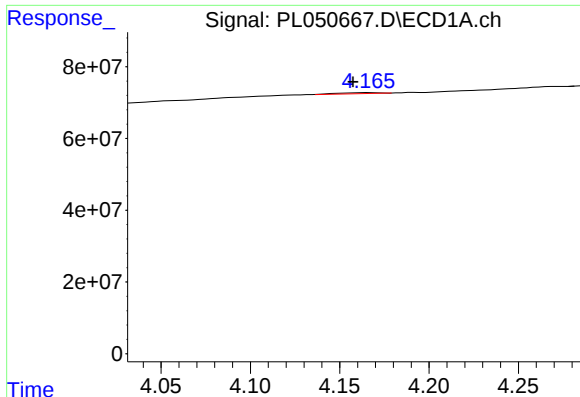

#23 Chlordane-1


R.T.: 4.166 min
Delta R.T.: 0.009 min
Response: 4449371
Conc: 12.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

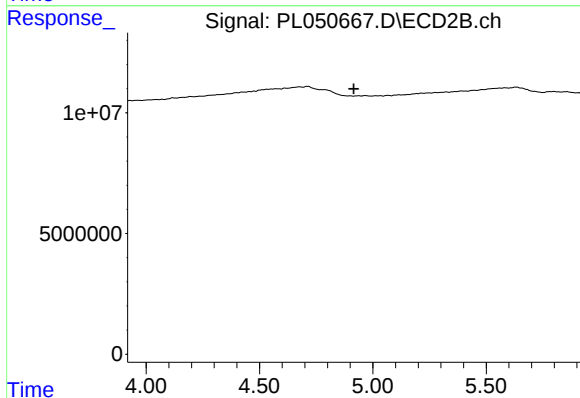


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.916 min
Response: 0
Conc: N.D.

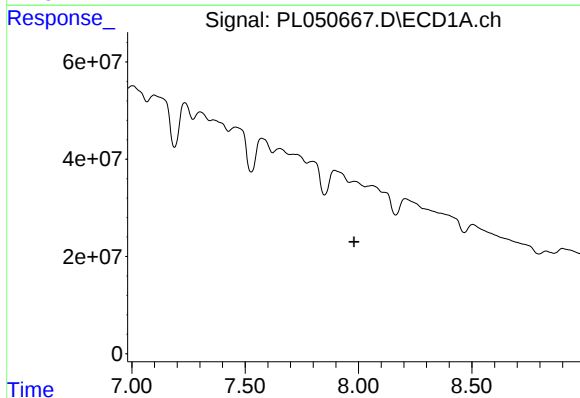

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.981 min
Response: 0
Conc: N.D.

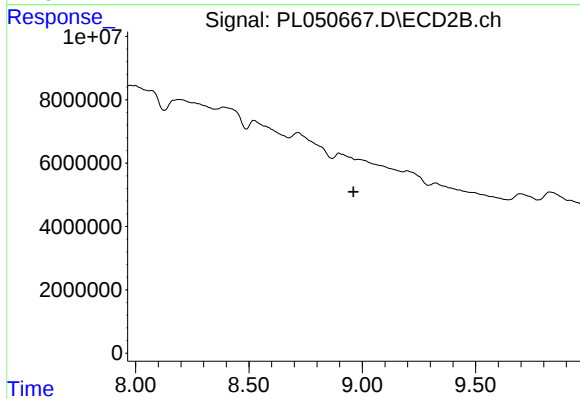

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.