

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072219\
 Data File : PL050685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2019 14:49
 Operator : SM\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:18:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.931	546.2E6	131.1E6	54.356	45.958
28)	SA Decachlor...	7.982	8.963	527.4E6	132.8E6	52.090	46.969
Target Compounds							
23)	Chlordane-1	4.159	4.916	176.6E6	51545749	479.978	475.122
24)	Chlordane-2	4.649	5.383	210.4E6	54089076	470.126	460.519
25)	Chlordane-3	5.204	6.027	656.5E6	225.3E6	468.994	468.352
26)	Chlordane-4	5.259	6.100	619.0E6	271.4E6	469.324	467.131
27)	Chlordane-5	6.081	6.902	227.2E6	43843874	447.346	459.739



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072219\
Data File : PL050685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2019 14:49
Operator : SM\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 01:18:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

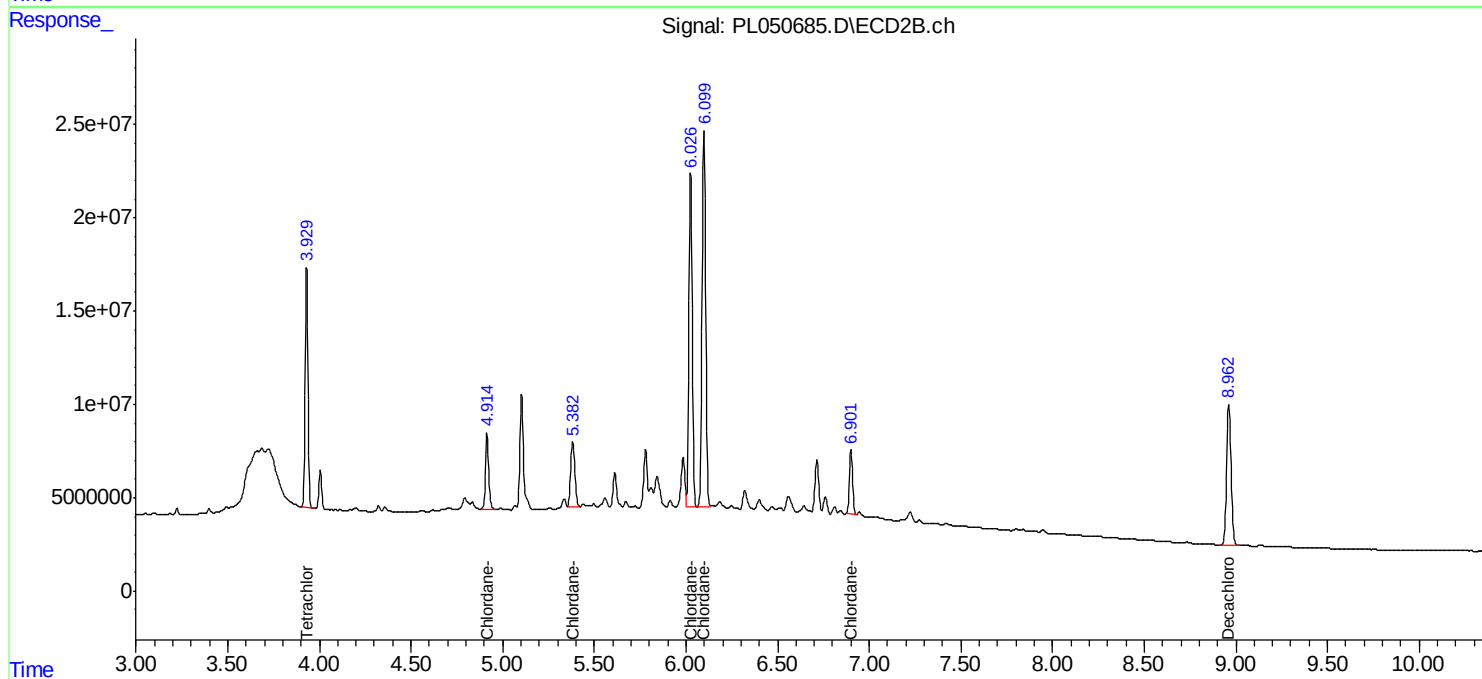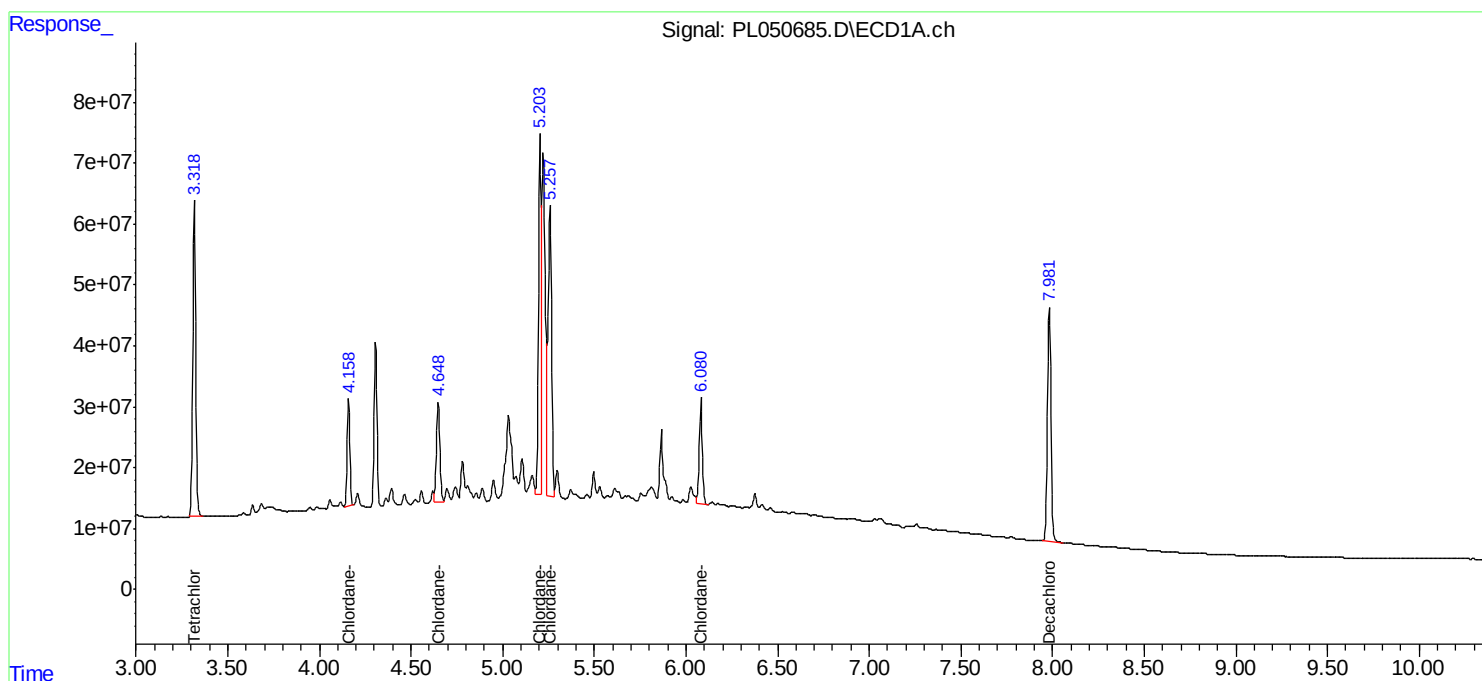


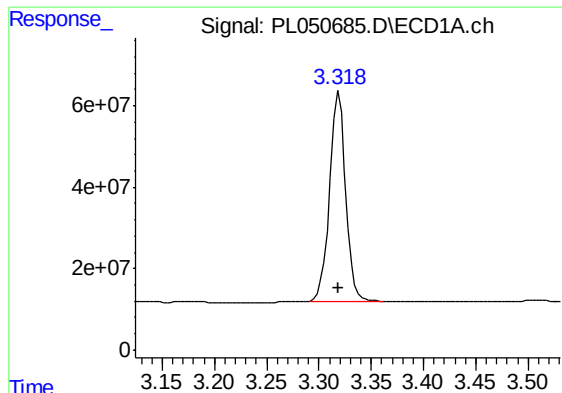

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.001 min
Response: 546163125
Conc: 54.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

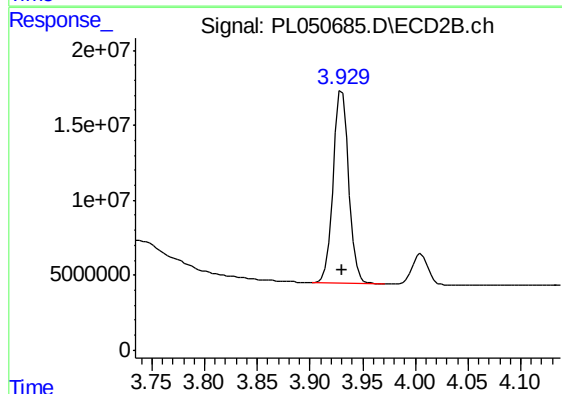


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 131128180
Conc: 45.96 ng/ml

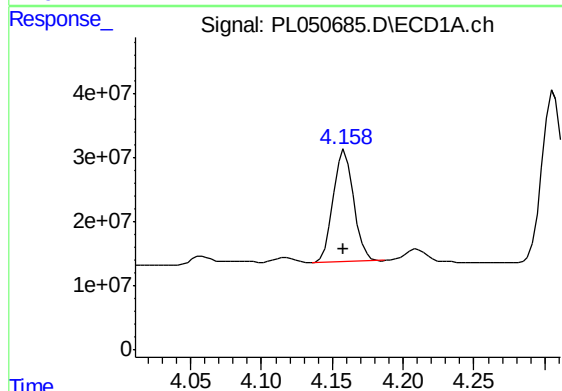


#23 Chlordane-1

R.T.: 4.159 min
Delta R.T.: 0.001 min
Response: 176608996
Conc: 479.98 ng/ml

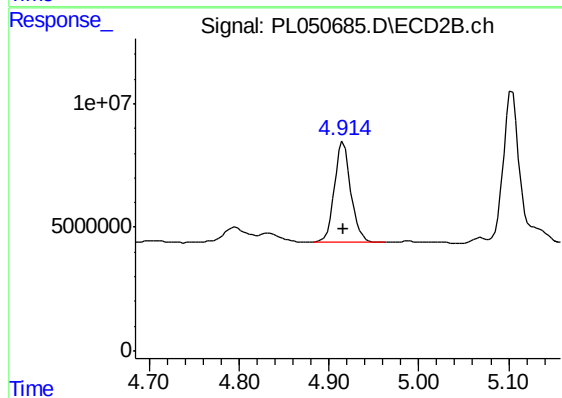

#23 Chlordane-1


R.T.: 4.916 min
Delta R.T.: 0.000 min
Response: 51545749
Conc: 475.12 ng/ml

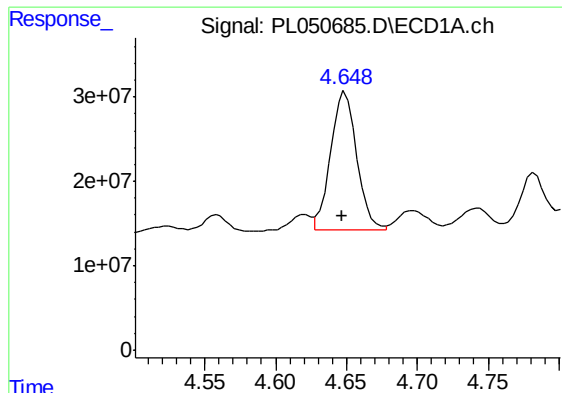

#24 Chlordane-2


R.T.: 4.649 min
Delta R.T.: 0.002 min
Response: 210431063
Conc: 470.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

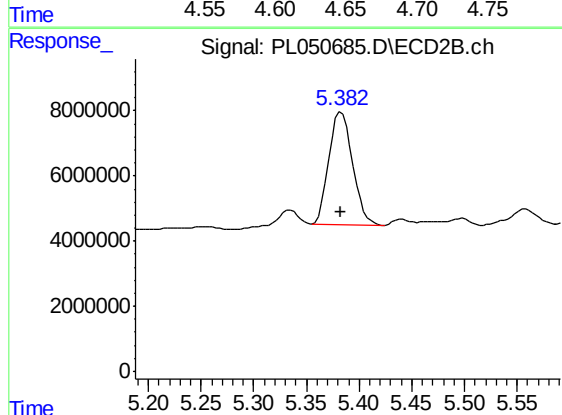


#24 Chlordane-2

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 54089076
Conc: 460.52 ng/ml

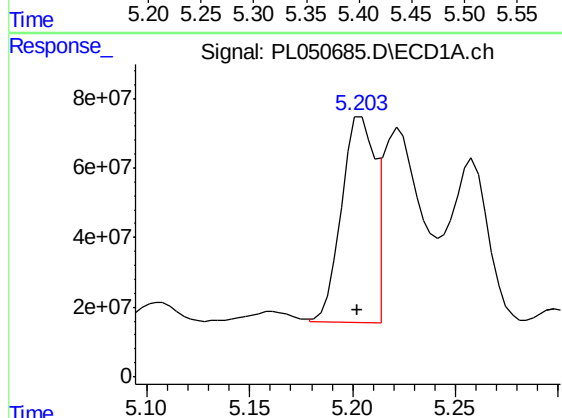


#25 Chlordane-3

R.T.: 5.204 min
Delta R.T.: 0.002 min
Response: 656492616
Conc: 468.99 ng/ml

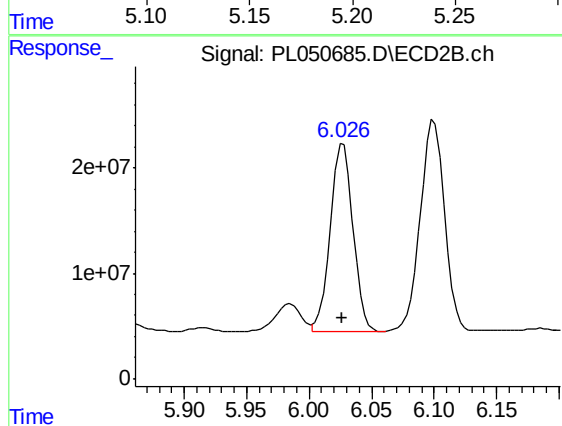

#25 Chlordane-3


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 225268229
Conc: 468.35 ng/ml

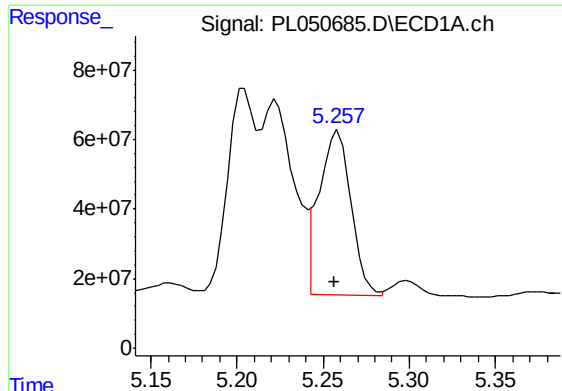

#26 Chlordane-4


R.T.: 5.259 min
Delta R.T.: 0.002 min
Response: 619028990
Conc: 469.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

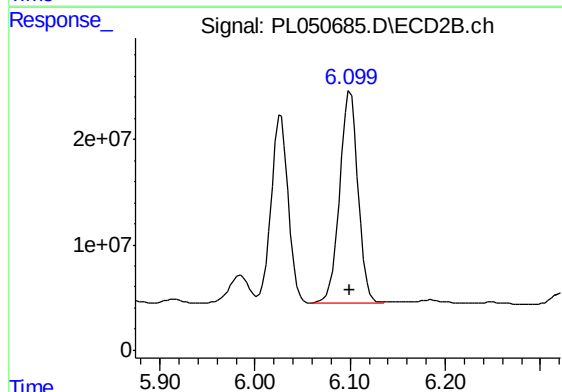


#26 Chlordane-4

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 271364993
Conc: 467.13 ng/ml

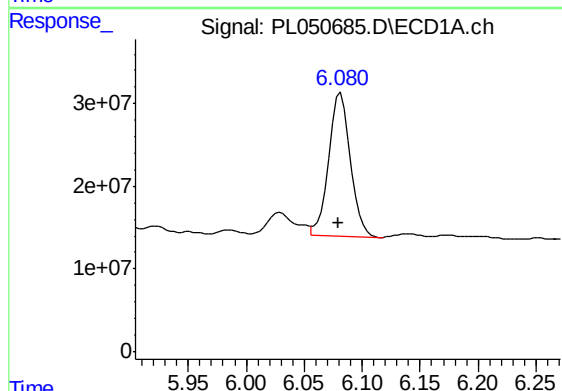


#27 Chlordane-5

R.T.: 6.081 min
Delta R.T.: 0.002 min
Response: 227223807
Conc: 447.35 ng/ml

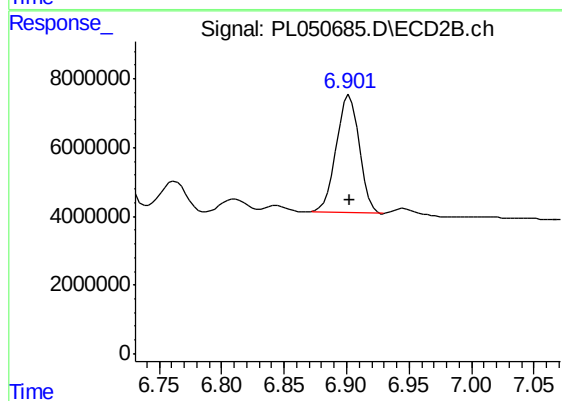

#27 Chlordane-5


R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 43843874
Conc: 459.74 ng/ml

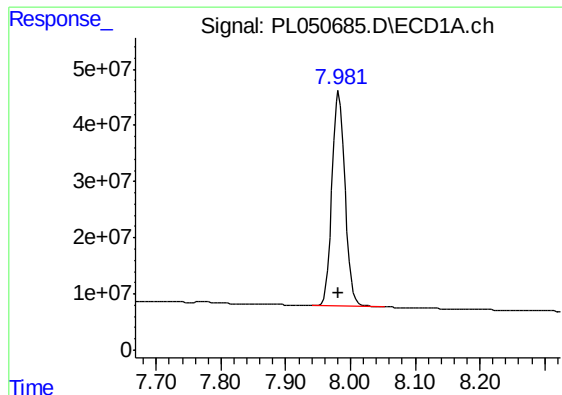

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: 0.002 min
Response: 527431166
Conc: 52.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

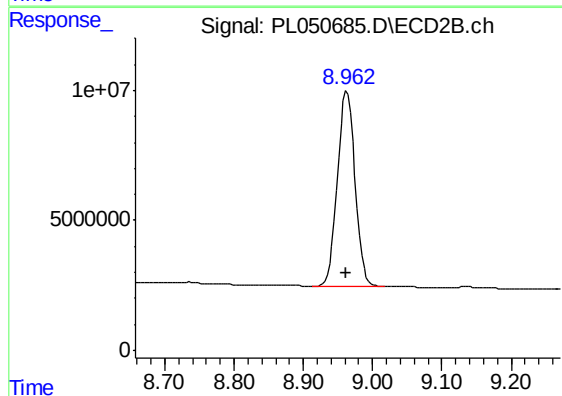

#28 Decachlorobiphenyl

R.T.: 8.963 min
Delta R.T.: 0.002 min
Response: 132823633
Conc: 46.97 ng/ml