

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072219\
 Data File : PL050694.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2019 17:09
 Operator : SM\AJ
 Sample : K3617-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-07-071919-B

Manual Integrations
 APPROVED

Ankita
 7/23/2019 2:08:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:11:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.319	3.931	99345371	28058120	9.887	9.834
28) SA Decachlor...	7.982	8.963	100.0E6	32491696	9.878	11.490
Target Compounds						
10) B gamma-Chl...	5.203	6.024	4366144	1591522	0.277m	0.431m#
11) B alpha-Chl...	5.257	6.098	4963138	2953702	0.325m	0.806m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072219\
Data File : PL050694.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2019 17:09
Operator : SM\AJ
Sample : K3617-03
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
NB-07-071919-B


Manual Integrations
APPROVED

Ankita
7/23/2019 2:08:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:11:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

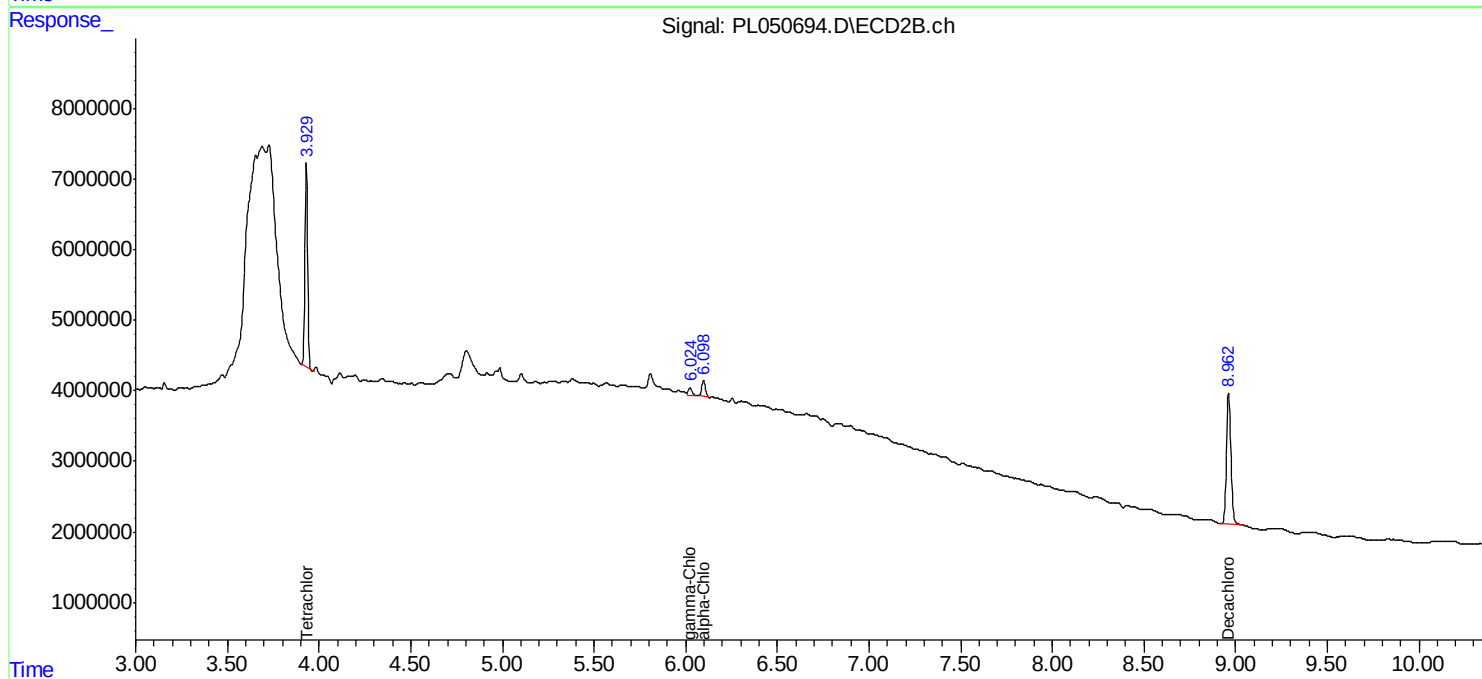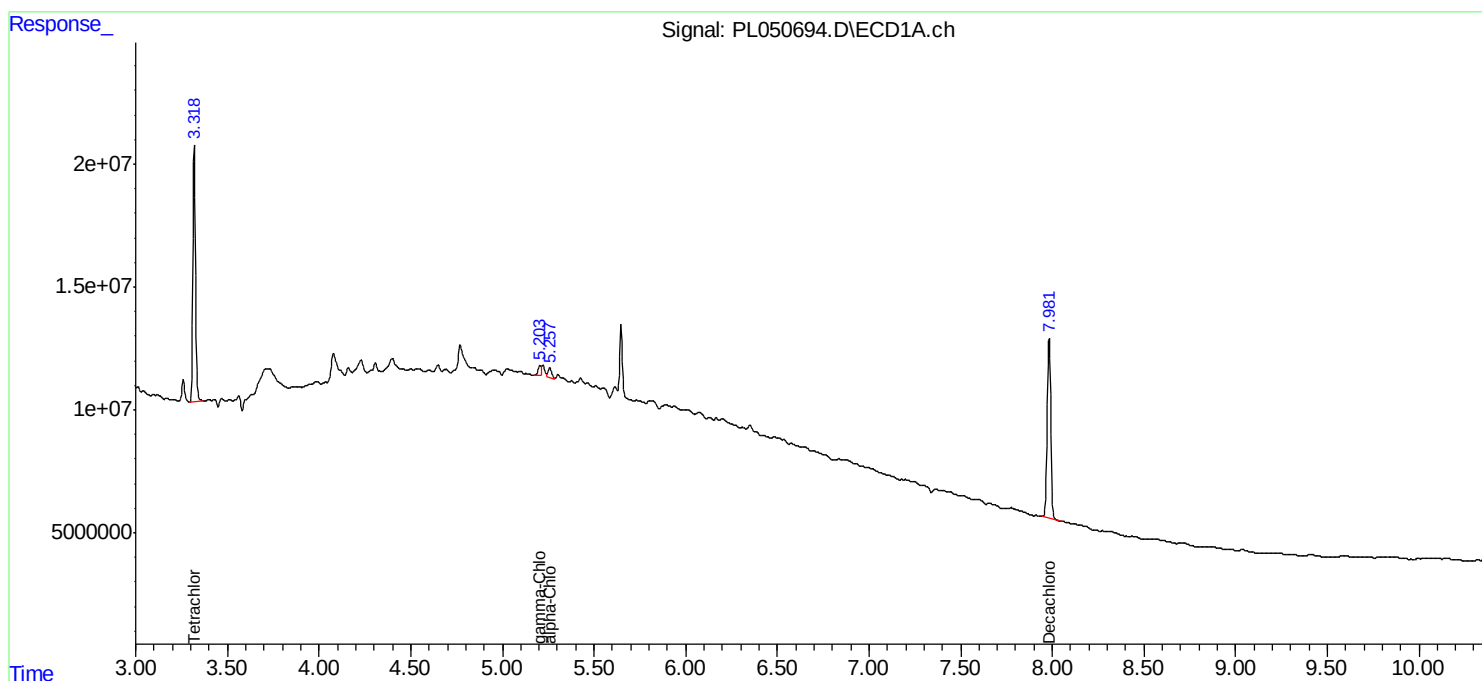

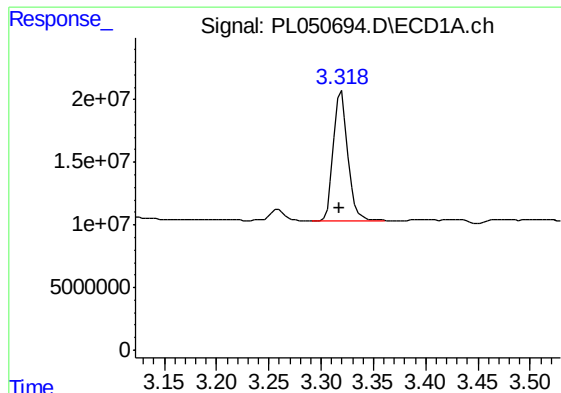


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: 0.001 min
Response: 99345371
Conc: 9.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-07-071919-B


Manual Integrations
APPROVED

Ankita
7/23/2019 2:08:50 PM

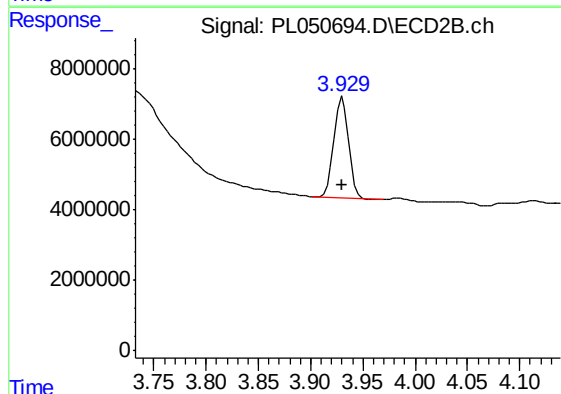


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 28058120
Conc: 9.83 ng/ml

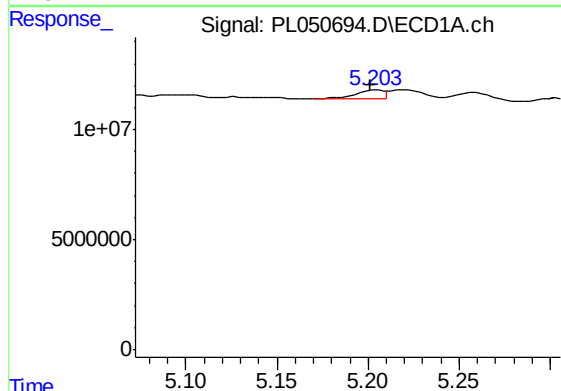


#10 gamma-Chlordane

R.T.: 5.203 min
Delta R.T.: 0.001 min
Response: 4366144
Conc: 0.28 ng/ml m

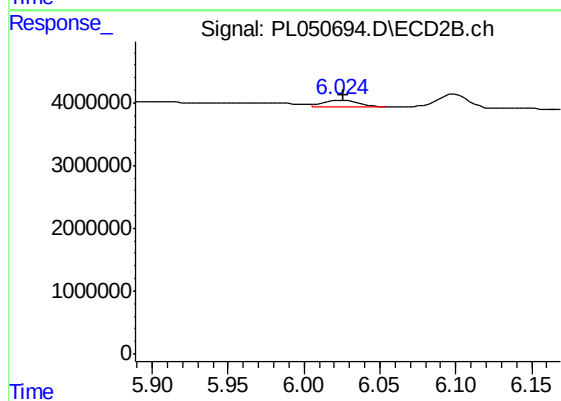

#10 gamma-Chlordane

R.T.: 6.024 min
Delta R.T.: -0.002 min
Response: 1591522
Conc: 0.43 ng/ml m

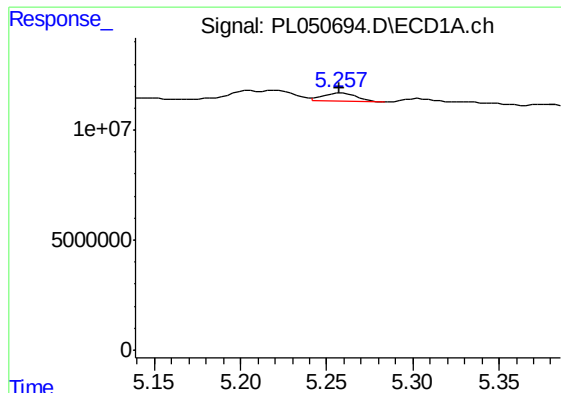


#11 alpha-Chlordane

R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 4963138
Conc: 0.33 ng/ml m

Instrument :
ECD_L
ClientSampleId :
NB-07-071919-B


Manual Integrations
APPROVED

Ankita
7/23/2019 2:08:50 PM

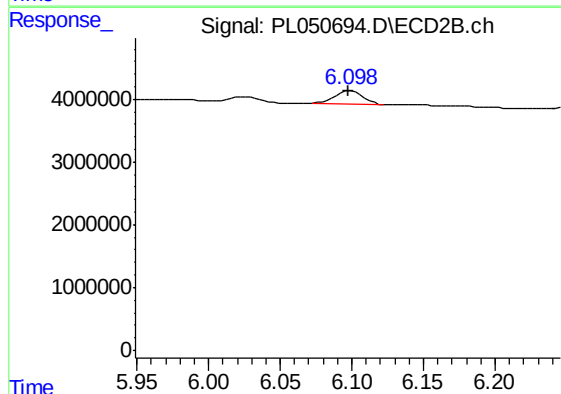


#11 alpha-Chlordane

R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 2953702
Conc: 0.81 ng/ml m

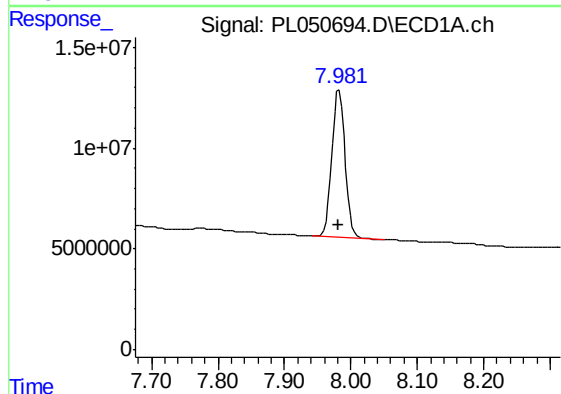

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: 0.002 min
Response: 100018571
Conc: 9.88 ng/ml

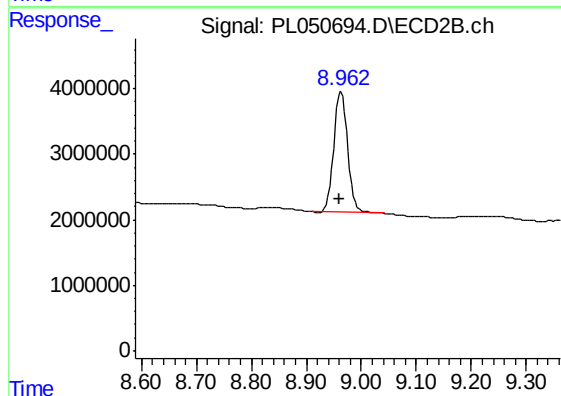

#28 Decachlorobiphenyl

R.T.: 8.963 min
Delta R.T.: 0.002 min
Response: 32491696
Conc: 11.49 ng/ml