

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
 Data File : PL060088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 14:52
 Operator : DD\AJ
 Sample : L3370-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:49:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	40144304	53518141	20.755	20.194
28)	SA Decachlor...	8.224	9.102	26035302	28180850	15.826	13.475
Target Compounds							
4)	MA Heptachlor	0.000	5.202	0	903667	N.D.	0.269 #
6)	B beta-BHC	4.447	0.000	776277	0	0.760	N.D. #
9)	A Endosulfan I	5.539f	0.000	1412219	0	0.839	N.D. #
11)	B alpha-Chl...	0.000	6.201	0	3283147	N.D.	1.148 #
12)	B 4,4'-DDE	5.631	6.356	7310901	11246759	4.390	4.202
17)	MA 4,4'-DDT	6.388	7.148	1423523	2436235	1.095	1.237
26)	Chlordane-4	0.000	6.201	0	3283147	N.D.	7.093 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
Data File : PL060088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 14:52
Operator : DD\AJ
Sample : L3370-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-3-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:49:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

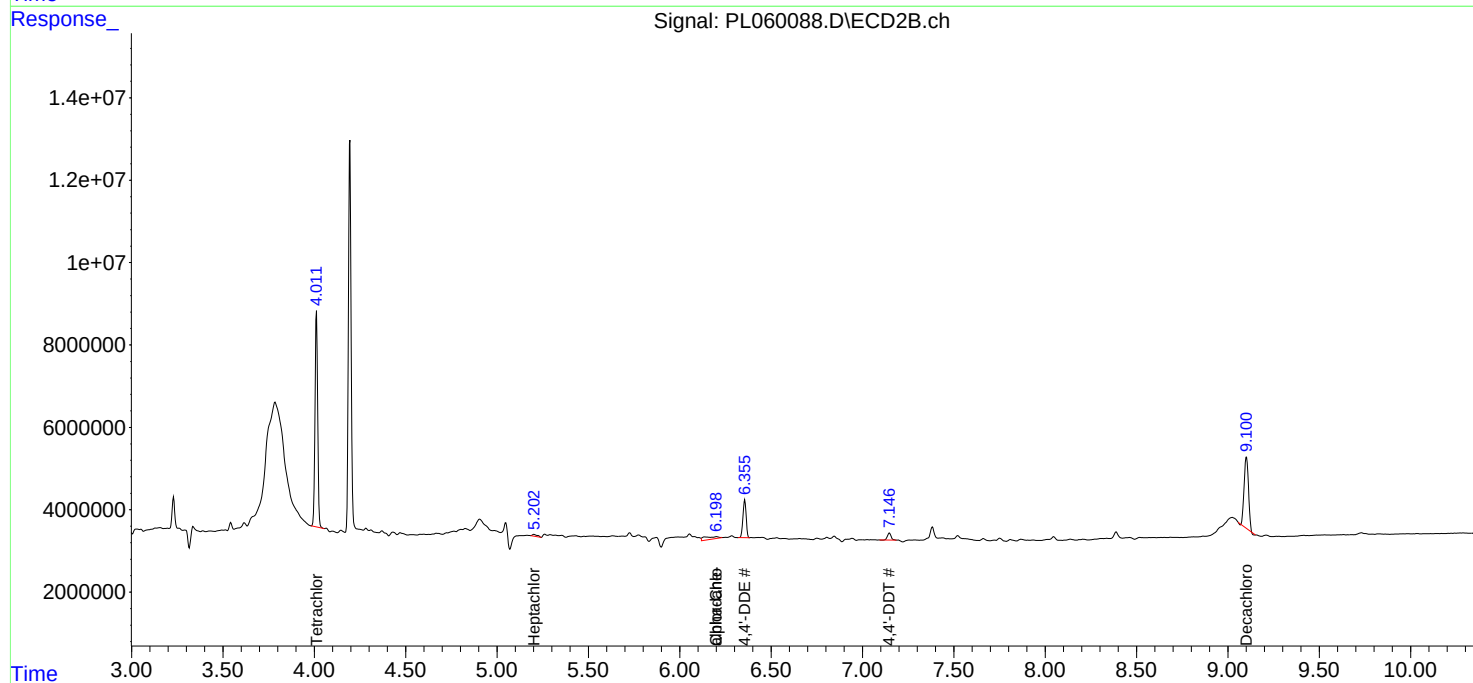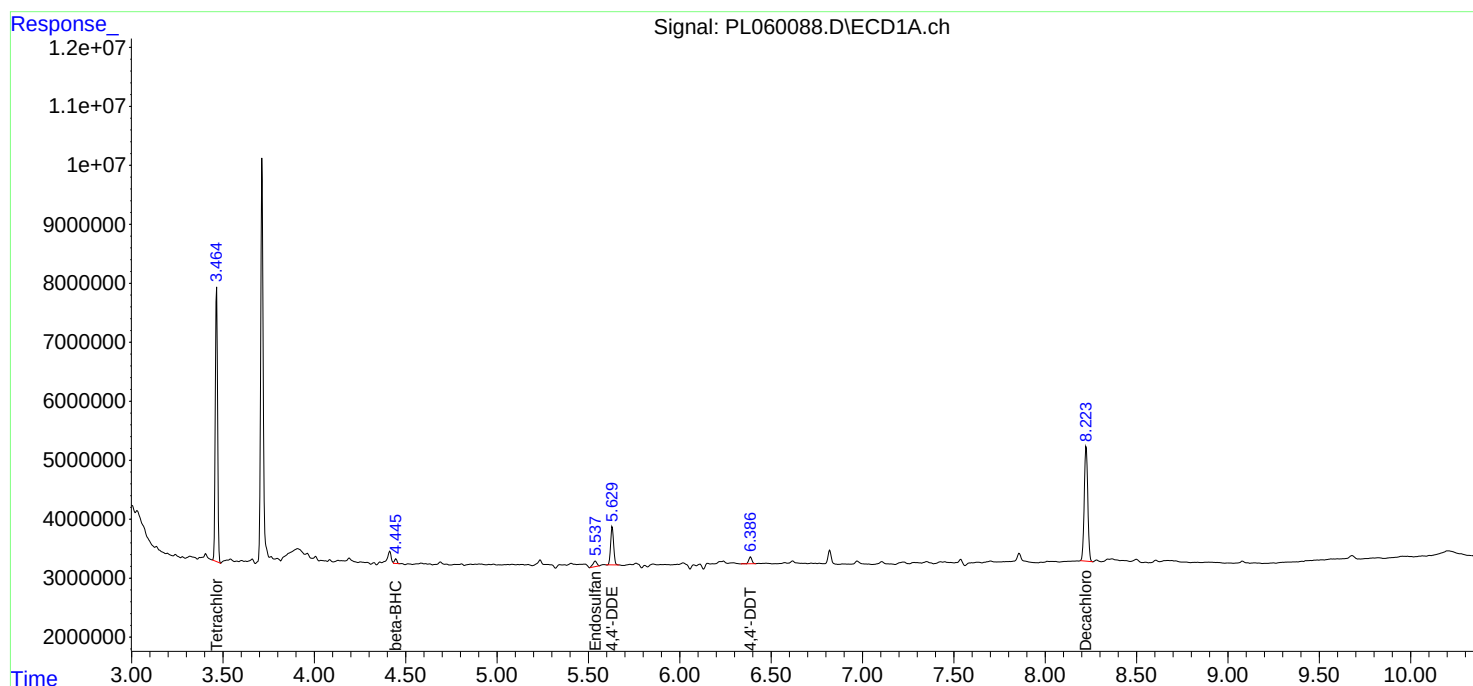


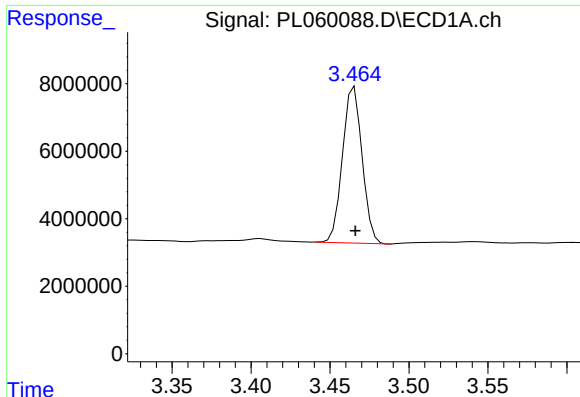

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 40144304
Conc: 20.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-S

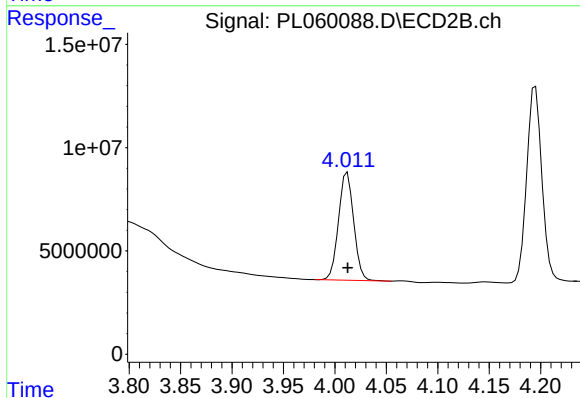


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 53518141
Conc: 20.19 ng/ml

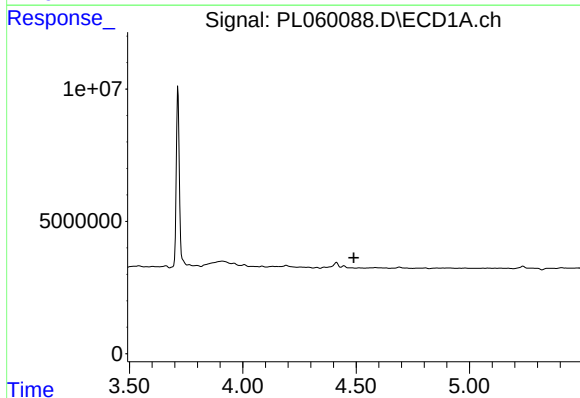


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

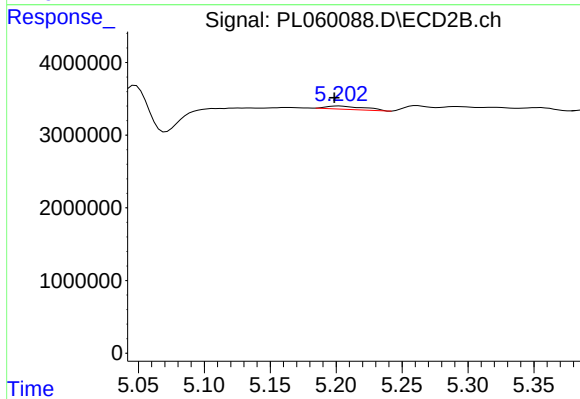

#4 Heptachlor


R.T.: 5.202 min
Delta R.T.: 0.004 min
Response: 903667
Conc: 0.27 ng/ml

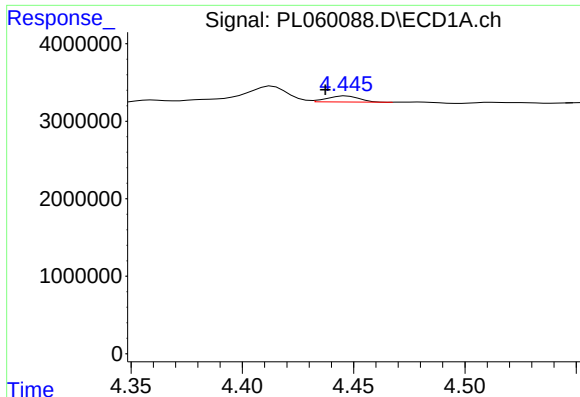

#6 beta-BHC


R.T.: 4.447 min
Delta R.T.: 0.009 min
Response: 776277
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-S

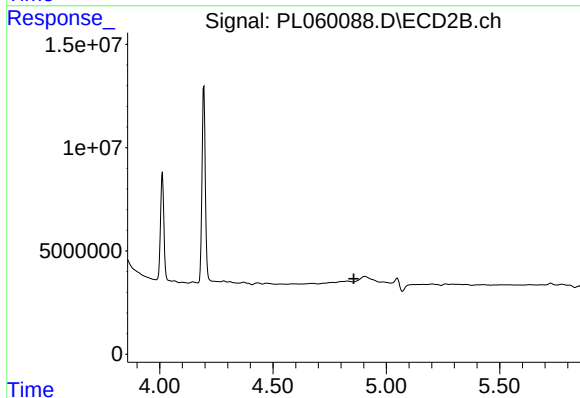


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

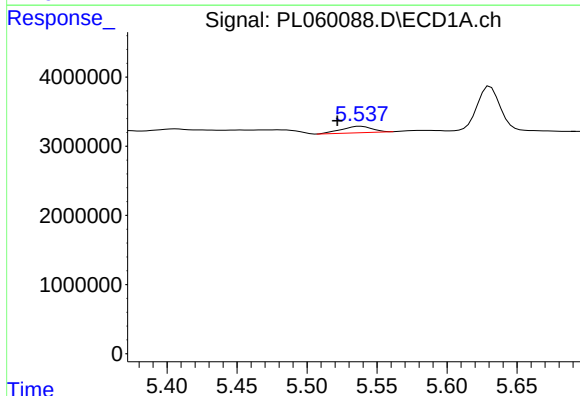


#9 Endosulfan I

R.T.: 5.539 min
Delta R.T.: 0.017 min
Response: 1412219
Conc: 0.84 ng/ml

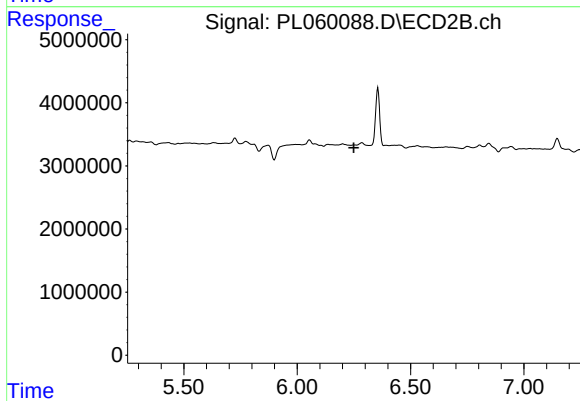

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

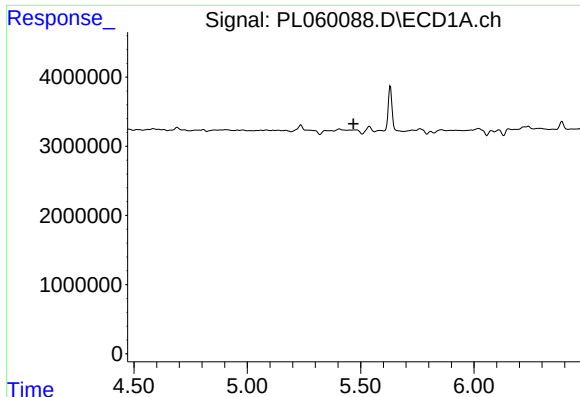

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3-S

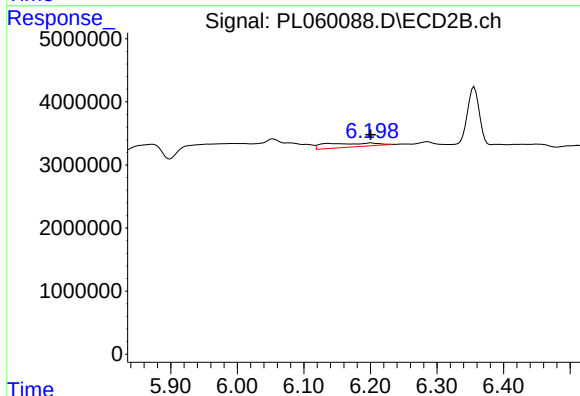


#11 alpha-Chlordane

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 3283147
Conc: 1.15 ng/ml

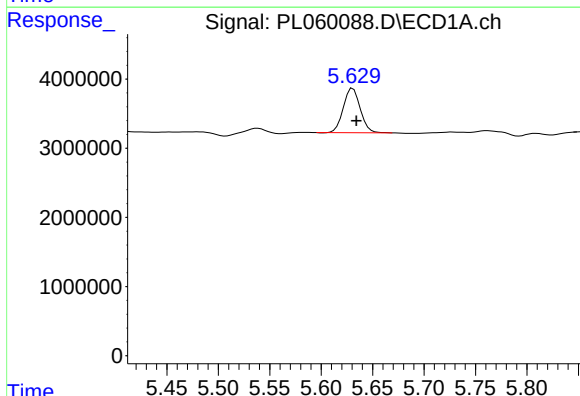


#12 4,4'-DDE

R.T.: 5.631 min
Delta R.T.: -0.003 min
Response: 7310901
Conc: 4.39 ng/ml

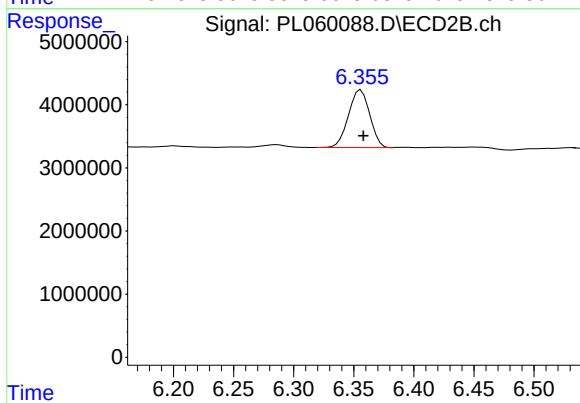

#12 4,4'-DDE


R.T.: 6.356 min
Delta R.T.: -0.002 min
Response: 11246759
Conc: 4.20 ng/ml

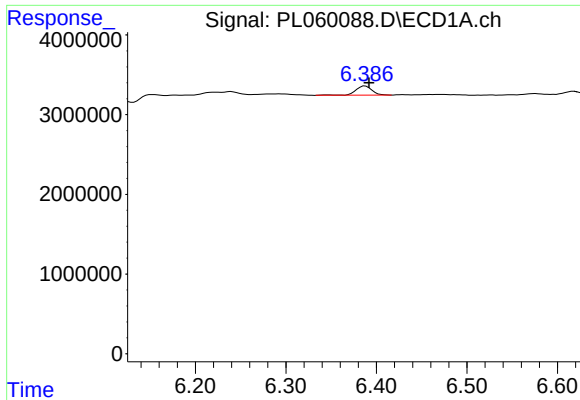

#17 4,4'-DDT


R.T.: 6.388 min
Delta R.T.: -0.004 min
Response: 1423523
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-S

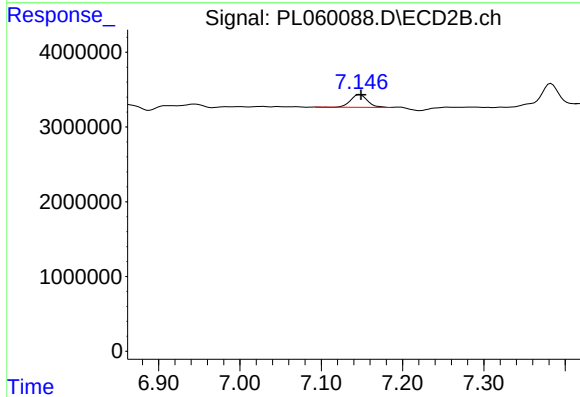


#17 4,4'-DDT

R.T.: 7.148 min
Delta R.T.: -0.001 min
Response: 2436235
Conc: 1.24 ng/ml

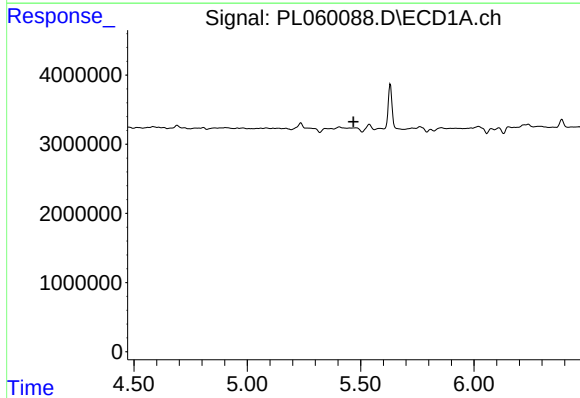


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.469 min
Response: 0
Conc: N.D.

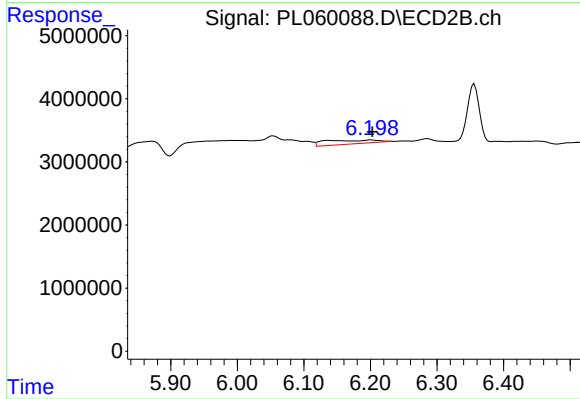

#26 Chlordane-4


R.T.: 6.201 min
Delta R.T.: -0.002 min
Response: 3283147
Conc: 7.09 ng/ml

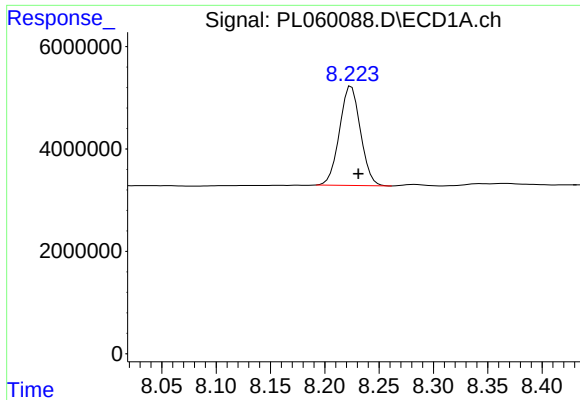

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.007 min
Response: 26035302
Conc: 15.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-S

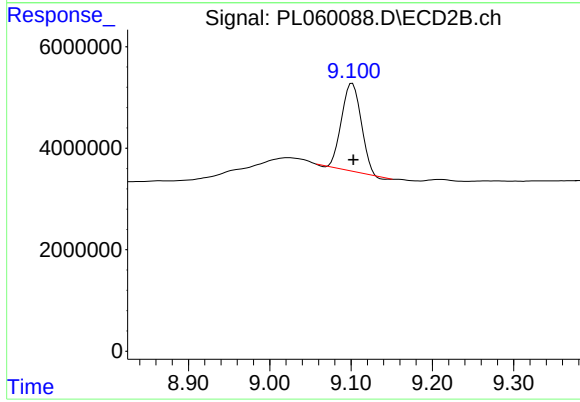

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: -0.001 min
Response: 28180850
Conc: 13.47 ng/ml