

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
 Data File : PL060092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 15:55
 Operator : DD\AJ
 Sample : L3372-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-04-011-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:50:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	41801261	58254235	21.611	21.981
28)	SA Decachlor...	8.226	9.101	30245116	38853070	18.385	18.578
Target Compounds							
4)	MA Heptachlor	0.000	5.204	0	614848	N.D.	0.183 #
8)	B Heptachlo...	0.000	5.871f	0	7493066	N.D.	2.782 #
10)	B gamma-Chl...	0.000	6.138	0	1672209	N.D.	0.584 #
15)	B Endosulfa...	6.286	0.000	52883	0	0.032	N.D. #
21)	B Endrin ke...	0.000	7.752	0	2611743	N.D.	1.011 #
25)	Chlordane-3	0.000	6.138	0	1672209	N.D.	4.322 #
27)	Chlordane-5	6.286f	0.000	52883	0	0.932	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
Data File : PL060092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 15:55
Operator : DD\AJ
Sample : L3372-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-04-011-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:50:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

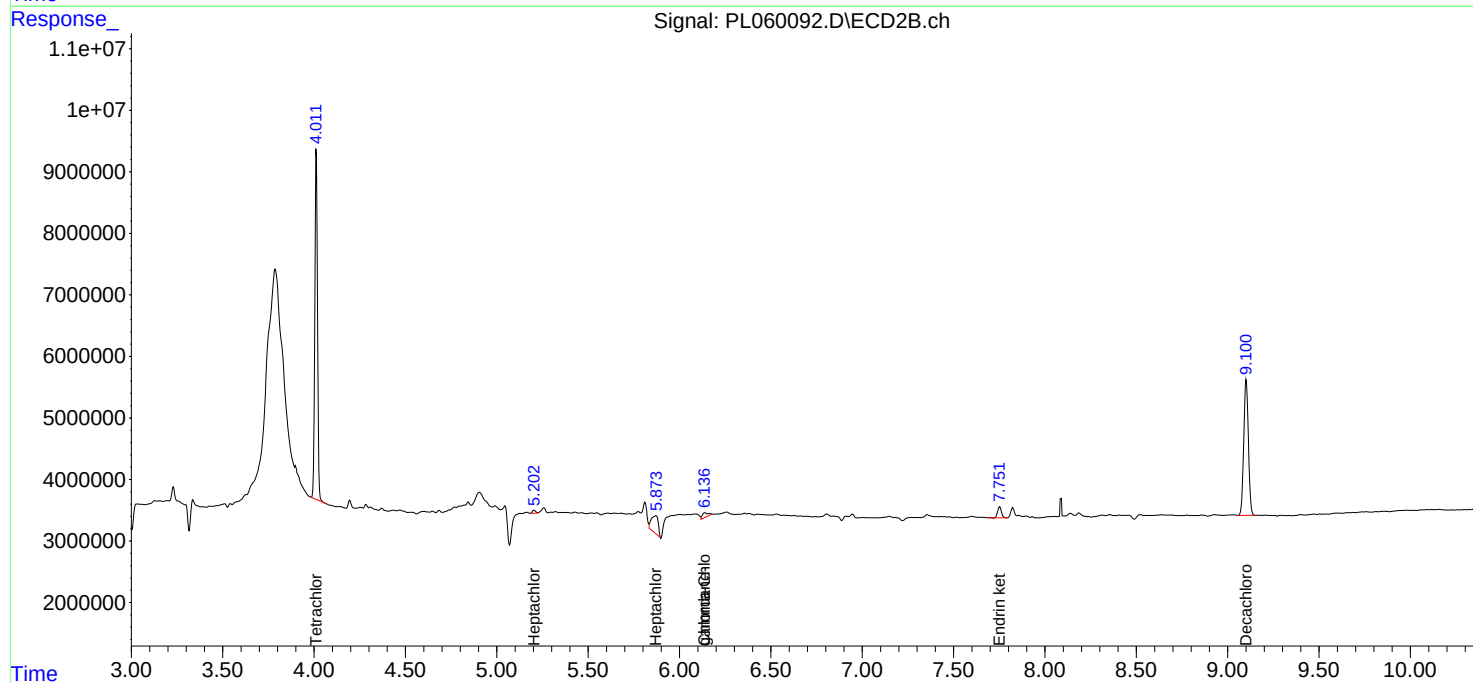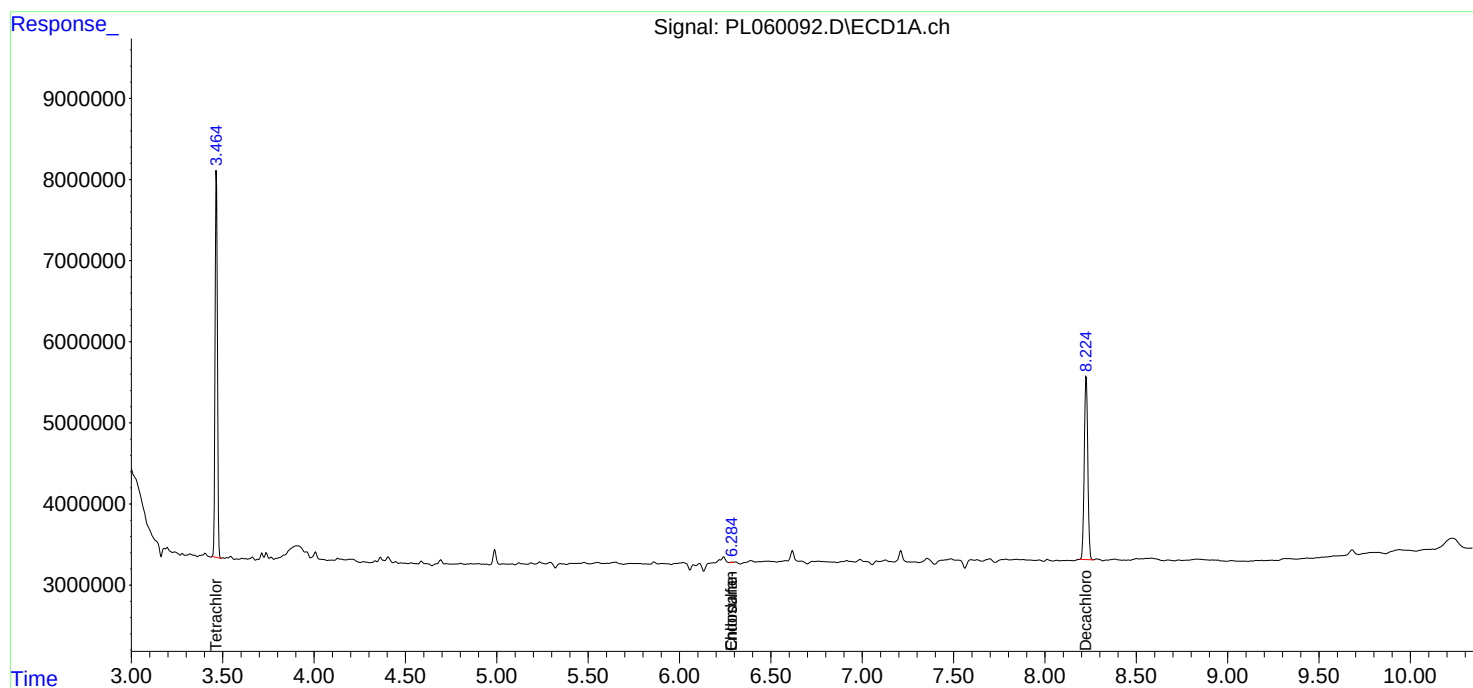


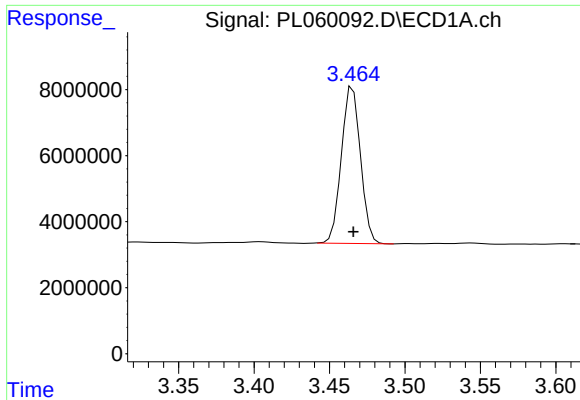

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 41801261
Conc: 21.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-04-011-ABCD

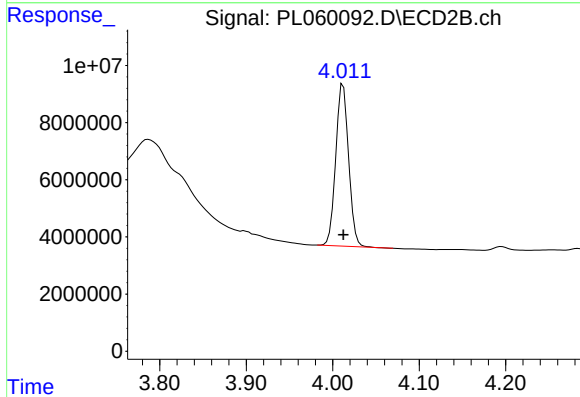


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 58254235
Conc: 21.98 ng/ml

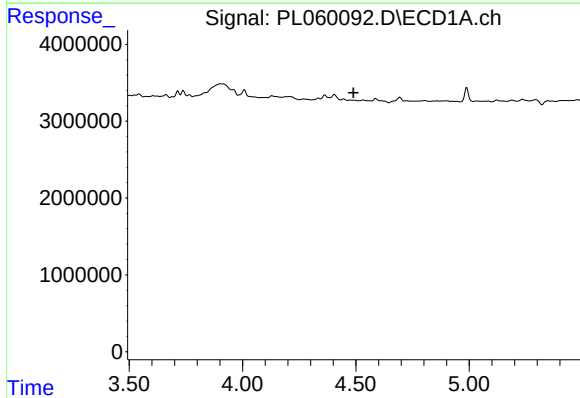


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

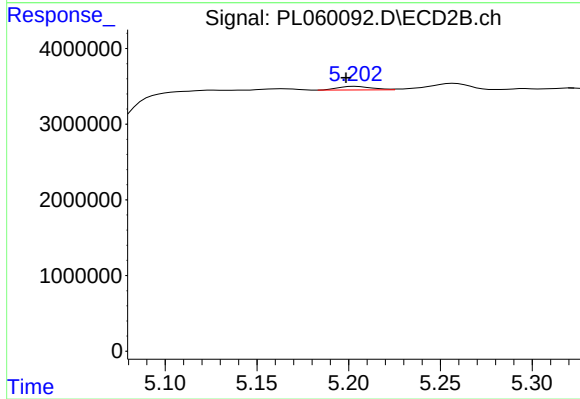

#4 Heptachlor


R.T.: 5.204 min
Delta R.T.: 0.005 min
Response: 614848
Conc: 0.18 ng/ml

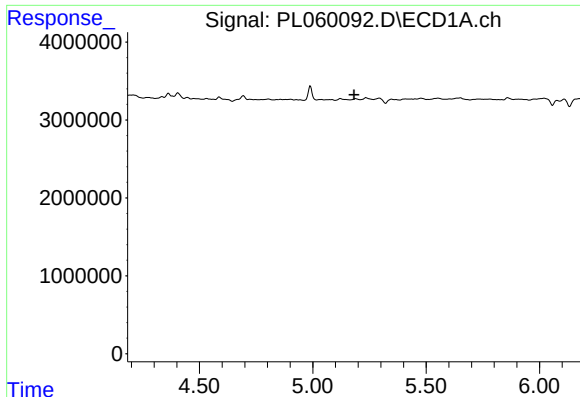

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-BPM-04-011-ABCD

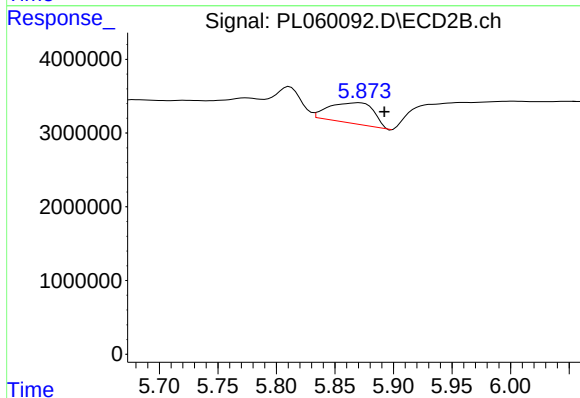


#8 Heptachlor epoxide

R.T.: 5.871 min
Delta R.T.: -0.021 min
Response: 7493066
Conc: 2.78 ng/ml

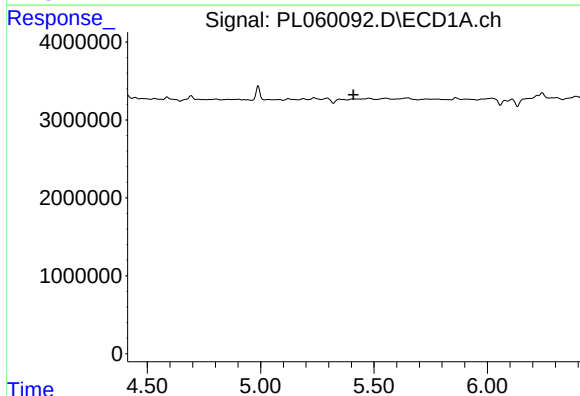


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.410 min
Response: 0
Conc: N.D.

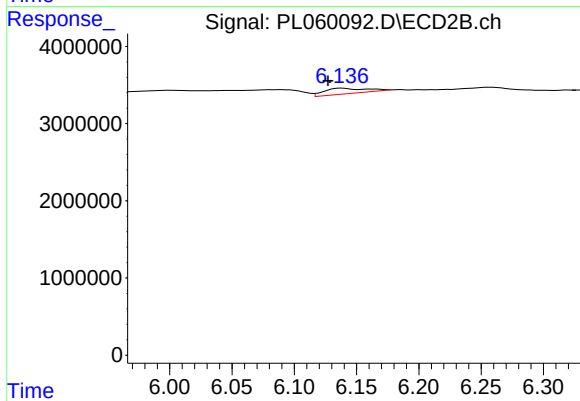

#10 gamma-Chlordane


R.T.: 6.138 min
Delta R.T.: 0.011 min
Response: 1672209
Conc: 0.58 ng/ml

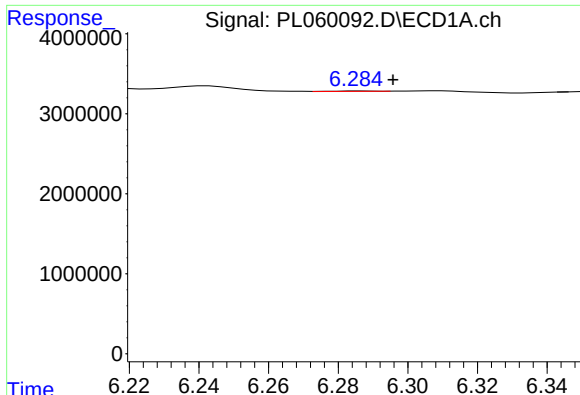

#15 Endosulfan II


R.T.: 6.286 min
Delta R.T.: -0.009 min
Response: 52883
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-04-011-ABCD

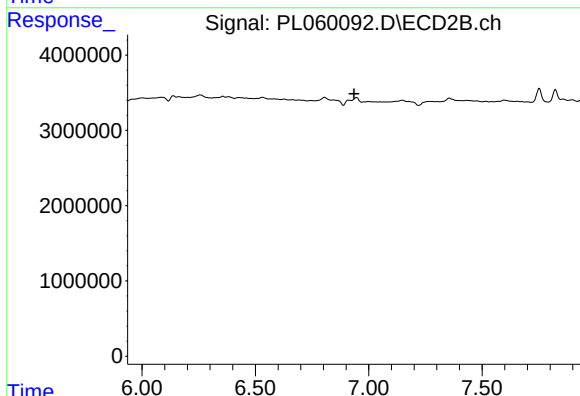


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

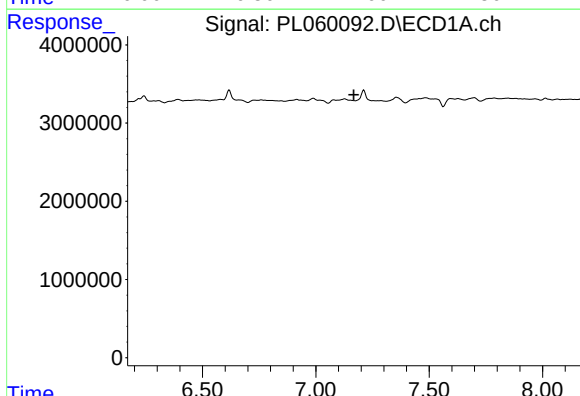


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.168 min
Response: 0
Conc: N.D.

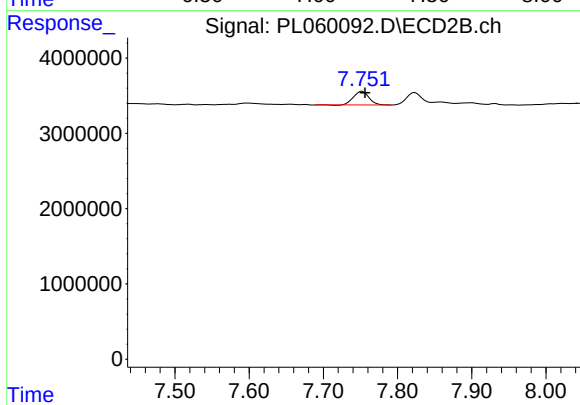

#21 Endrin ketone


R.T.: 7.752 min
Delta R.T.: -0.004 min
Response: 2611743
Conc: 1.01 ng/ml

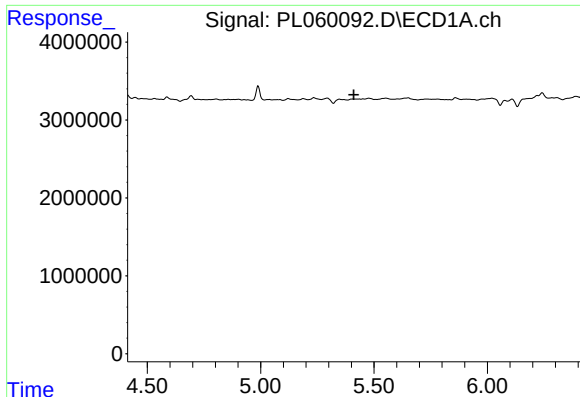

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-BPM-04-011-ABCD

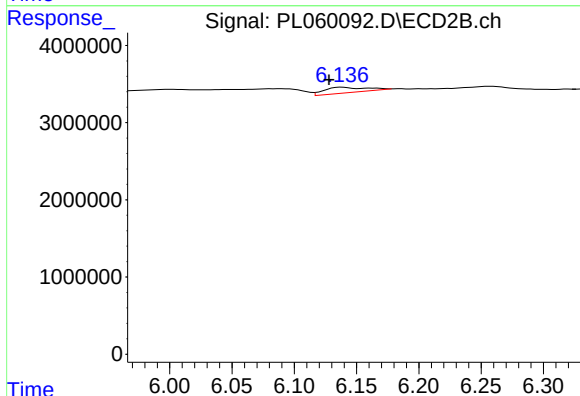


#25 Chlordane-3

R.T.: 6.138 min
Delta R.T.: 0.010 min
Response: 1672209
Conc: 4.32 ng/ml

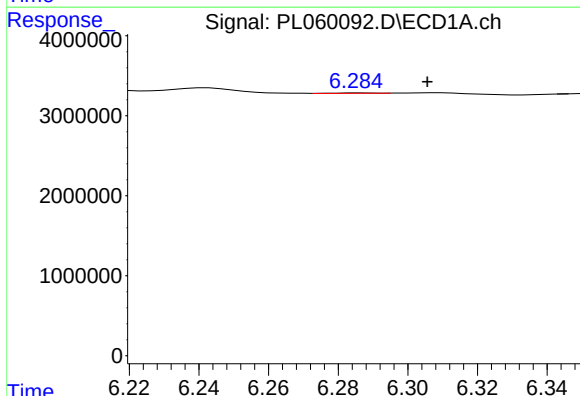


#27 Chlordane-5

R.T.: 6.286 min
Delta R.T.: -0.019 min
Response: 52883
Conc: 0.93 ng/ml

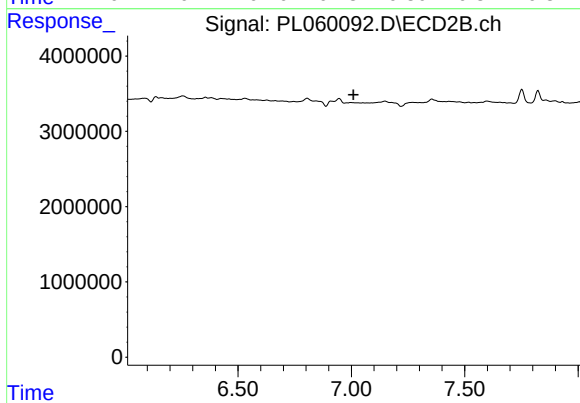

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 7.010 min
Response: 0
Conc: N.D.

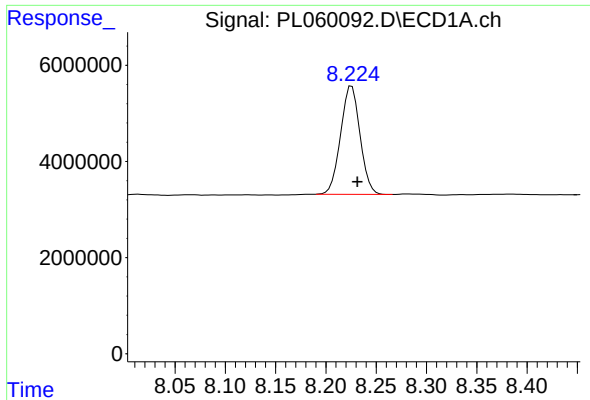

#28 Decachlorobiphenyl

R.T.: 8.226 min
Delta R.T.: -0.005 min
Response: 30245116
Conc: 18.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-04-011-ABCD

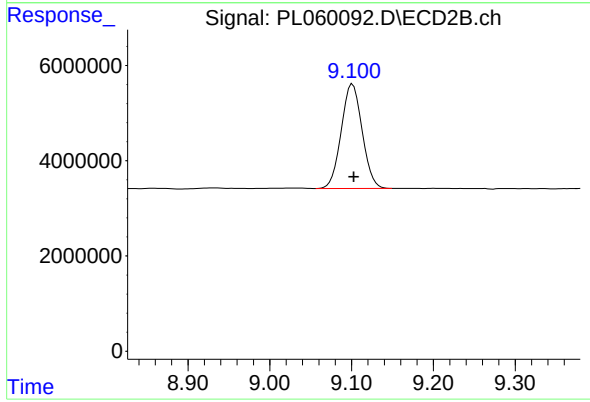

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: -0.001 min
Response: 38853070
Conc: 18.58 ng/ml