

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
 Data File : PL060100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 17:49
 Operator : DD\AJ
 Sample : L3184-17
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-03-072020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:52:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.013	38018280	52219308	19.655	19.704
28)	SA Decachlor...	8.225	9.102	34441321	44602881	20.936	21.327
Target Compounds							
10)	B gamma-Chl...	0.000	6.107f	0	4159831	N.D.	1.453 #
25)	Chlordane-3	0.000	6.107f	0	4159831	N.D.	10.751 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
Data File : PL060100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 17:49
Operator : DD\AJ
Sample : L3184-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EO-03-072020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:52:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

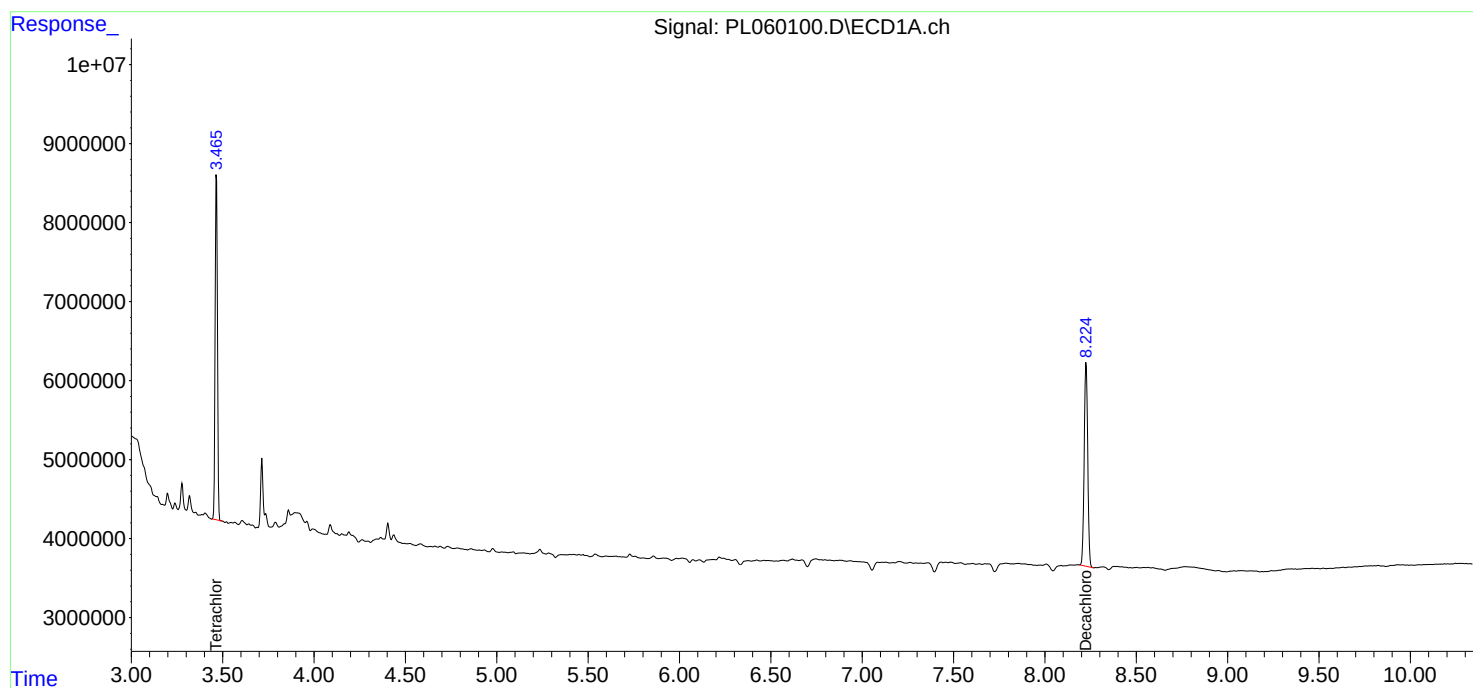


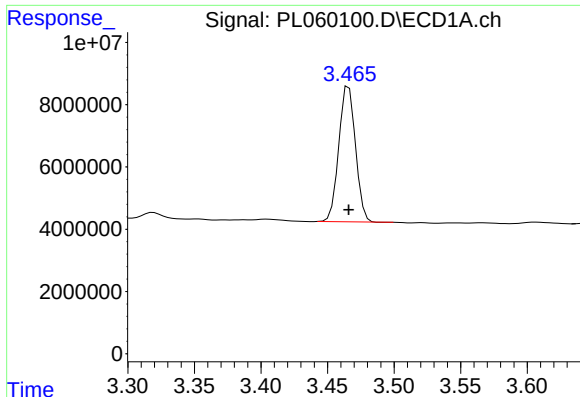

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 38018280
Conc: 19.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-03-072020

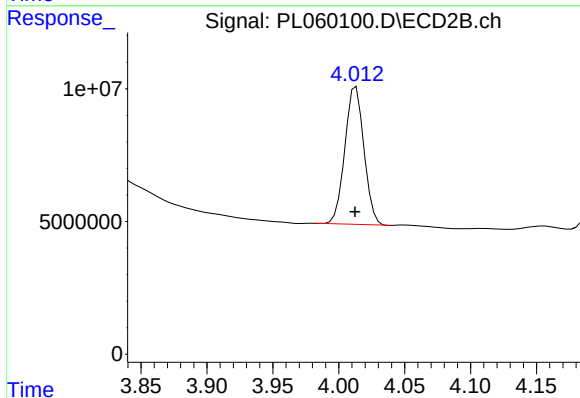


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 52219308
Conc: 19.70 ng/ml

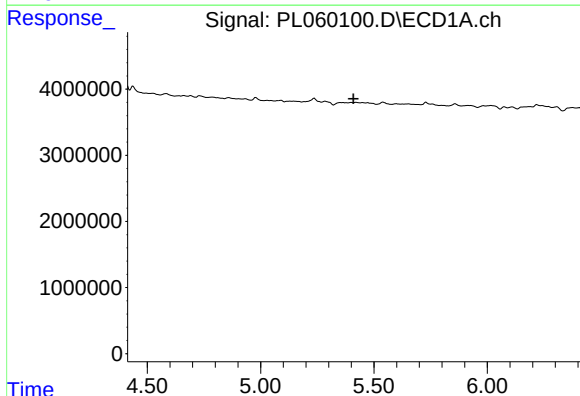


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.410 min
Response: 0
Conc: N.D.

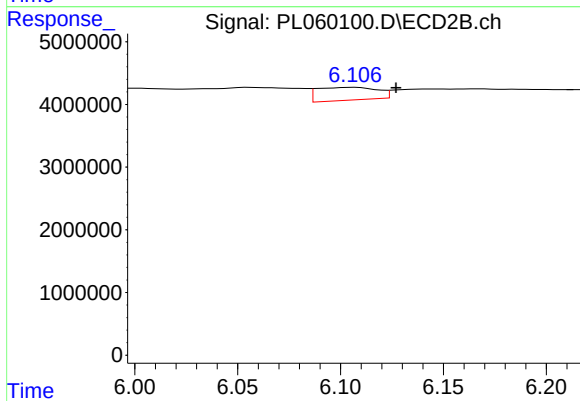

#10 gamma-Chlordane


R.T.: 6.107 min
Delta R.T.: -0.020 min
Response: 4159831
Conc: 1.45 ng/ml

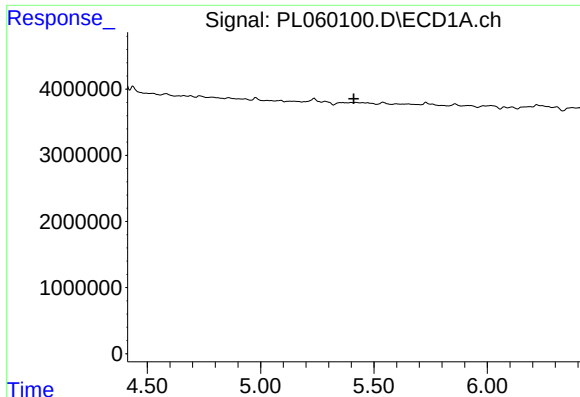

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-03-072020

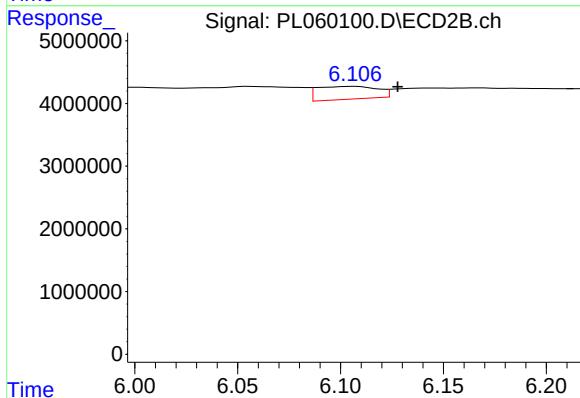


#25 Chlordane-3

R.T.: 6.107 min
Delta R.T.: -0.021 min
Response: 4159831
Conc: 10.75 ng/ml

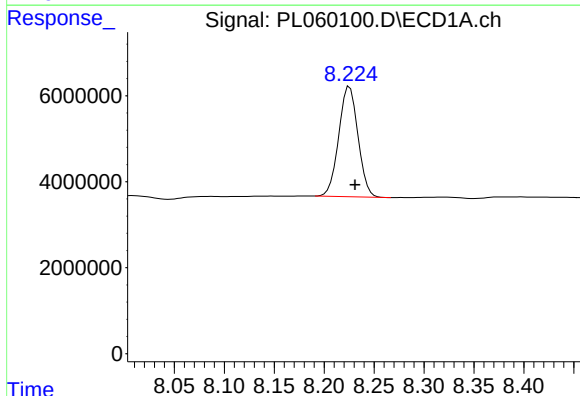

#28 Decachlorobiphenyl

R.T.: 8.225 min
Delta R.T.: -0.006 min
Response: 34441321
Conc: 20.94 ng/ml

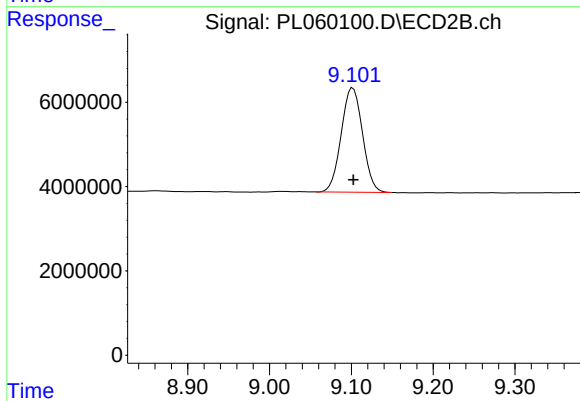

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: 0.000 min
Response: 44602881
Conc: 21.33 ng/ml