

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
 Data File : PL060104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 18:45
 Operator : DD\AJ
 Sample : L3187-13
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-04-072120

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:53:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.012	37226881	51342785	19.246	19.373
28)	SA Decachlor...	8.224	9.100	30543512	39258030	18.566	18.771
Target Compounds							
4)	MA Heptachlor	0.000	5.200	0	759227	N.D.	0.226 #
6)	B beta-BHC	4.437	0.000	1179679	0	1.155	N.D. #
10)	B gamma-Chl...	0.000	6.102f	0	1182058	N.D.	0.413 #
11)	B alpha-Chl...	0.000	6.209	0	1354397	N.D.	0.474 #
18)	B Endrin al...	6.469	0.000	1895383	0	1.329	N.D. #
19)	B Endosulfa...	6.686	7.285	5580736	2842013	3.395	1.215 #
25)	Chlordane-3	0.000	6.102f	0	1182058	N.D.	3.055 #
26)	Chlordane-4	0.000	6.209	0	1354397	N.D.	2.926 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
Data File : PL060104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 18:45
Operator : DD\AJ
Sample : L3187-13
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SU-04-072120

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:53:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

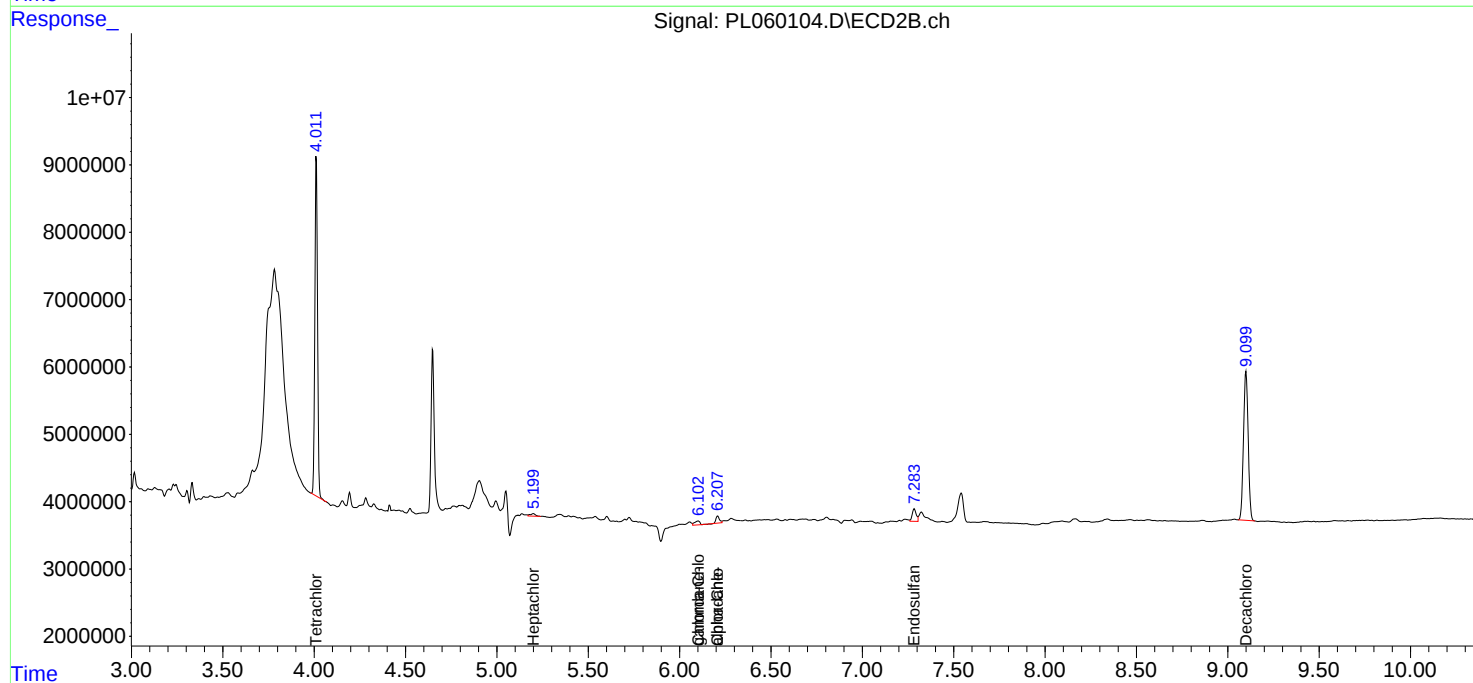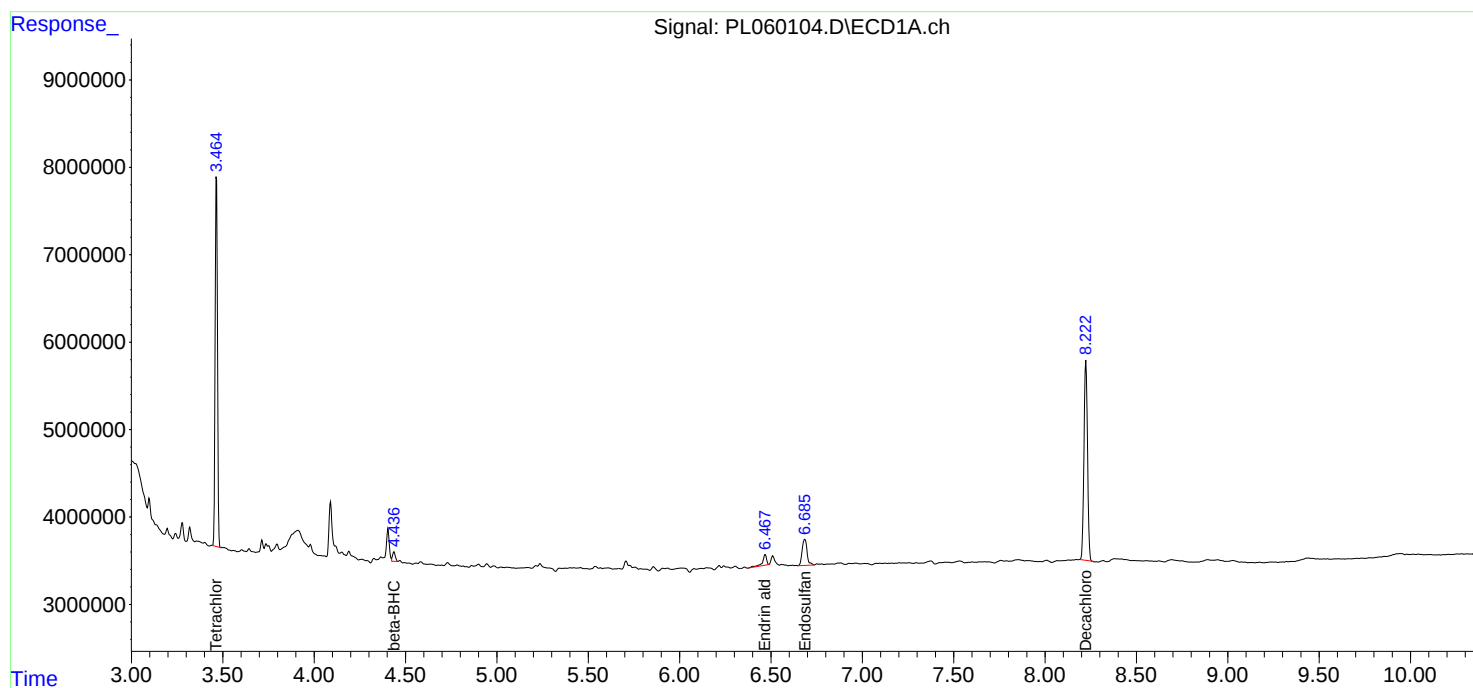


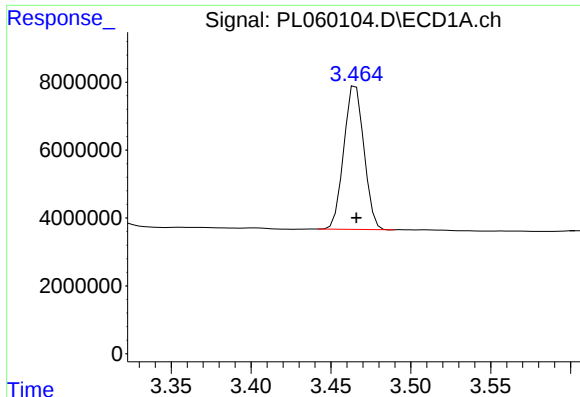

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 37226881
Conc: 19.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-04-072120

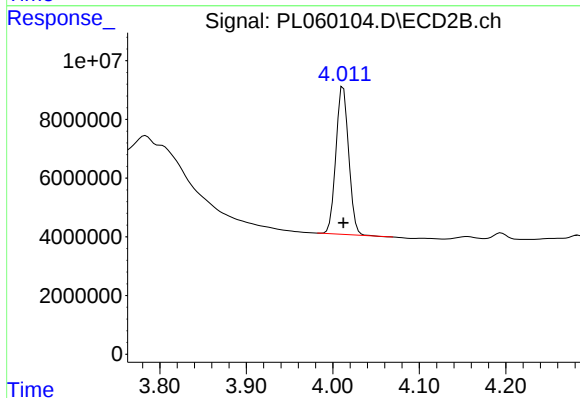


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 51342785
Conc: 19.37 ng/ml

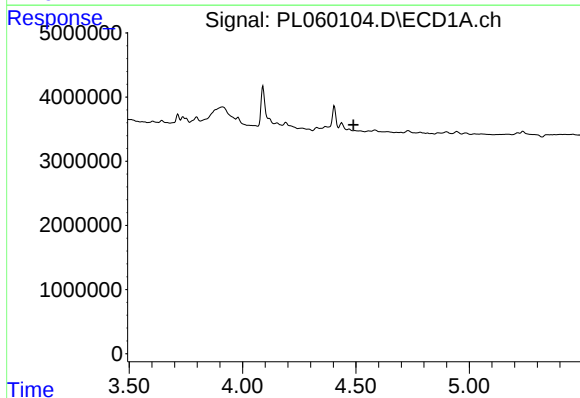


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

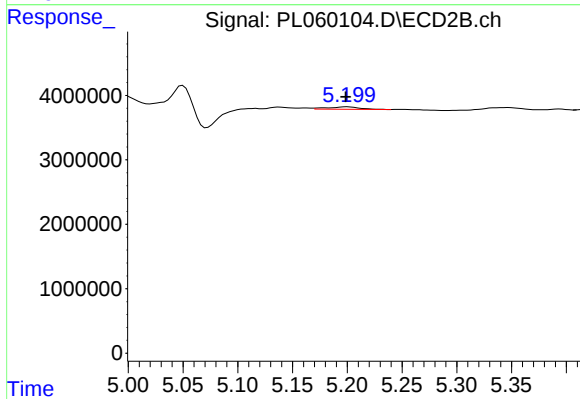

#4 Heptachlor


R.T.: 5.200 min
Delta R.T.: 0.002 min
Response: 759227
Conc: 0.23 ng/ml

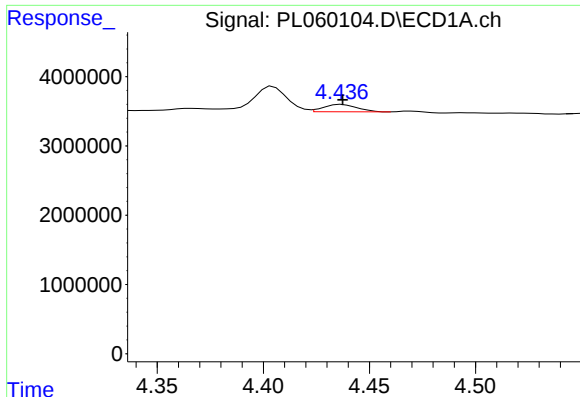

#6 beta-BHC


R.T.: 4.437 min
Delta R.T.: 0.000 min
Response: 1179679
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-04-072120

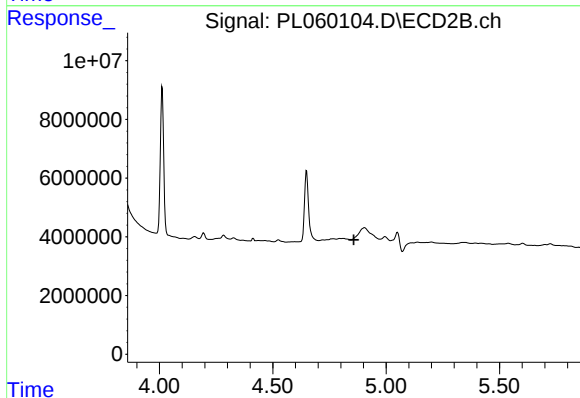


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

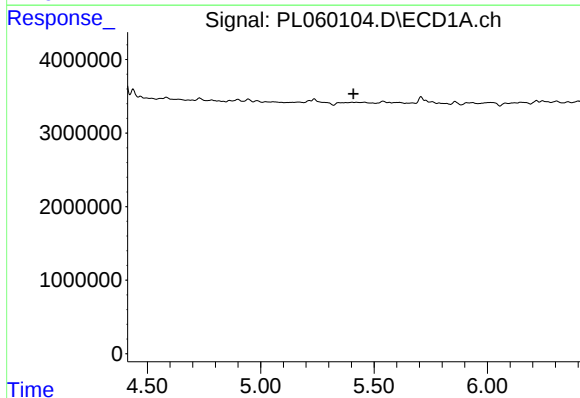


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.410 min
Response: 0
Conc: N.D.

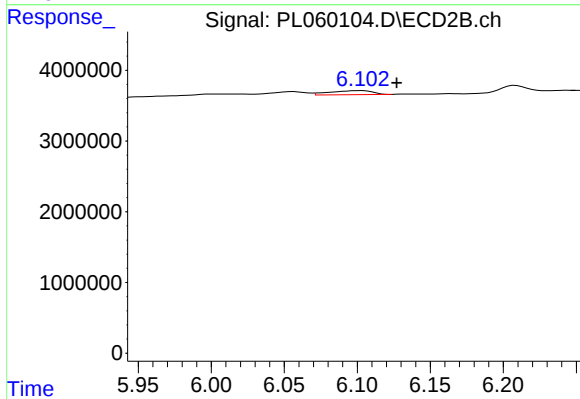

#10 gamma-Chlordane


R.T.: 6.102 min
Delta R.T.: -0.025 min
Response: 1182058
Conc: 0.41 ng/ml

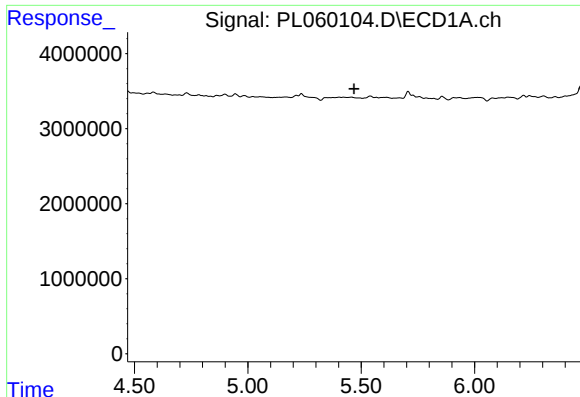

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SU-04-072120

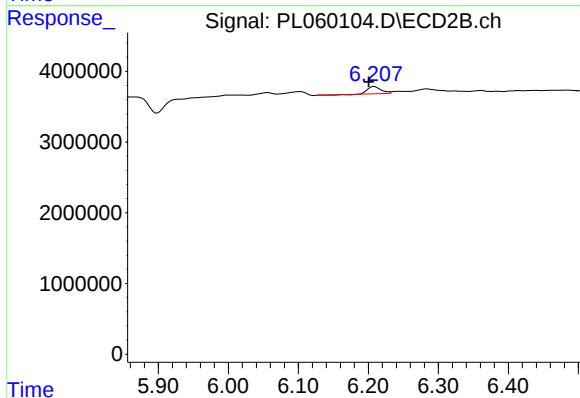


#11 alpha-Chlordane

R.T.: 6.209 min
Delta R.T.: 0.008 min
Response: 1354397
Conc: 0.47 ng/ml

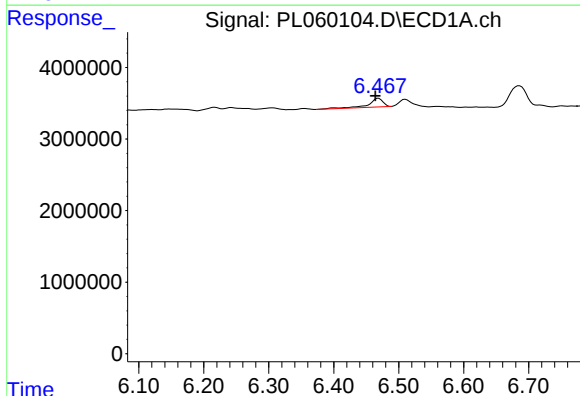


#18 Endrin aldehyde

R.T.: 6.469 min
Delta R.T.: 0.005 min
Response: 1895383
Conc: 1.33 ng/ml

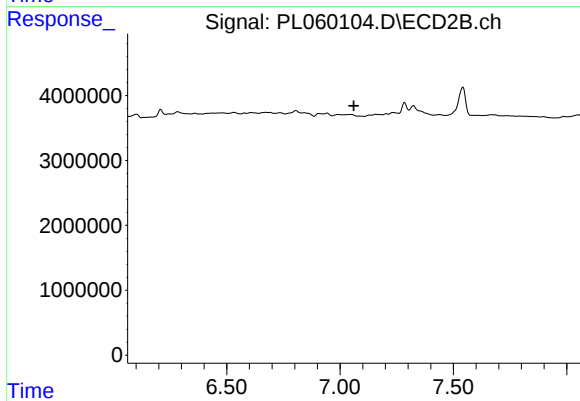

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.060 min
Response: 0
Conc: N.D.

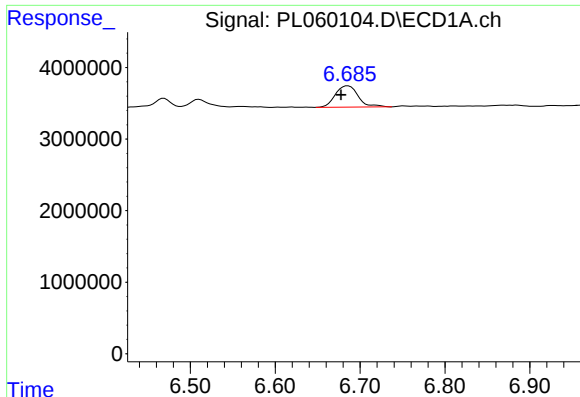

#19 Endosulfan Sulfate


R.T.: 6.686 min
Delta R.T.: 0.008 min
Response: 5580736
Conc: 3.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-04-072120

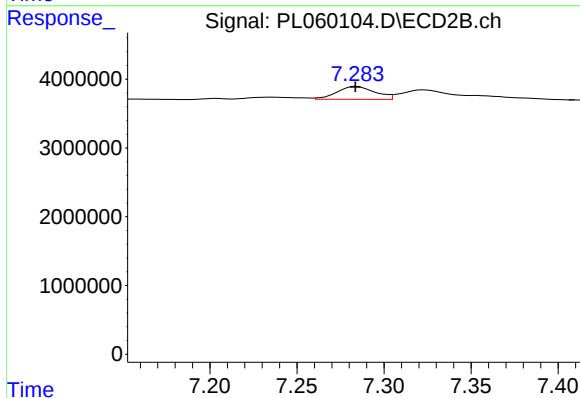


#19 Endosulfan Sulfate

R.T.: 7.285 min
Delta R.T.: 0.000 min
Response: 2842013
Conc: 1.22 ng/ml

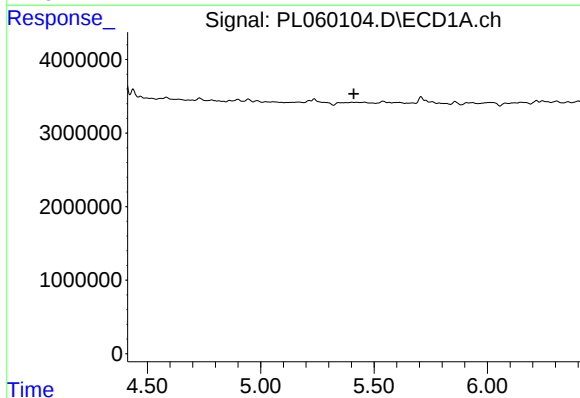


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.411 min
Response: 0
Conc: N.D.

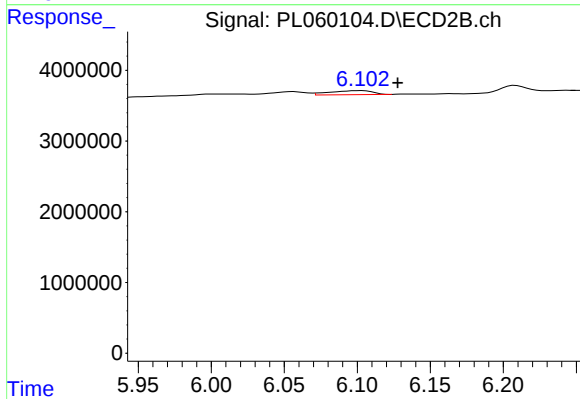

#25 Chlordane-3


R.T.: 6.102 min
Delta R.T.: -0.026 min
Response: 1182058
Conc: 3.06 ng/ml

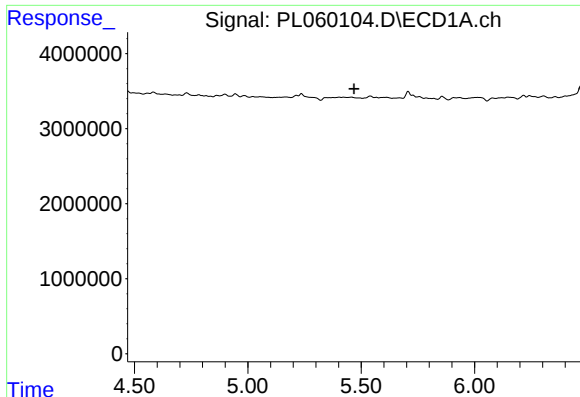

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SU-04-072120

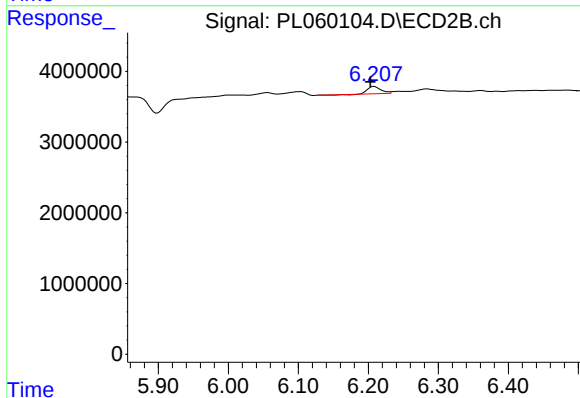


#26 Chlordane-4

R.T.: 6.209 min
Delta R.T.: 0.006 min
Response: 1354397
Conc: 2.93 ng/ml

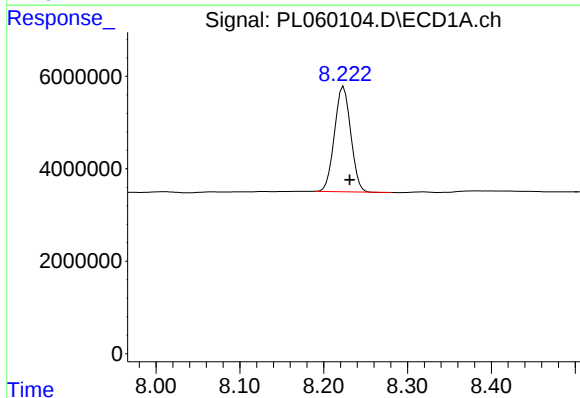

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.007 min
Response: 30543512
Conc: 18.57 ng/ml

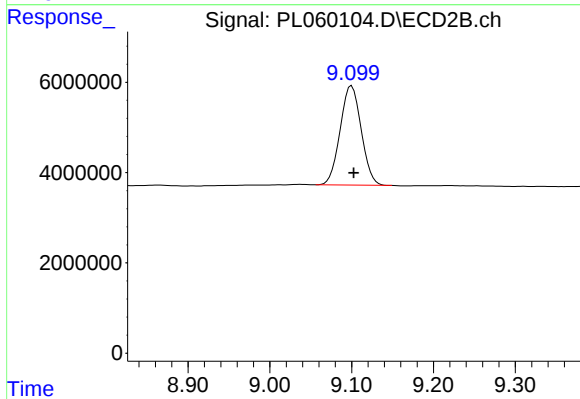

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: -0.003 min
Response: 39258030
Conc: 18.77 ng/ml