

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
 Data File : PL060106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 19:13
 Operator : DD\AJ
 Sample : L3352-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HS-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:53:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.013	36856322	50876070	19.055	19.197
28)	SA Decachlor...	8.223	9.100	33016069	42437227	20.069	20.291
Target Compounds							
5)	MB Aldrin	4.729	0.000	961326	0	0.487	N.D. #
8)	B Heptachlo...	0.000	5.867f	0	11281613	N.D.	4.189 #
9)	A Endosulfan I	0.000	6.274f	0	15338226	N.D.	5.750 #
11)	B alpha-Chl...	0.000	6.172f	0	12062419	N.D.	4.219 #
12)	B 4,4'-DDE	0.000	6.385f	0	8267793	N.D.	3.089 #
13)	MA Dieldrin	5.766	0.000	1534221	0	0.869	N.D. #
15)	B Endosulfa...	0.000	6.944	0	1279572	N.D.	0.509 #
23)	Chlordane-1	4.327	0.000	818190	0	13.355	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
Data File : PL060106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 19:13
Operator : DD\AJ
Sample : L3352-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HS-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:53:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

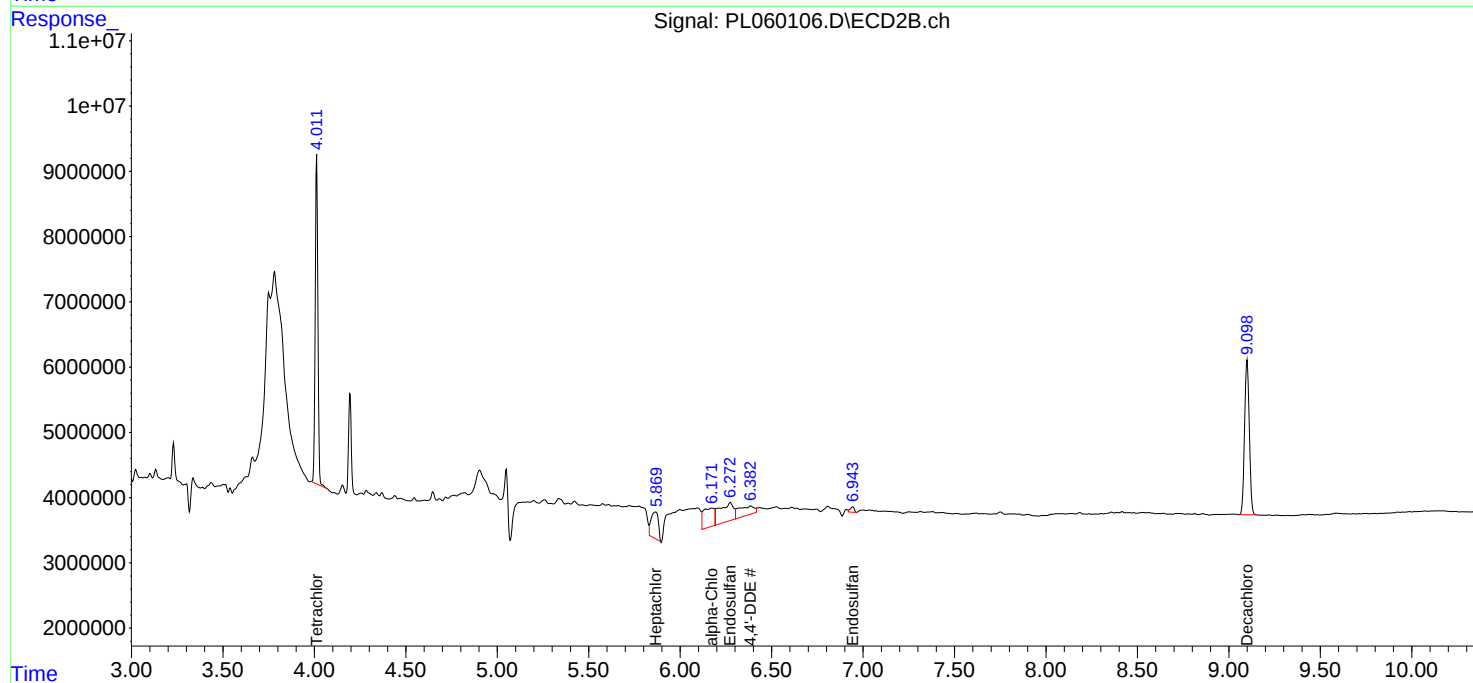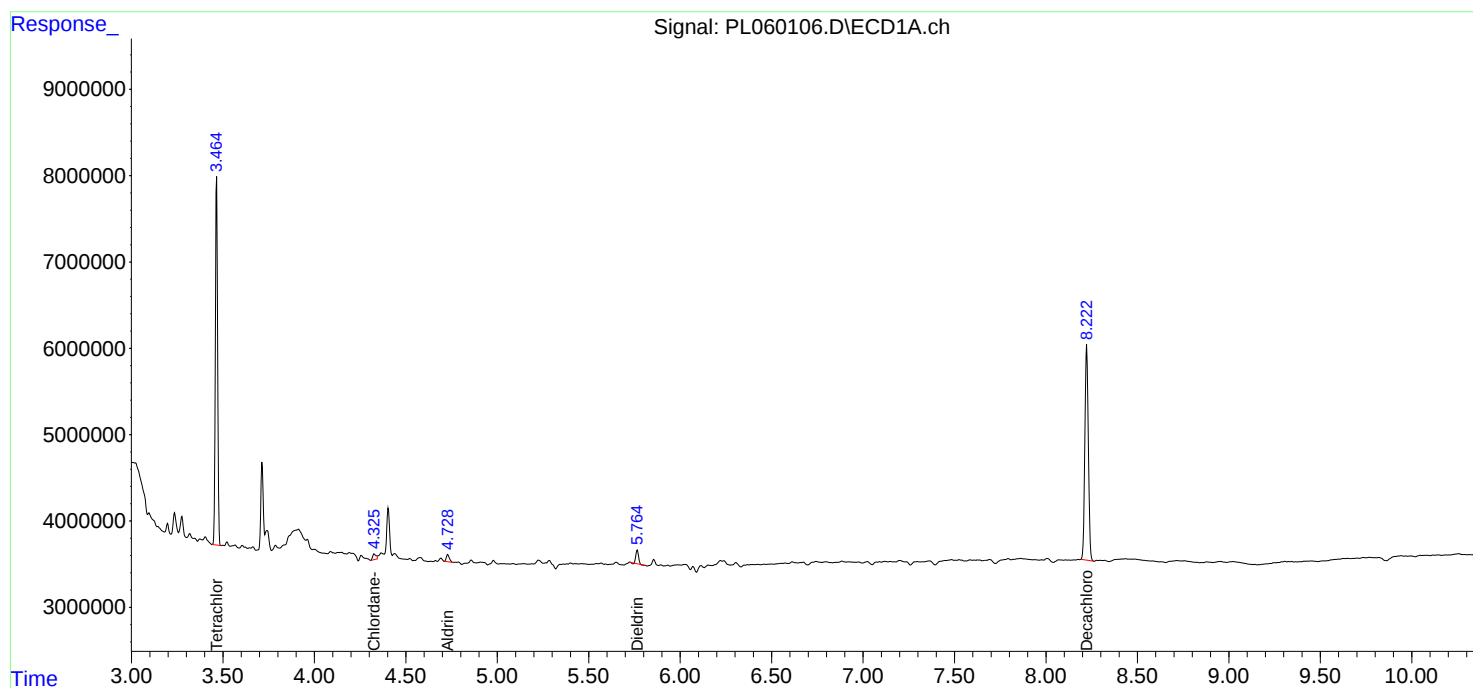


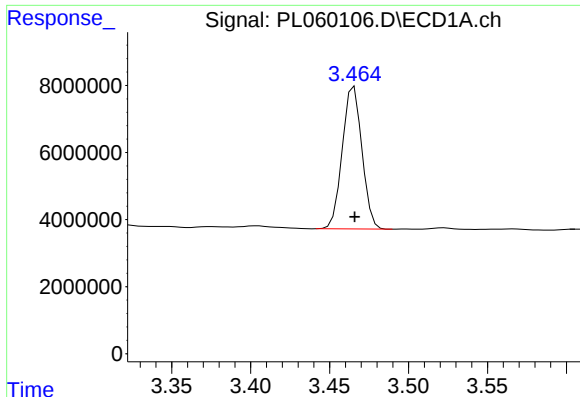

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 36856322
Conc: 19.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
HS-01

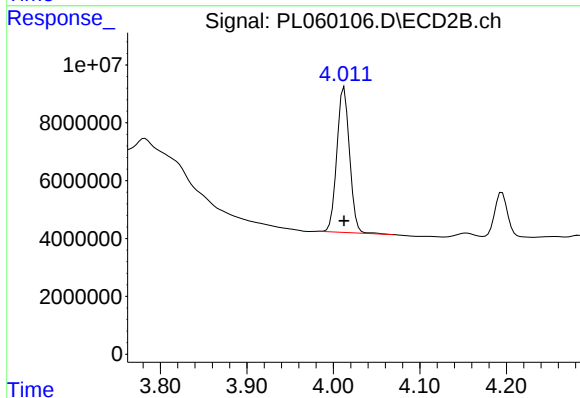


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 50876070
Conc: 19.20 ng/ml

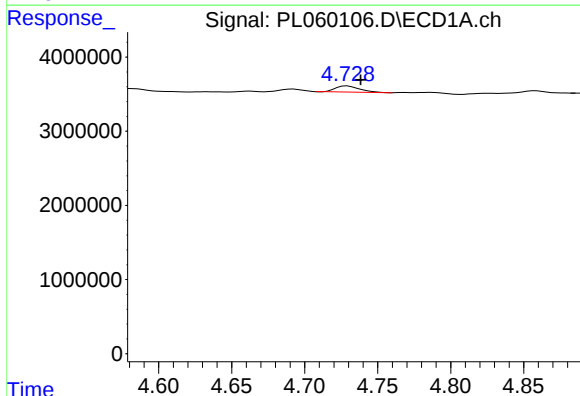


#5 Aldrin

R.T.: 4.729 min
Delta R.T.: -0.009 min
Response: 961326
Conc: 0.49 ng/ml

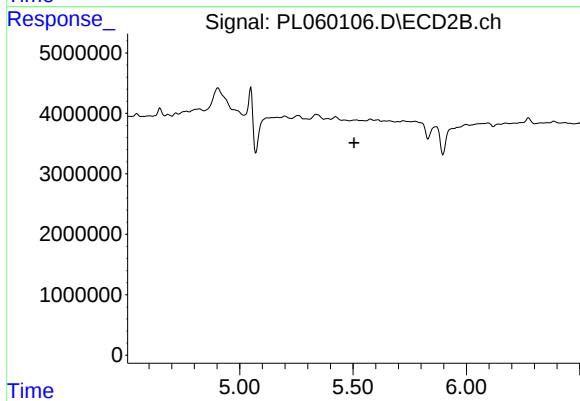

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.505 min
Response: 0
Conc: N.D.

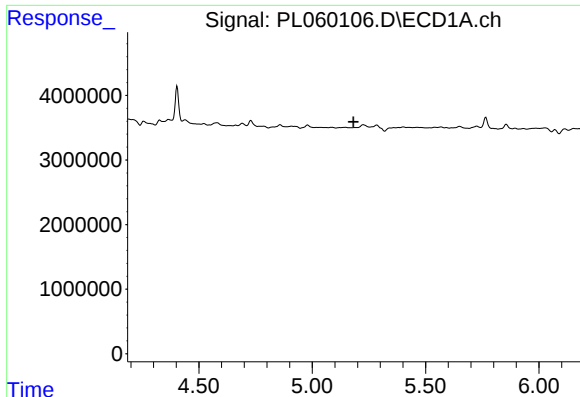

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HS-01

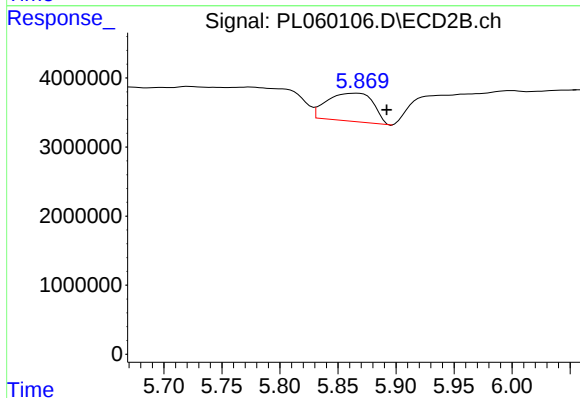


#8 Heptachlor epoxide

R.T.: 5.867 min
Delta R.T.: -0.025 min
Response: 11281613
Conc: 4.19 ng/ml

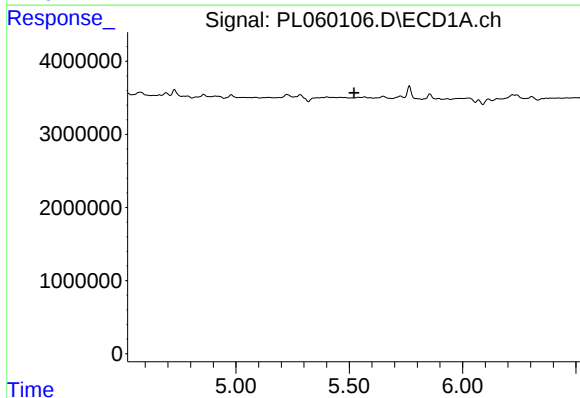


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.522 min
Response: 0
Conc: N.D.

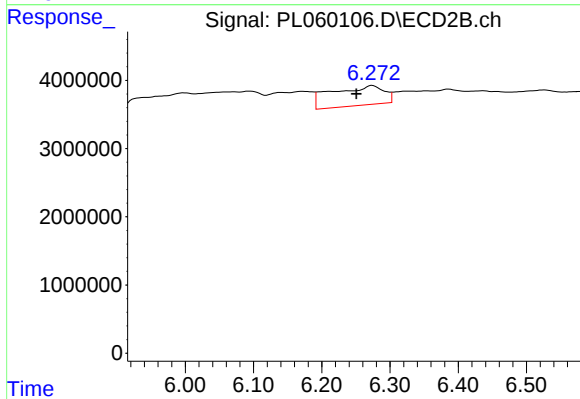

#9 Endosulfan I


R.T.: 6.274 min
Delta R.T.: 0.024 min
Response: 15338226
Conc: 5.75 ng/ml

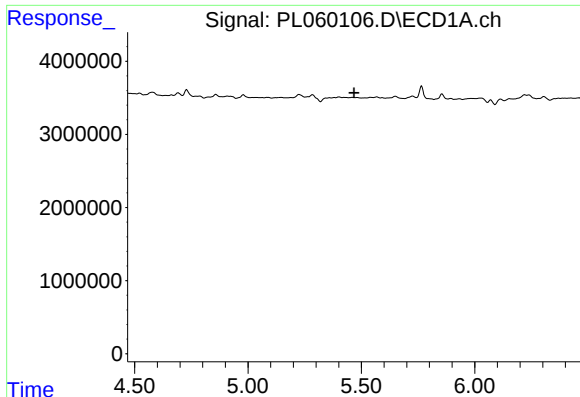

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HS-01

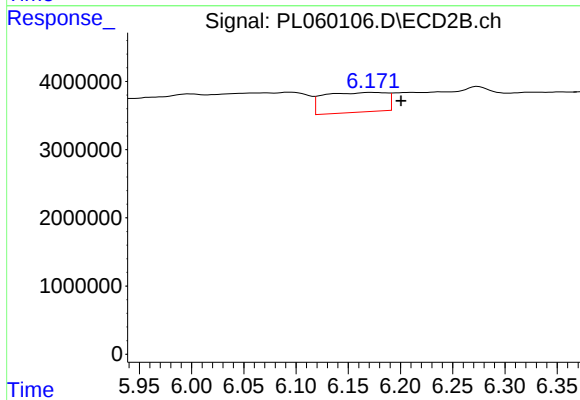


#11 alpha-Chlordane

R.T.: 6.172 min
Delta R.T.: -0.028 min
Response: 12062419
Conc: 4.22 ng/ml

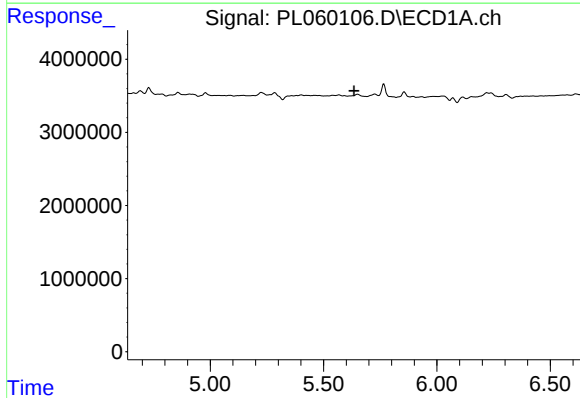


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.634 min
Response: 0
Conc: N.D.

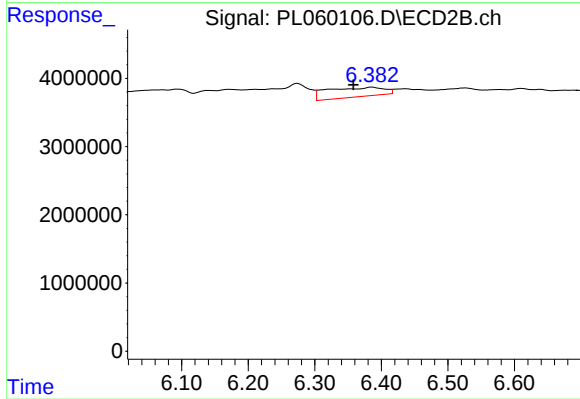

#12 4,4'-DDE


R.T.: 6.385 min
Delta R.T.: 0.027 min
Response: 8267793
Conc: 3.09 ng/ml

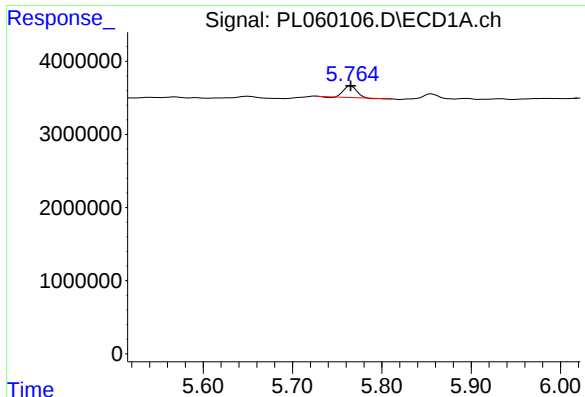

#13 Dieldrin


R.T.: 5.766 min
Delta R.T.: 0.000 min
Response: 1534221
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
HS-01

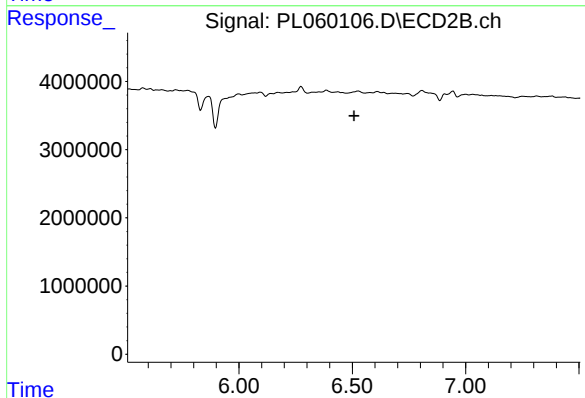


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.508 min
Response: 0
Conc: N.D.

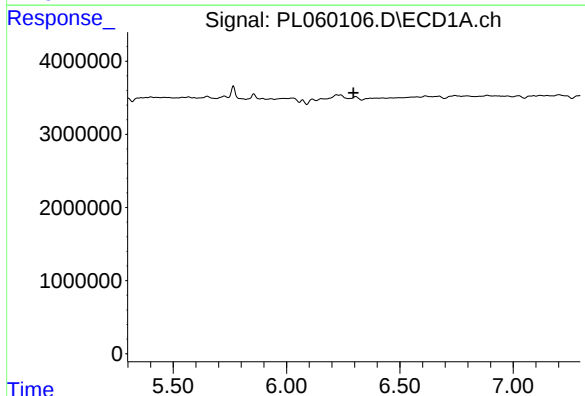


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.296 min
Response: 0
Conc: N.D.

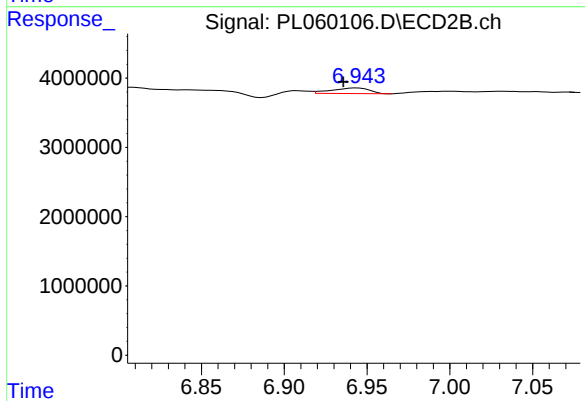

#15 Endosulfan II


R.T.: 6.944 min
Delta R.T.: 0.009 min
Response: 1279572
Conc: 0.51 ng/ml

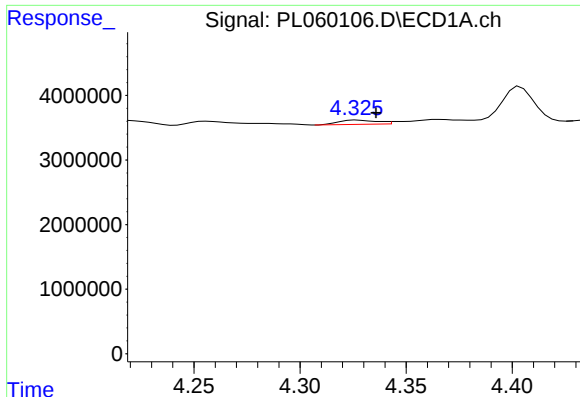

#23 Chlordane-1


R.T.: 4.327 min
Delta R.T.: -0.009 min
Response: 818190
Conc: 13.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
HS-01

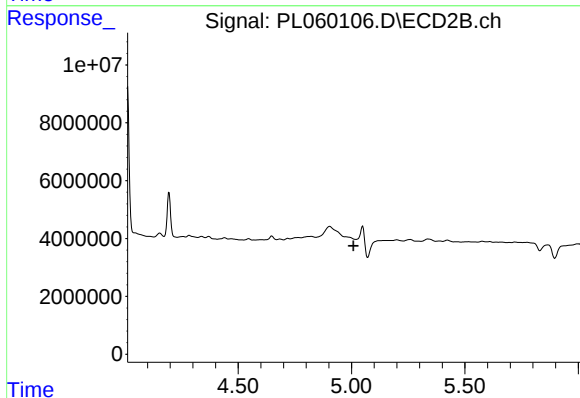


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.009 min
Response: 0
Conc: N.D.

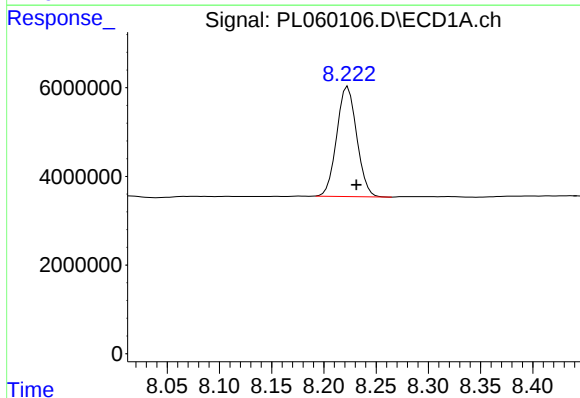

#28 Decachlorobiphenyl

R.T.: 8.223 min
Delta R.T.: -0.008 min
Response: 33016069
Conc: 20.07 ng/ml

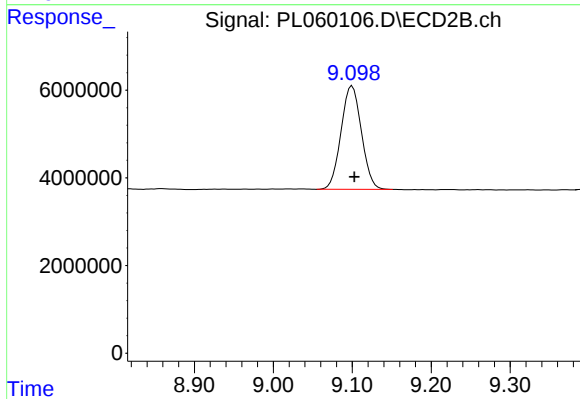

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: -0.003 min
Response: 42437227
Conc: 20.29 ng/ml