

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
 Data File : PL060115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 21:21
 Operator : DD\AJ
 Sample : L3370-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3-GW

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:55:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.013	35857036	49032534	18.538	18.501
28)	SA Decachlor...	8.224	9.101	27174168	34407034	16.518	16.452
Target Compounds							
2)	A alpha-BHC	0.000	4.420f	0	4087898	N.D.	1.059 #
3)	MA gamma-BHC...	4.184	0.000	48626220	0	19.690	N.D. #
4)	MA Heptachlor	0.000	5.202	0	982130	N.D.	0.292 #
5)	MB Aldrin	0.000	5.533f	0	1388188	N.D.	0.446 #
11)	B alpha-Chl...	0.000	6.196	0	3504942	N.D.	1.226 #
15)	B Endosulfa...	0.000	6.946	0	3212251	N.D.	1.279 #
17)	MA 4,4'-DDT	0.000	7.147	0	4548017	N.D.	2.310 #
18)	B Endrin al...	0.000	7.055	0	3235120	N.D.	1.490 #
19)	B Endosulfa...	6.653f	0.000	1821932	0	1.108	N.D. #
26)	Chlordane-4	0.000	6.196	0	3504942	N.D.	7.572 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
Data File : PL060115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 21:21
Operator : DD\AJ
Sample : L3370-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-3-GW

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:55:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

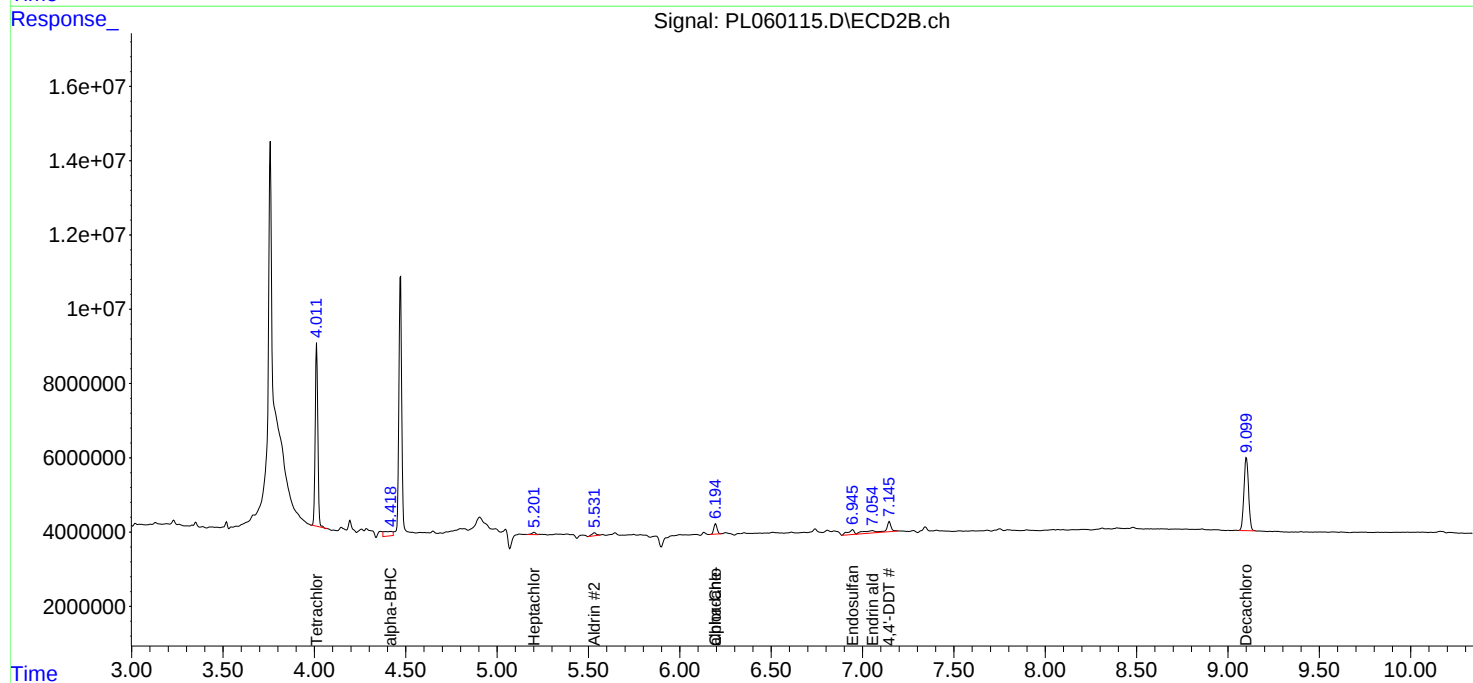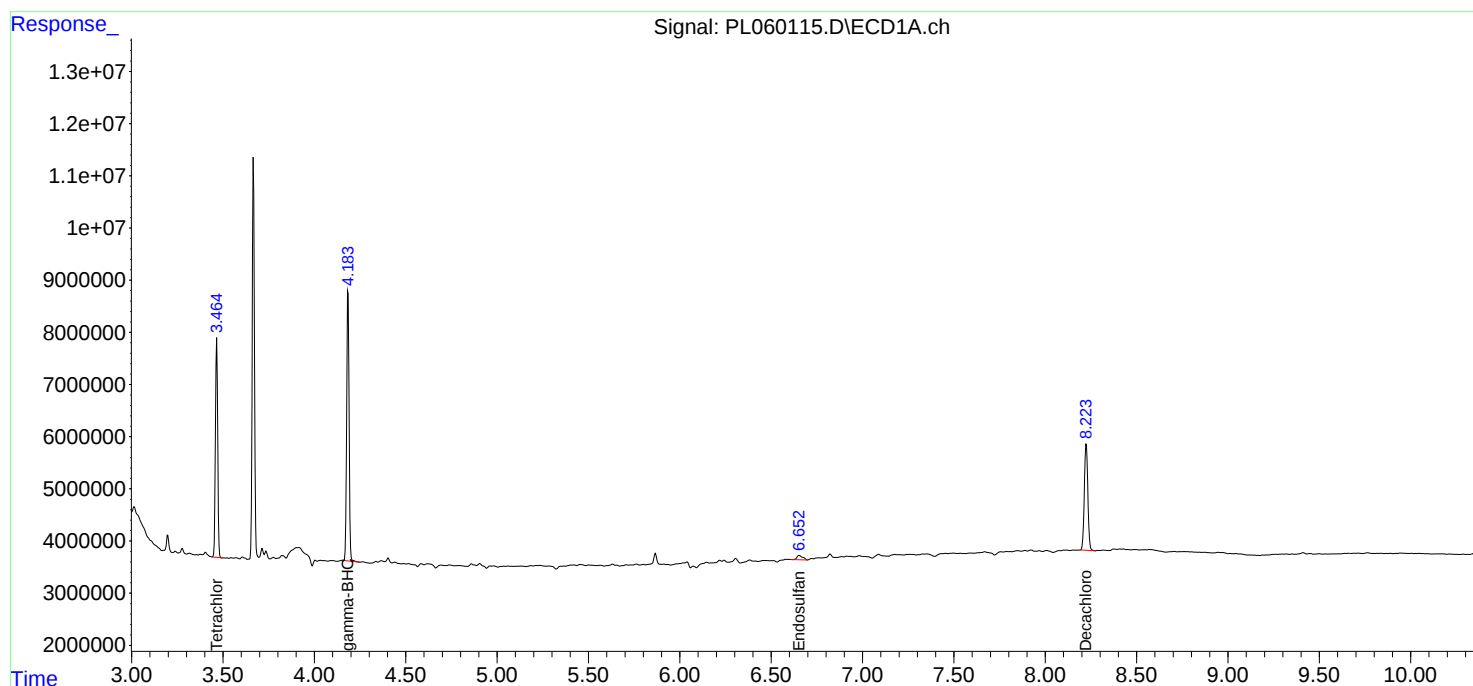


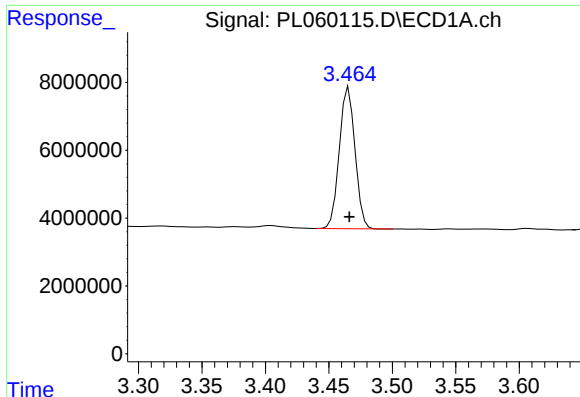

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 35857036
Conc: 18.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-GW

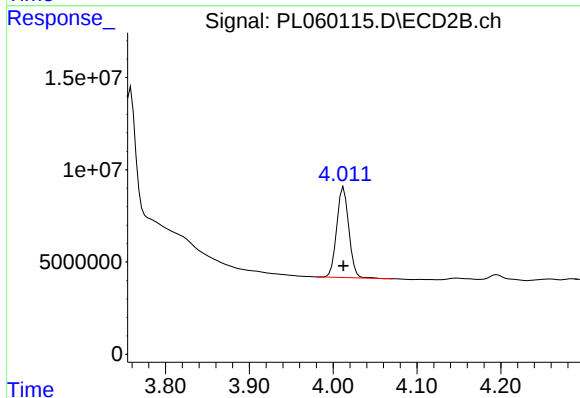


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 49032534
Conc: 18.50 ng/ml

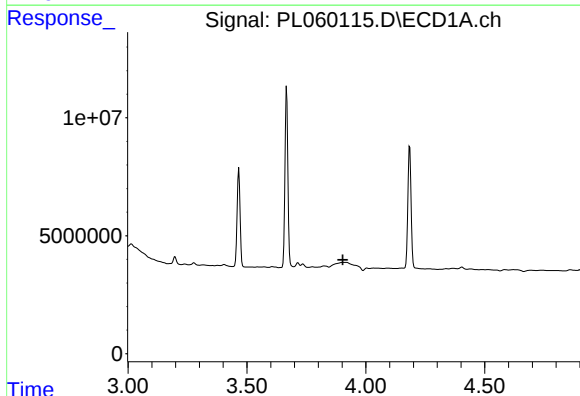


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.903 min
Response: 0
Conc: N.D.

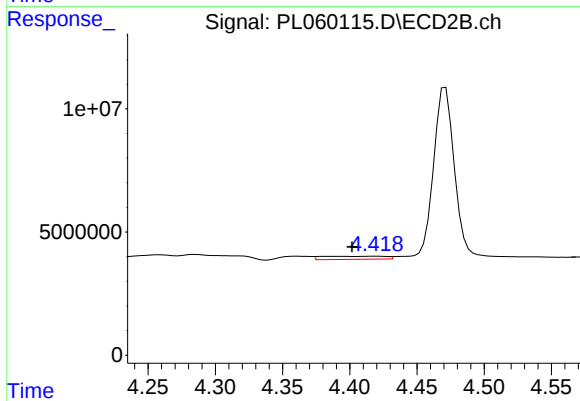

#2 alpha-BHC


R.T.: 4.420 min
Delta R.T.: 0.018 min
Response: 4087898
Conc: 1.06 ng/ml

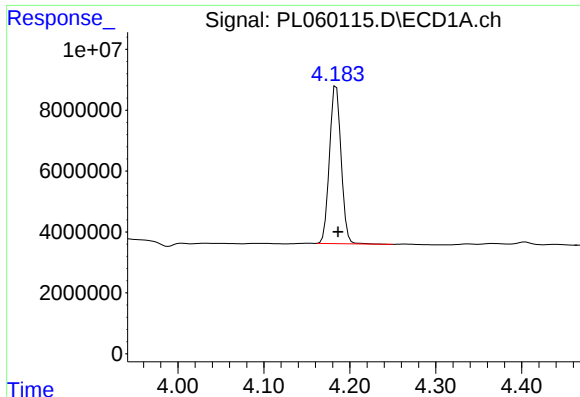

#3 gamma-BHC (Lindane)


R.T.: 4.184 min
Delta R.T.: -0.002 min
Response: 48626220
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-GW

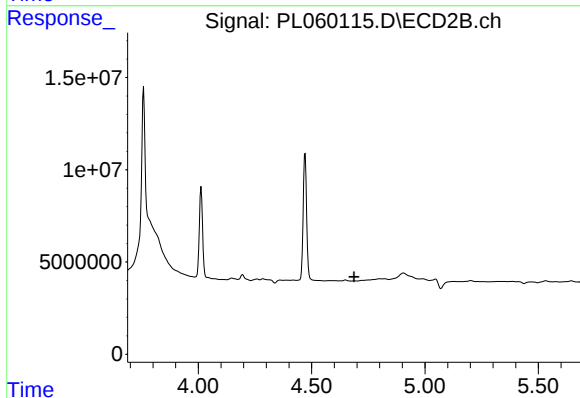


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.687 min
Response: 0
Conc: N.D.

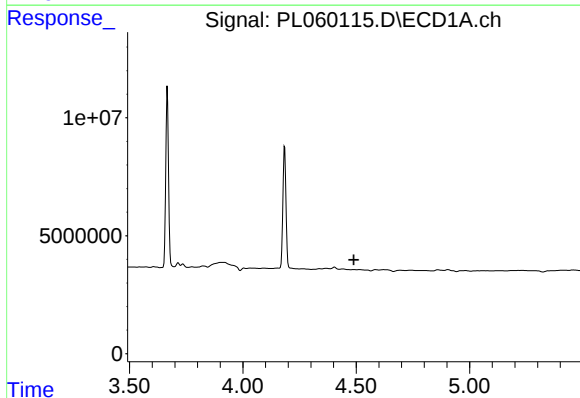


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

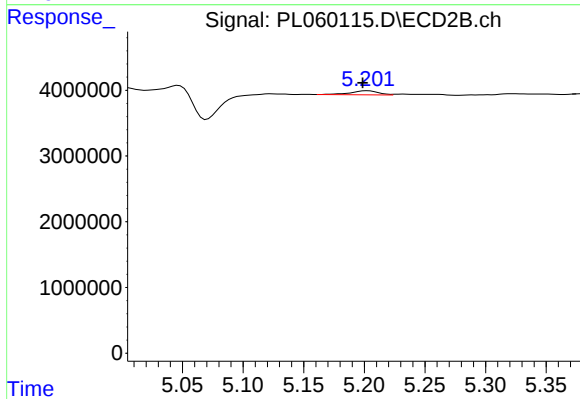

#4 Heptachlor


R.T.: 5.202 min
Delta R.T.: 0.004 min
Response: 982130
Conc: 0.29 ng/ml

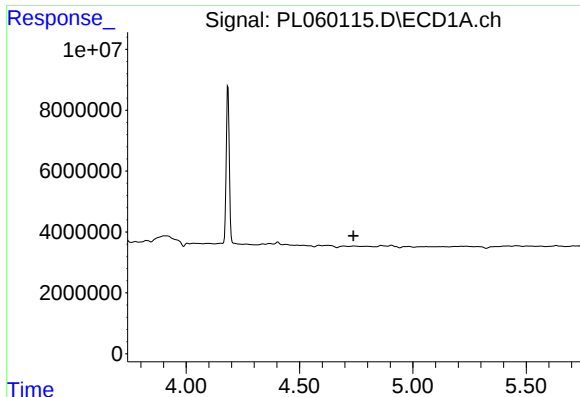

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3-GW

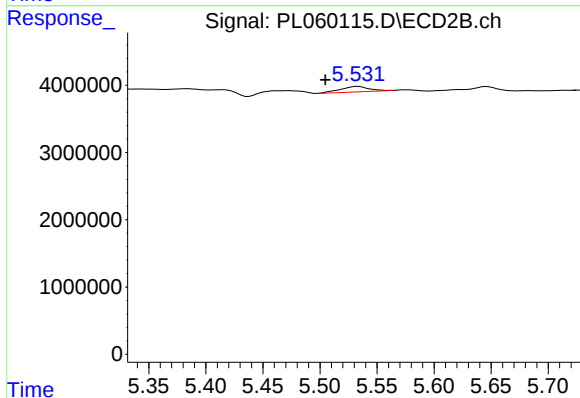


#5 Aldrin

R.T.: 5.533 min
Delta R.T.: 0.029 min
Response: 1388188
Conc: 0.45 ng/ml

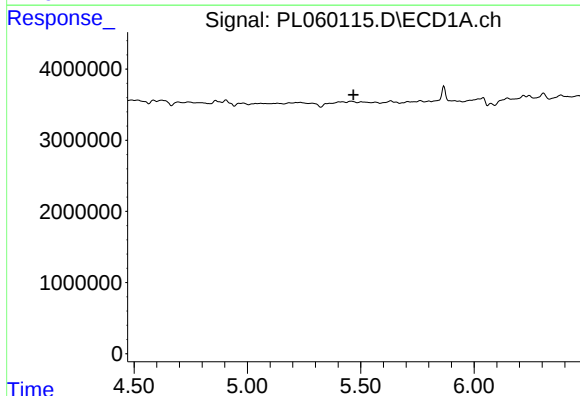


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.469 min
Response: 0
Conc: N.D.

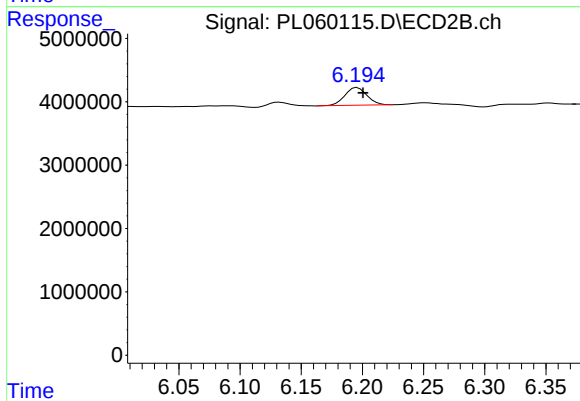

#11 alpha-Chlordane


R.T.: 6.196 min
Delta R.T.: -0.005 min
Response: 3504942
Conc: 1.23 ng/ml

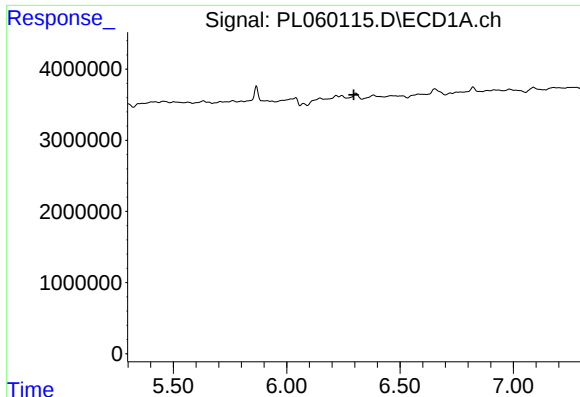

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3-GW

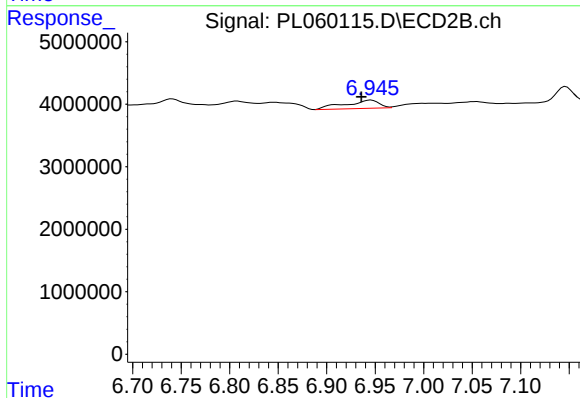


#15 Endosulfan II

R.T.: 6.946 min
Delta R.T.: 0.010 min
Response: 3212251
Conc: 1.28 ng/ml

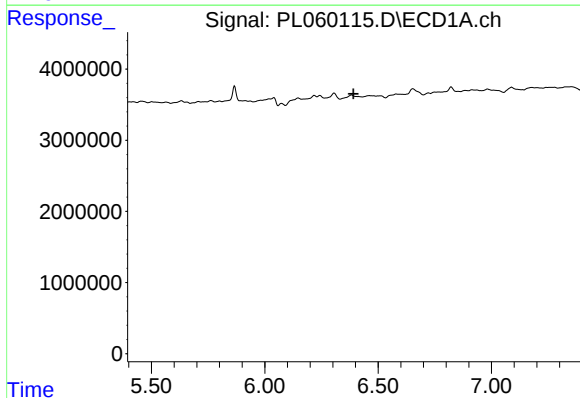


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.392 min
Response: 0
Conc: N.D.

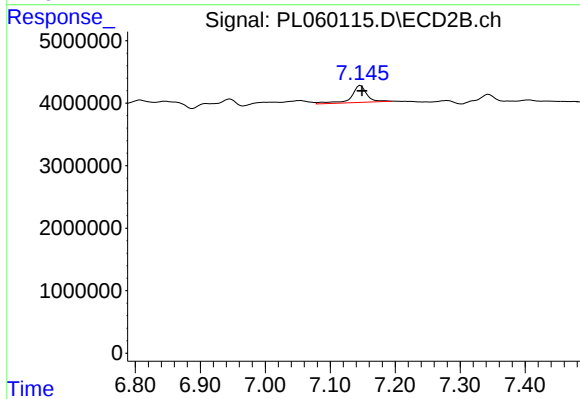

#17 4,4'-DDT


R.T.: 7.147 min
Delta R.T.: -0.002 min
Response: 4548017
Conc: 2.31 ng/ml

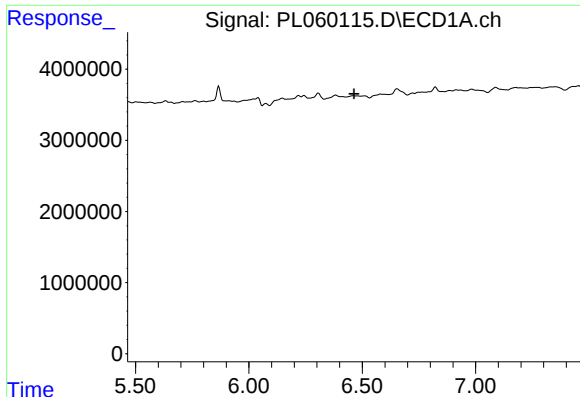

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3-GW

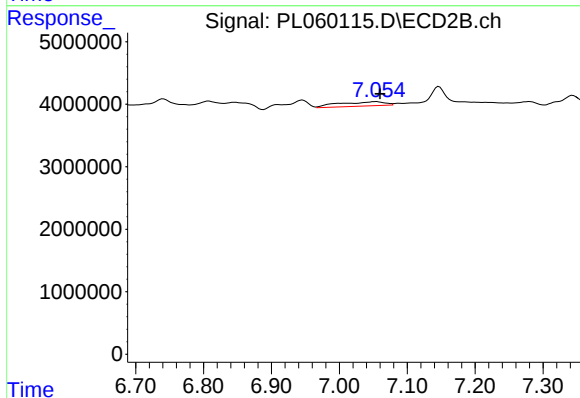


#18 Endrin aldehyde

R.T.: 7.055 min
Delta R.T.: -0.005 min
Response: 3235120
Conc: 1.49 ng/ml

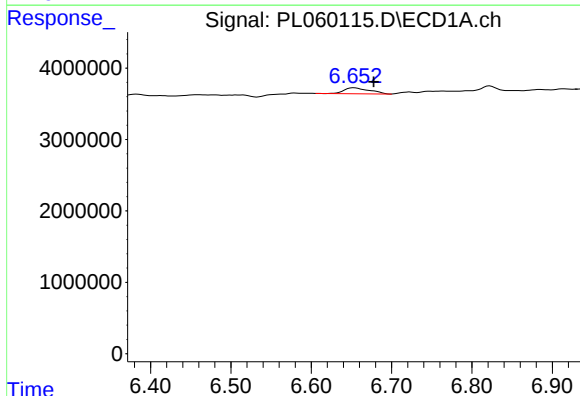


#19 Endosulfan Sulfate

R.T.: 6.653 min
Delta R.T.: -0.025 min
Response: 1821932
Conc: 1.11 ng/ml

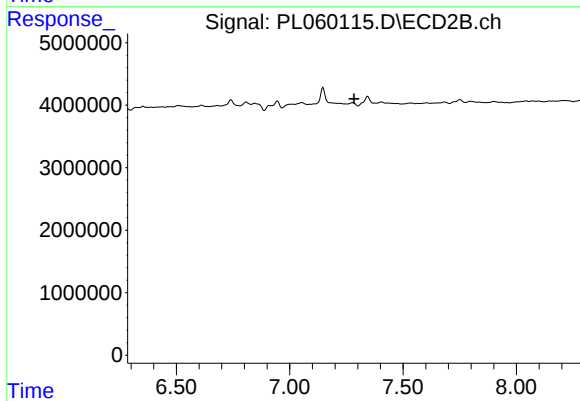

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

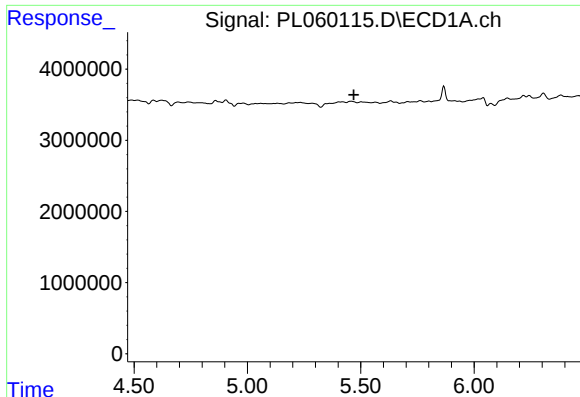

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3-GW

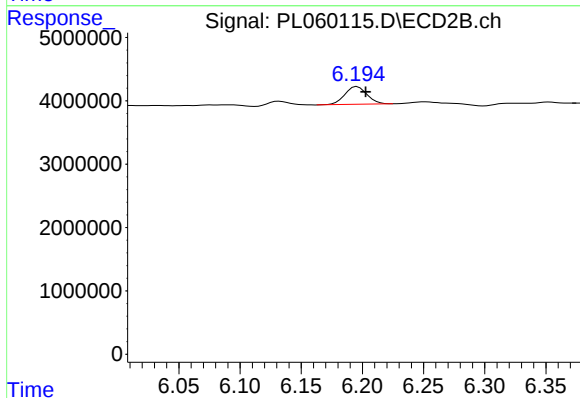


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: -0.007 min
Response: 3504942
Conc: 7.57 ng/ml

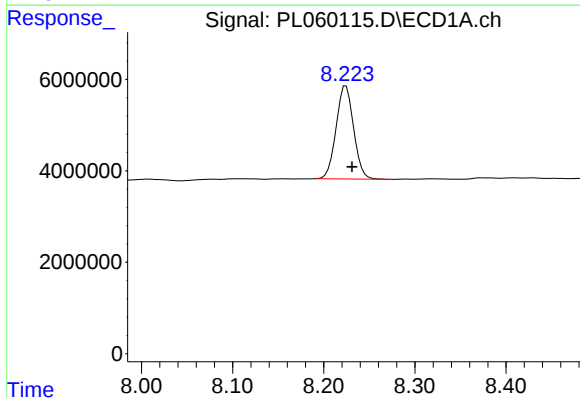

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.007 min
Response: 27174168
Conc: 16.52 ng/ml

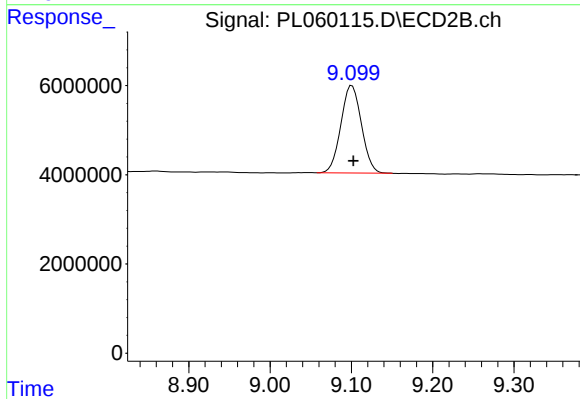

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: -0.002 min
Response: 34407034
Conc: 16.45 ng/ml