

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
 Data File : PL060116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 21:35
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:55:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.013	37418557	50053452	19.345	18.887
28)	SA Decachlor...	8.225	9.102	29495994	37201782	17.930	17.788
Target Compounds							
4)	MA Heptachlor	0.000	5.203	0	361759	N.D.	0.108 #
8)	B Heptachlo...	0.000	5.883	0	10322376	N.D.	3.833 #
9)	A Endosulfan I	0.000	6.280f	0	37046179	N.D.	13.889 #
12)	B 4,4'-DDE	0.000	6.340f	0	14435483	N.D.	5.393 #
13)	MA Dieldrin	0.000	6.498	0	9917346	N.D.	3.585 #
16)	A 4,4'-DDD	0.000	6.841	0	2342567	N.D.	1.021 #
18)	B Endrin al...	0.000	7.030f	0	1472766	N.D.	0.678 #
27)	Chlordane-5	0.000	7.030f	0	1472766	N.D.	18.963 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072220\
Data File : PL060116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 21:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:55:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

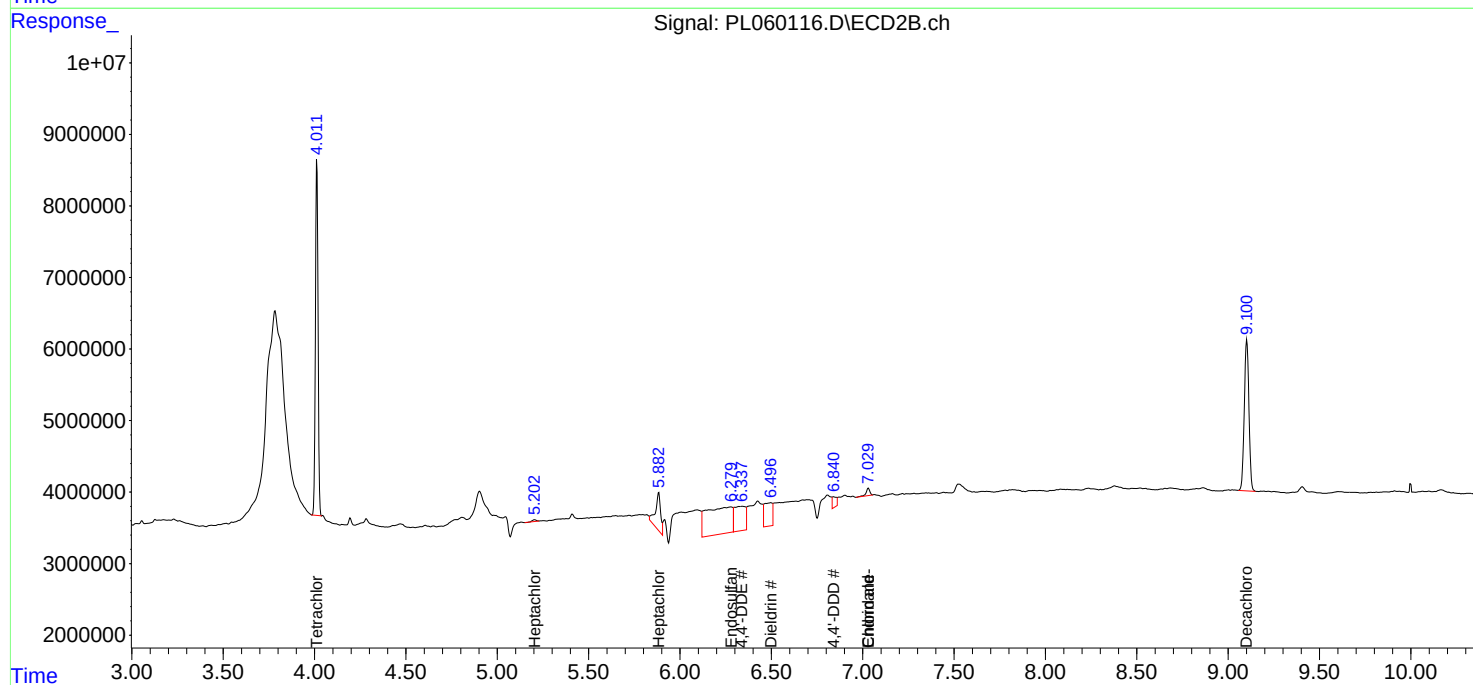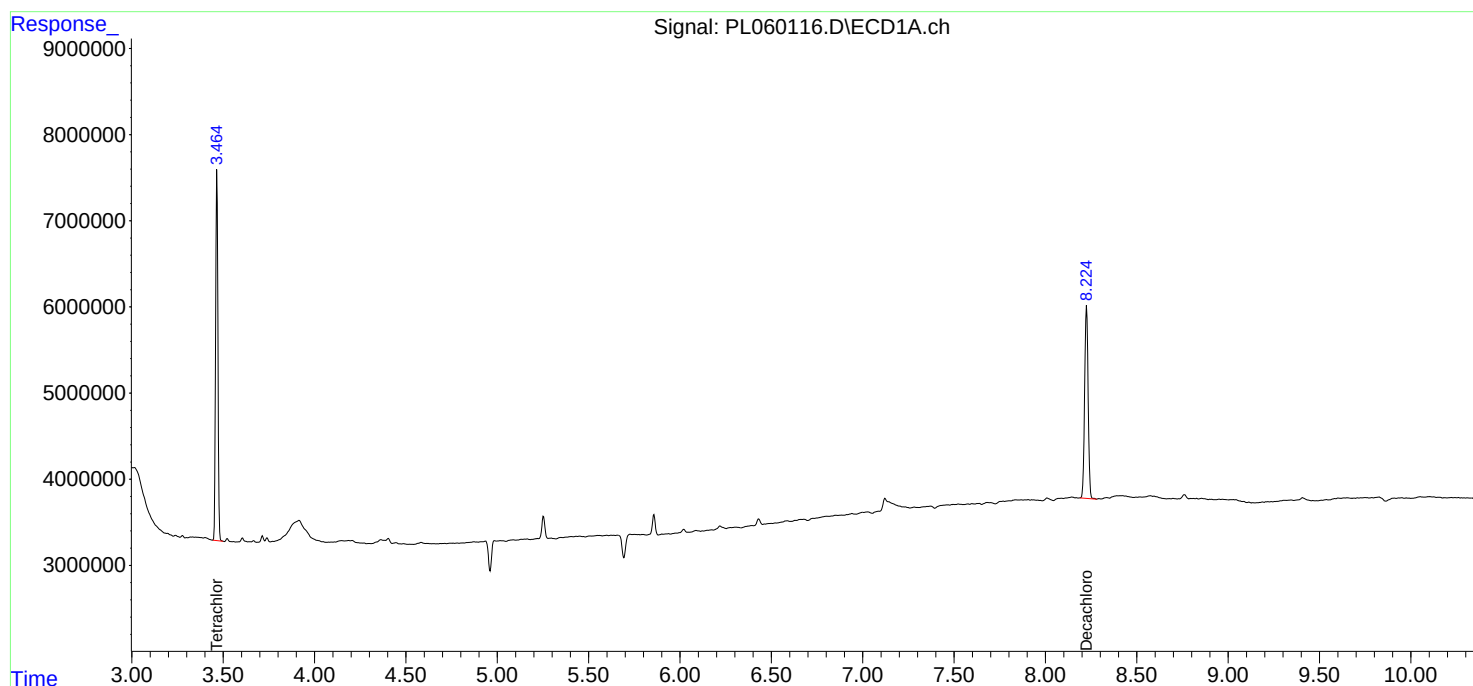


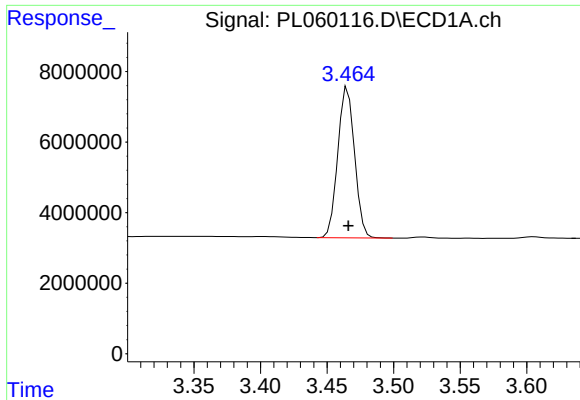

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 37418557
Conc: 19.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

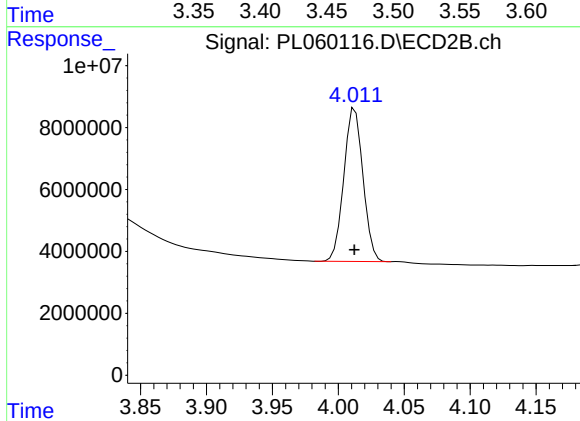


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 50053452
Conc: 18.89 ng/ml

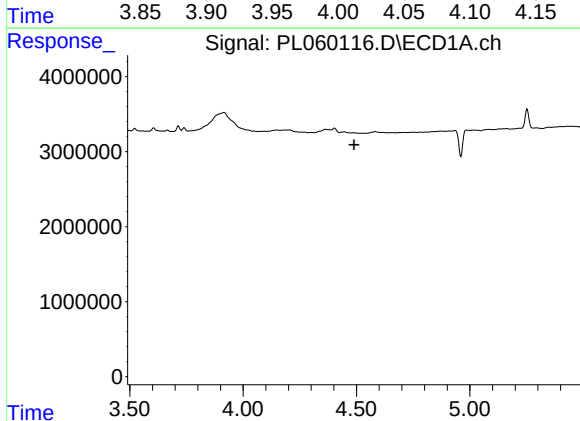


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

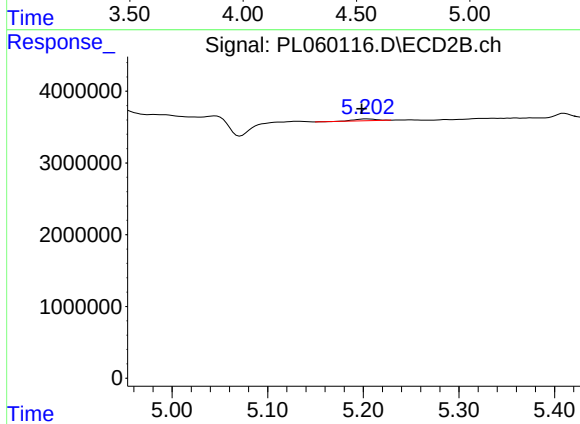

#4 Heptachlor


R.T.: 5.203 min
Delta R.T.: 0.005 min
Response: 361759
Conc: 0.11 ng/ml

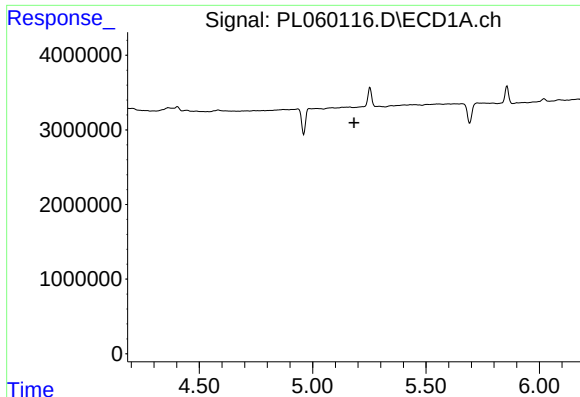

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

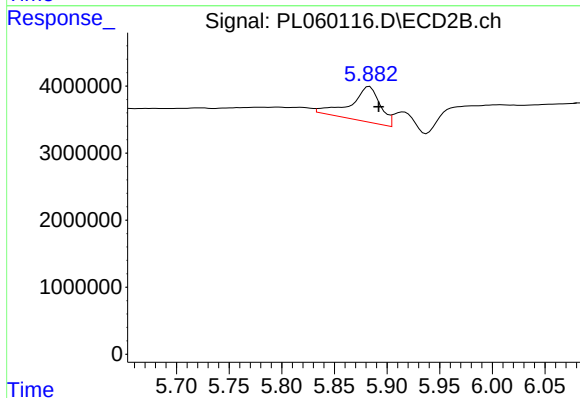


#8 Heptachlor epoxide

R.T.: 5.883 min
Delta R.T.: -0.009 min
Response: 10322376
Conc: 3.83 ng/ml

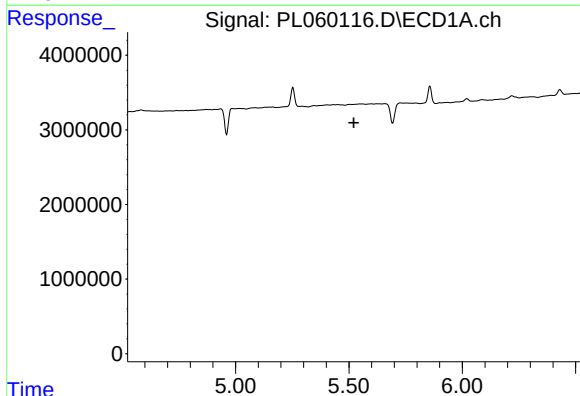


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.522 min
Response: 0
Conc: N.D.

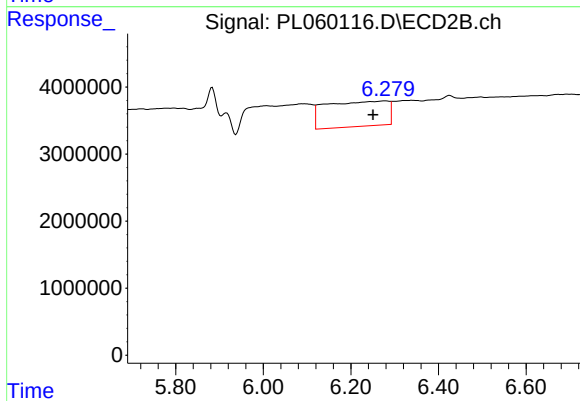

#9 Endosulfan I


R.T.: 6.280 min
Delta R.T.: 0.029 min
Response: 37046179
Conc: 13.89 ng/ml

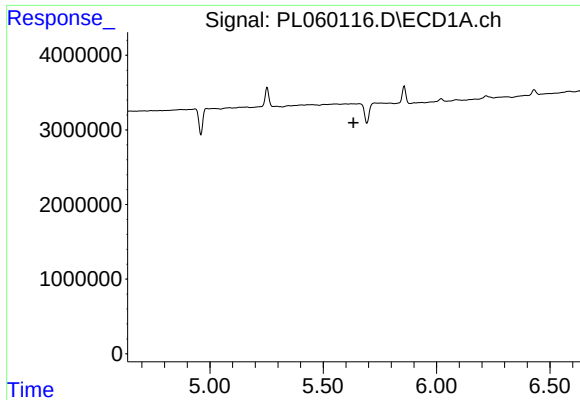

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

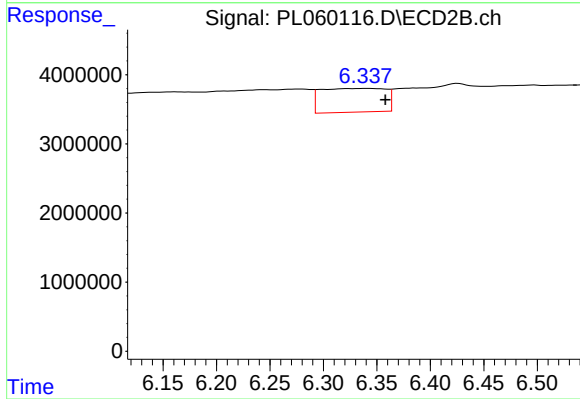


#12 4,4'-DDE

R.T.: 6.340 min
Delta R.T.: -0.018 min
Response: 14435483
Conc: 5.39 ng/ml

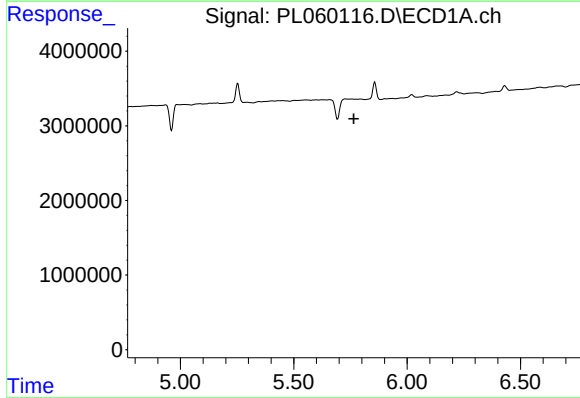


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.765 min
Response: 0
Conc: N.D.

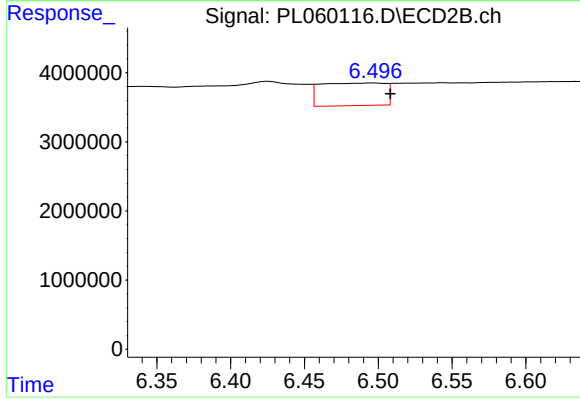

#13 Dieldrin


R.T.: 6.498 min
Delta R.T.: -0.011 min
Response: 9917346
Conc: 3.59 ng/ml

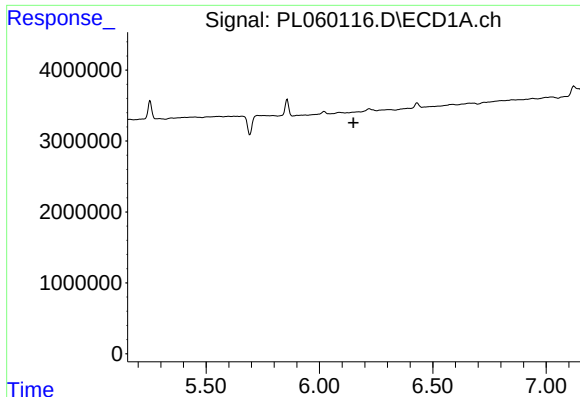

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

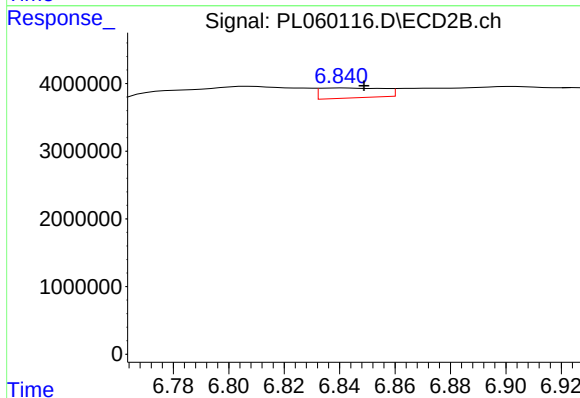


#16 4,4'-DDD

R.T.: 6.841 min
Delta R.T.: -0.008 min
Response: 2342567
Conc: 1.02 ng/ml

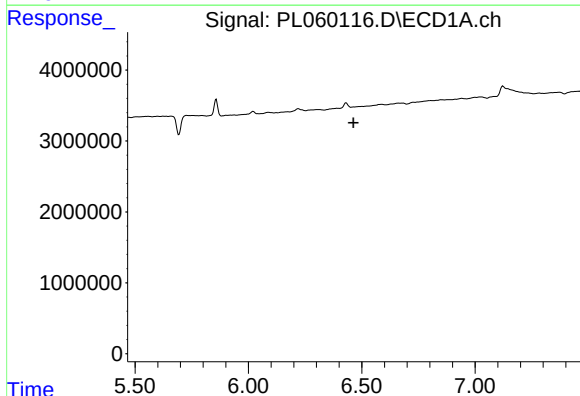


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.464 min
Response: 0
Conc: N.D.

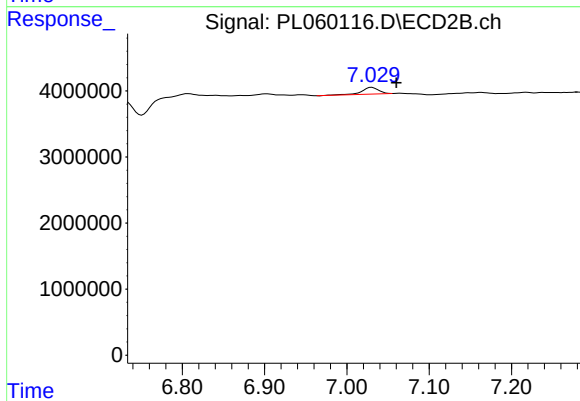

#18 Endrin aldehyde


R.T.: 7.030 min
Delta R.T.: -0.030 min
Response: 1472766
Conc: 0.68 ng/ml

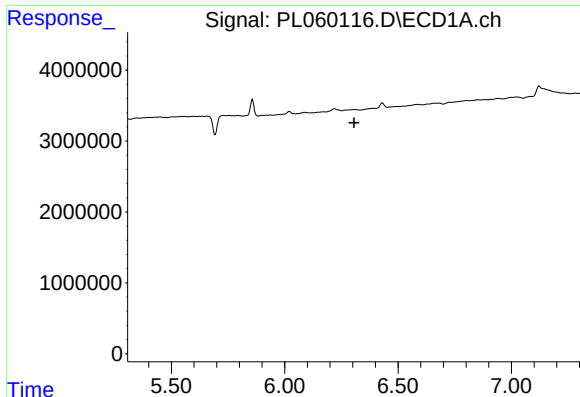

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

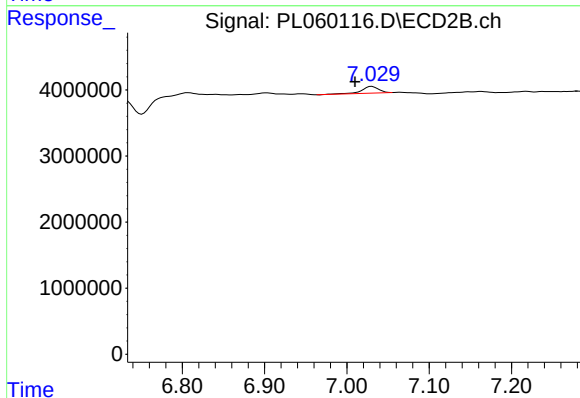


#27 Chlordane-5

R.T.: 7.030 min
Delta R.T.: 0.021 min
Response: 1472766
Conc: 18.96 ng/ml

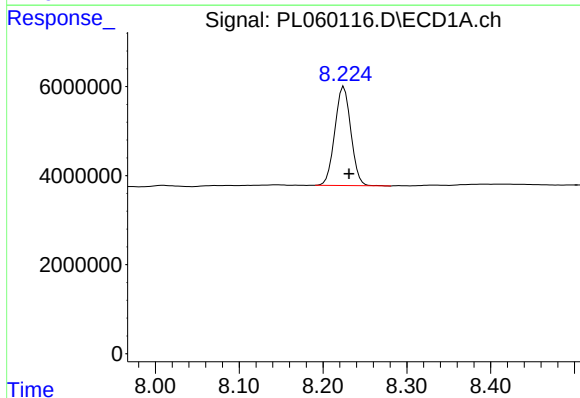

#28 Decachlorobiphenyl

R.T.: 8.225 min
Delta R.T.: -0.006 min
Response: 29495994
Conc: 17.93 ng/ml

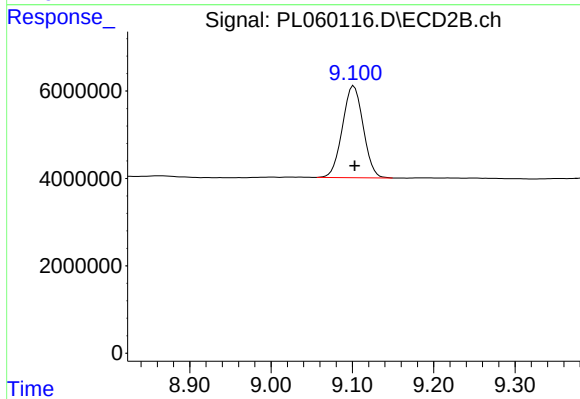

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: 0.000 min
Response: 37201782
Conc: 17.79 ng/ml