

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072221\
 Data File : PL068375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2021 13:06
 Operator : AR\AJ
 Sample : PB137780BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:13:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.643	5.570	8065350	18121781	18.792	17.759
28)	SA Decachlor...	10.420	11.493	12186818	18238877	21.669	20.447
Target Compounds							
15)	B Endosulfa...	0.000	9.217f	0	262167	N.D.	0.289 #
23)	Chlordane-1	0.000	6.980f	0	182157	N.D.	4.497 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072221\
Data File : PL068375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2021 13:06
Operator : AR\AJ
Sample : PB137780BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:13:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

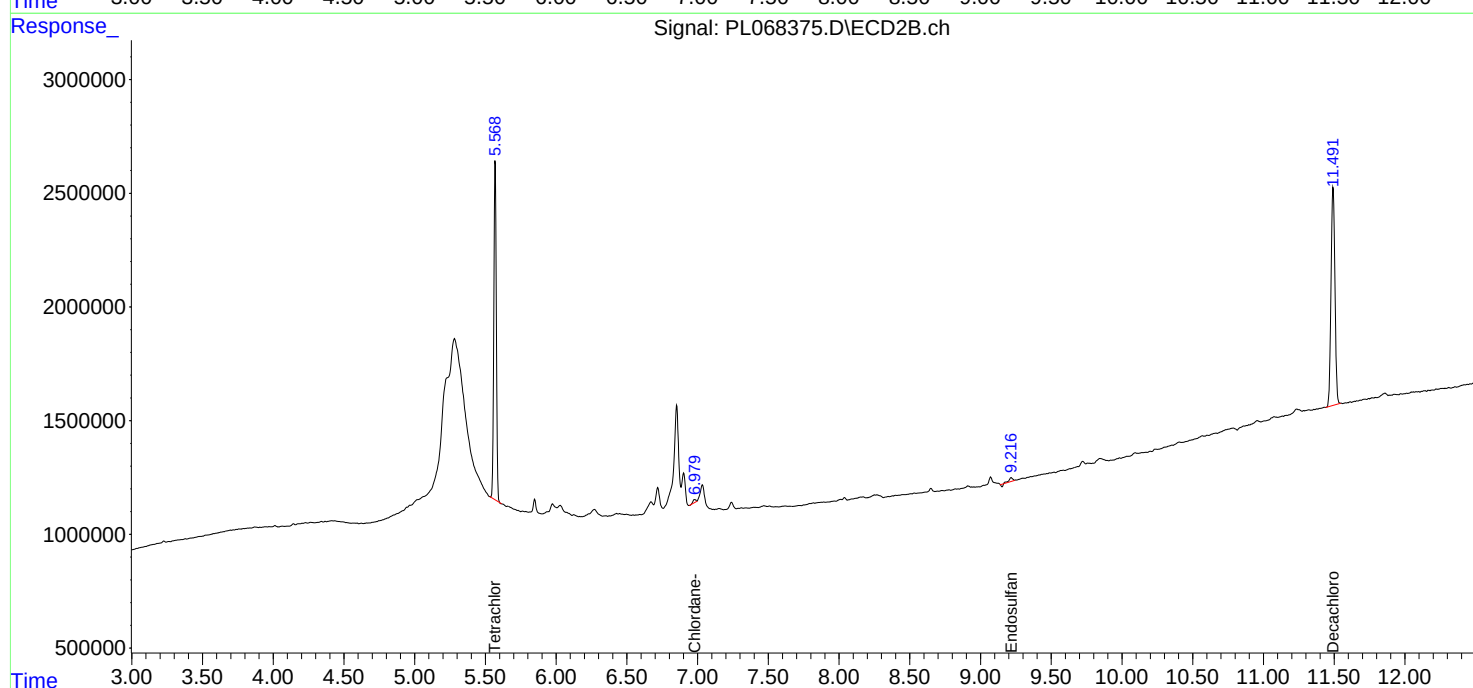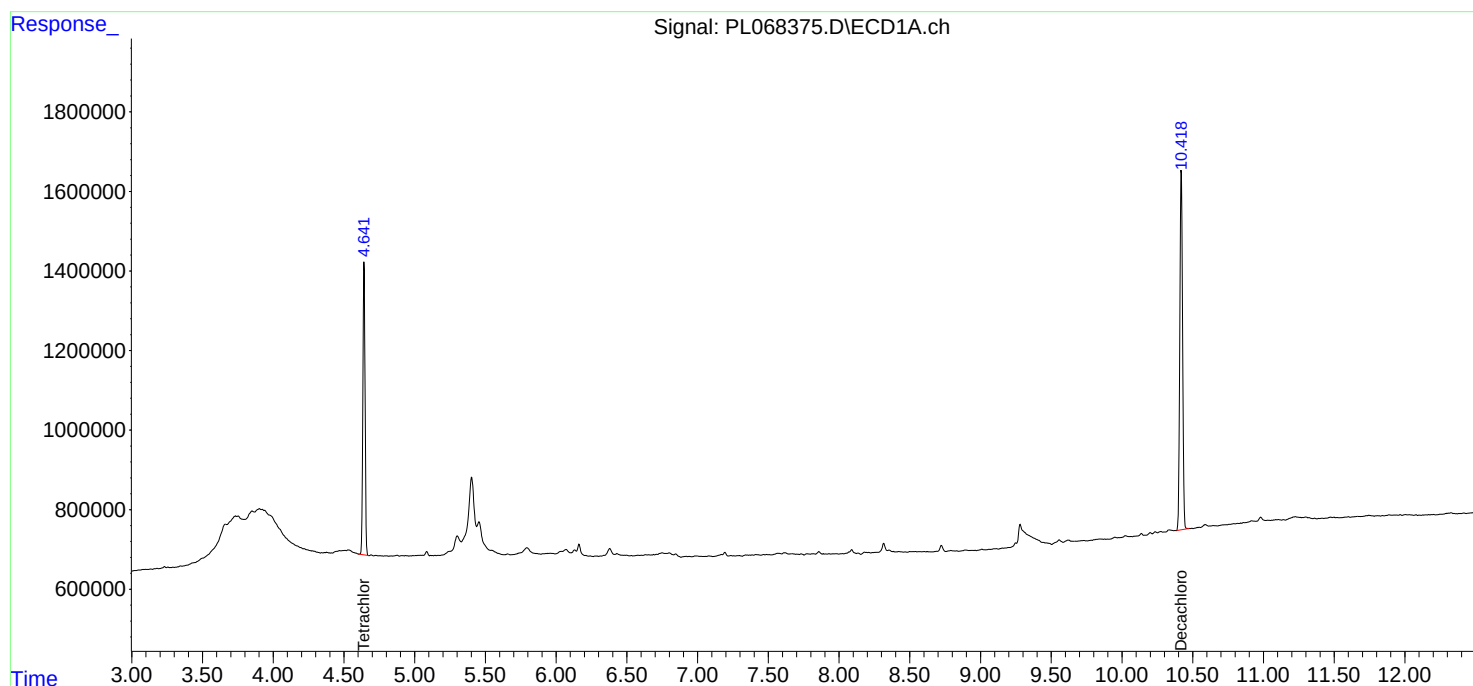


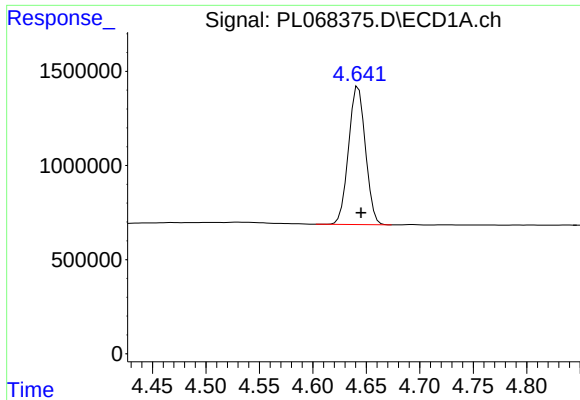

#1 Tetrachloro-m-xylene


R.T.: 4.643 min
Delta R.T.: -0.002 min
Response: 8065350
Conc: 18.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

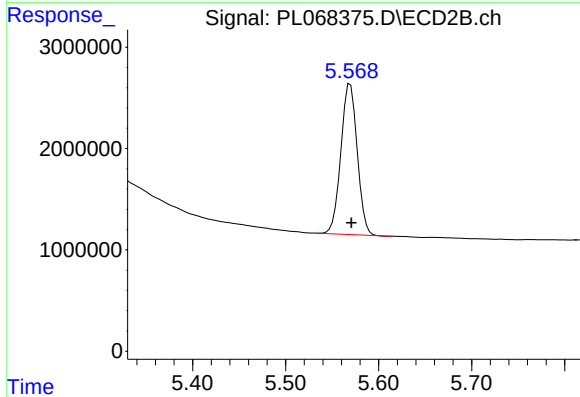


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: -0.001 min
Response: 18121781
Conc: 17.76 ng/ml

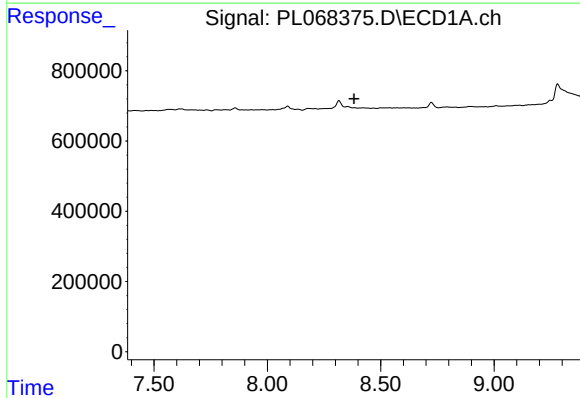


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

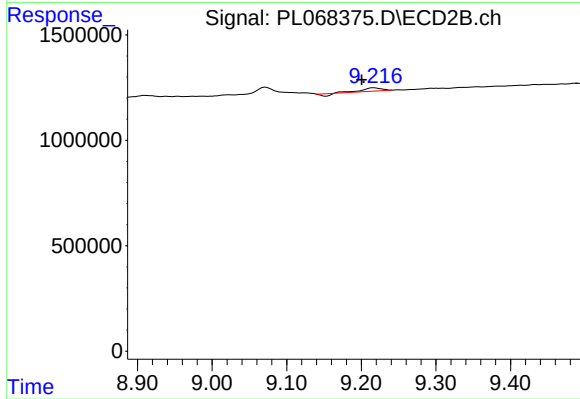

#15 Endosulfan II


R.T.: 9.217 min
Delta R.T.: 0.016 min
Response: 262167
Conc: 0.29 ng/ml

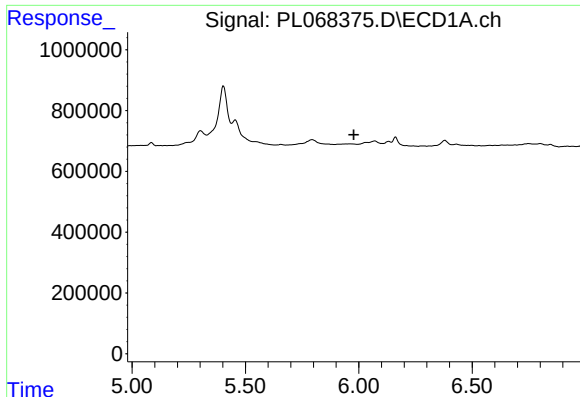

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

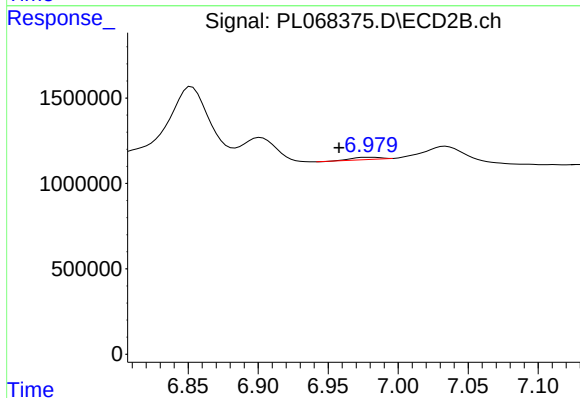


#23 Chlordane-1

R.T.: 6.980 min
Delta R.T.: 0.022 min
Response: 182157
Conc: 4.50 ng/ml

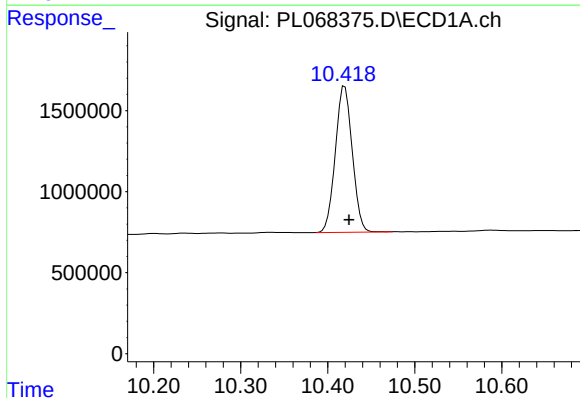

#28 Decachlorobiphenyl

R.T.: 10.420 min
Delta R.T.: -0.005 min
Response: 12186818
Conc: 21.67 ng/ml

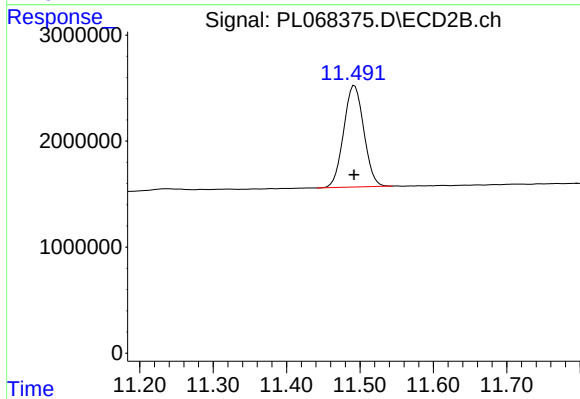

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 18238877
Conc: 20.45 ng/ml