

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072221\
 Data File : PL068386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2021 16:16
 Operator : AR\AJ
 Sample : M3117-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:15:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.643	5.569	8210126	18228769	19.130	17.864
28)	SA Decachlor...	10.419	11.491	9175207	15829233	16.314	17.746
Target Compounds							
11)	B alpha-Chl...	0.000	8.384	0	412978	N.D.	0.367 #
12)	B 4,4'-DDE	7.648	8.568	1500142	2407084	2.977	2.336
14)	MA Endrin	8.088f	0.000	575956	0	1.152	N.D. #
17)	MA 4,4'-DDT	8.495	9.425	1929695	2323012	3.847	2.461 #
26)	Chlordane-4	0.000	8.384	0	412978	N.D.	2.203 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072221\
Data File : PL068386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2021 16:16
Operator : AR\AJ
Sample : M3117-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:15:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

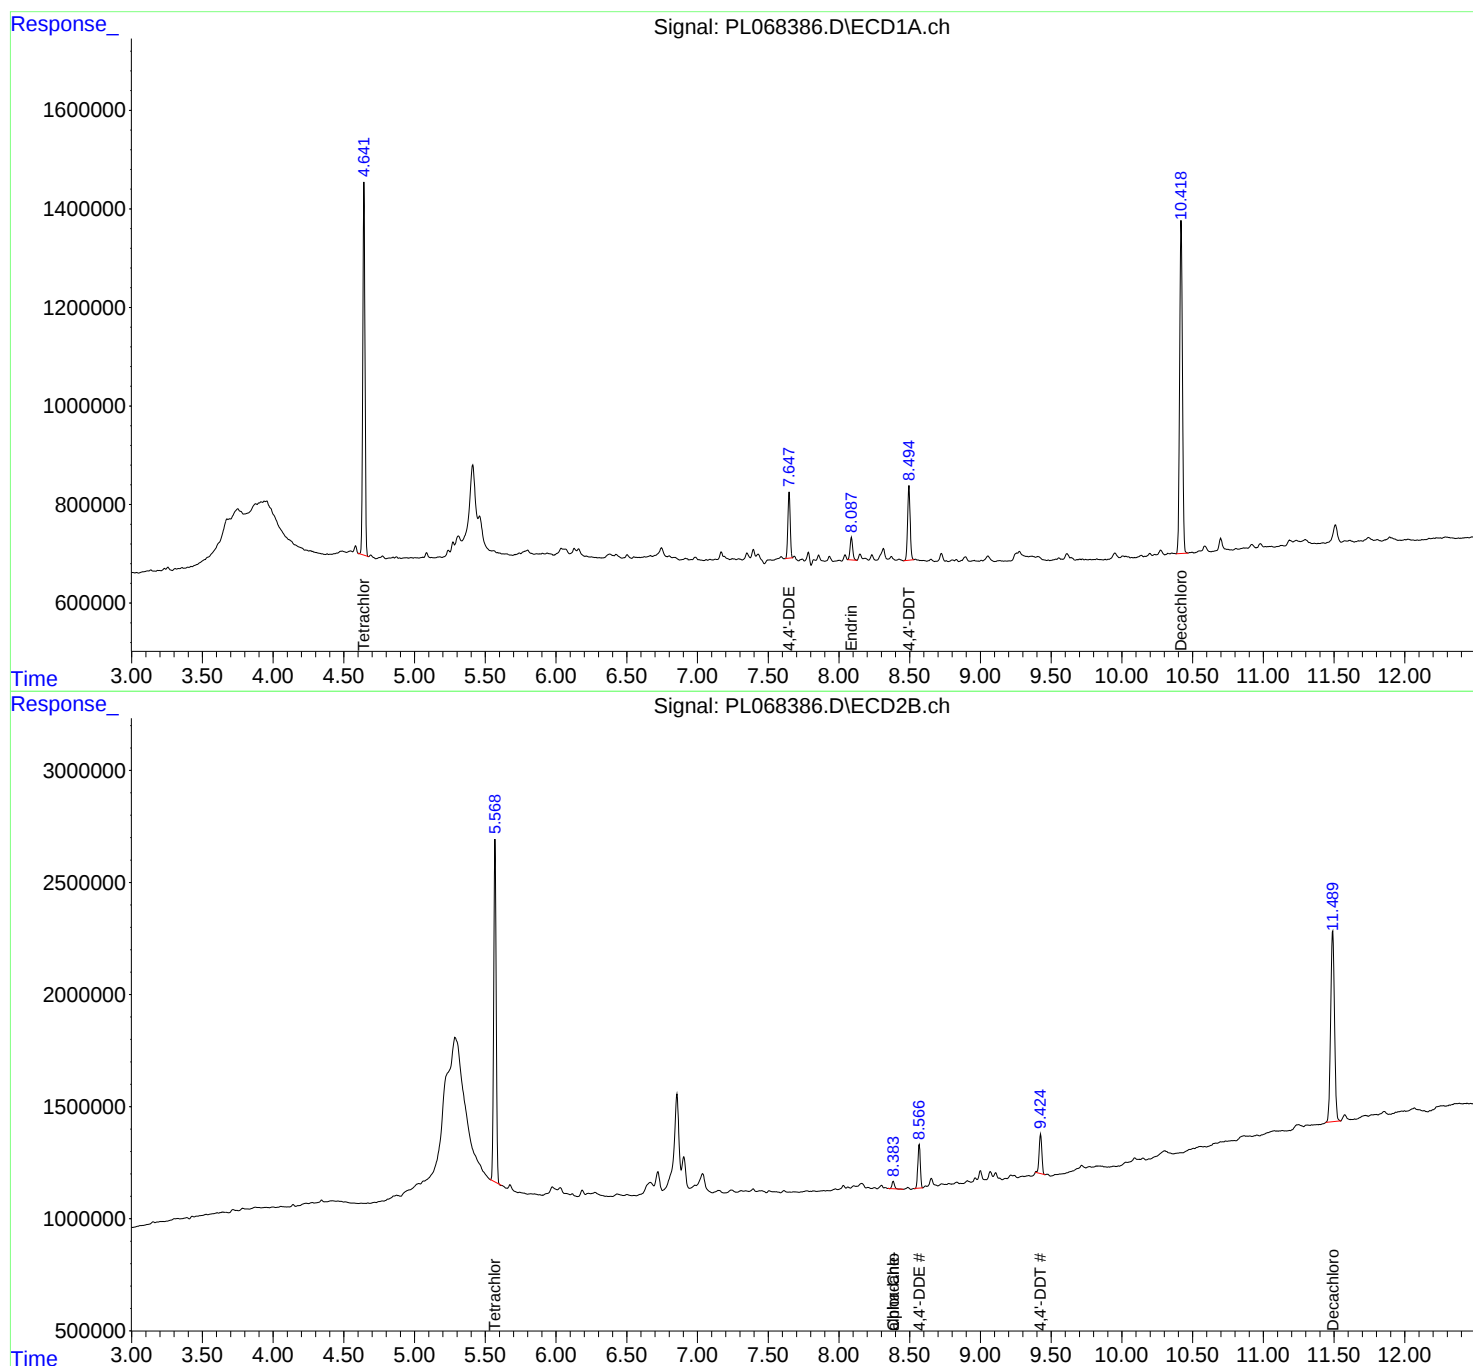


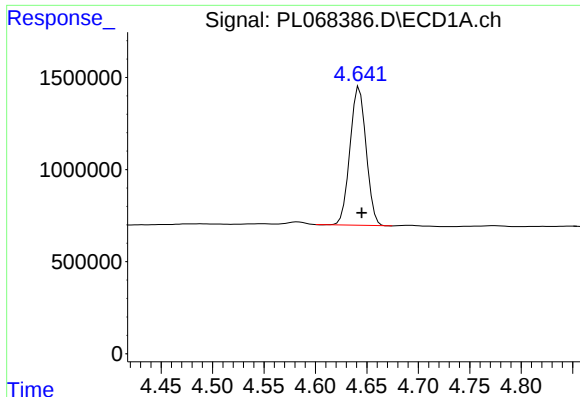

#1 Tetrachloro-m-xylene


R.T.: 4.643 min
Delta R.T.: -0.002 min
Response: 8210126
Conc: 19.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

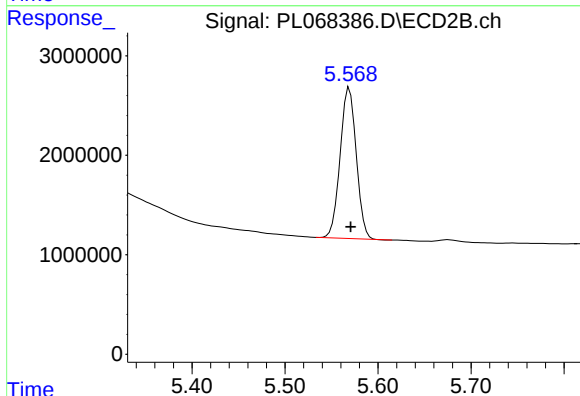


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.001 min
Response: 18228769
Conc: 17.86 ng/ml

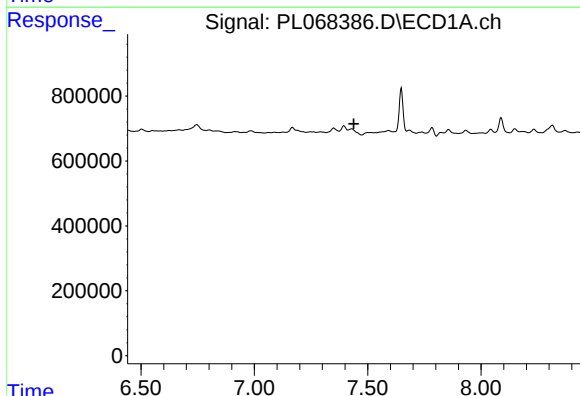


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.438 min
Response: 0
Conc: N.D.

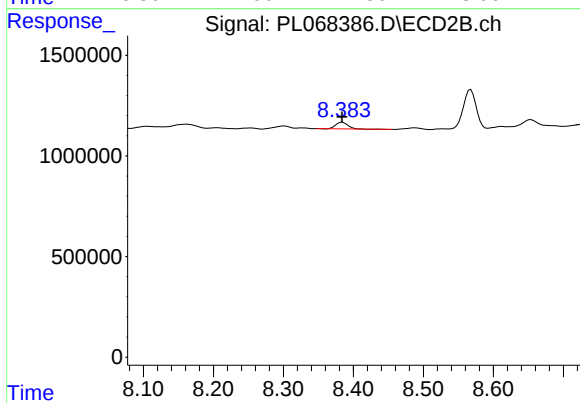

#11 alpha-Chlordane


R.T.: 8.384 min
Delta R.T.: 0.000 min
Response: 412978
Conc: 0.37 ng/ml

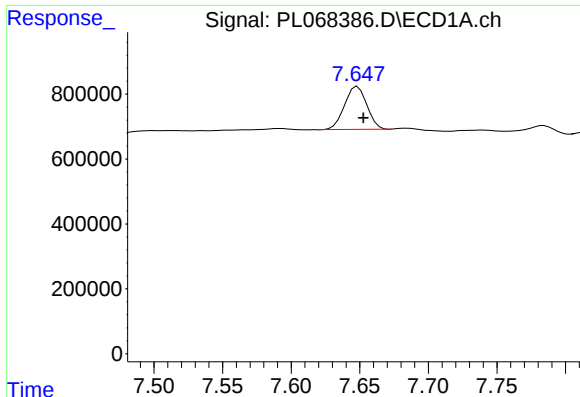

#12 4,4'-DDE


R.T.: 7.648 min
Delta R.T.: -0.004 min
Response: 1500142
Conc: 2.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

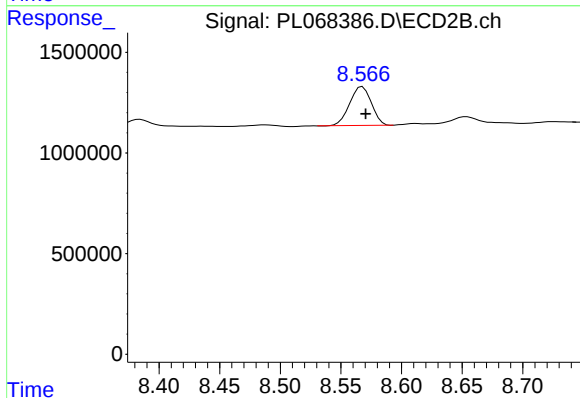


#12 4,4'-DDE

R.T.: 8.568 min
Delta R.T.: -0.003 min
Response: 2407084
Conc: 2.34 ng/ml

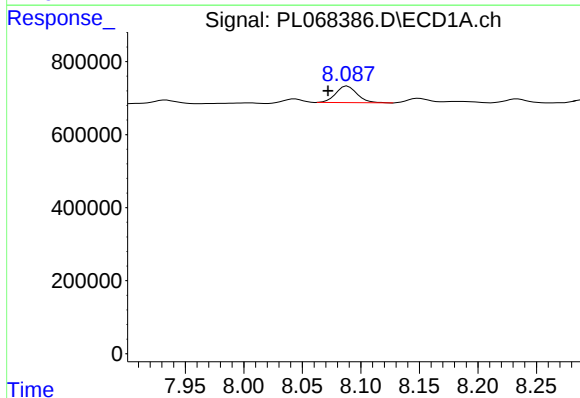


#14 Endrin

R.T.: 8.088 min
Delta R.T.: 0.016 min
Response: 575956
Conc: 1.15 ng/ml

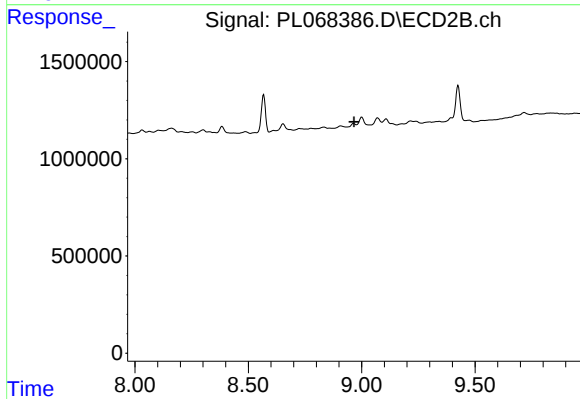

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.966 min
Response: 0
Conc: N.D.

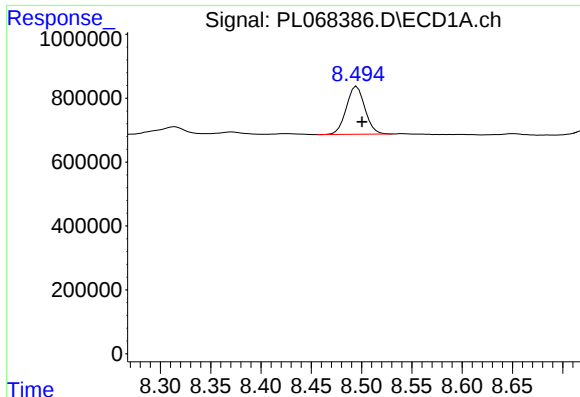

#17 4,4'-DDT


R.T.: 8.495 min
Delta R.T.: -0.005 min
Response: 1929695
Conc: 3.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

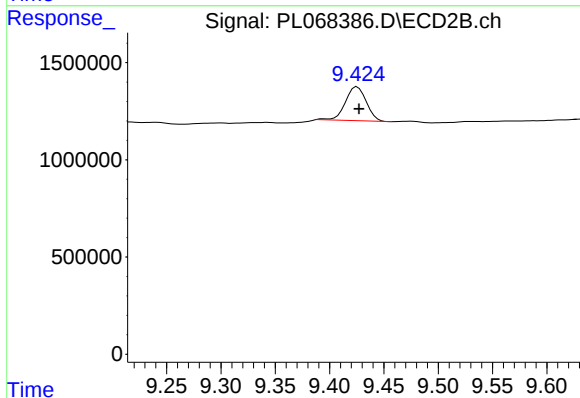


#17 4,4'-DDT

R.T.: 9.425 min
Delta R.T.: -0.002 min
Response: 2323012
Conc: 2.46 ng/ml

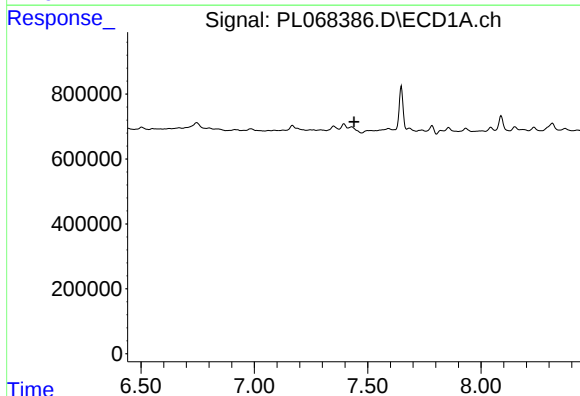


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

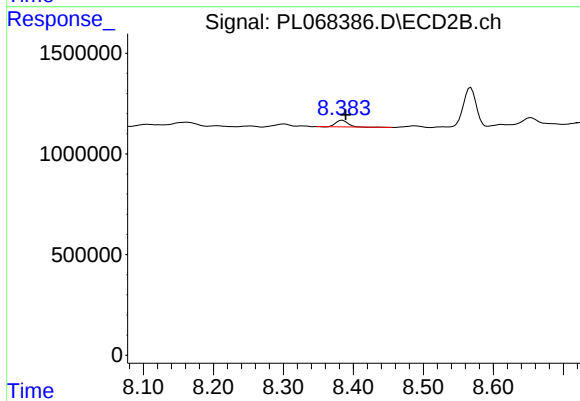

#26 Chlordane-4


R.T.: 8.384 min
Delta R.T.: -0.005 min
Response: 412978
Conc: 2.20 ng/ml

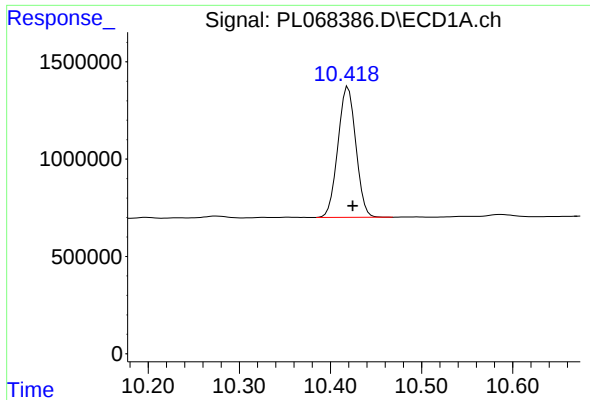

#28 Decachlorobiphenyl

R.T.: 10.419 min
Delta R.T.: -0.005 min
Response: 9175207
Conc: 16.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

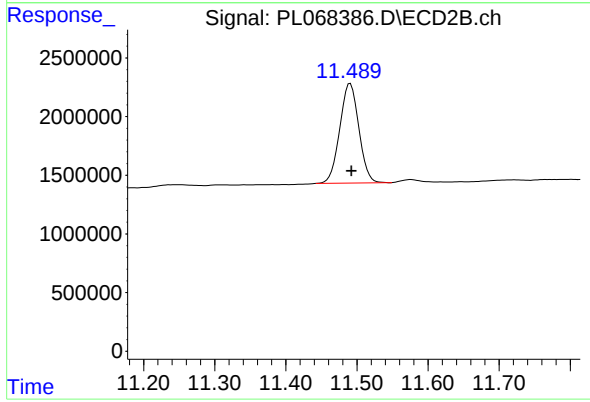

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: -0.002 min
Response: 15829233
Conc: 17.75 ng/ml