

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072221\
 Data File : PL068388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2021 16:49
 Operator : AR\AJ
 Sample : M3117-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NJ-CLEAN-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:16:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.643	5.569	5747322	12739154	13.391	12.484
28)	SA Decachlor...	10.418	11.491	5509718	9032714	9.796	10.126
Target Compounds							
12)	B 4,4'-DDE	0.000	8.567	0	301613	N.D.	0.293 #
23)	Chlordane-1	0.000	6.977f	0	270068	N.D.	6.667 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072221\
Data File : PL068388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2021 16:49
Operator : AR\AJ
Sample : M3117-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NJ-CLEAN-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:16:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

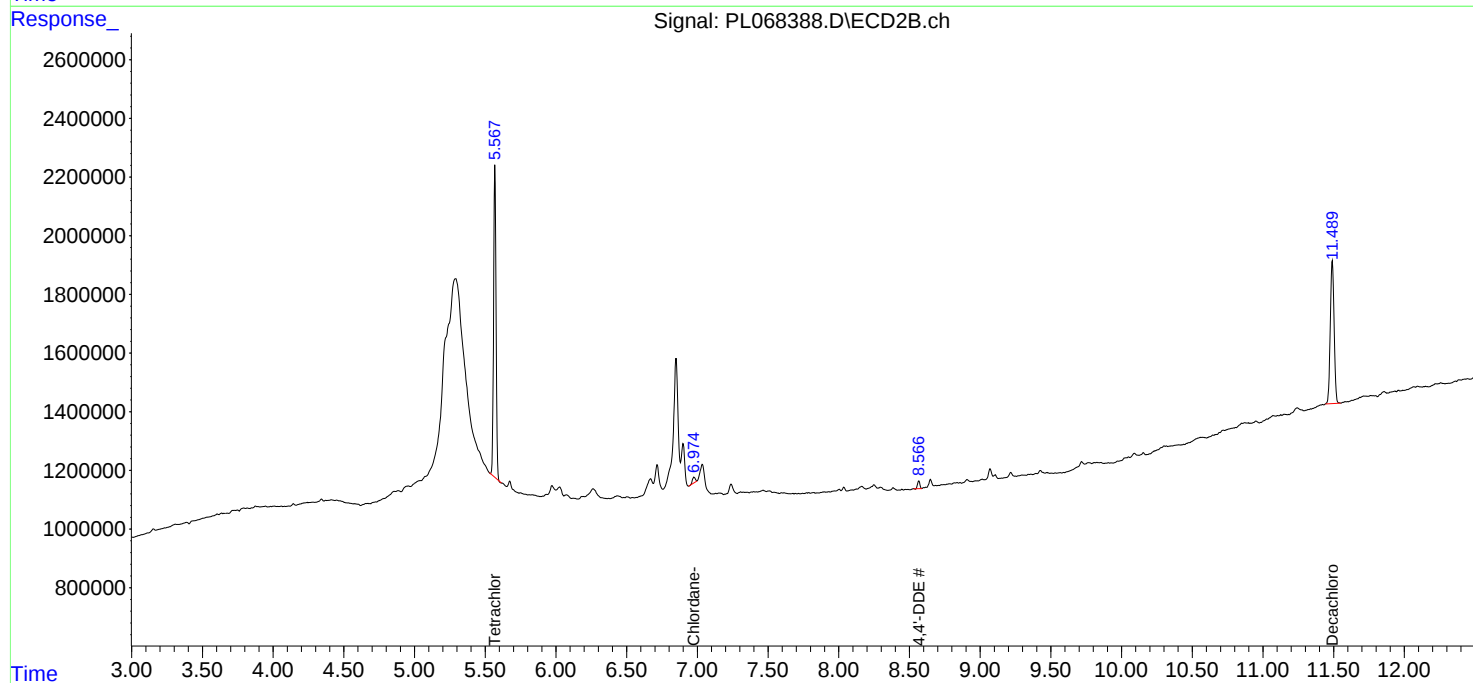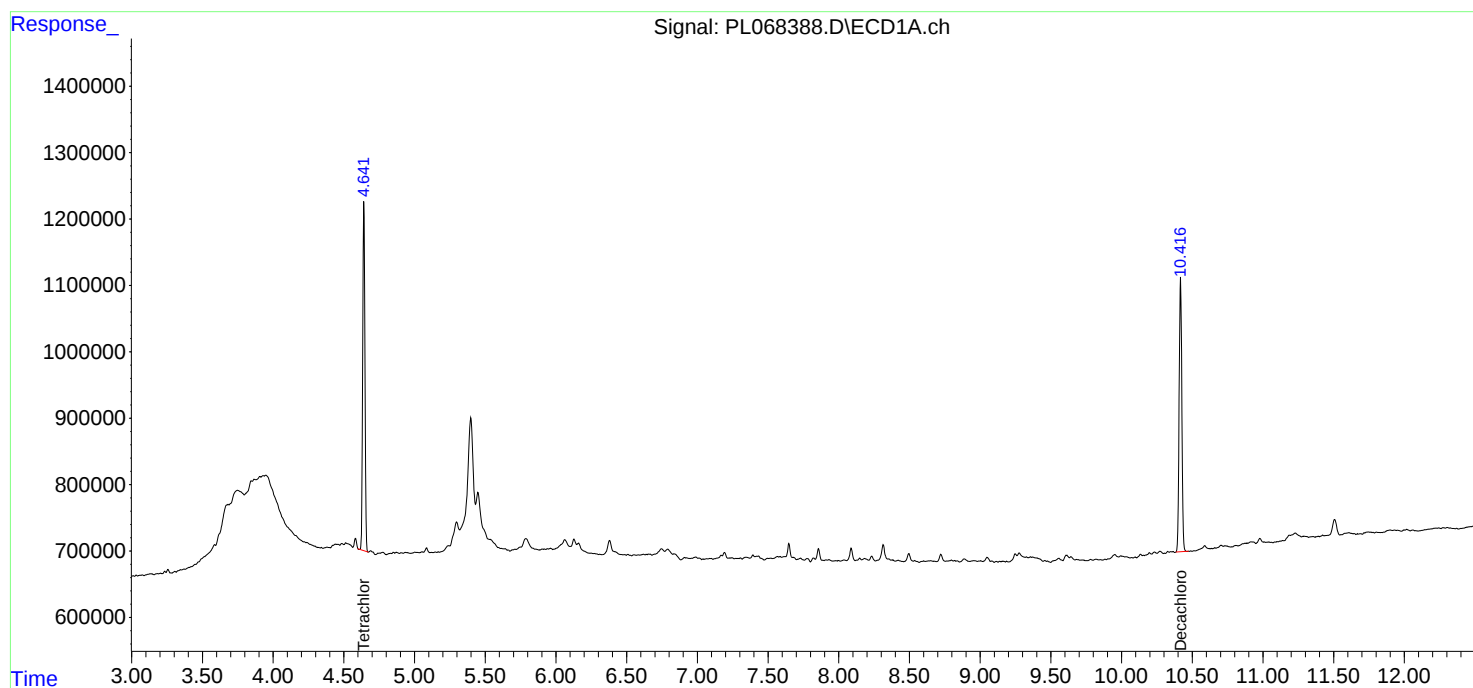


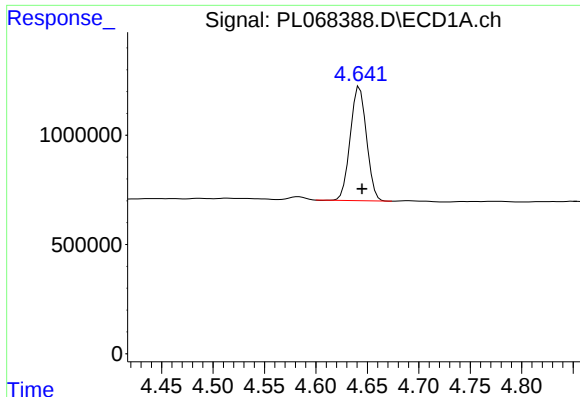

#1 Tetrachloro-m-xylene


R.T.: 4.643 min
Delta R.T.: -0.002 min
Response: 5747322
Conc: 13.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
NJ-CLEAN-8

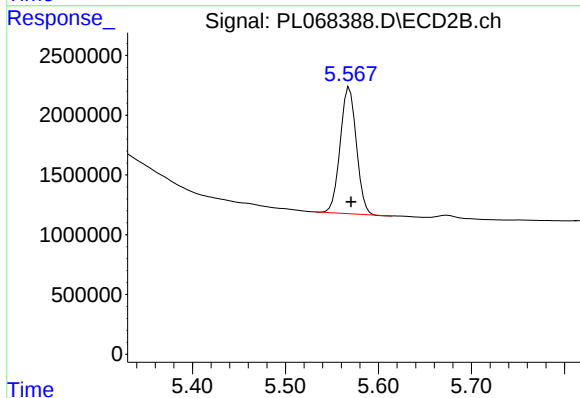


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 12739154
Conc: 12.48 ng/ml

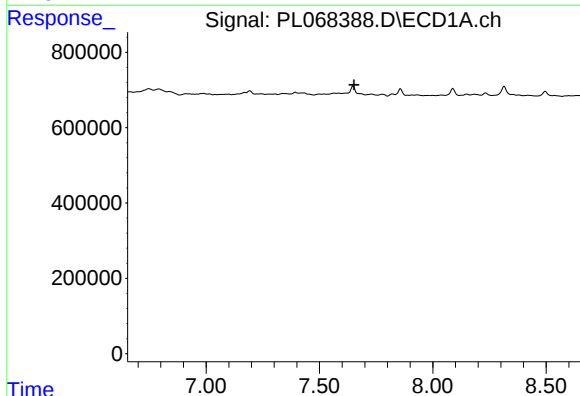


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 7.653 min
Response: 0
Conc: N.D.

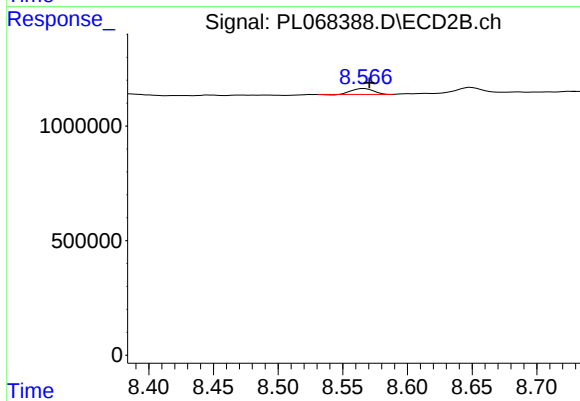

#12 4,4'-DDE


R.T.: 8.567 min
Delta R.T.: -0.004 min
Response: 301613
Conc: 0.29 ng/ml

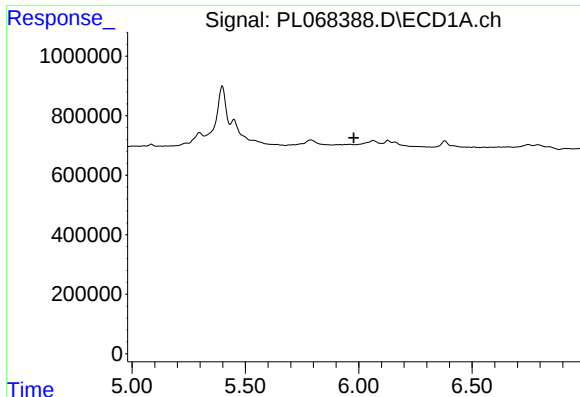

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NJ-CLEAN-8

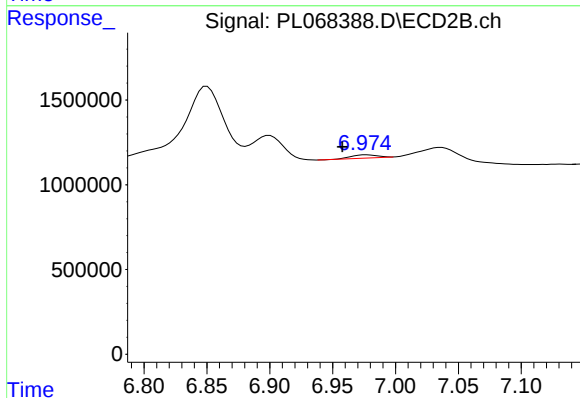


#23 Chlordane-1

R.T.: 6.977 min
Delta R.T.: 0.019 min
Response: 270068
Conc: 6.67 ng/ml

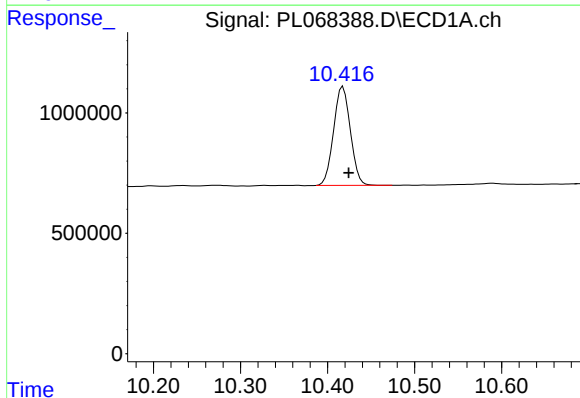

#28 Decachlorobiphenyl

R.T.: 10.418 min
Delta R.T.: -0.007 min
Response: 5509718
Conc: 9.80 ng/ml

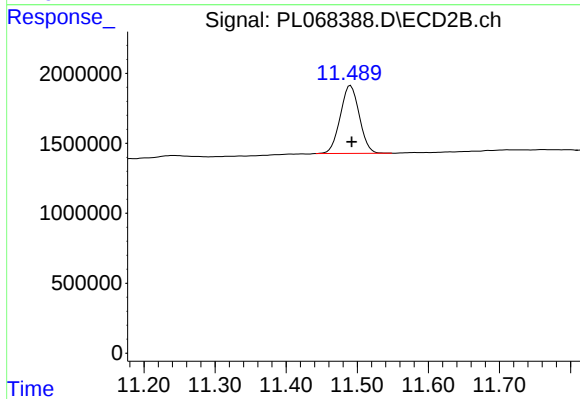

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: -0.002 min
Response: 9032714
Conc: 10.13 ng/ml