

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072221\
 Data File : PL068413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2021 00:24
 Operator : AR\AJ
 Sample : M3135-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-L

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:22:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.569	8274836	18609874	19.280	18.237
28)	SA Decachlor...	10.417	11.490	9392444	15093103	16.700	16.921
Target Compounds							
10)	B gamma-Chl...	7.394f	0.000	332492	0	0.579	N.D. #
11)	B alpha-Chl...	0.000	8.383	0	1050956	N.D.	0.934 #
25)	Chlordane-3	7.394f	0.000	332492	0	6.174	N.D. #
26)	Chlordane-4	0.000	8.383	0	1050956	N.D.	5.606 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072221\
Data File : PL068413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2021 00:24
Operator : AR\AJ
Sample : M3135-07
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-L

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:22:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

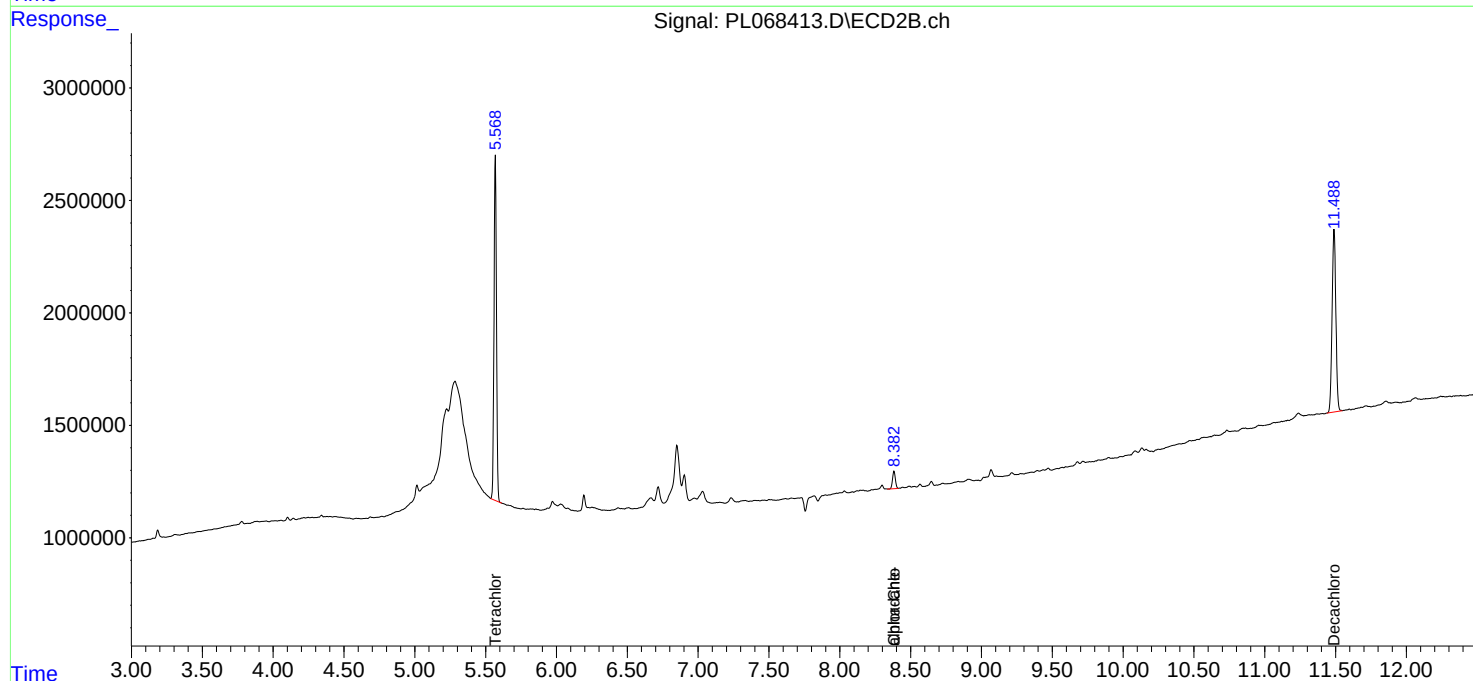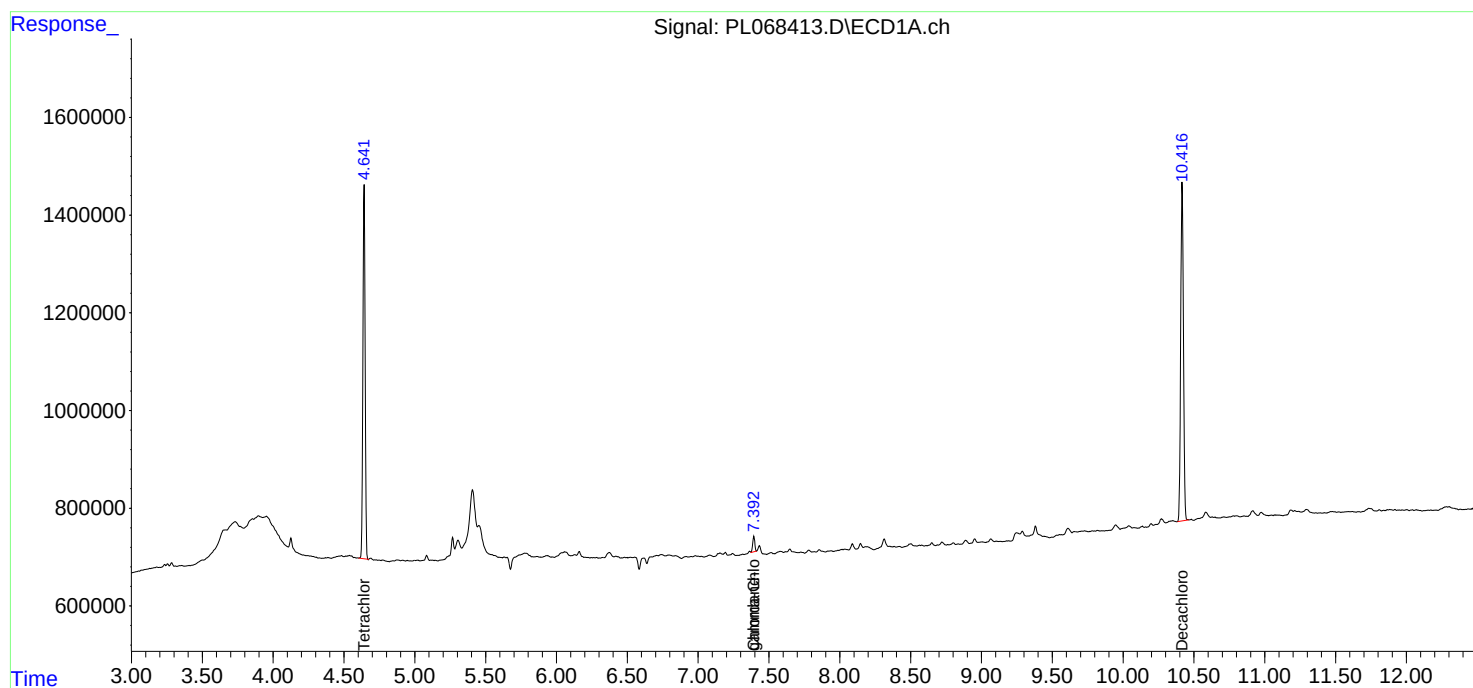


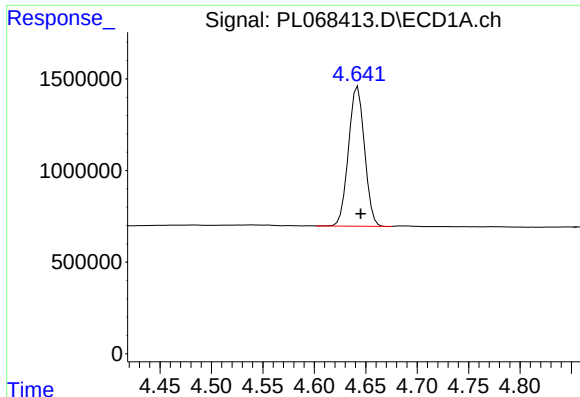

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 8274836
Conc: 19.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-L

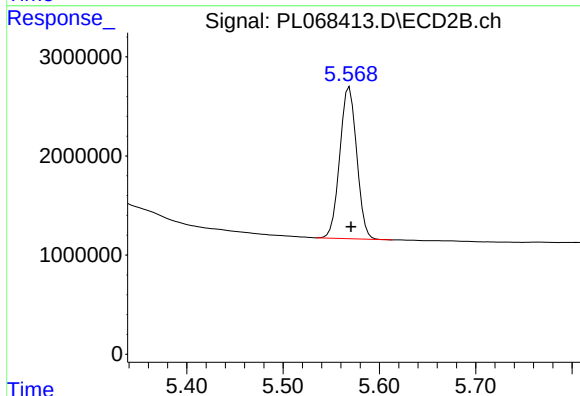


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 18609874
Conc: 18.24 ng/ml

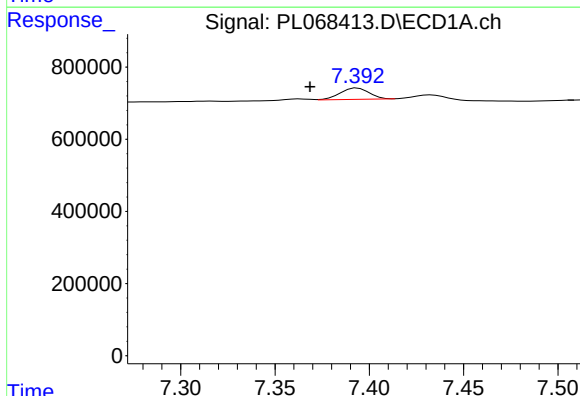


#10 gamma-Chlordane

R.T.: 7.394 min
Delta R.T.: 0.025 min
Response: 332492
Conc: 0.58 ng/ml

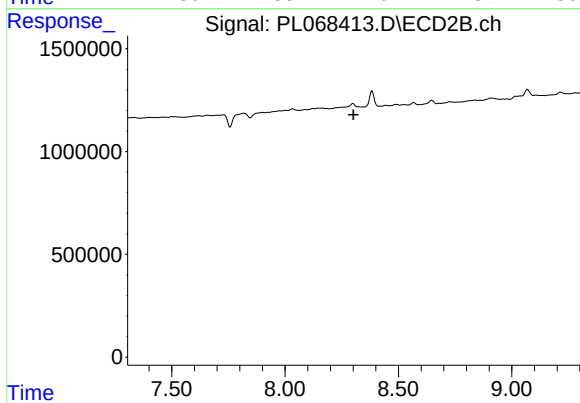

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.302 min
Response: 0
Conc: N.D.

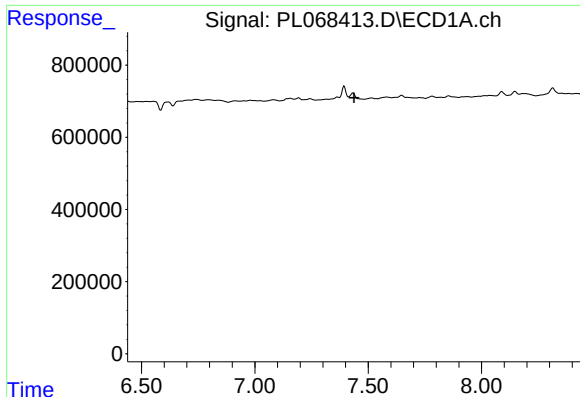

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-L

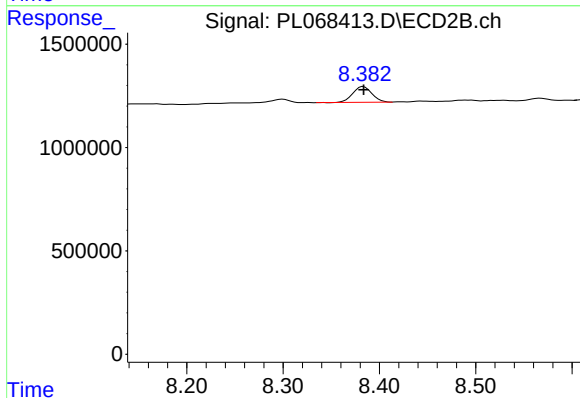


#11 alpha-Chlordane

R.T.: 8.383 min
Delta R.T.: 0.000 min
Response: 1050956
Conc: 0.93 ng/ml

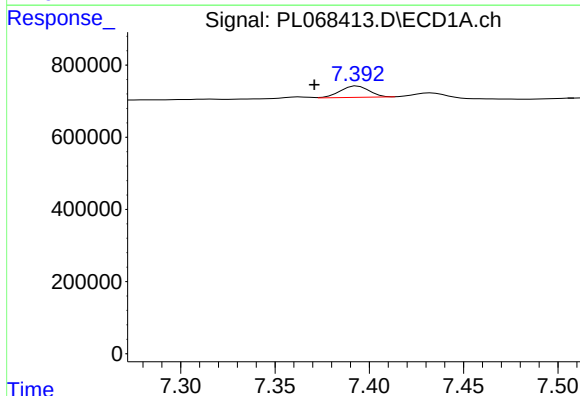


#25 Chlordane-3

R.T.: 7.394 min
Delta R.T.: 0.023 min
Response: 332492
Conc: 6.17 ng/ml

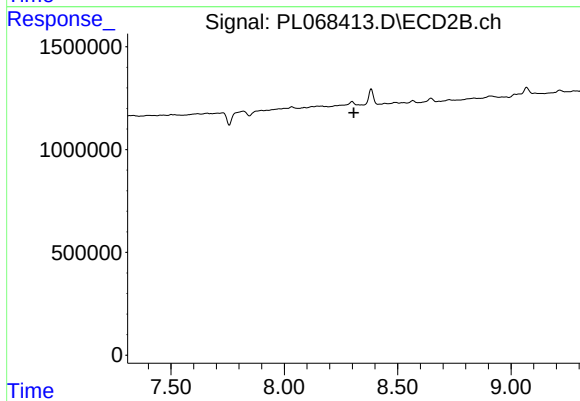

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.306 min
Response: 0
Conc: N.D.

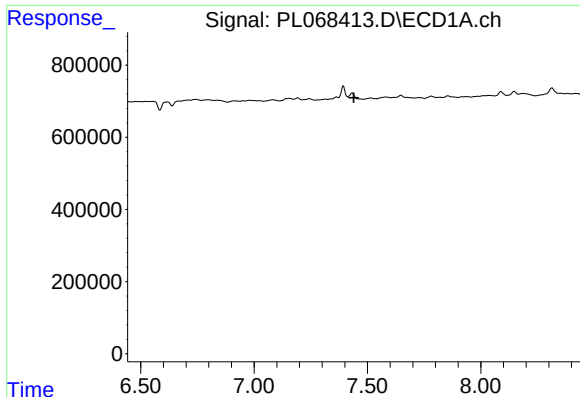

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-L

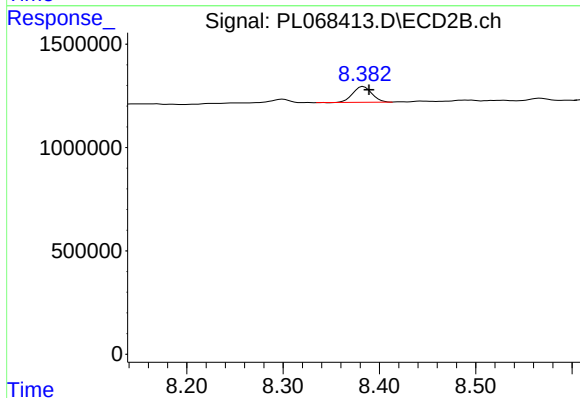


#26 Chlordane-4

R.T.: 8.383 min
Delta R.T.: -0.006 min
Response: 1050956
Conc: 5.61 ng/ml

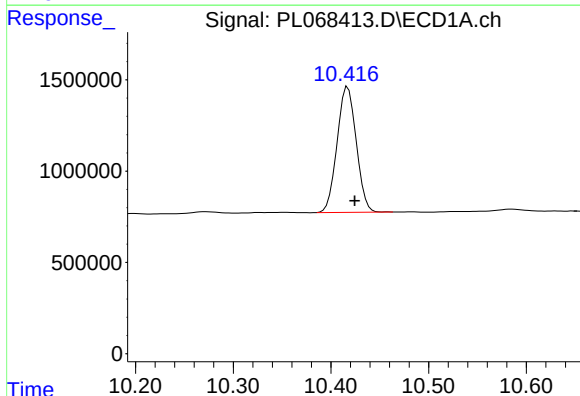

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.007 min
Response: 9392444
Conc: 16.70 ng/ml

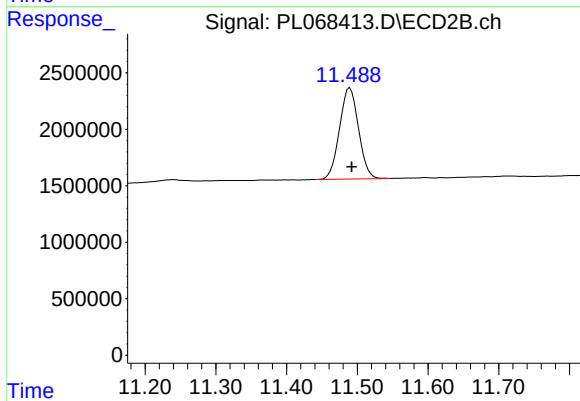

#28 Decachlorobiphenyl

R.T.: 11.490 min
Delta R.T.: -0.003 min
Response: 15093103
Conc: 16.92 ng/ml