

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072221\
 Data File : PL068414.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2021 00:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:23:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.569	9335465	21012657	21.752	20.592
28)	SA Decachlor...	10.417	11.490	12640415	19765985	22.475	22.159
Target Compounds							
4)	MA Heptachlor	6.161f	0.000	642899	0	1.055	N.D. #
6)	B beta-BHC	6.161	0.000	642899	0	2.197	N.D. #
8)	B Heptachlo...	0.000	8.037	0	870856	N.D.	0.770 #
14)	MA Endrin	8.089f	0.000	779850	0	1.559	N.D. #
15)	B Endosulfa...	0.000	9.217f	0	63896	N.D.	0.070 #
27)	Chlordane-5	0.000	9.272	0	548154	N.D.	17.103 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072221\
Data File : PL068414.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2021 00:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:23:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

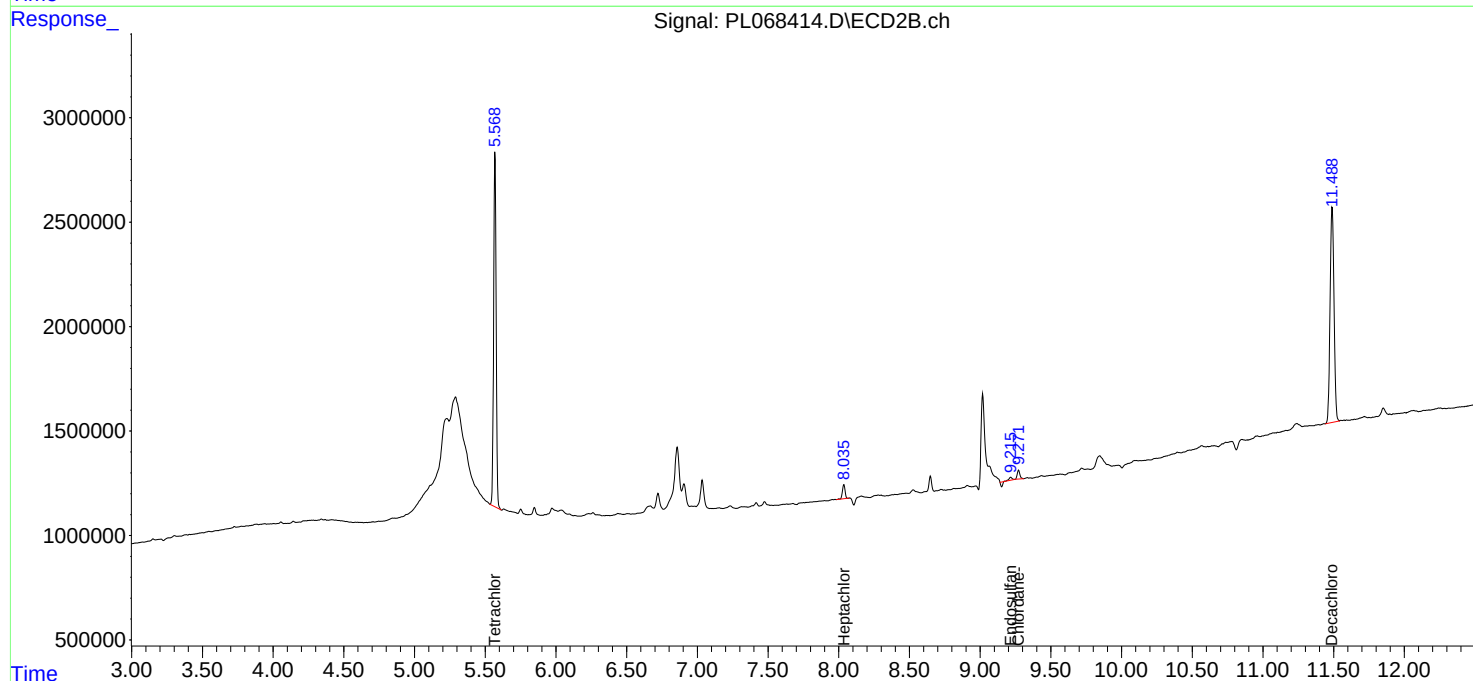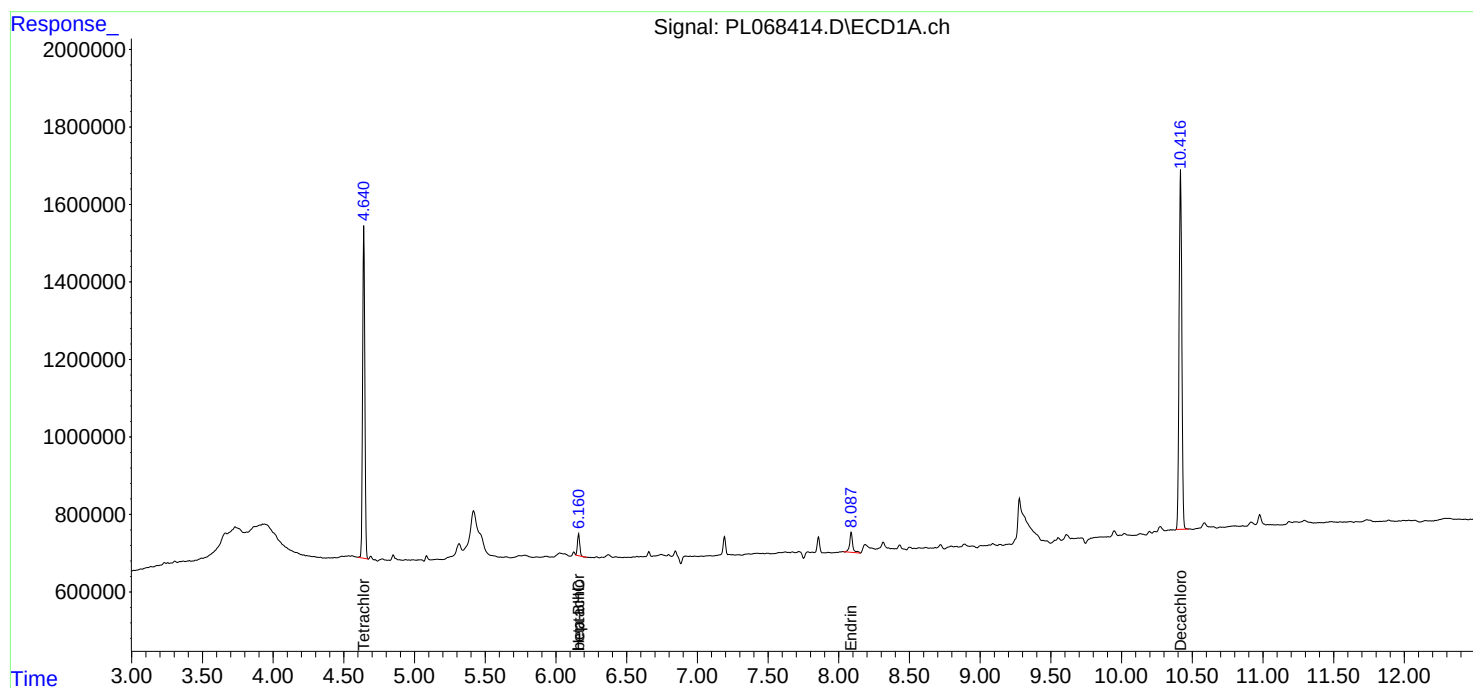


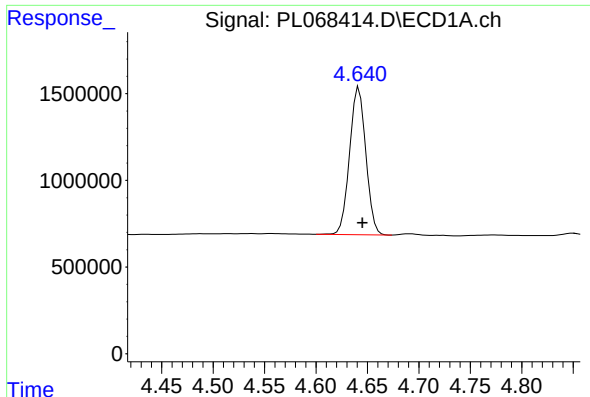

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 9335465
Conc: 21.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

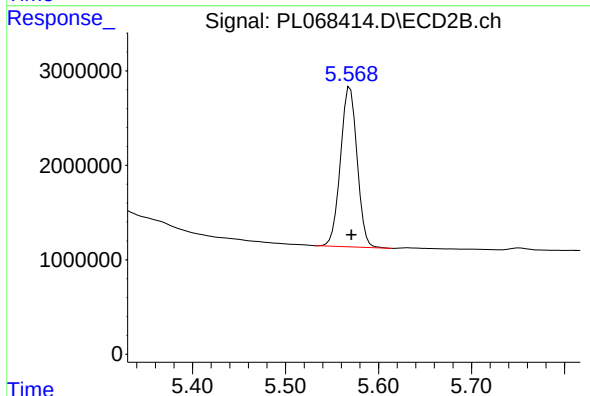


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.001 min
Response: 21012657
Conc: 20.59 ng/ml

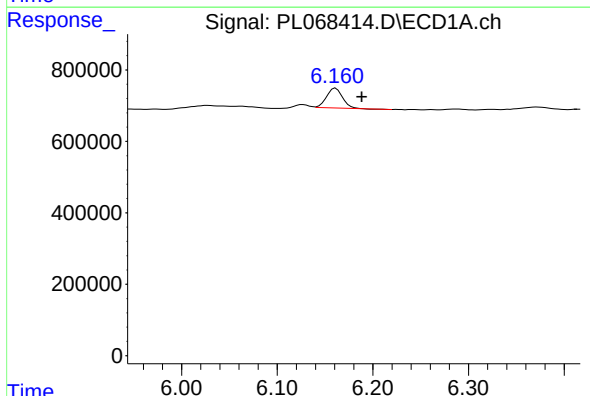


#4 Heptachlor

R.T.: 6.161 min
Delta R.T.: -0.027 min
Response: 642899
Conc: 1.05 ng/ml

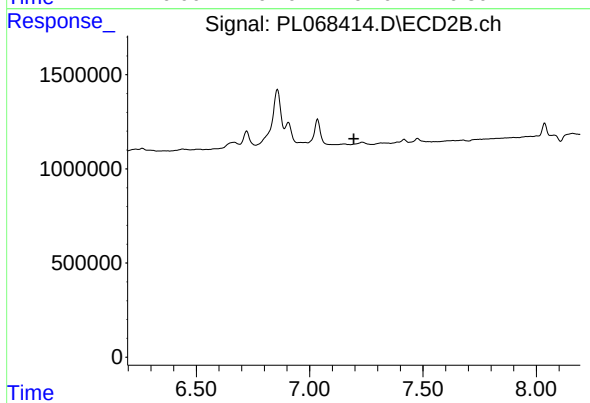

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.195 min
Response: 0
Conc: N.D.

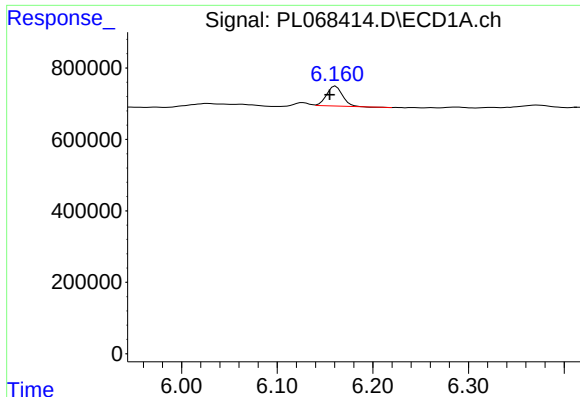

#6 beta-BHC


R.T.: 6.161 min
Delta R.T.: 0.006 min
Response: 642899
Conc: 2.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

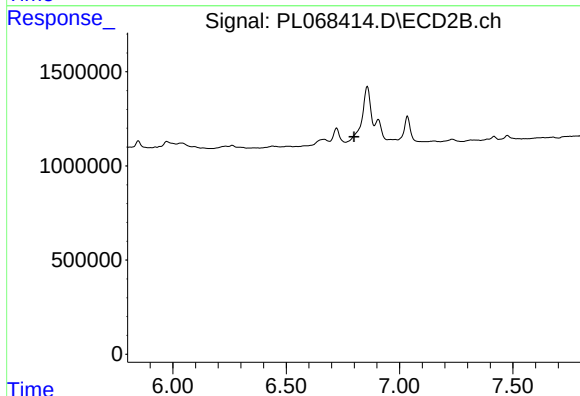


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

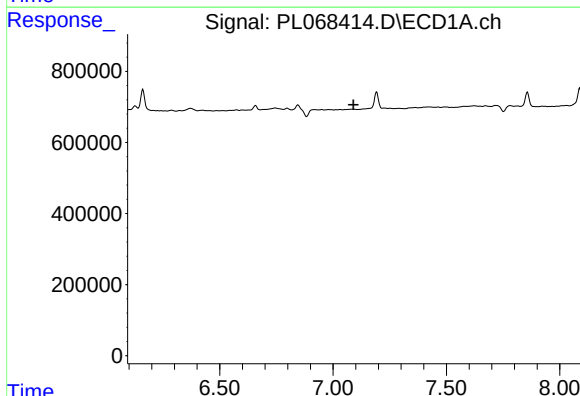


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

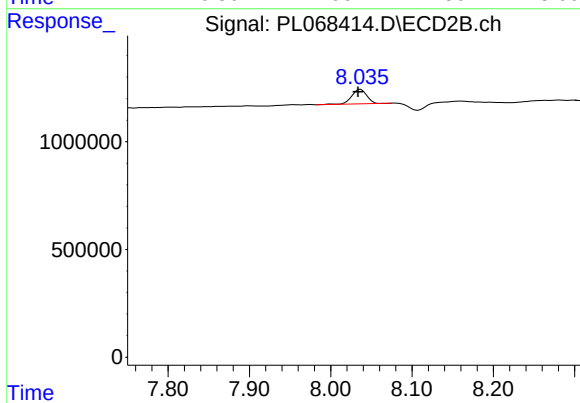

#8 Heptachlor epoxide


R.T.: 8.037 min
Delta R.T.: 0.003 min
Response: 870856
Conc: 0.77 ng/ml

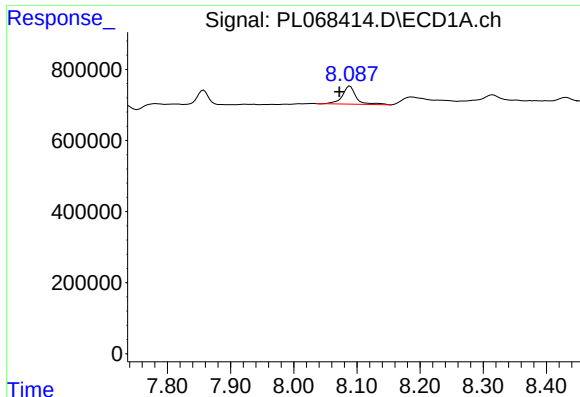

#14 Endrin


R.T.: 8.089 min
Delta R.T.: 0.017 min
Response: 779850
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

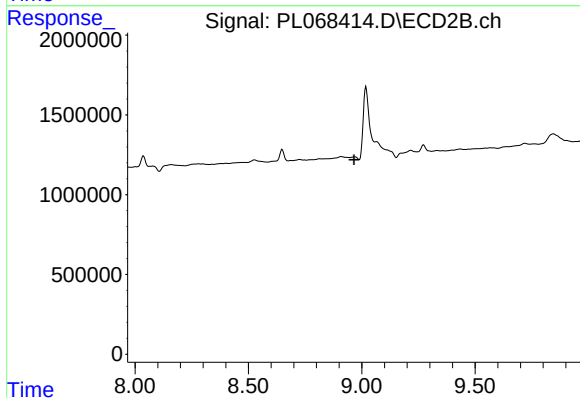


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.966 min
Response: 0
Conc: N.D.

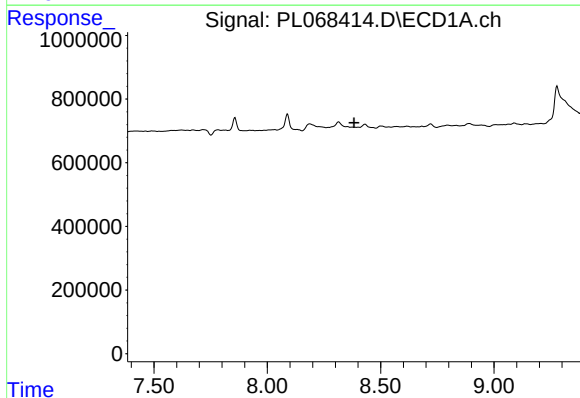


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

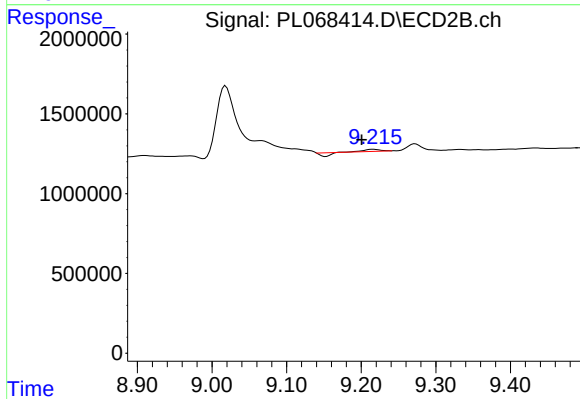

#15 Endosulfan II


R.T.: 9.217 min
Delta R.T.: 0.016 min
Response: 63896
Conc: 0.07 ng/ml

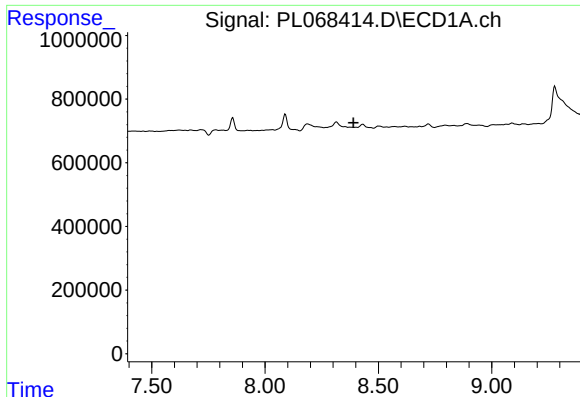

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

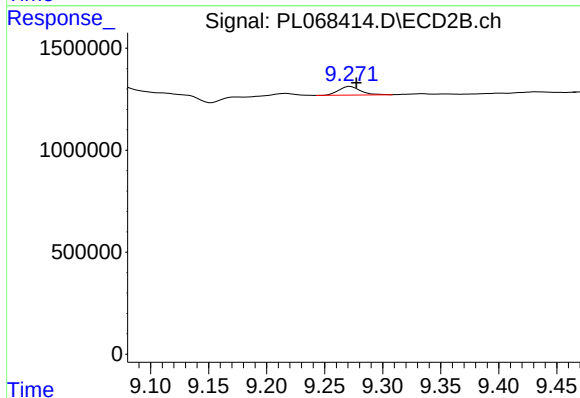


#27 Chlordane-5

R.T.: 9.272 min
Delta R.T.: -0.005 min
Response: 548154
Conc: 17.10 ng/ml

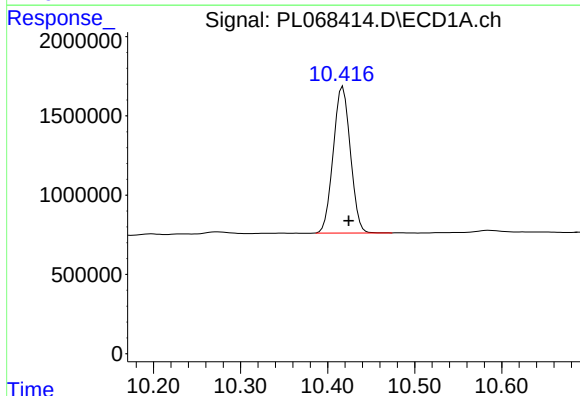

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.007 min
Response: 12640415
Conc: 22.48 ng/ml

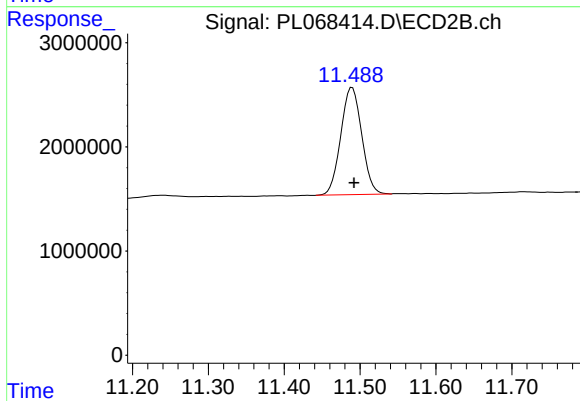

#28 Decachlorobiphenyl

R.T.: 11.490 min
Delta R.T.: -0.003 min
Response: 19765985
Conc: 22.16 ng/ml