

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072223\
 Data File : PL084097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2023 14:28
 Operator : AR\AJ
 Sample : 03680-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/21/2023
 Supervised By :Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 21:31:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.476	2.688	41242615	20668122	20.623	18.610
2) SA Decachlor...	9.023	7.871	24033244	18364094	18.464	16.527
Target Compounds						
13) MA Dieldrin	6.293	5.290	1627340	892695	0.681m	0.685

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072223\
Data File : PL084097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2023 14:28
Operator : AR\AJ
Sample : 03680-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/21/2023
Supervised By : Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 21:31:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

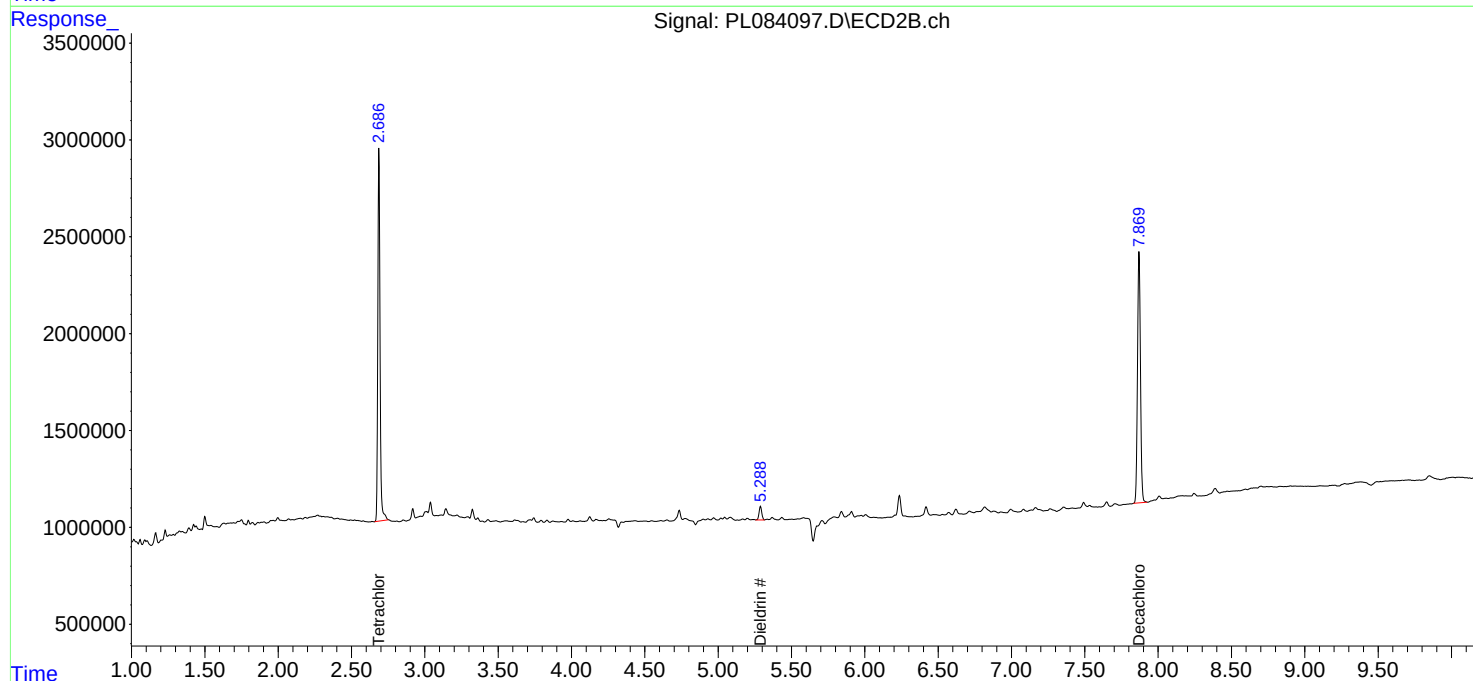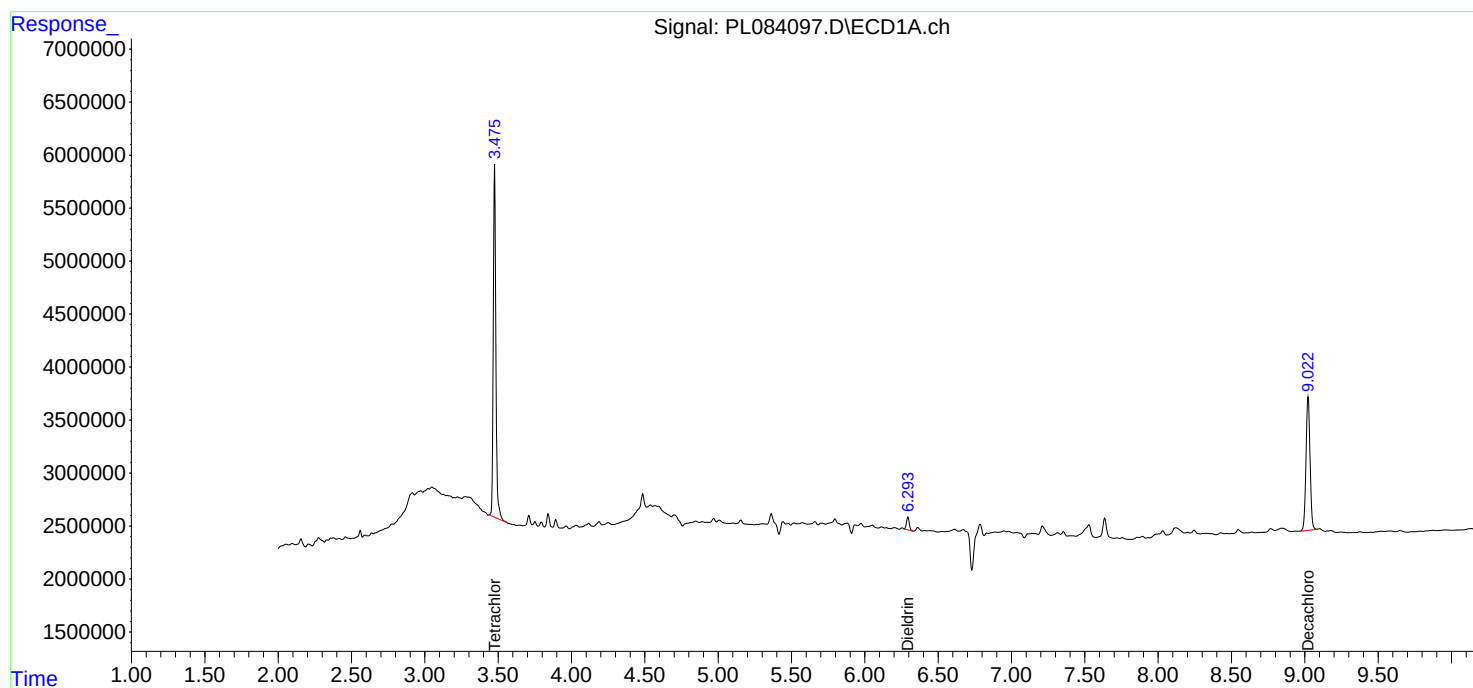

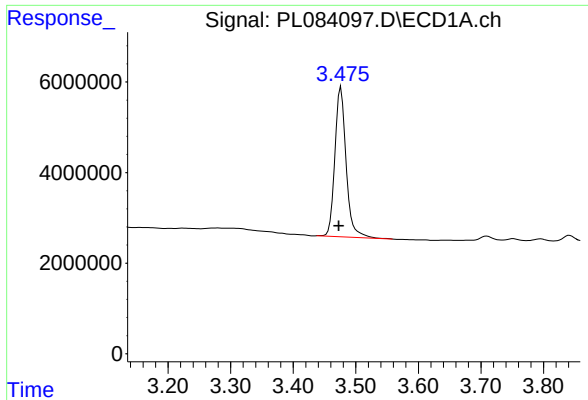


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 41242615
Conc: 20.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023

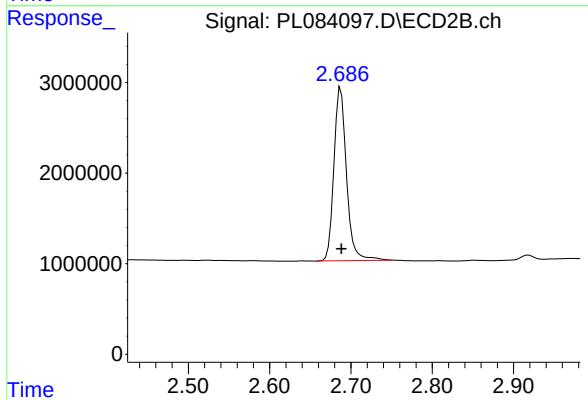


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: 0.000 min
Response: 20668122
Conc: 18.61 ng/ml

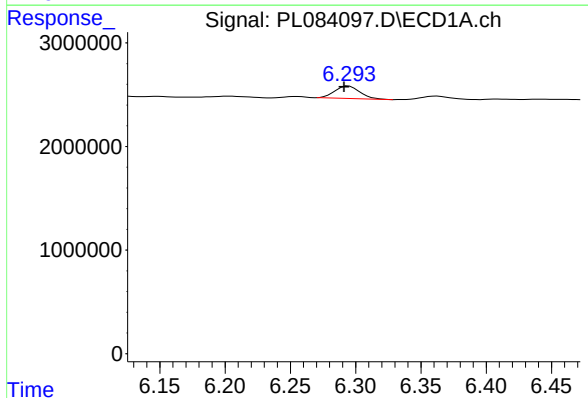


#13 Dieldrin

R.T.: 6.293 min
Delta R.T.: 0.002 min
Response: 1627340
Conc: 0.68 ng/ml m

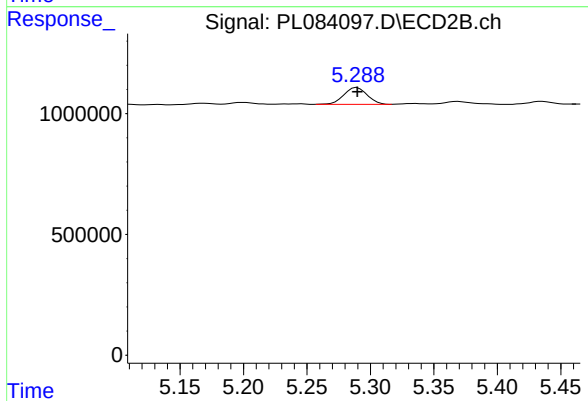

#13 Dieldrin

R.T.: 5.290 min
Delta R.T.: 0.000 min
Response: 892695
Conc: 0.69 ng/ml

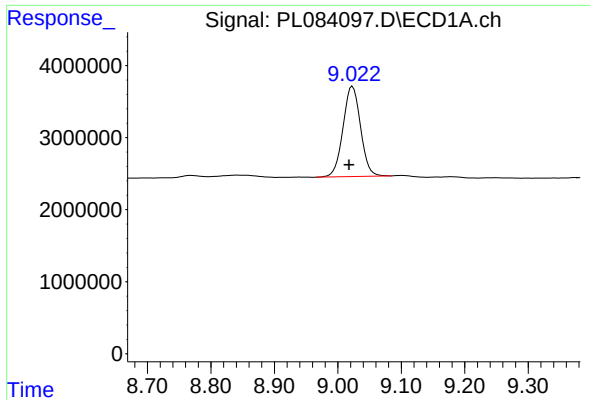


#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.006 min
Response: 24033244
Conc: 18.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023

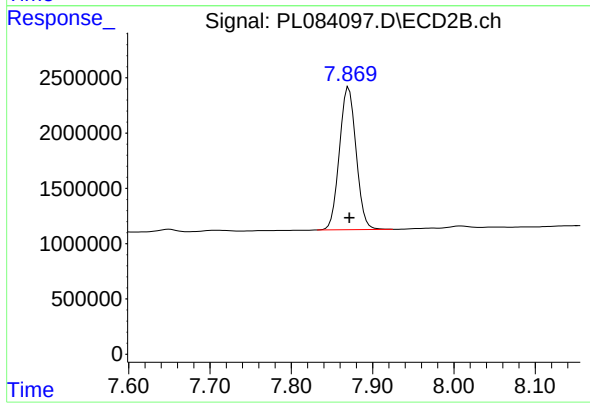

#28 Decachlorobiphenyl

R.T.: 7.871 min
Delta R.T.: 0.000 min
Response: 18364094
Conc: 16.53 ng/ml