

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072223\
 Data File : PL084106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2023 16:52
 Operator : AR\AJ
 Sample : 03683-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NORTH-TURNPIKE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/21/2023
 Supervised By :Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 21:43:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.688	35806202	18176613	17.904	16.367
28)	SA Decachlor...	9.023	7.871	20298172	12965020	15.594m	11.668 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072223\
Data File : PL084106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2023 16:52
Operator : AR\AJ
Sample : 03683-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NORTH-TURNPIKE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/21/2023
Supervised By : Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 21:43:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

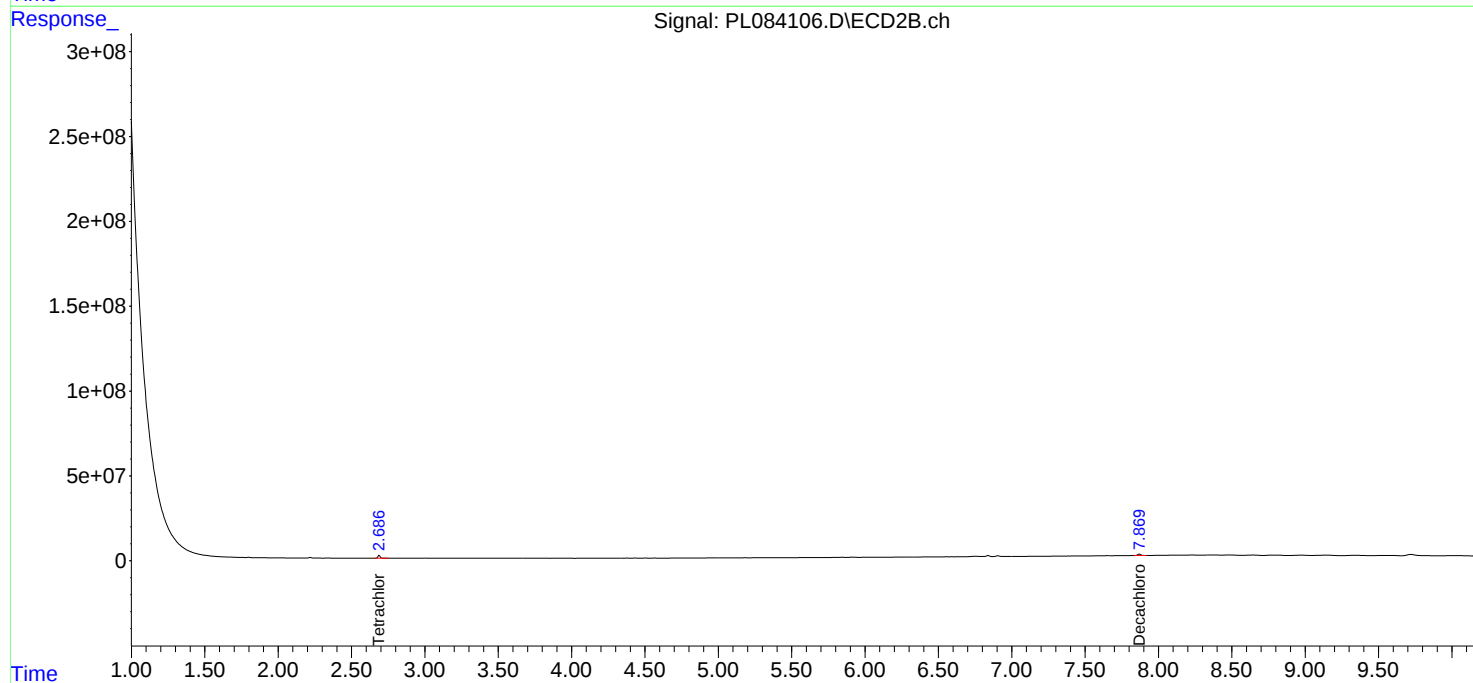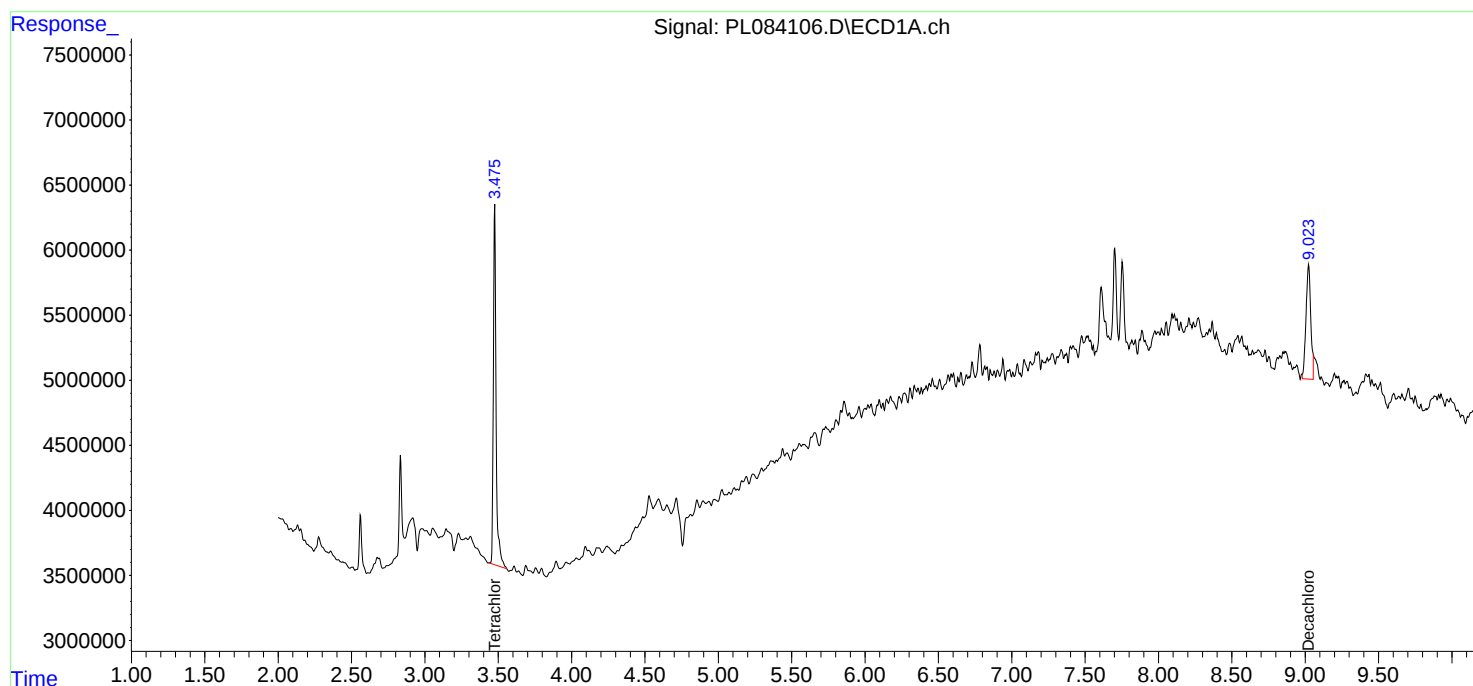

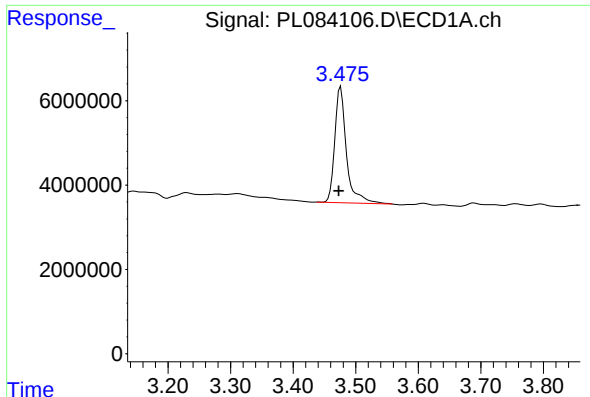


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 35806202
Conc: 17.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
NORTH-TURNPIKE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023

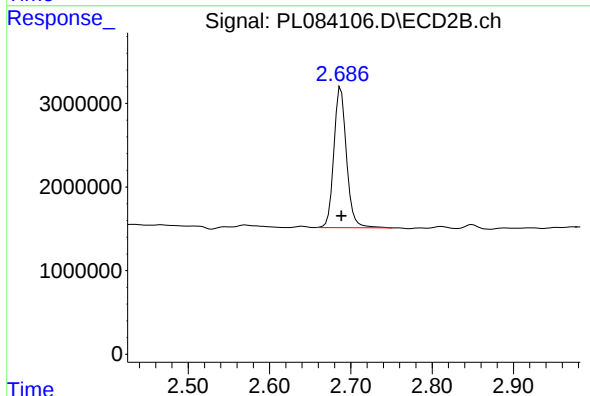


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: 0.000 min
Response: 18176613
Conc: 16.37 ng/ml

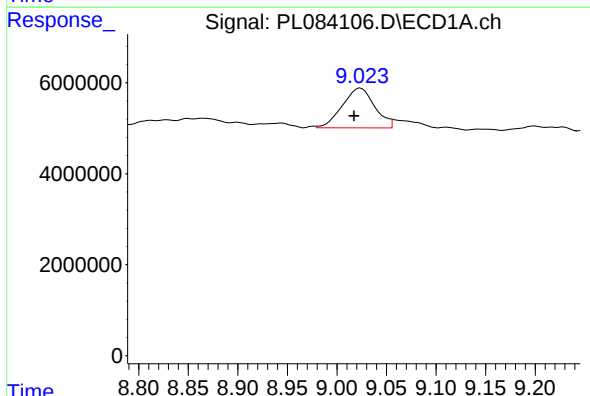

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.005 min
Response: 20298172
Conc: 15.59 ng/ml m

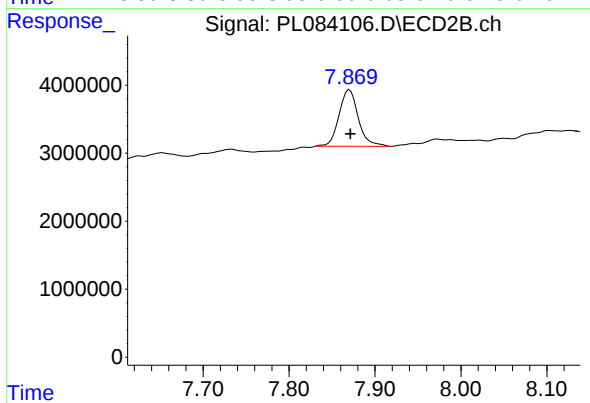

#28 Decachlorobiphenyl

R.T.: 7.871 min
Delta R.T.: -0.001 min
Response: 12965020
Conc: 11.67 ng/ml