

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072225\
 Data File : PL096518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 17:16
 Operator : AR\AJ
 Sample : Q2649-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:49:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.534	2.828	62258674	107.3E6	17.062m	18.593
28) SA Decachlor...	9.017	7.993	41313800	75861603	14.686	15.213

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072225\
Data File : PL096518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2025 17:16
Operator : AR\AJ
Sample : Q2649-05
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/23/2025
Supervised By : mohammad ahmed 07/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 01:49:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

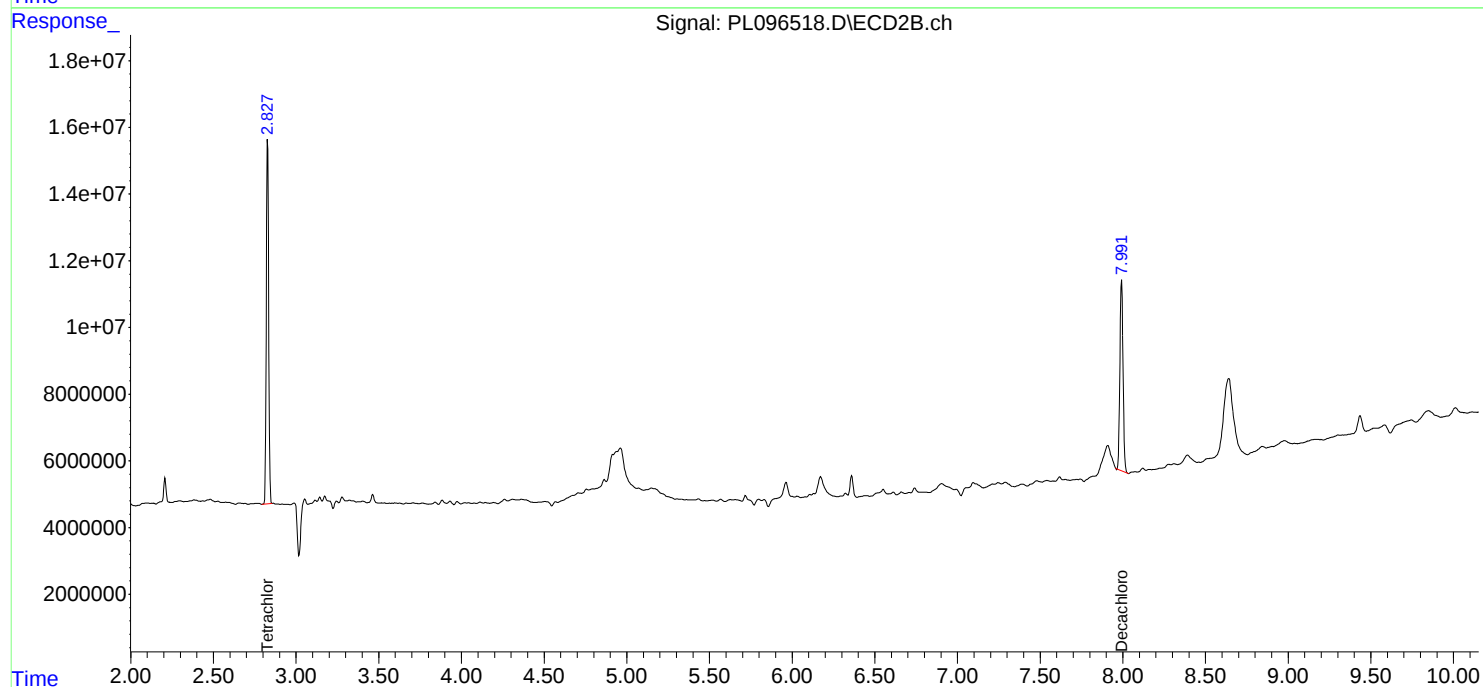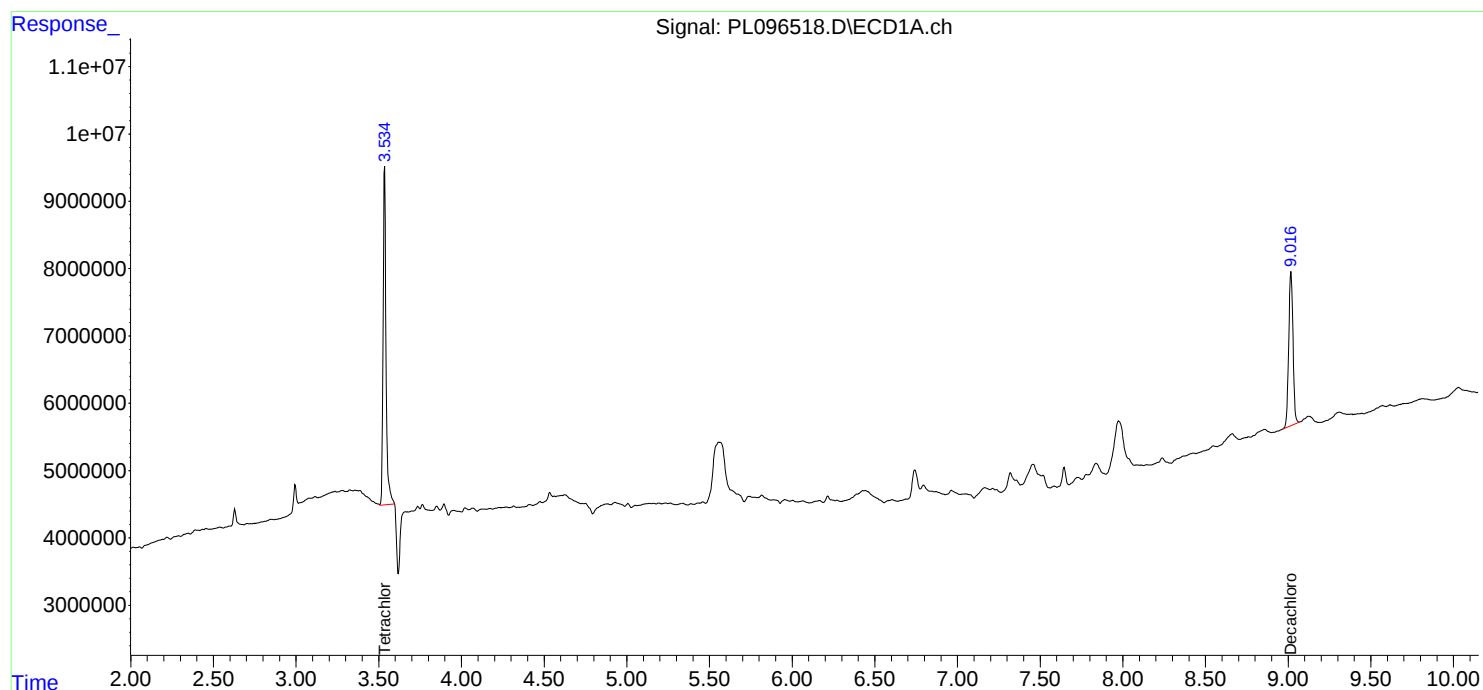

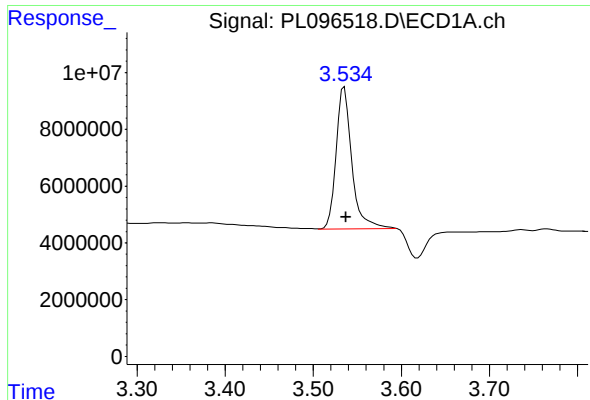


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: -0.003 min
Response: 62258674
Conc: 17.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/23/2025
Supervised By :mohammad ahmed 07/24/2025

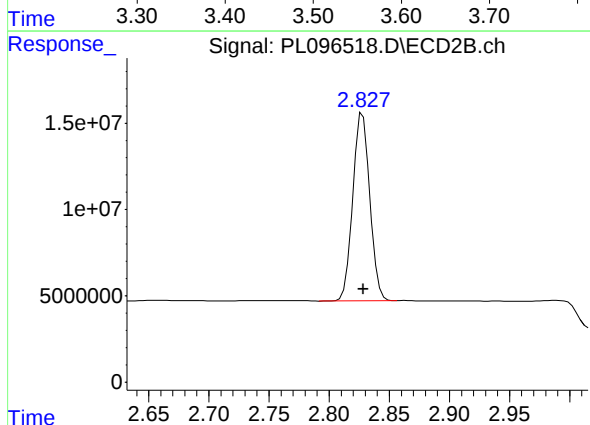


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 107301958
Conc: 18.59 ng/ml

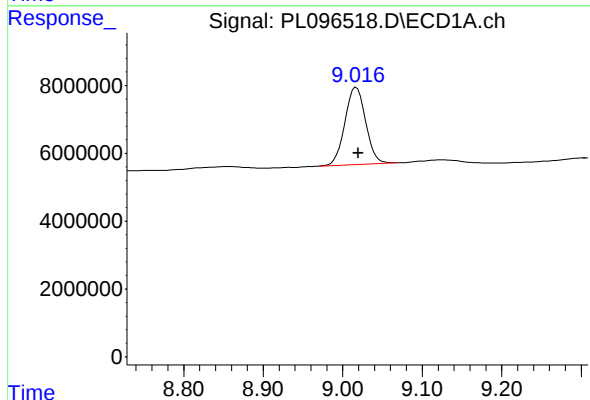

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: -0.003 min
Response: 41313800
Conc: 14.69 ng/ml

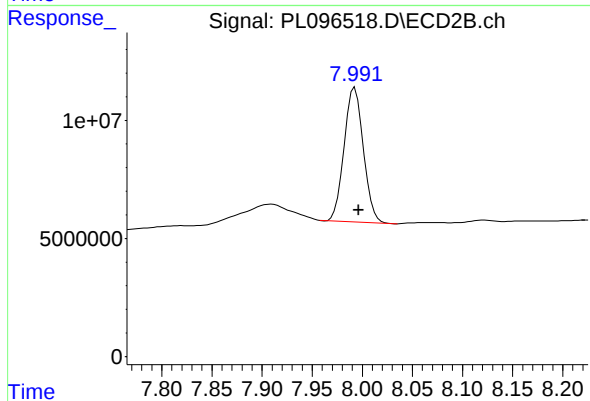

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.004 min
Response: 75861603
Conc: 15.21 ng/ml