

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072318\
 Data File : PL038432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2018 11:45
 Operator : AJ\SJ
 Sample : J3827-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 03:26:57 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.334	3.928	130.6E6	55781879	17.542	21.251
28)	SA Decachlor...	8.003	8.937	139.1E6	49536987	18.338	20.265
Target Compounds							
4)	MA Heptachlor	4.250f	0.000	16583802	0	1.559	N.D. #
6)	B beta-BHC	4.250f	0.000	16583802	0	3.513	N.D. #
7)	B delta-BHC	0.000	4.958	0	7013556	N.D.	2.115 #
14)	MA Endrin	0.000	6.671f	0	5900309	N.D.	2.471 #
15)	B Endosulfa...	6.033f	6.802	20366182	-30908	2.568	N.D. #
16)	A 4,4'-DDD	0.000	6.671f	0	5900309	N.D.	2.757 #
23)	Chlordane-1	0.000	4.958	0	7013556	N.D.	60.522 #
27)	Chlordane-5	0.000	6.829	0	1015419	N.D.	11.335 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072318\
Data File : PL038432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2018 11:45
Operator : AJ\SJ
Sample : J3827-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 03:26:57 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

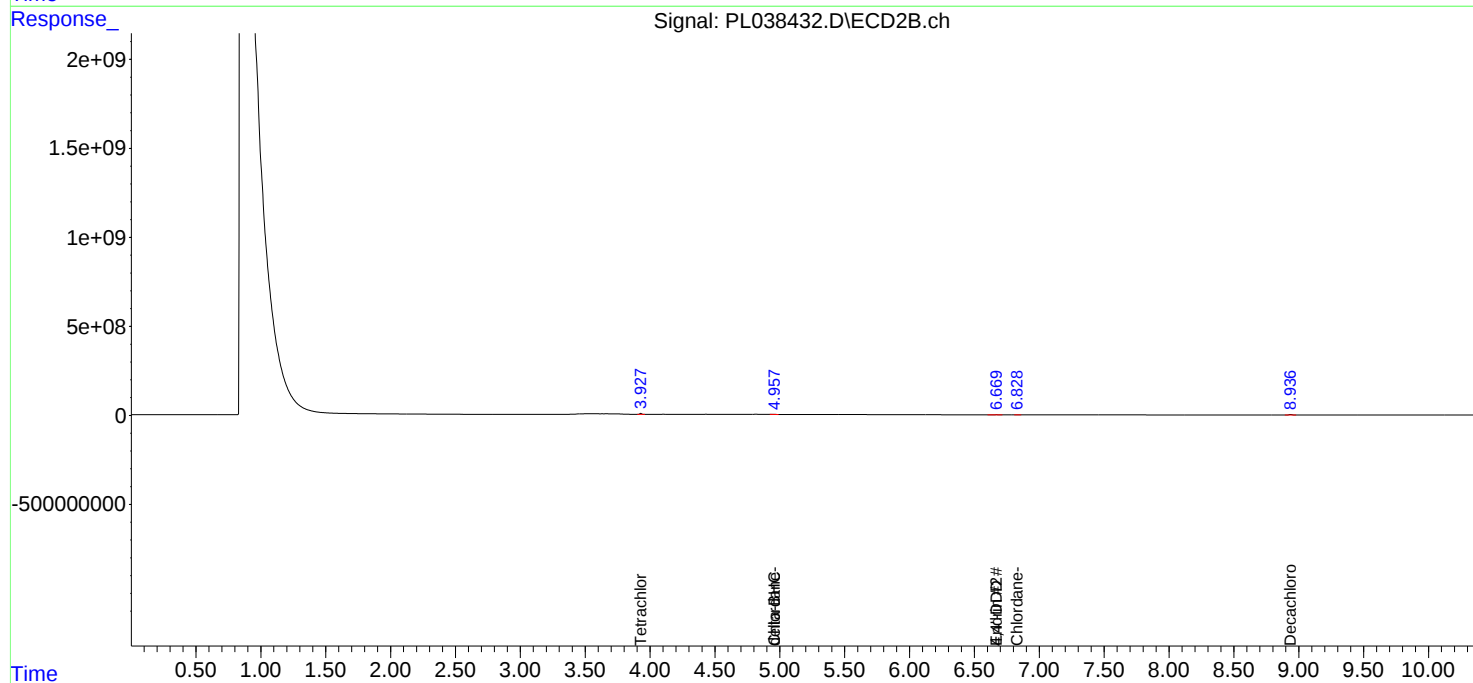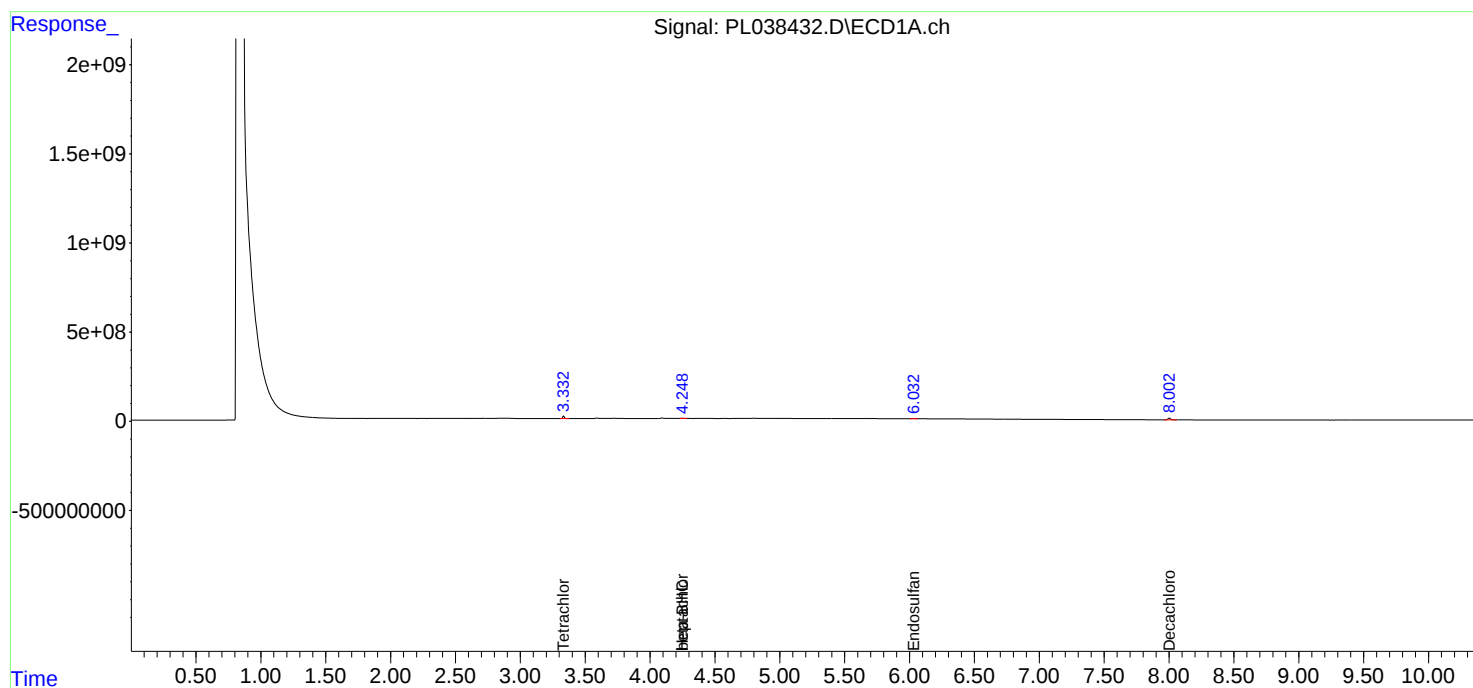


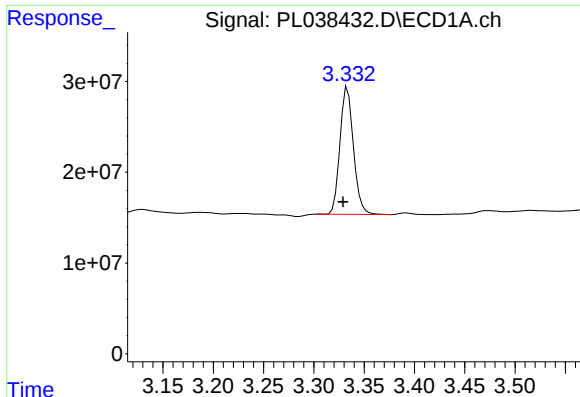

#1 Tetrachloro-m-xylene


R.T.: 3.334 min
Delta R.T.: 0.005 min
Response: 130624752
Conc: 17.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

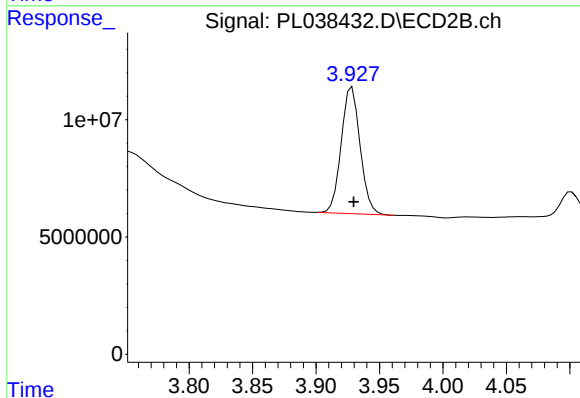


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.001 min
Response: 55781879
Conc: 21.25 ng/ml

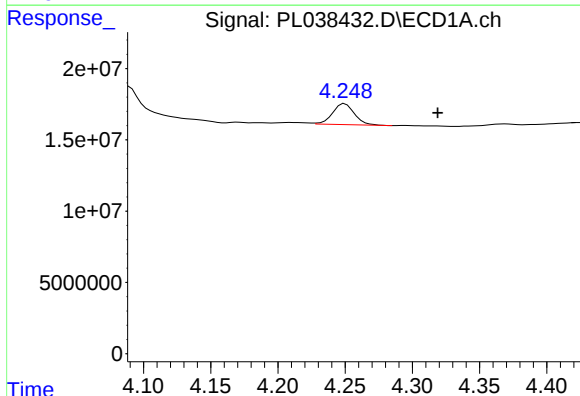


#4 Heptachlor

R.T.: 4.250 min
Delta R.T.: -0.069 min
Response: 16583802
Conc: 1.56 ng/ml

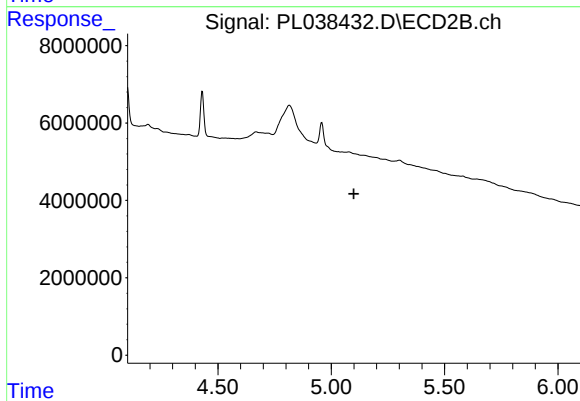

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.099 min
Response: 0
Conc: N.D.

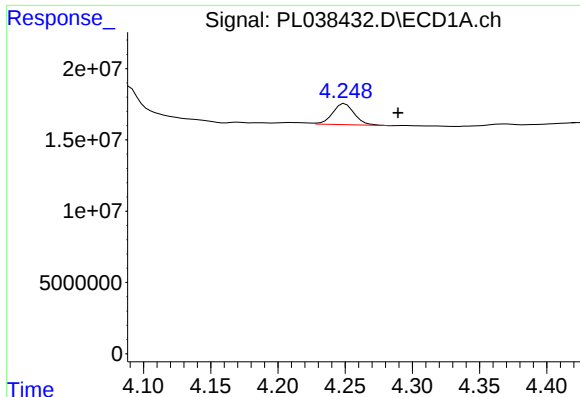

#6 beta-BHC


R.T.: 4.250 min
Delta R.T.: -0.040 min
Response: 16583802
Conc: 3.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

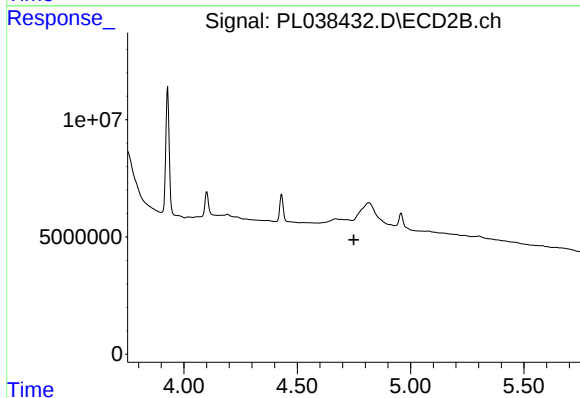


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

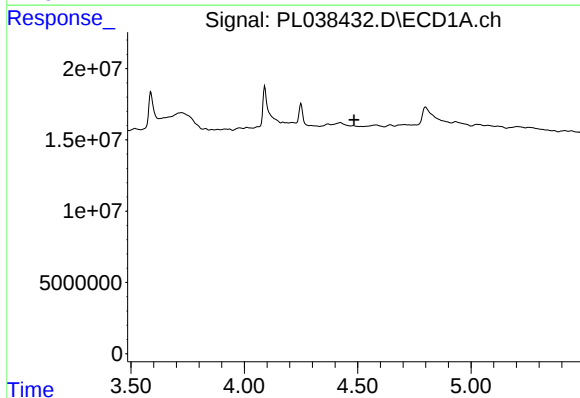


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

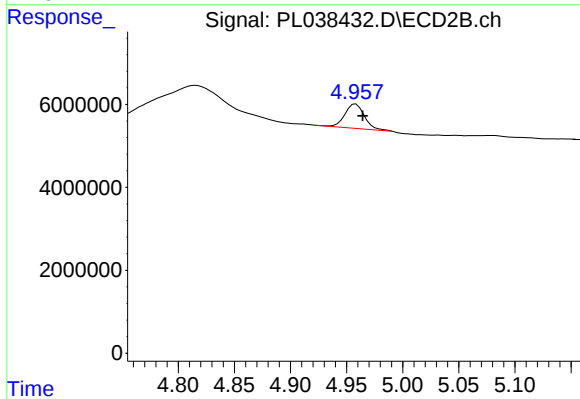

#7 delta-BHC


R.T.: 4.958 min
Delta R.T.: -0.006 min
Response: 7013556
Conc: 2.11 ng/ml

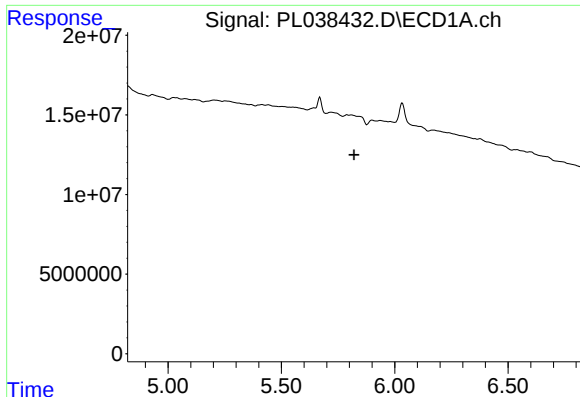

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

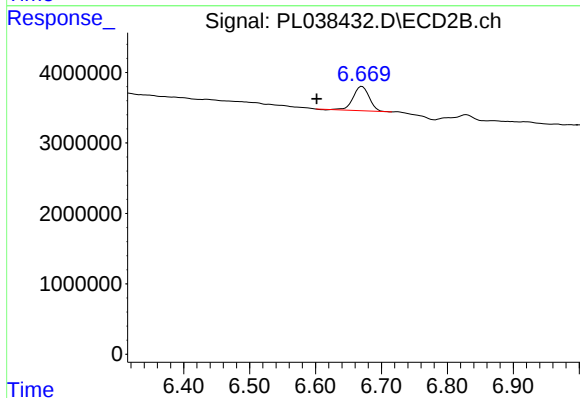


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.069 min
Response: 5900309
Conc: 2.47 ng/ml

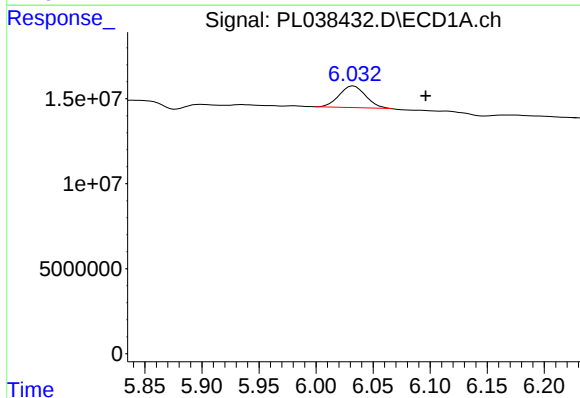


#15 Endosulfan II

R.T.: 6.033 min
Delta R.T.: -0.063 min
Response: 20366182
Conc: 2.57 ng/ml

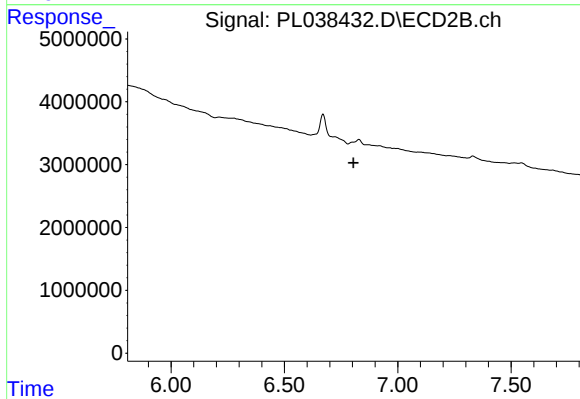

#15 Endosulfan II


R.T.: 6.802 min
Delta R.T.: -0.003 min
Response: -30908
Conc: N.D.

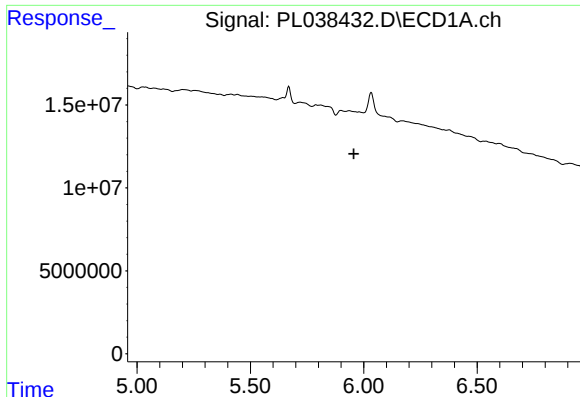

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

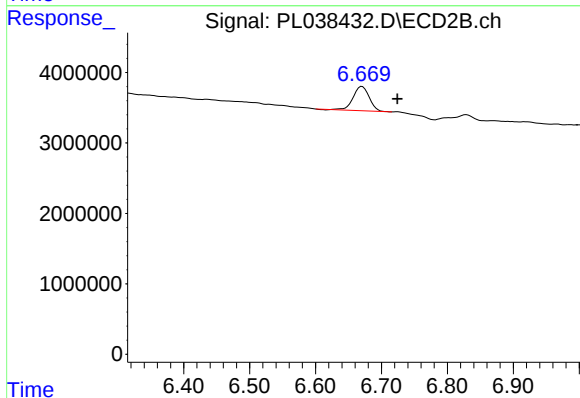


#16 4,4'-DDD

R.T.: 6.671 min
Delta R.T.: -0.054 min
Response: 5900309
Conc: 2.76 ng/ml

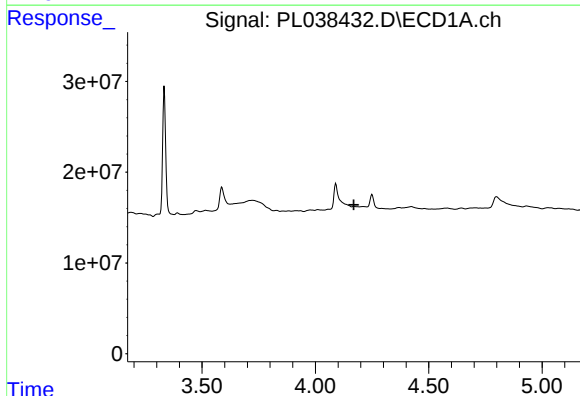


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.169 min
Response: 0
Conc: N.D.

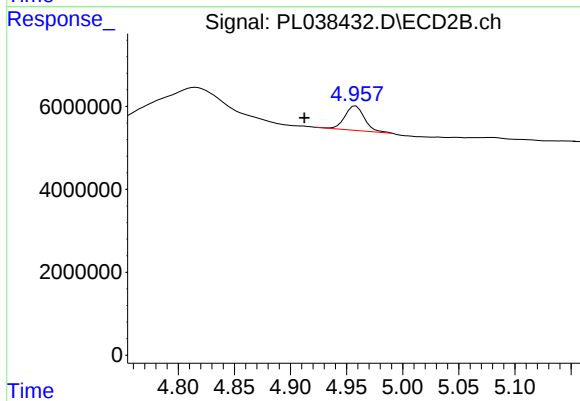

#23 Chlordane-1


R.T.: 4.958 min
Delta R.T.: 0.046 min
Response: 7013556
Conc: 60.52 ng/ml

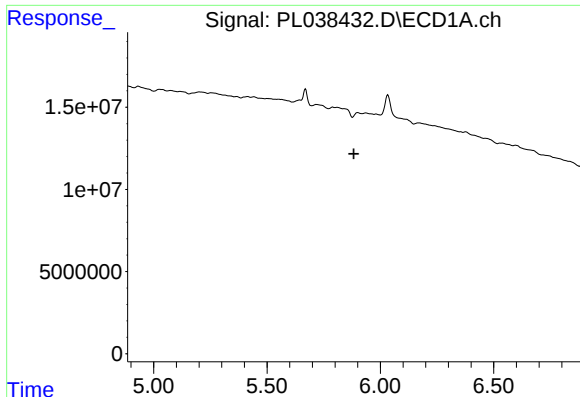

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

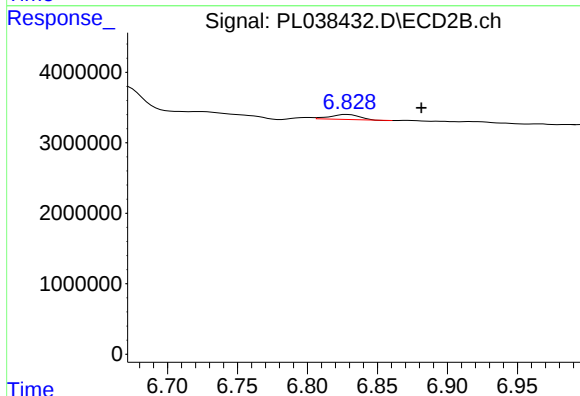


#27 Chlordane-5

R.T.: 6.829 min
Delta R.T.: -0.053 min
Response: 1015419
Conc: 11.34 ng/ml

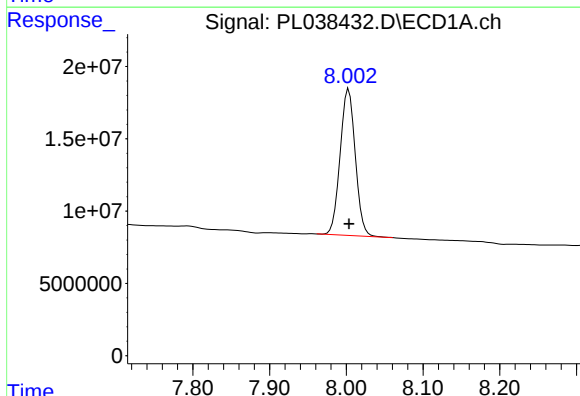

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 139107347
Conc: 18.34 ng/ml

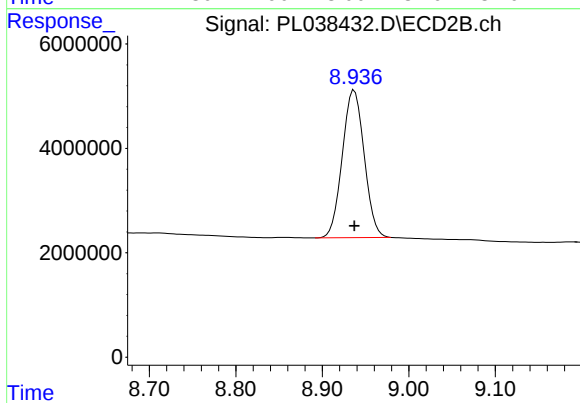

#28 Decachlorobiphenyl

R.T.: 8.937 min
Delta R.T.: 0.000 min
Response: 49536987
Conc: 20.27 ng/ml