

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072318\
 Data File : PL038434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2018 12:14
 Operator : AJ\SJ
 Sample : J4062-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 03:27:23 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.929	130.9E6	56329384	17.575	21.459
28)	SA Decachlor...	7.995	8.935	133.5E6	49226518	17.592	20.138
Target Compounds							
2)	A alpha-BHC	0.000	4.321	0	1031906	N.D.	0.267 #
3)	MA gamma-BHC...	4.082f	0.000	43418936	0	4.142	N.D. #
6)	B beta-BHC	4.241f	0.000	18422249	0	3.903	N.D. #
7)	B delta-BHC	0.000	4.957	0	5502118	N.D.	1.659 #
15)	B Endosulfa...	6.030f	6.804	8987809	-394678	1.133	N.D. #
16)	A 4,4'-DDD	0.000	6.675f	0	3416261	N.D.	1.596 #
19)	B Endosulfa...	6.538f	0.000	29023955	0	3.843	N.D. #
23)	Chlordane-1	0.000	4.957	0	5502118	N.D.	47.479 #
27)	Chlordane-5	0.000	6.827	0	282022	N.D.	3.148 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072318\
Data File : PL038434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2018 12:14
Operator : AJ\SJ
Sample : J4062-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 03:27:23 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

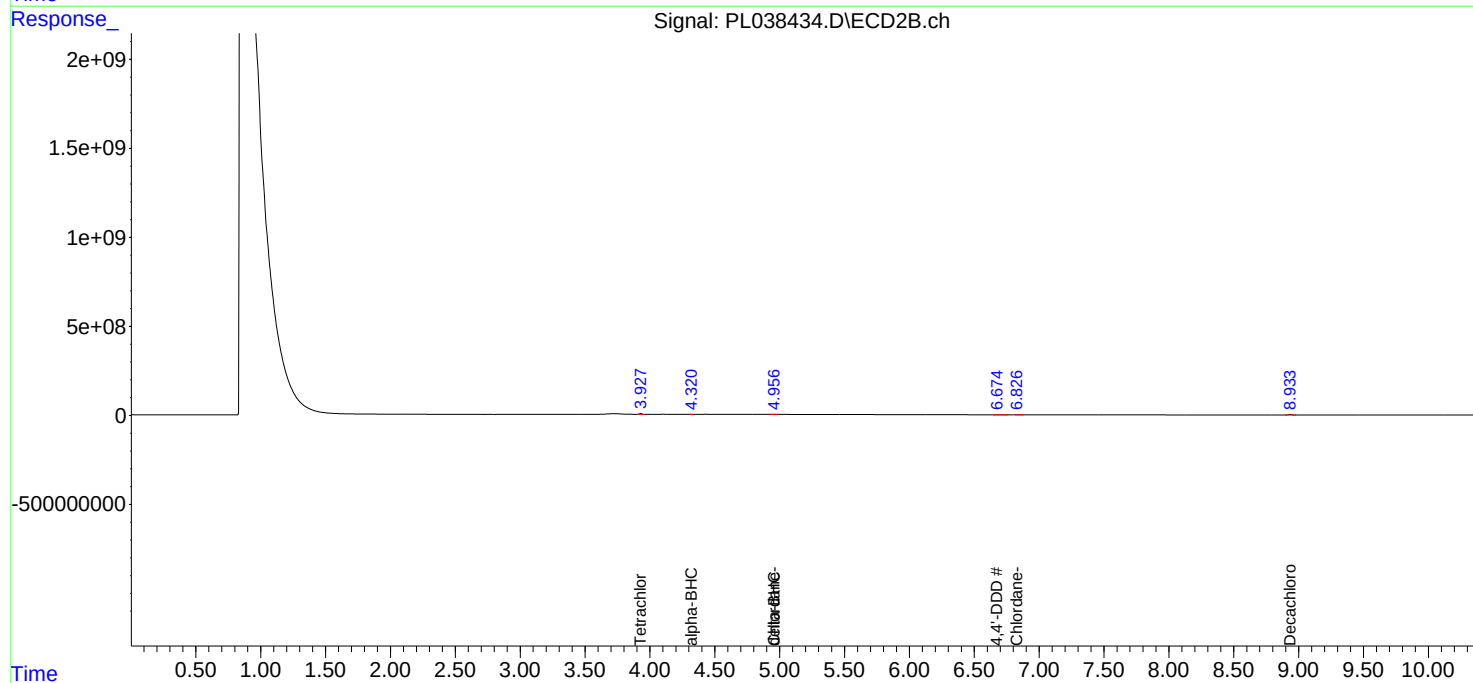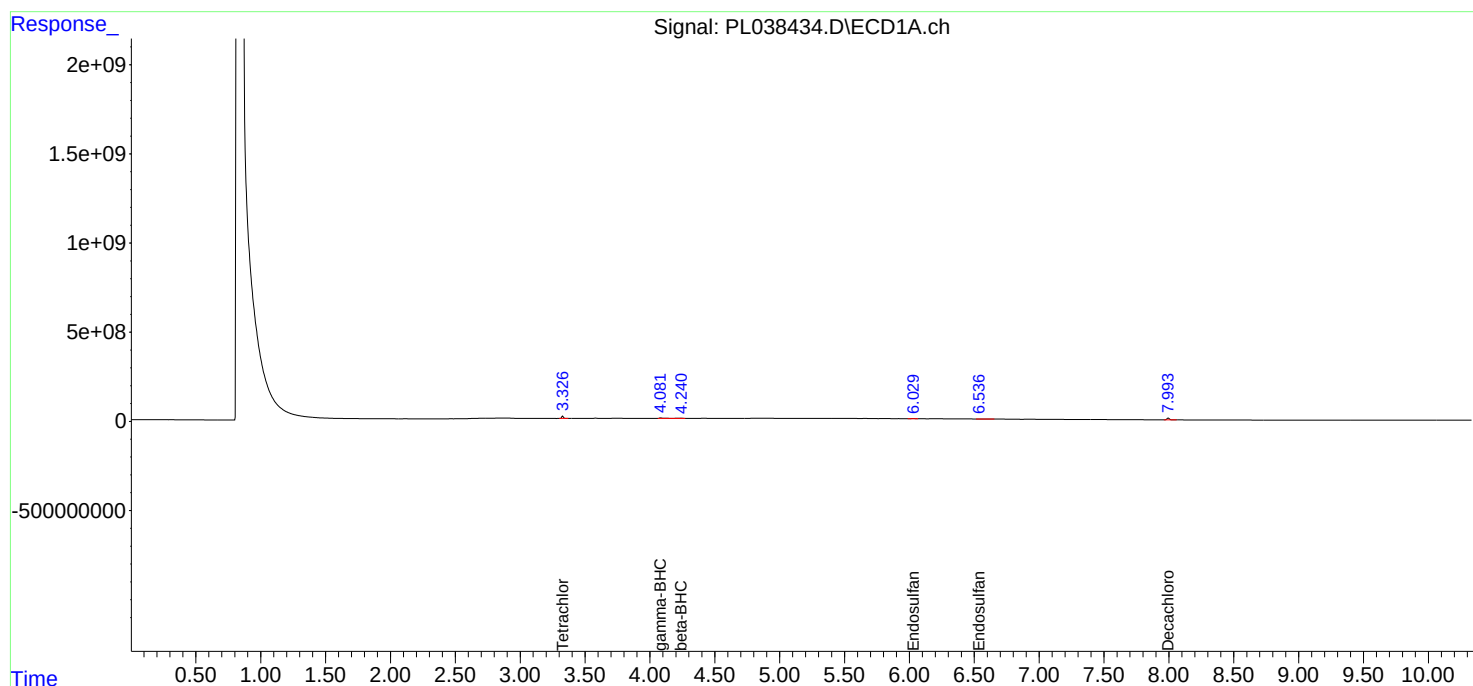


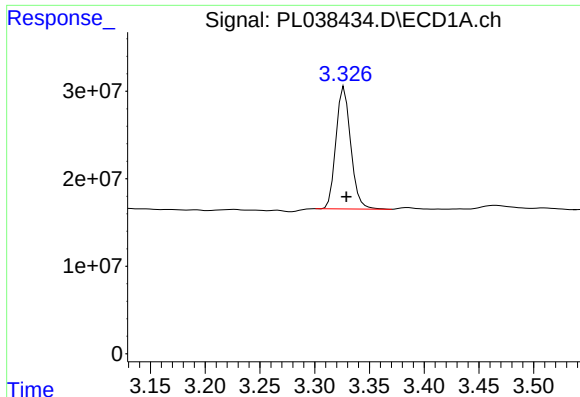

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: -0.002 min
Response: 130870847
Conc: 17.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

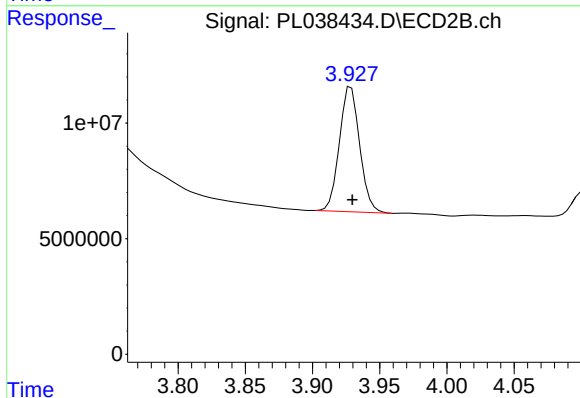


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.001 min
Response: 56329384
Conc: 21.46 ng/ml

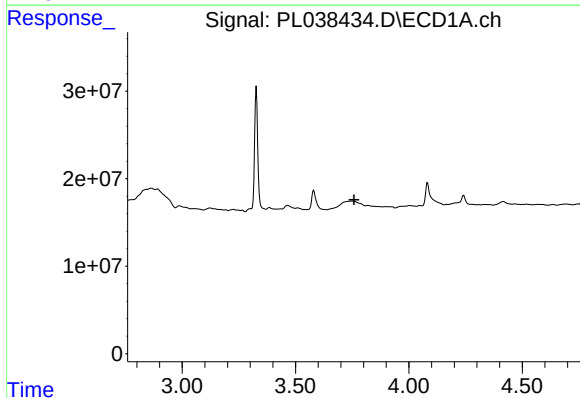


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

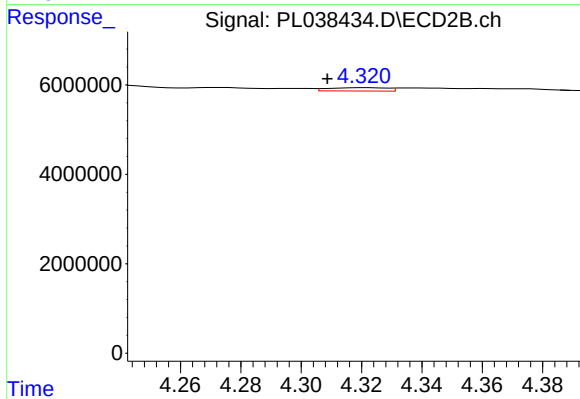

#2 alpha-BHC


R.T.: 4.321 min
Delta R.T.: 0.013 min
Response: 1031906
Conc: 0.27 ng/ml

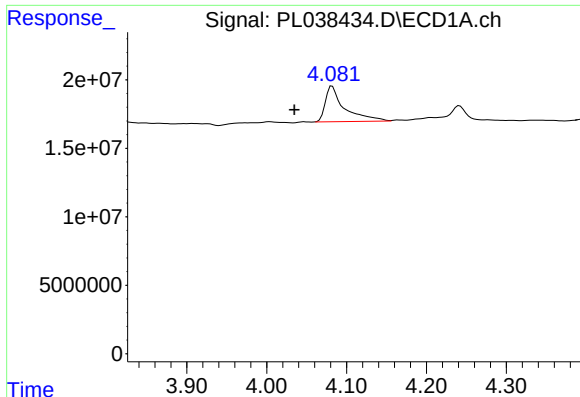

#3 gamma-BHC (Lindane)


R.T.: 4.082 min
Delta R.T.: 0.047 min
Response: 43418936
Conc: 4.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

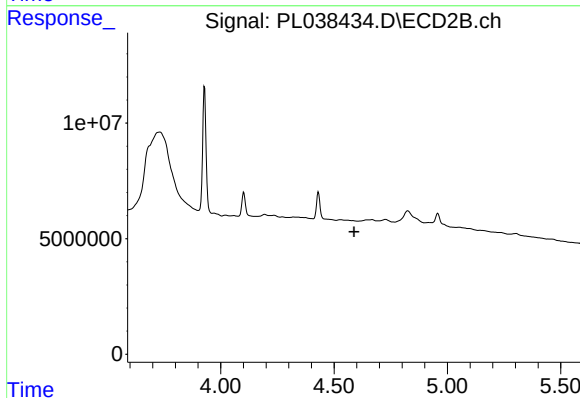


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.588 min
Response: 0
Conc: N.D.

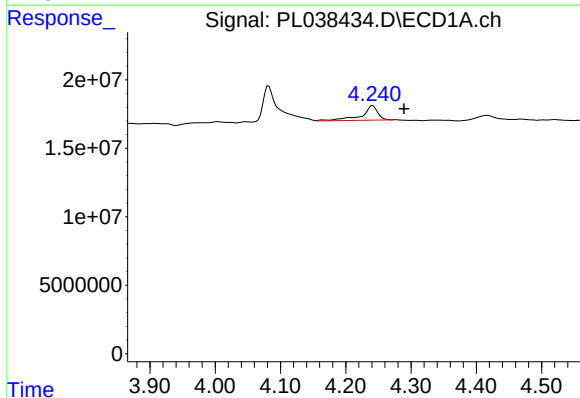


#6 beta-BHC

R.T.: 4.241 min
Delta R.T.: -0.048 min
Response: 18422249
Conc: 3.90 ng/ml

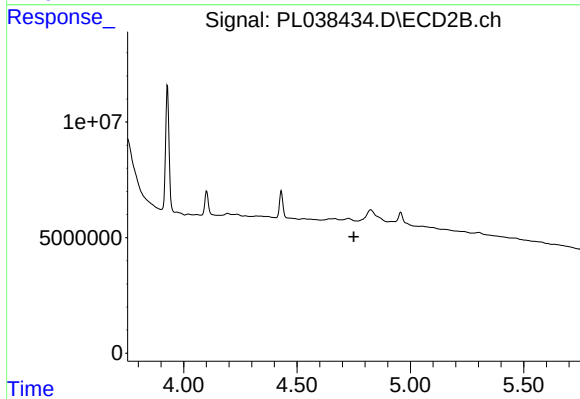

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

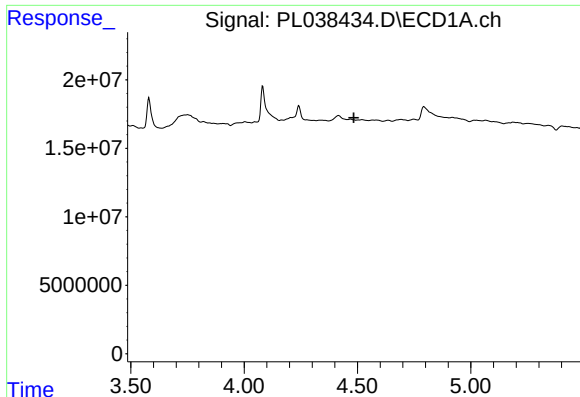

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

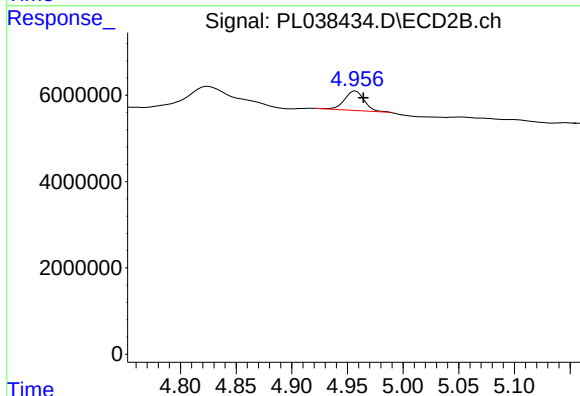


#7 delta-BHC

R.T.: 4.957 min
Delta R.T.: -0.007 min
Response: 5502118
Conc: 1.66 ng/ml

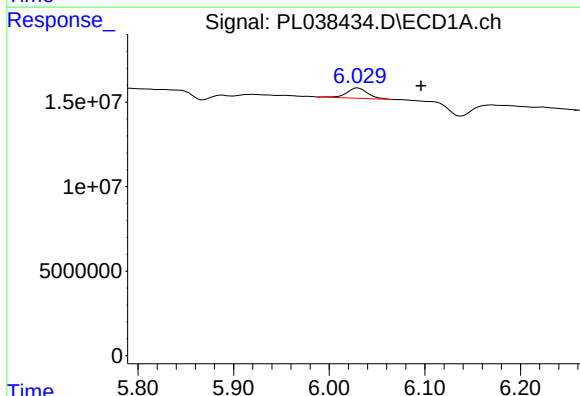


#15 Endosulfan II

R.T.: 6.030 min
Delta R.T.: -0.066 min
Response: 8987809
Conc: 1.13 ng/ml

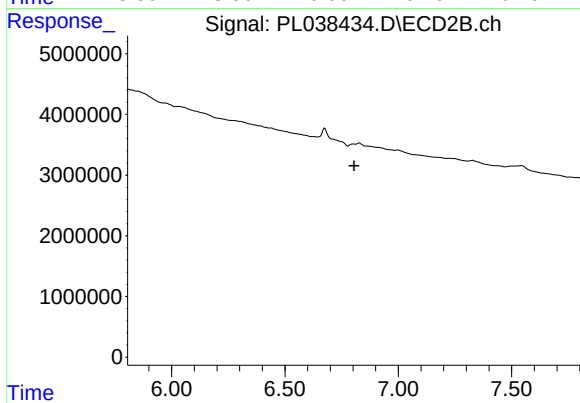

#15 Endosulfan II


R.T.: 6.804 min
Delta R.T.: -0.001 min
Response: -394678
Conc: N.D.

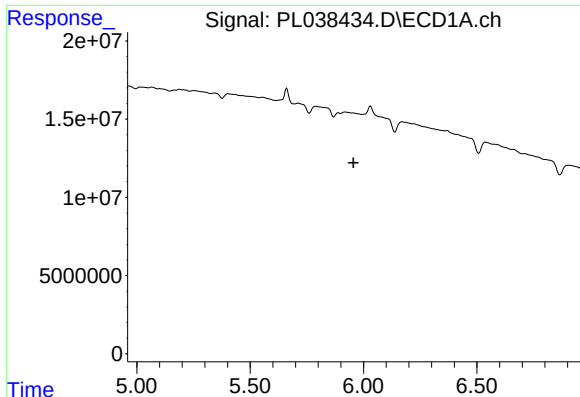

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

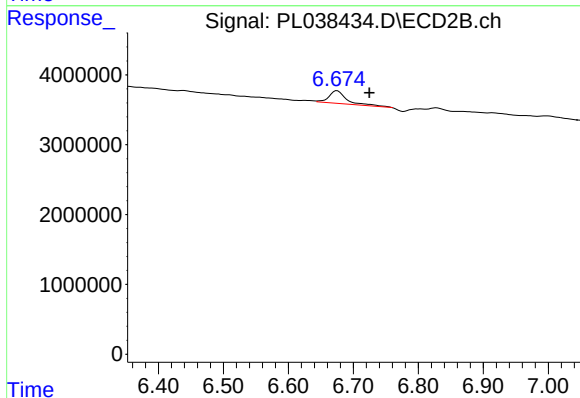


#16 4,4'-DDD

R.T.: 6.675 min
Delta R.T.: -0.050 min
Response: 3416261
Conc: 1.60 ng/ml

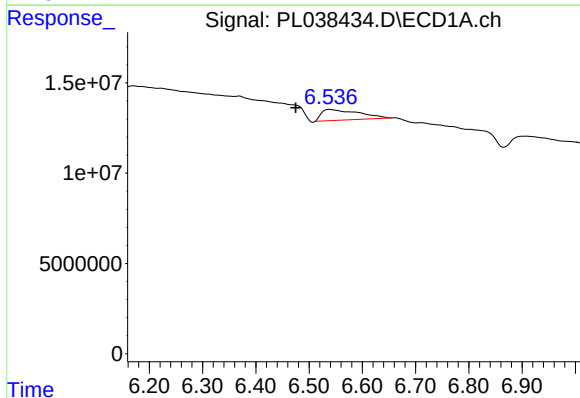


#19 Endosulfan Sulfate

R.T.: 6.538 min
Delta R.T.: 0.063 min
Response: 29023955
Conc: 3.84 ng/ml

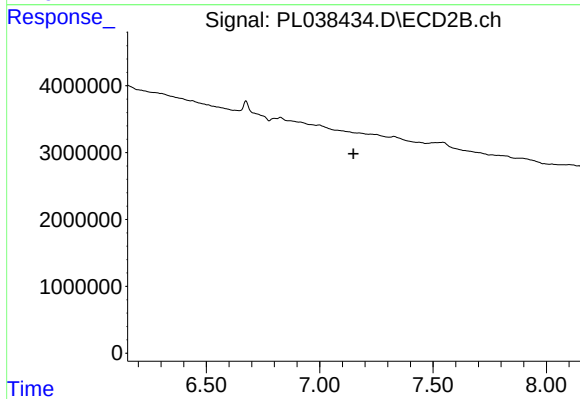

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.149 min
Response: 0
Conc: N.D.

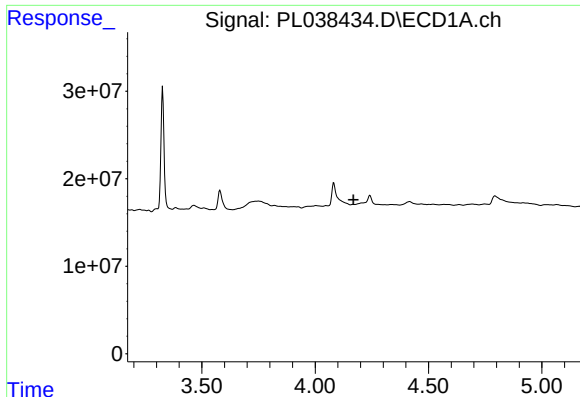

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

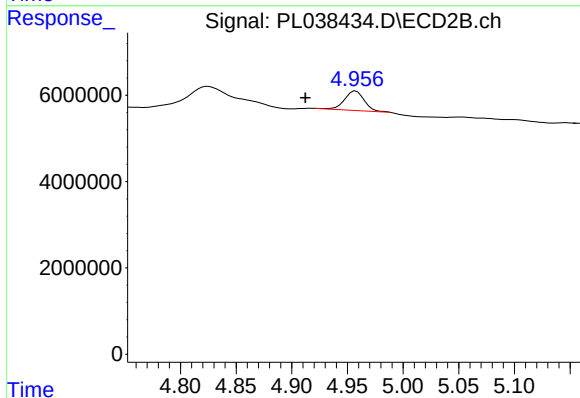


#23 Chlordane-1

R.T.: 4.957 min
Delta R.T.: 0.045 min
Response: 5502118
Conc: 47.48 ng/ml

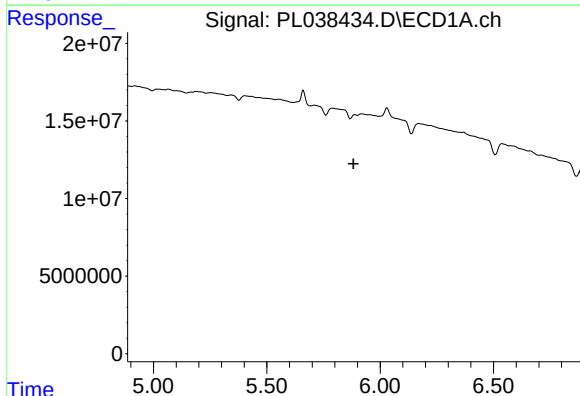


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.883 min
Response: 0
Conc: N.D.

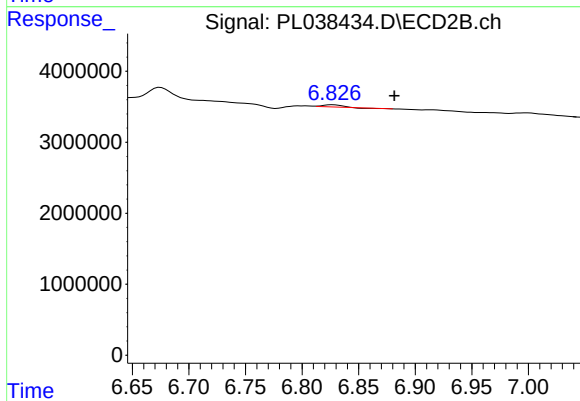

#27 Chlordane-5


R.T.: 6.827 min
Delta R.T.: -0.054 min
Response: 282022
Conc: 3.15 ng/ml

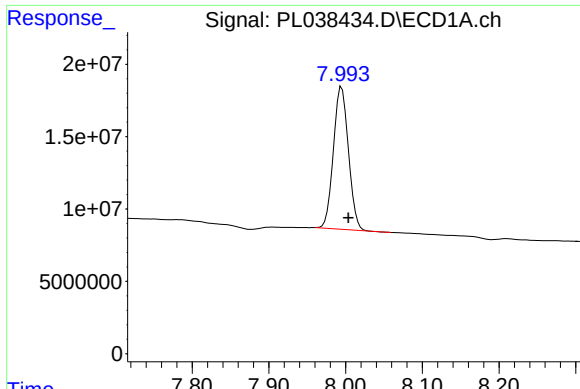

#28 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: -0.009 min
Response: 133451449
Conc: 17.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

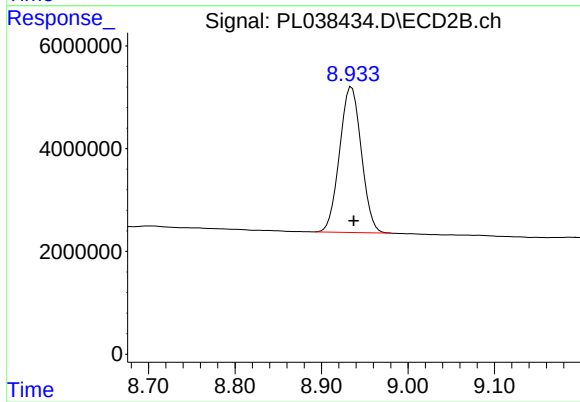

#28 Decachlorobiphenyl

R.T.: 8.935 min
Delta R.T.: -0.002 min
Response: 49226518
Conc: 20.14 ng/ml