

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072319\
 Data File : PL050723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2019 16:42
 Operator : SM\AJ
 Sample : K3934-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Ankita
 7/24/2019 11:06:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 01:10:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.929	96366808	26410890	9.591m	9.257
28)	SA Decachlor...	7.980	8.960	131.6E6	36221584	12.992	12.809

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072319\
Data File : PL050723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2019 16:42
Operator : SM\AJ
Sample : K3934-16
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-3


Manual Integrations
APPROVED

Ankita
7/24/2019 11:06:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 01:10:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

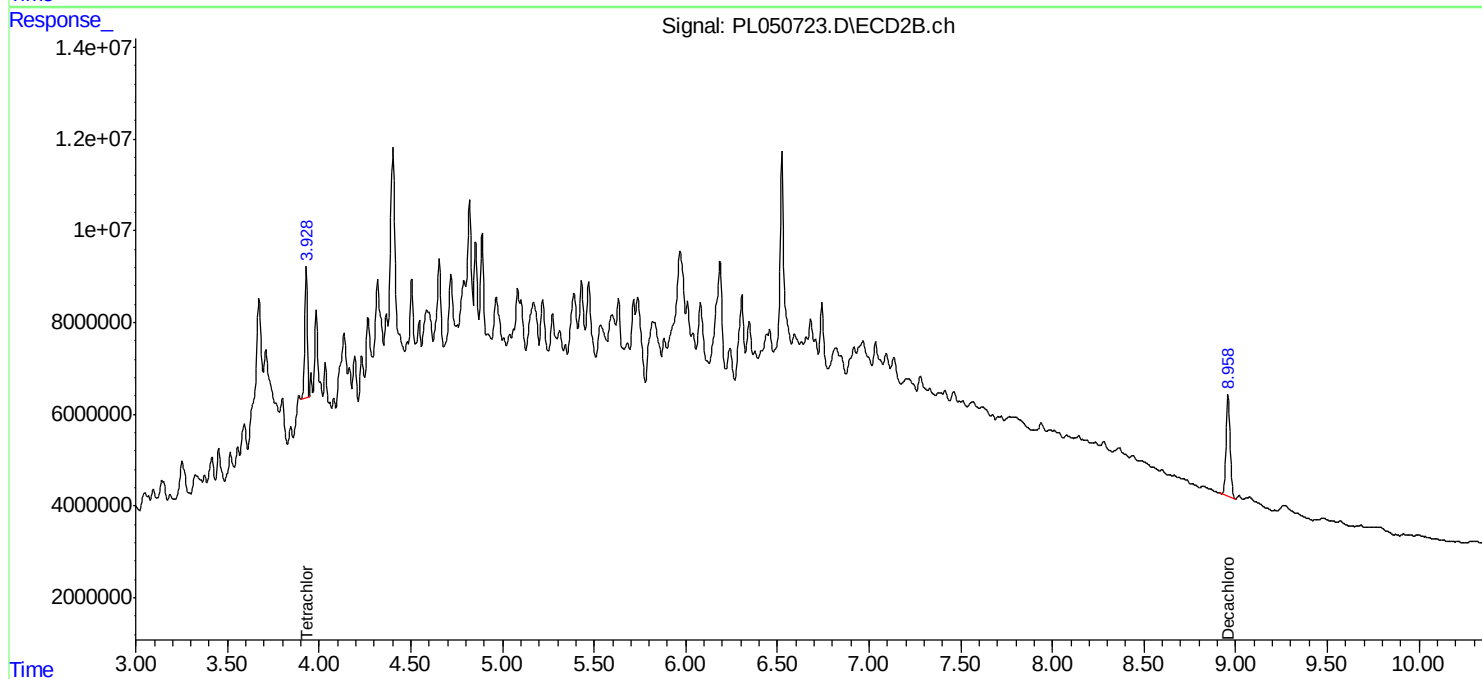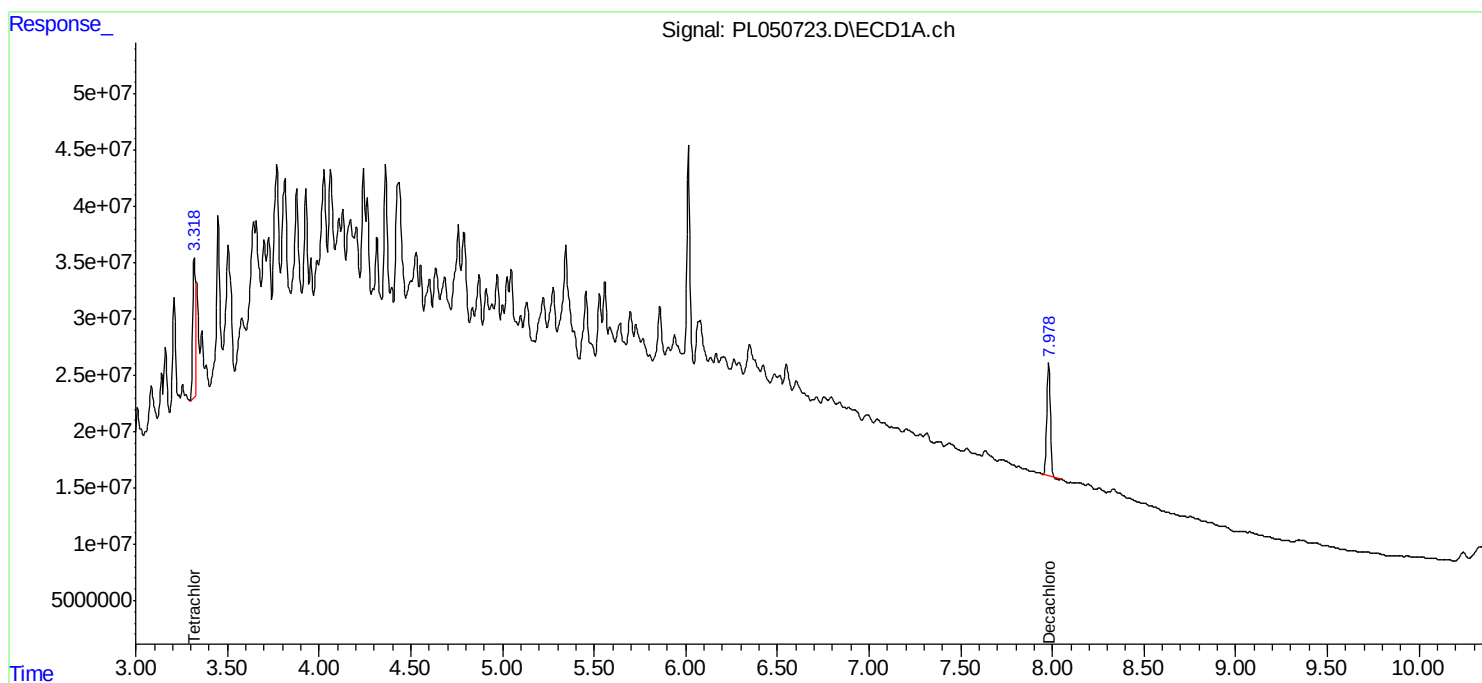

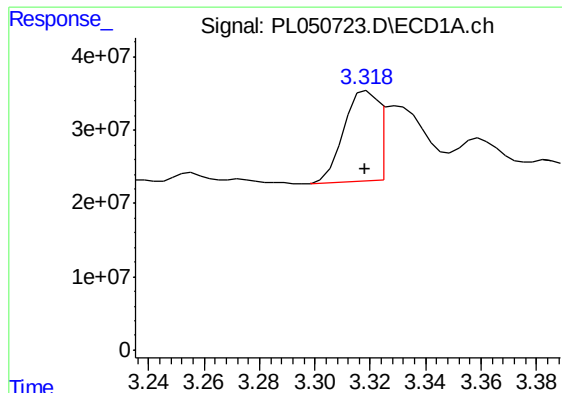


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 96366808
Conc: 9.59 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
7/24/2019 11:06:29 AM

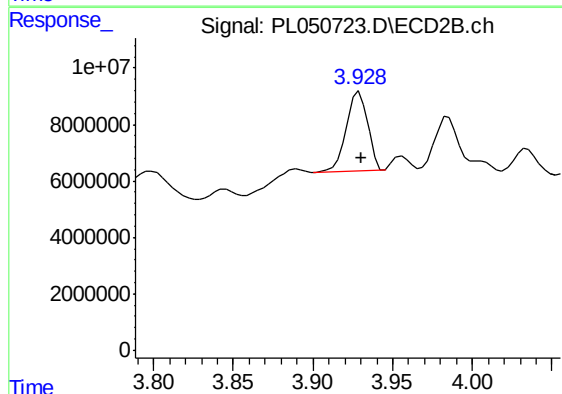


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.001 min
Response: 26410890
Conc: 9.26 ng/ml

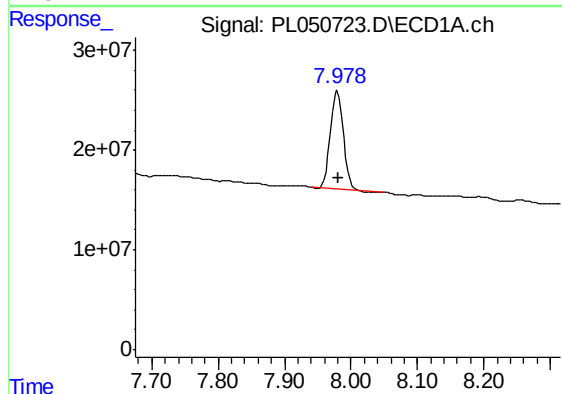

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 131550492
Conc: 12.99 ng/ml

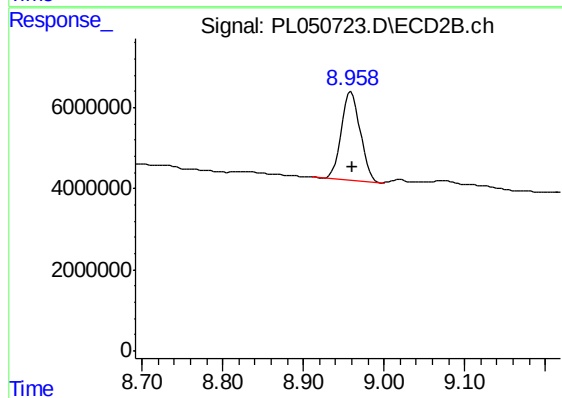

#28 Decachlorobiphenyl

R.T.: 8.960 min
Delta R.T.: -0.002 min
Response: 36221584
Conc: 12.81 ng/ml