

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072320\
 Data File : PL060122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2020 10:15
 Operator : DD\AJ
 Sample : L3370-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 01:56:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.014	37837780	49696573	19.562	18.752
28)	SA Decachlor...	8.232	9.107	20955343	25699807	12.738	12.288
Target Compounds							
4)	MA Heptachlor	0.000	5.203	0	3809307	N.D.	1.132 #
6)	B beta-BHC	4.421f	4.882f	2106945	7642017	2.063	5.055 #
8)	B Heptachlo...	0.000	5.886	0	22276012	N.D.	8.271 #
10)	B gamma-Chl...	0.000	6.141	0	2727346	N.D.	0.952 #
15)	B Endosulfa...	0.000	6.949	0	2348380	N.D.	0.935 #
16)	A 4,4'-DDD	0.000	6.870f	0	936350	N.D.	0.408 #
17)	MA 4,4'-DDT	0.000	7.160	0	992918	N.D.	0.504 #
18)	B Endrin al...	0.000	7.063	0	2848508	N.D.	1.312 #
21)	B Endrin ke...	0.000	7.758	0	2535210	N.D.	0.982 #
25)	Chlordane-3	0.000	6.141	0	2727346	N.D.	7.049 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072320\
Data File : PL060122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2020 10:15
Operator : DD\AJ
Sample : L3370-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-3-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 01:56:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

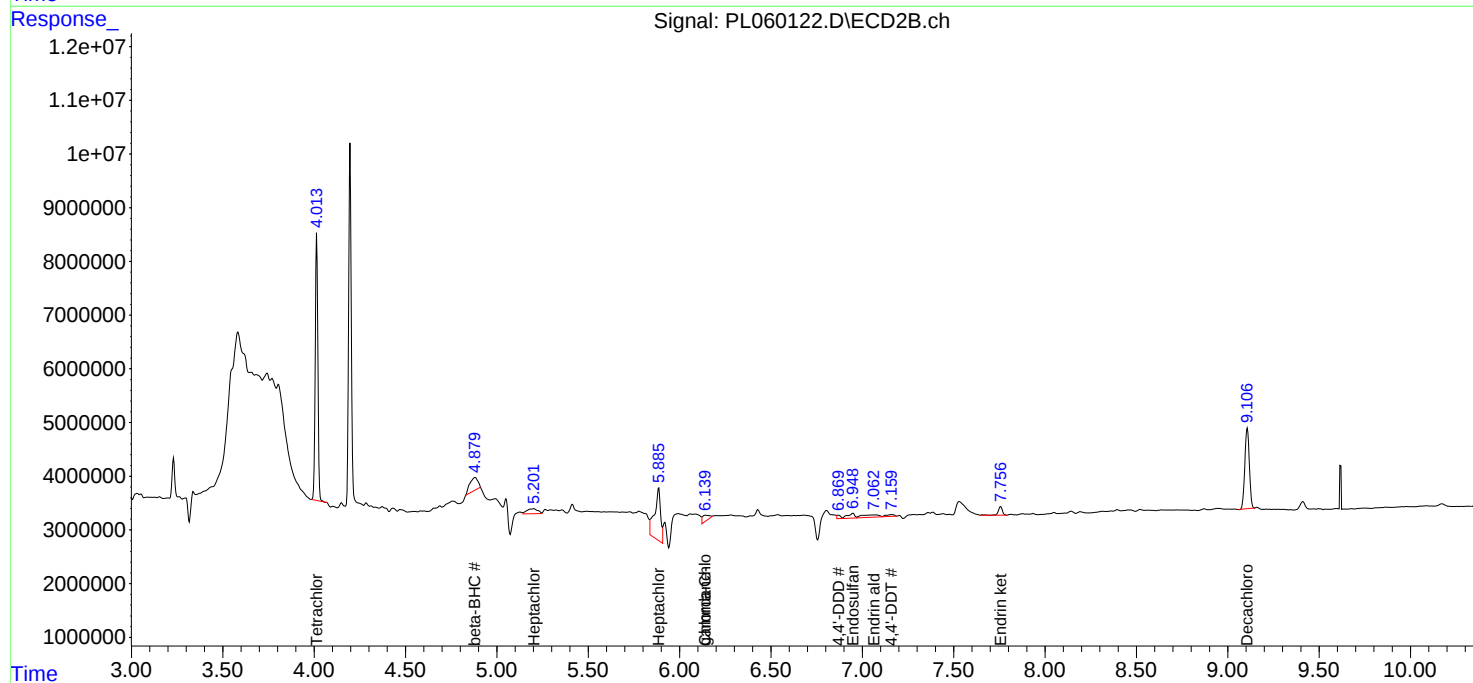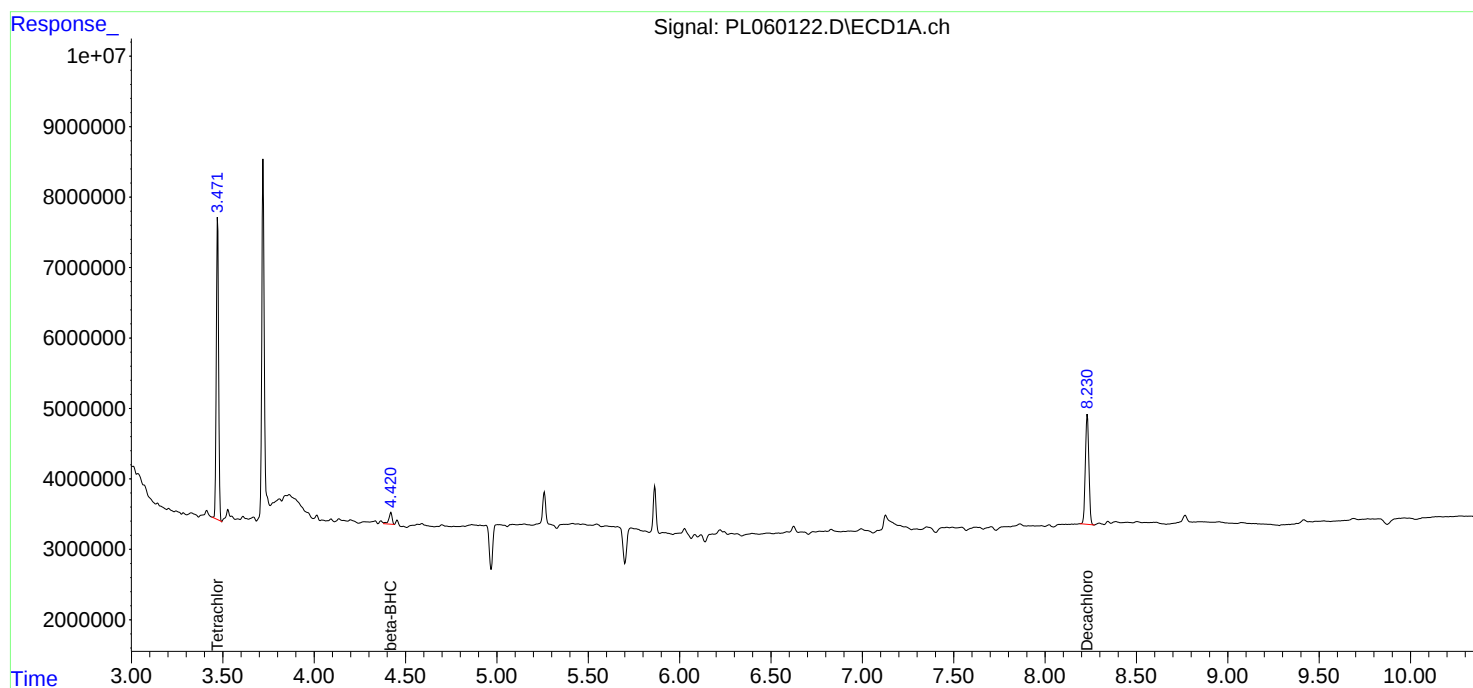


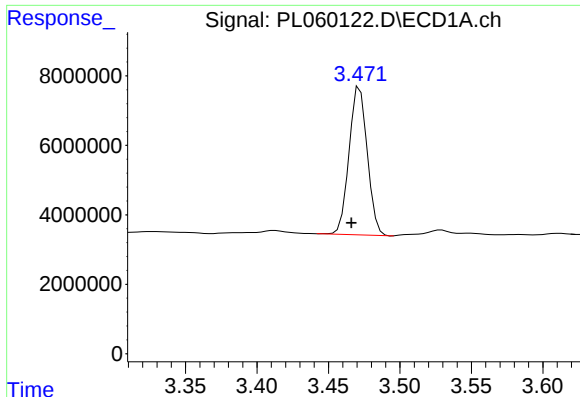

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: 0.006 min
Response: 37837780
Conc: 19.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-D

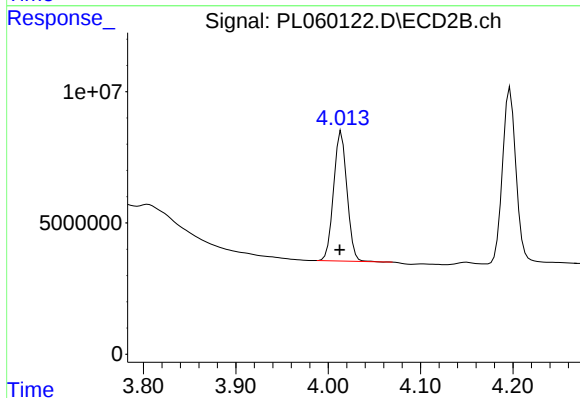


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.002 min
Response: 49696573
Conc: 18.75 ng/ml

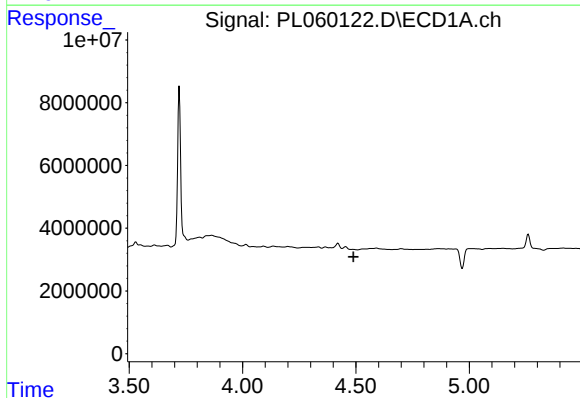


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

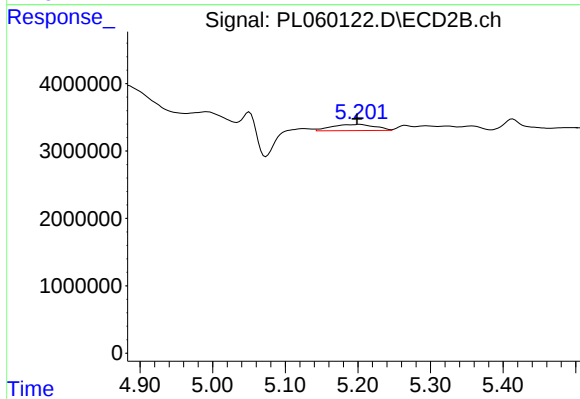

#4 Heptachlor


R.T.: 5.203 min
Delta R.T.: 0.004 min
Response: 3809307
Conc: 1.13 ng/ml

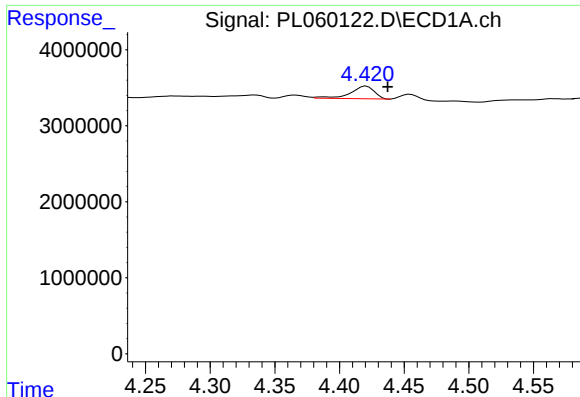

#6 beta-BHC


R.T.: 4.421 min
Delta R.T.: -0.016 min
Response: 2106945
Conc: 2.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-D

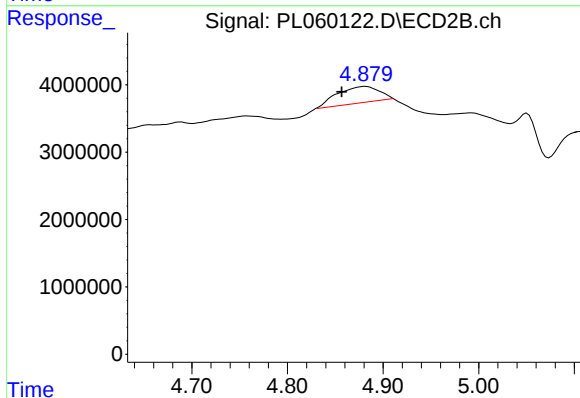


#6 beta-BHC

R.T.: 4.882 min
Delta R.T.: 0.025 min
Response: 7642017
Conc: 5.05 ng/ml

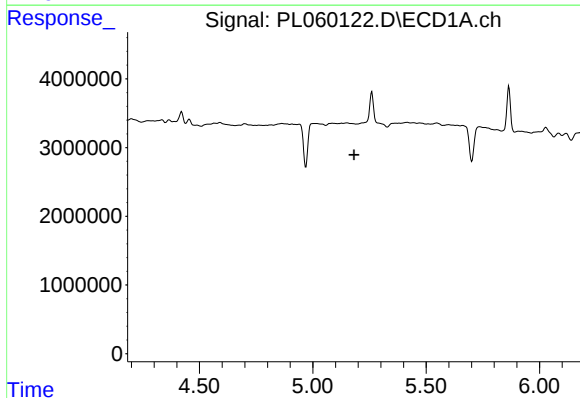


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.183 min
Response: 0
Conc: N.D.

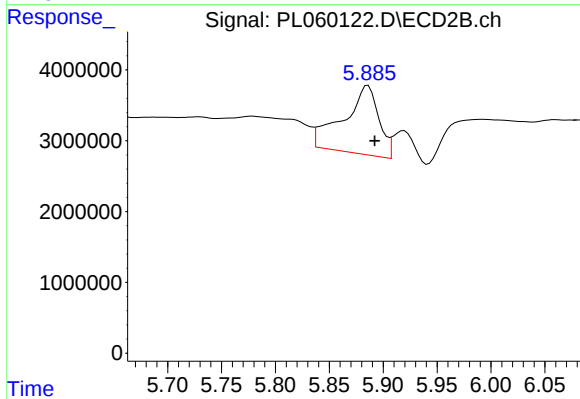

#8 Heptachlor epoxide


R.T.: 5.886 min
Delta R.T.: -0.006 min
Response: 22276012
Conc: 8.27 ng/ml

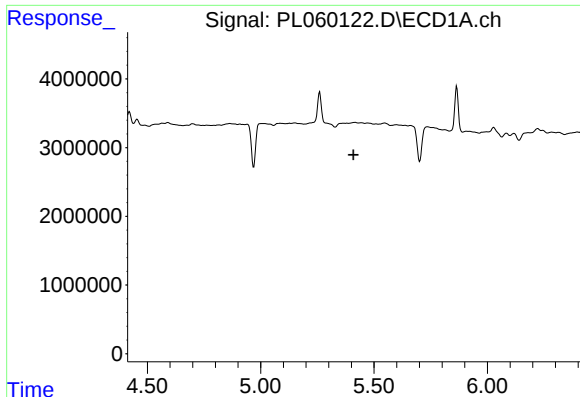

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3-D

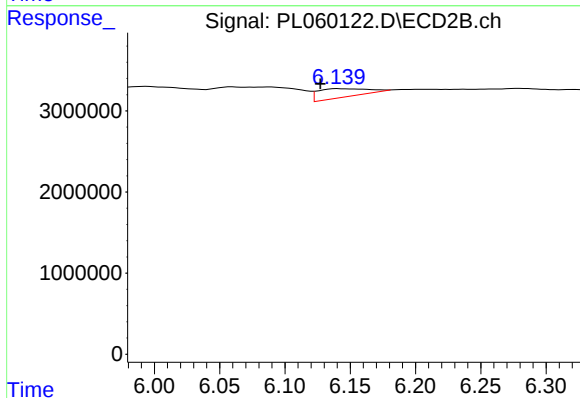


#10 gamma-Chlordane

R.T.: 6.141 min
Delta R.T.: 0.014 min
Response: 2727346
Conc: 0.95 ng/ml

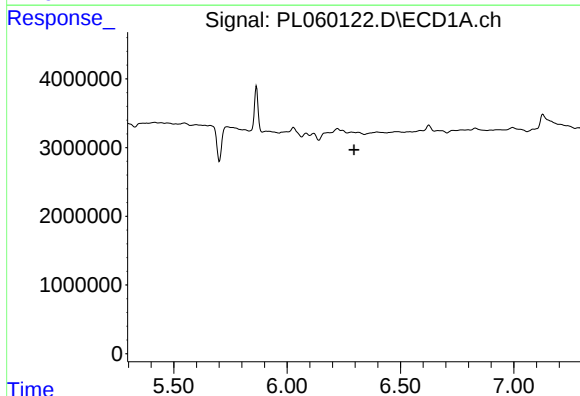


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.296 min
Response: 0
Conc: N.D.

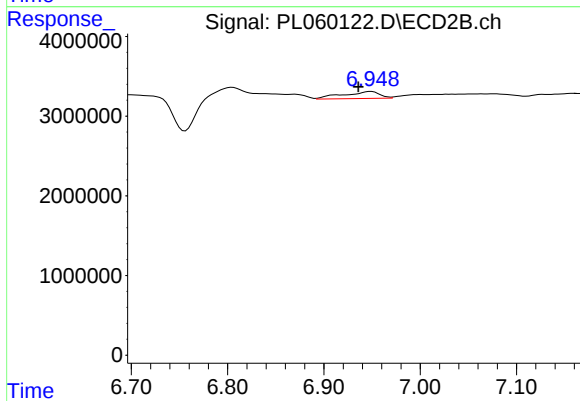

#15 Endosulfan II


R.T.: 6.949 min
Delta R.T.: 0.013 min
Response: 2348380
Conc: 0.94 ng/ml

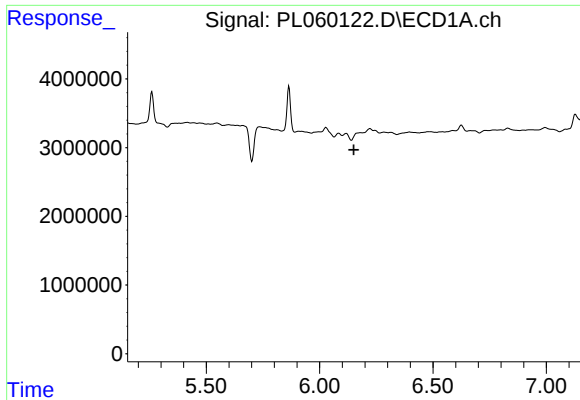

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3-D

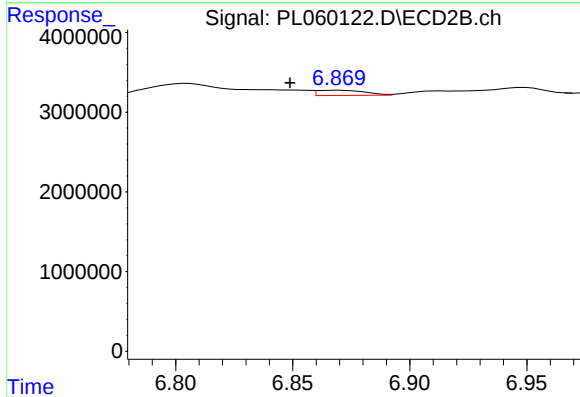


#16 4,4'-DDD

R.T.: 6.870 min
Delta R.T.: 0.021 min
Response: 936350
Conc: 0.41 ng/ml

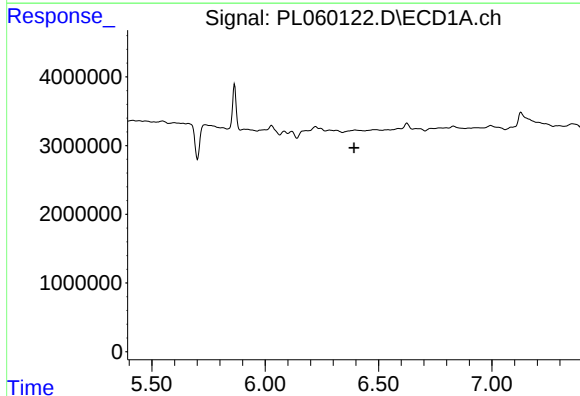


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.392 min
Response: 0
Conc: N.D.

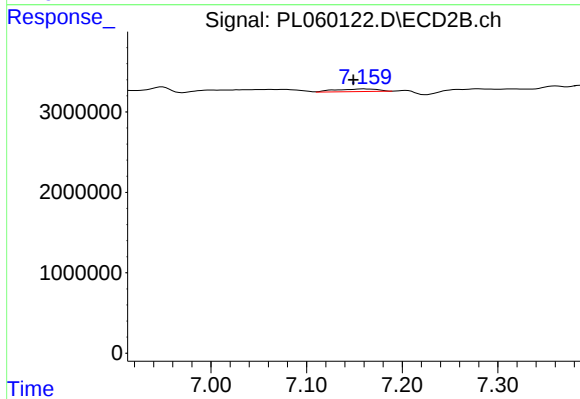

#17 4,4'-DDT


R.T.: 7.160 min
Delta R.T.: 0.011 min
Response: 992918
Conc: 0.50 ng/ml

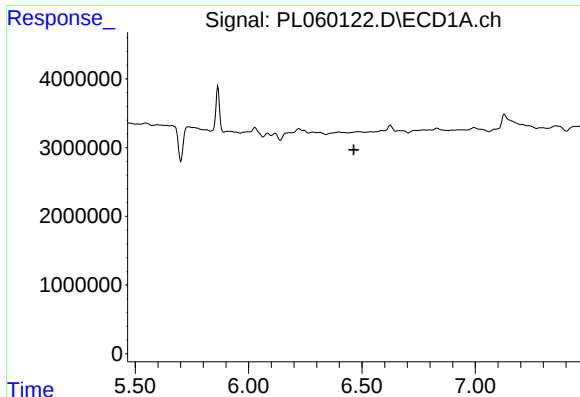

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3-D

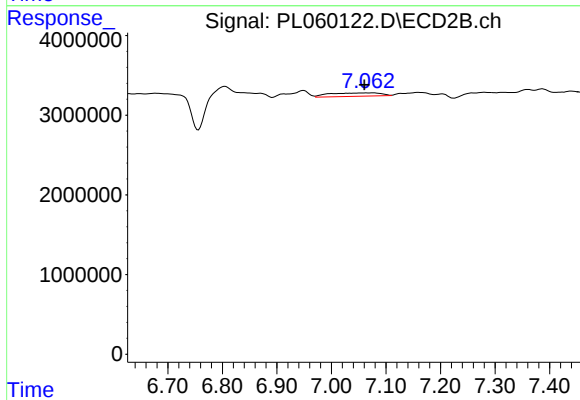


#18 Endrin aldehyde

R.T.: 7.063 min
Delta R.T.: 0.003 min
Response: 2848508
Conc: 1.31 ng/ml

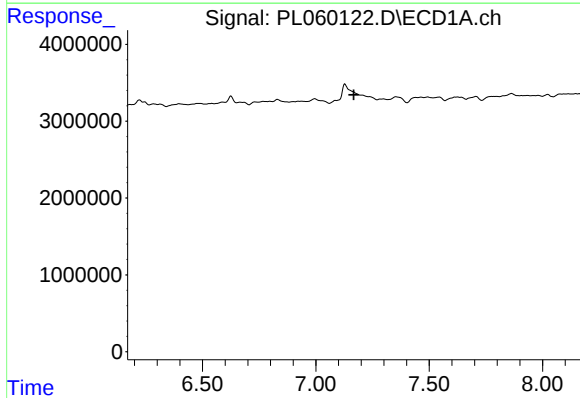


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.168 min
Response: 0
Conc: N.D.

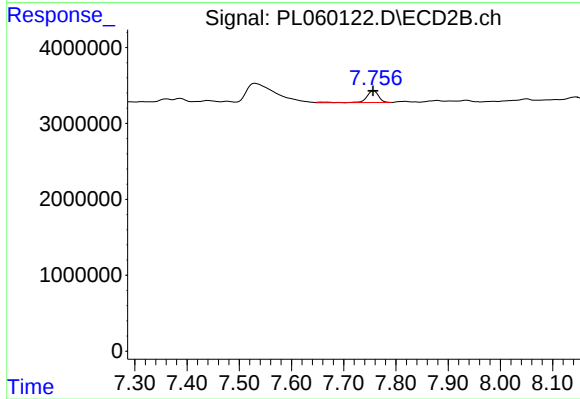

#21 Endrin ketone


R.T.: 7.758 min
Delta R.T.: 0.001 min
Response: 2535210
Conc: 0.98 ng/ml

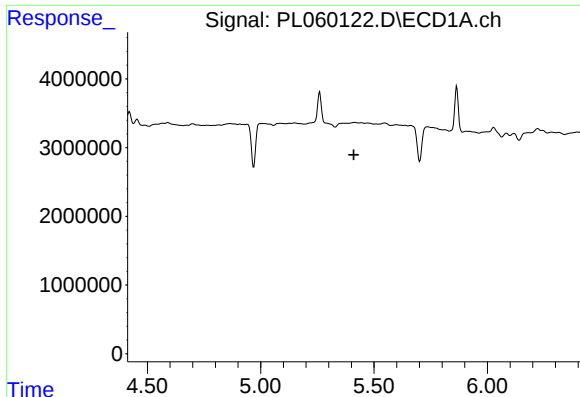

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3-D

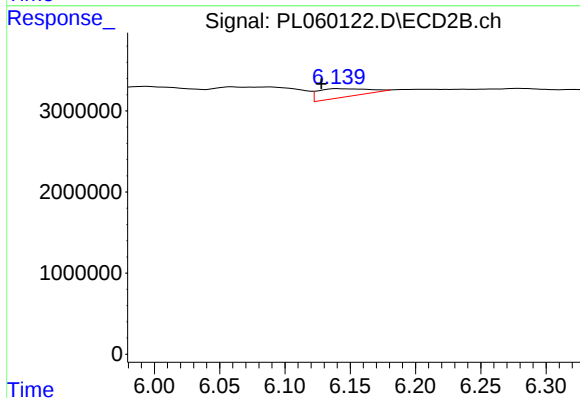


#25 Chlordane-3

R.T.: 6.141 min
Delta R.T.: 0.013 min
Response: 2727346
Conc: 7.05 ng/ml

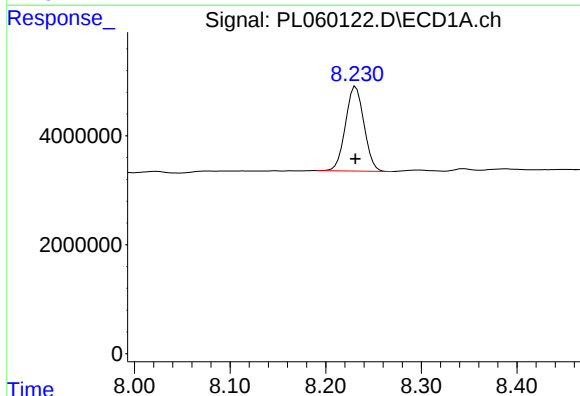

#28 Decachlorobiphenyl

R.T.: 8.232 min
Delta R.T.: 0.000 min
Response: 20955343
Conc: 12.74 ng/ml

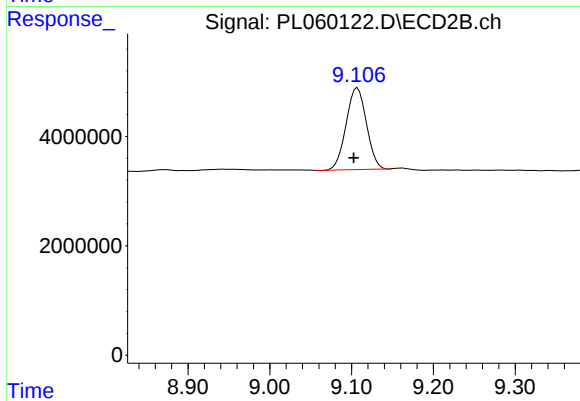

#28 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.004 min
Response: 25699807
Conc: 12.29 ng/ml