

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072320\
 Data File : PL060133.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2020 13:45
 Operator : DD\AJ
 Sample : L3380-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 02:00:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.013	18059977	23488775	9.337	8.863
28)	SA Decachlor...	8.224	9.099	33332050	32630271	20.261	15.602
Target Compounds							
10)	B gamma-Chl...	5.431f	0.000	399883	0	0.220	N.D. #
11)	B alpha-Chl...	0.000	6.201	0	2255226	N.D.	0.789 #
12)	B 4,4'-DDE	0.000	6.356	0	1388195	N.D.	0.519 #
14)	MA Endrin	0.000	6.704f	0	1088315	N.D.	0.511 #
17)	MA 4,4'-DDT	6.386	7.147	922758	1026325	0.710	0.521 #
18)	B Endrin al...	0.000	7.066	0	313932	N.D.	0.145 #
25)	Chlordane-3	5.431f	0.000	399883	0	2.365	N.D. #
26)	Chlordane-4	0.000	6.201	0	2255226	N.D.	4.872 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072320\
Data File : PL060133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2020 13:45
Operator : DD\AJ
Sample : L3380-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VNJ-242

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 02:00:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

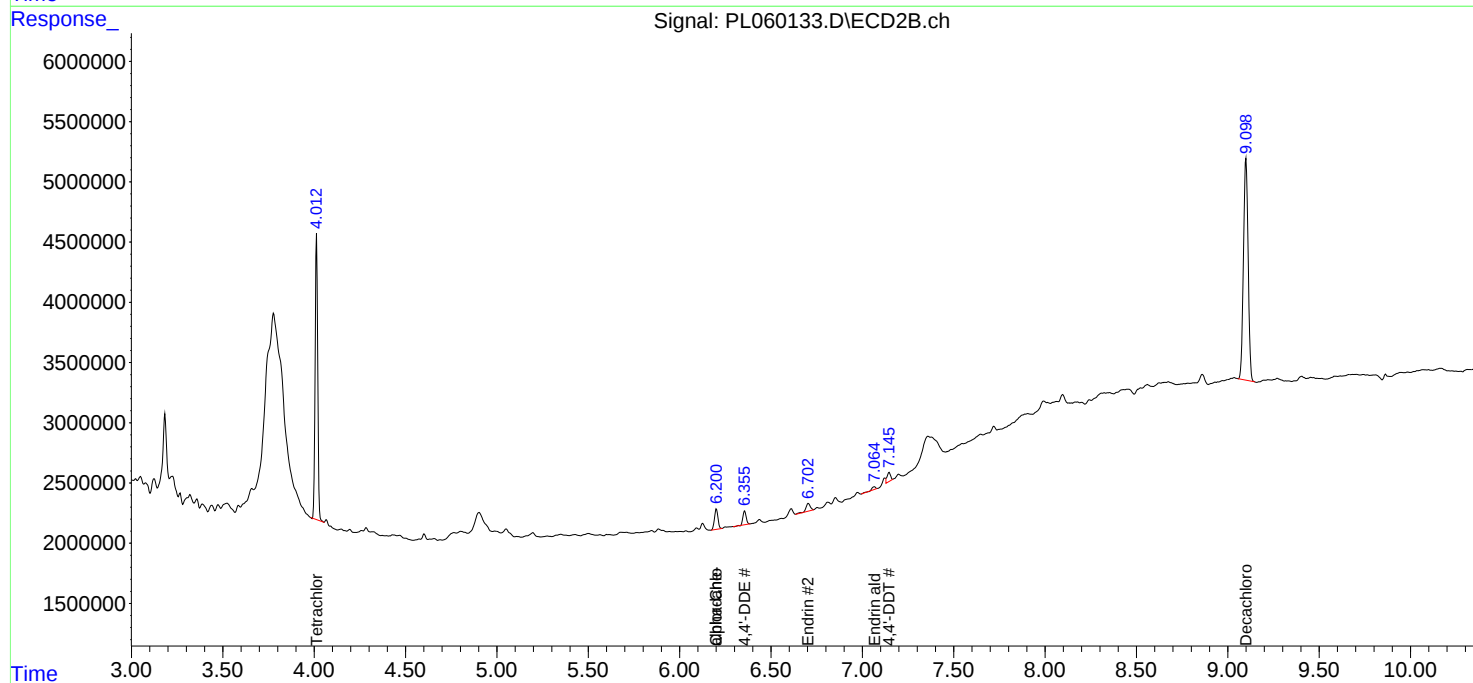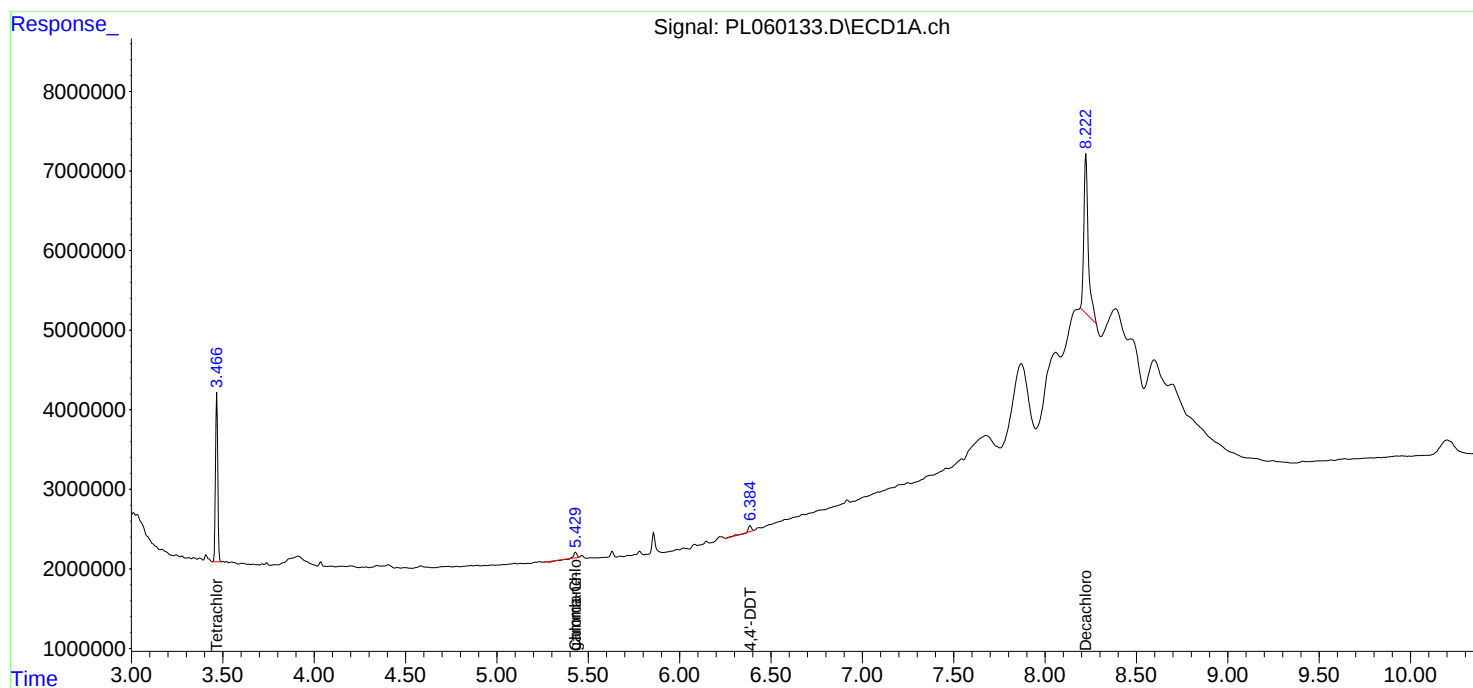


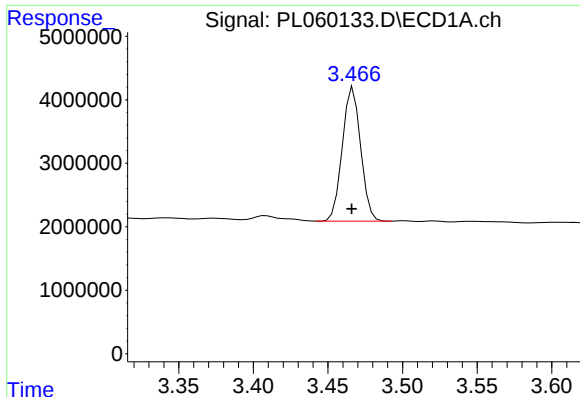

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 18059977
Conc: 9.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-242

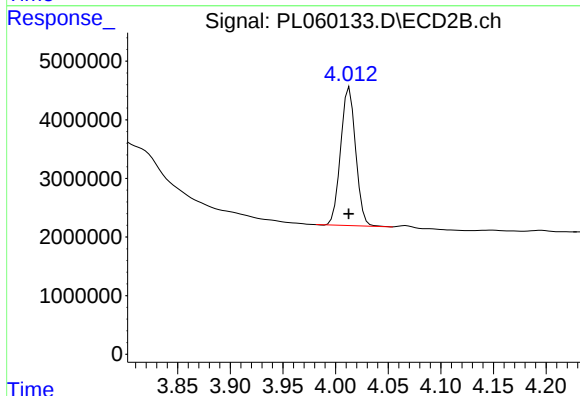


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 23488775
Conc: 8.86 ng/ml

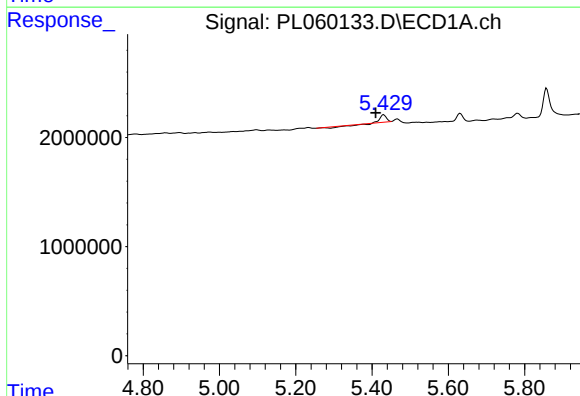


#10 gamma-Chlordane

R.T.: 5.431 min
Delta R.T.: 0.021 min
Response: 399883
Conc: 0.22 ng/ml

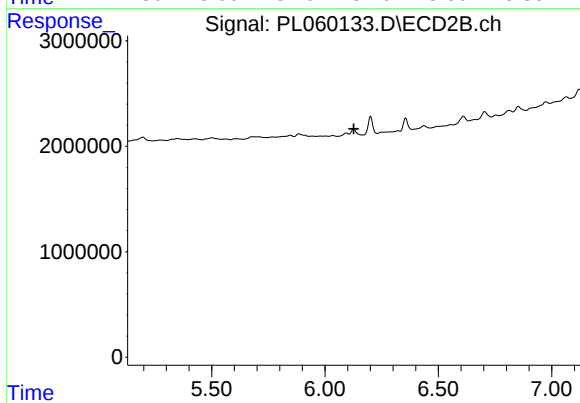

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.127 min
Response: 0
Conc: N.D.

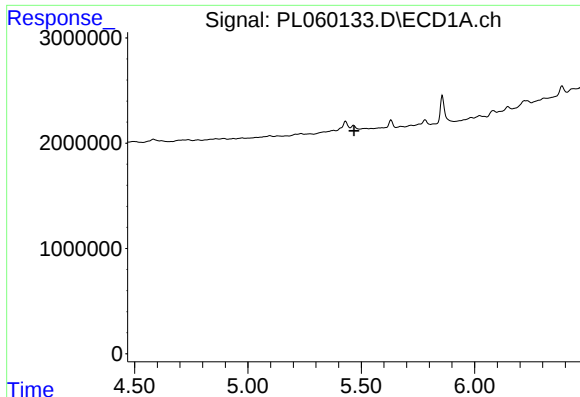

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VNJ-242

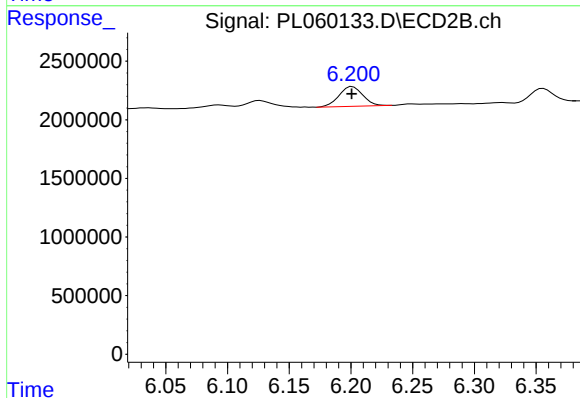


#11 alpha-Chlordane

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 2255226
Conc: 0.79 ng/ml

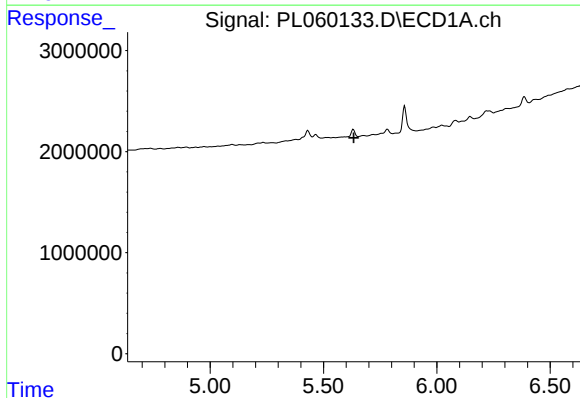


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.634 min
Response: 0
Conc: N.D.

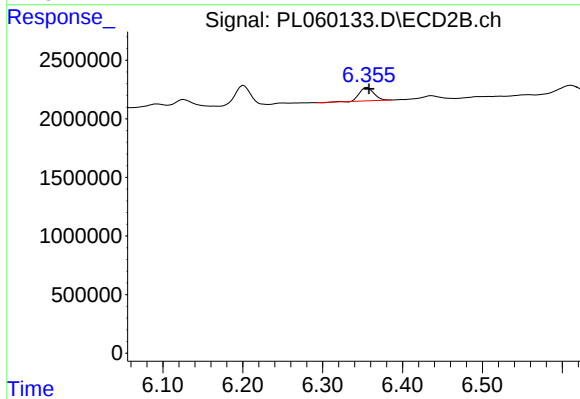

#12 4,4'-DDE


R.T.: 6.356 min
Delta R.T.: -0.002 min
Response: 1388195
Conc: 0.52 ng/ml

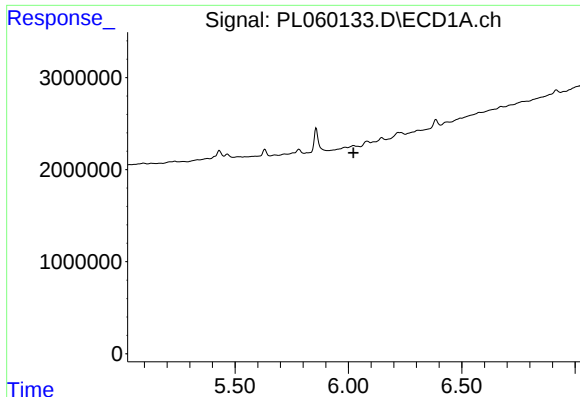

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VNJ-242

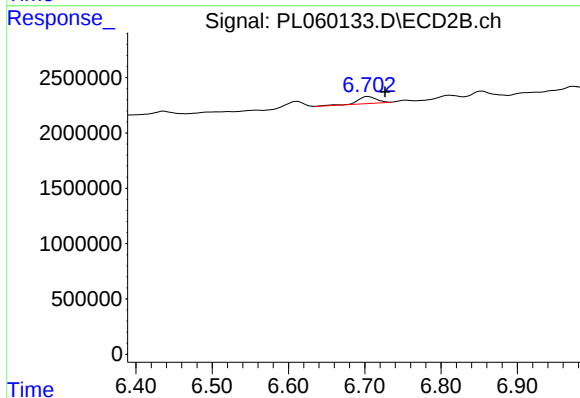


#14 Endrin

R.T.: 6.704 min
Delta R.T.: -0.022 min
Response: 1088315
Conc: 0.51 ng/ml

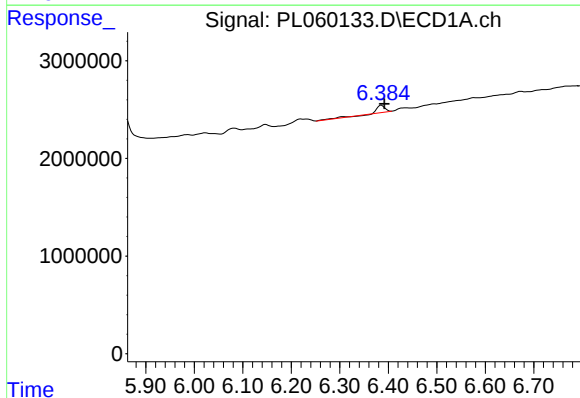


#17 4,4'-DDT

R.T.: 6.386 min
Delta R.T.: -0.006 min
Response: 922758
Conc: 0.71 ng/ml

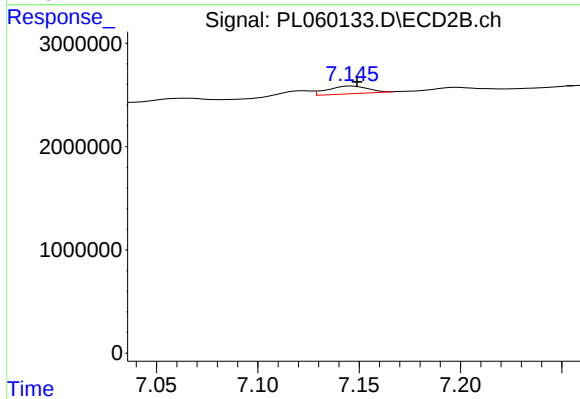

#17 4,4'-DDT


R.T.: 7.147 min
Delta R.T.: -0.002 min
Response: 1026325
Conc: 0.52 ng/ml

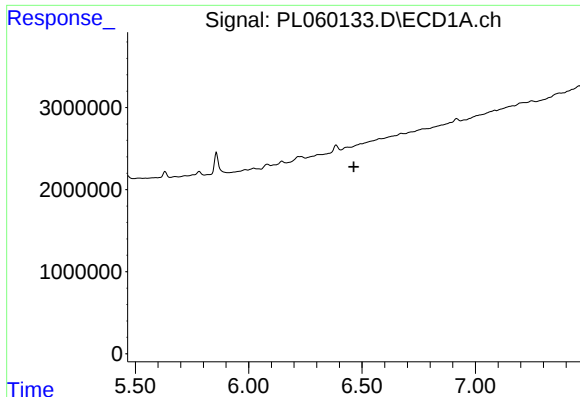

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VNJ-242

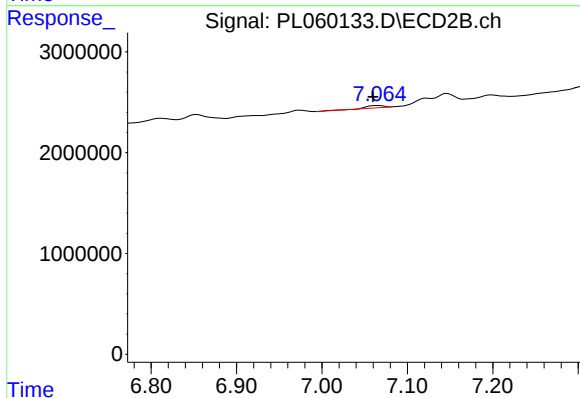


#18 Endrin aldehyde

R.T.: 7.066 min
Delta R.T.: 0.005 min
Response: 313932
Conc: 0.14 ng/ml

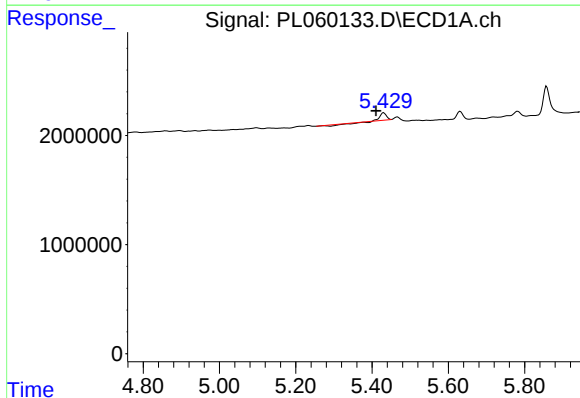


#25 Chlordane-3

R.T.: 5.431 min
Delta R.T.: 0.020 min
Response: 399883
Conc: 2.36 ng/ml

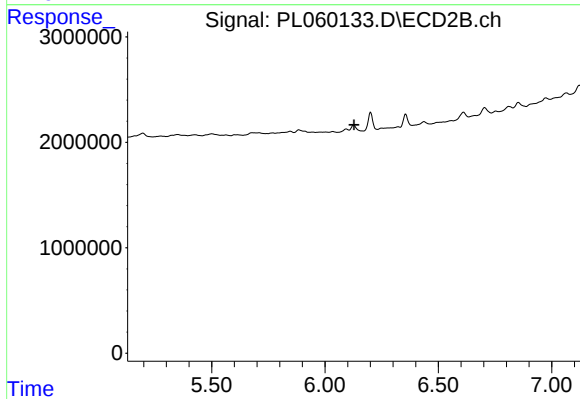

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.128 min
Response: 0
Conc: N.D.

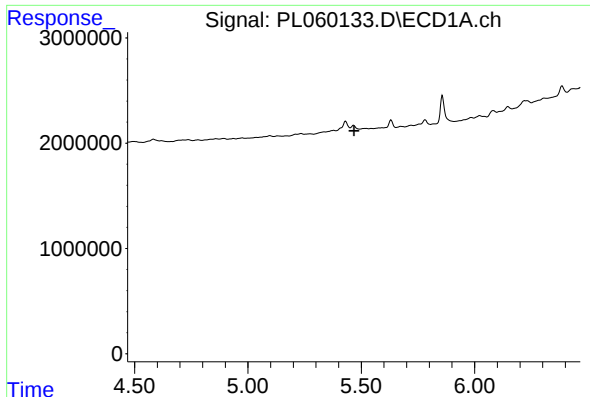

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VNJ-242

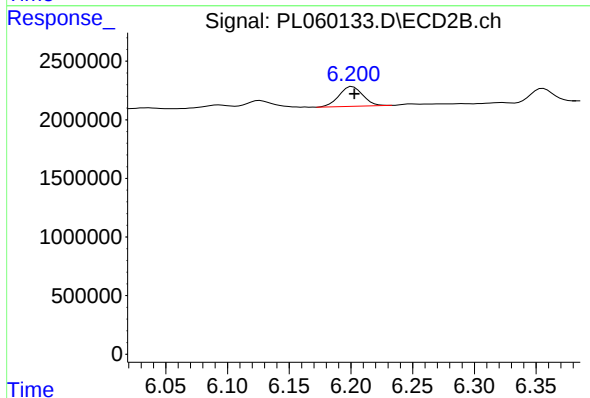


#26 Chlordane-4

R.T.: 6.201 min
Delta R.T.: -0.002 min
Response: 2255226
Conc: 4.87 ng/ml

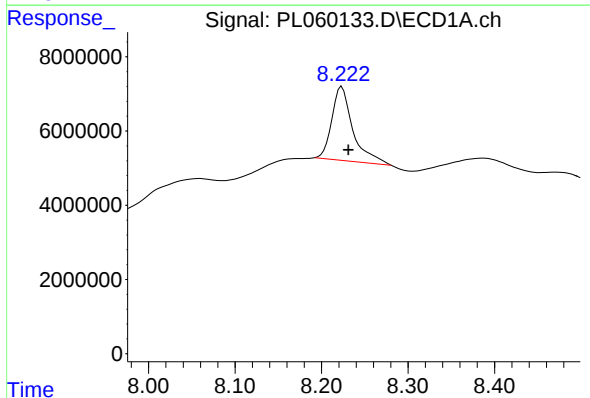

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.008 min
Response: 33332050
Conc: 20.26 ng/ml

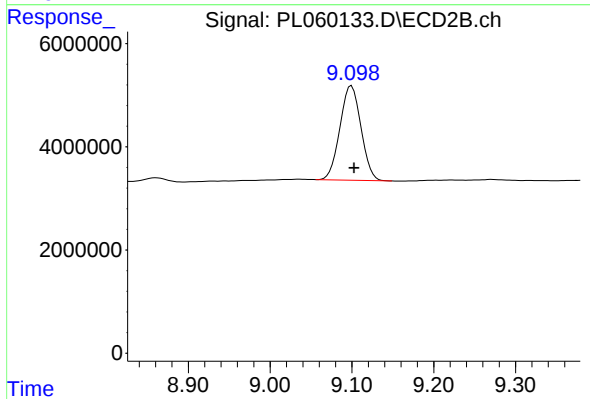

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.003 min
Response: 32630271
Conc: 15.60 ng/ml