

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072320\
 Data File : PL060138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2020 15:10
 Operator : DD\AJ
 Sample : L3381-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 339-GRID-B3-B4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 02:01:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	29549449	40001218	15.277	15.094
28)	SA Decachlor...	8.224	9.100	21592364	27952023	13.125	13.365
Target Compounds							
4)	MA Heptachlor	0.000	5.199	0	717688	N.D.	0.213 #
13)	MA Dieldrin	0.000	6.496	0	2878223	N.D.	1.040 #
15)	B Endosulfa...	0.000	6.920f	0	1689909	N.D.	0.673 #
16)	A 4,4'-DDD	0.000	6.852	0	6881239	N.D.	2.998 #
17)	MA 4,4'-DDT	6.382	0.000	4747402	0	3.651	N.D. #
18)	B Endrin al...	6.477	0.000	1608380	0	1.127	N.D. #
19)	B Endosulfa...	6.671	0.000	3563780	0	2.168	N.D. #
20)	A Methoxychlor	6.916f	0.000	1917158	0	2.563	N.D. #
21)	B Endrin ke...	7.192f	0.000	1078708	0	0.575	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072320\
Data File : PL060138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2020 15:10
Operator : DD\AJ
Sample : L3381-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
339-GRID-B3-B4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 02:01:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

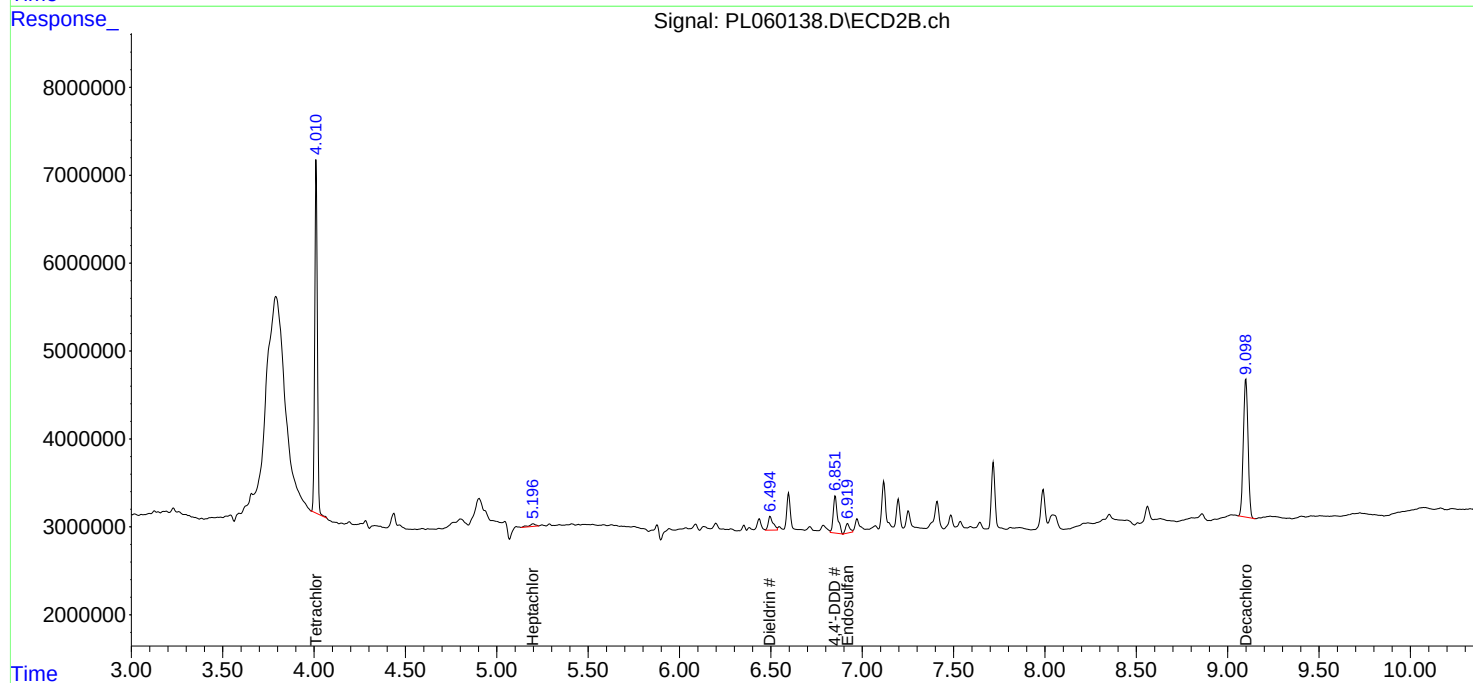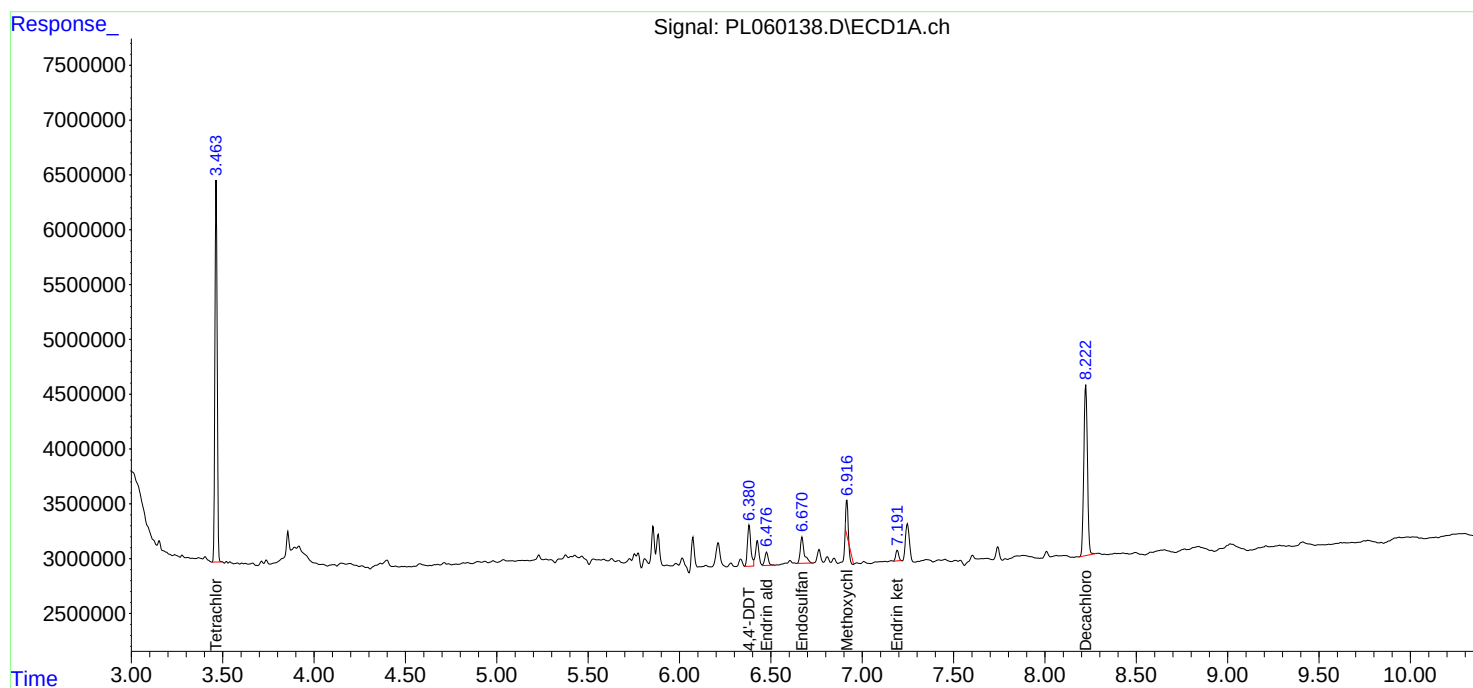


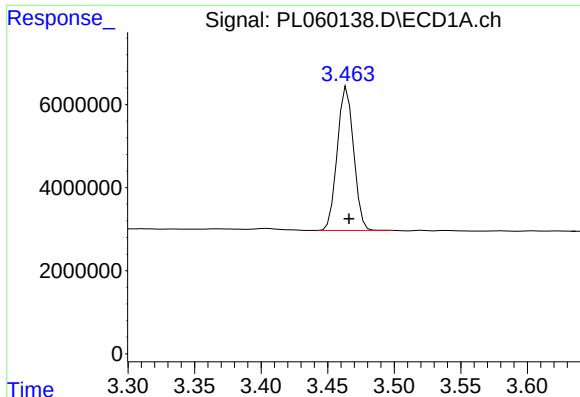

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: -0.001 min
Response: 29549449
Conc: 15.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
339-GRID-B3-B4

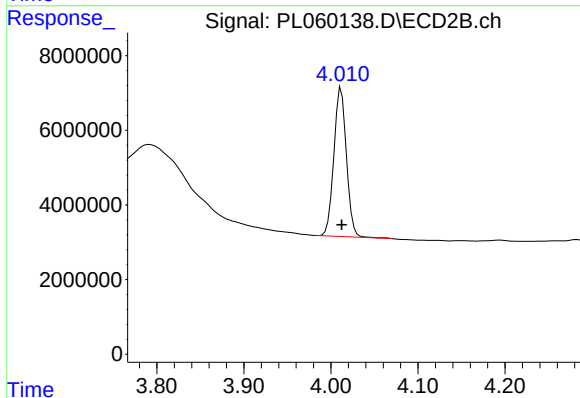


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 40001218
Conc: 15.09 ng/ml

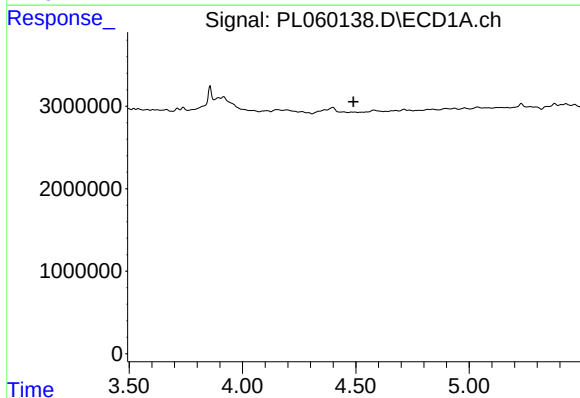


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

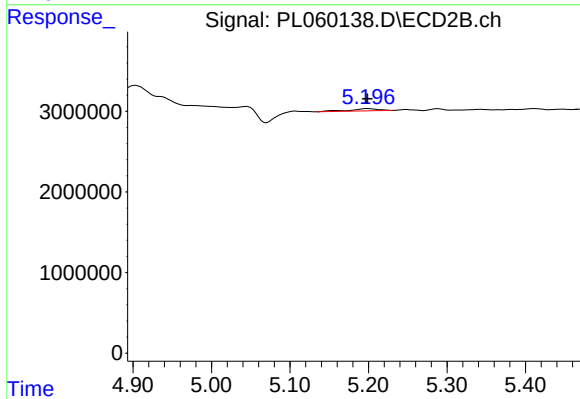

#4 Heptachlor


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 717688
Conc: 0.21 ng/ml

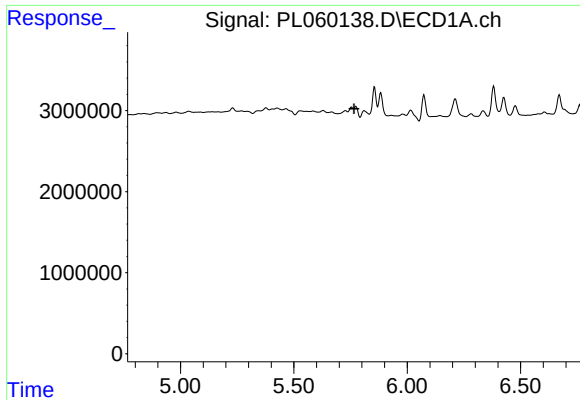

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
339-GRID-B3-B4

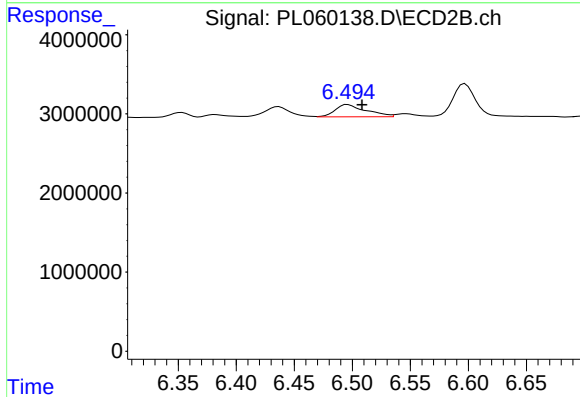


#13 Dieldrin

R.T.: 6.496 min
Delta R.T.: -0.012 min
Response: 2878223
Conc: 1.04 ng/ml

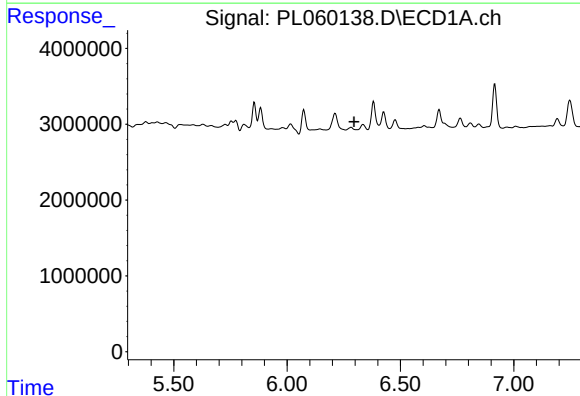


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.296 min
Response: 0
Conc: N.D.

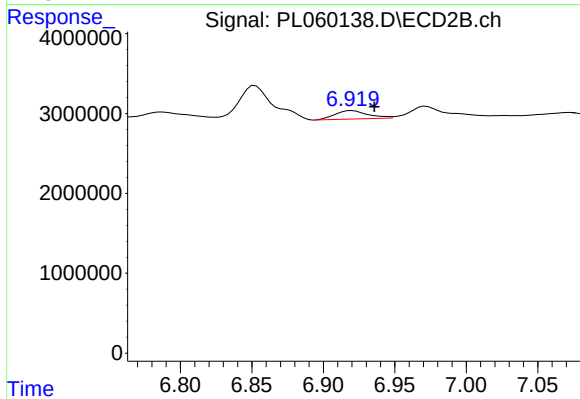

#15 Endosulfan II


R.T.: 6.920 min
Delta R.T.: -0.016 min
Response: 1689909
Conc: 0.67 ng/ml

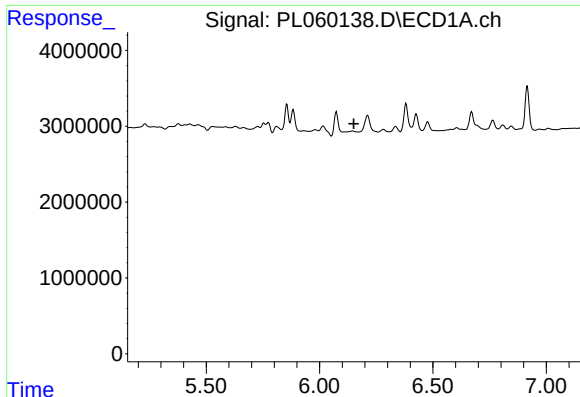

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
339-GRID-B3-B4

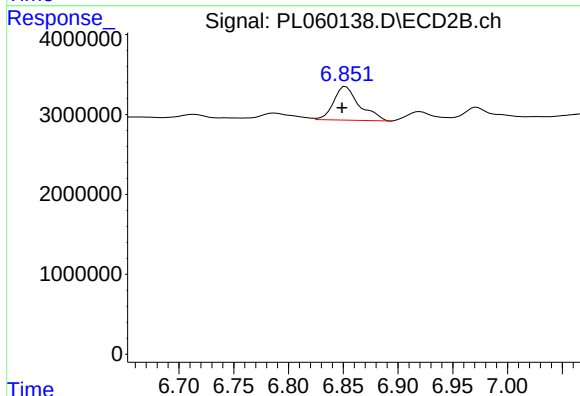


#16 4,4'-DDD

R.T.: 6.852 min
Delta R.T.: 0.004 min
Response: 6881239
Conc: 3.00 ng/ml

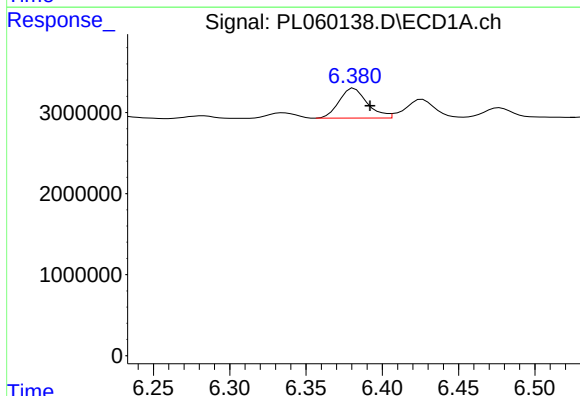


#17 4,4'-DDT

R.T.: 6.382 min
Delta R.T.: -0.010 min
Response: 4747402
Conc: 3.65 ng/ml

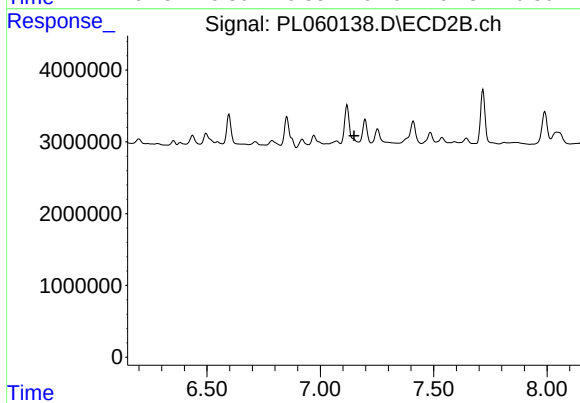

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.149 min
Response: 0
Conc: N.D.

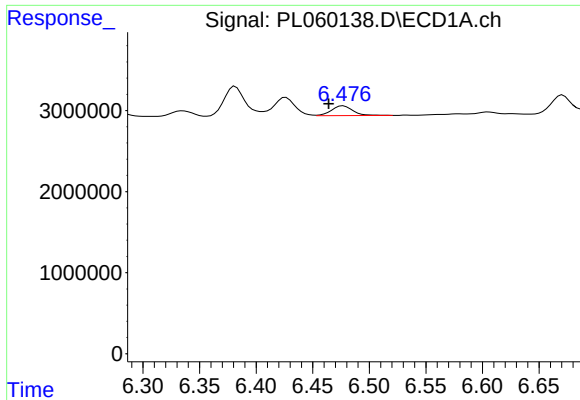

#18 Endrin aldehyde


R.T.: 6.477 min
Delta R.T.: 0.013 min
Response: 1608380
Conc: 1.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
339-GRID-B3-B4

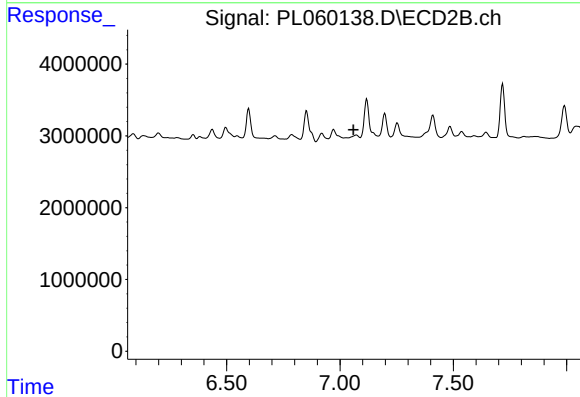


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

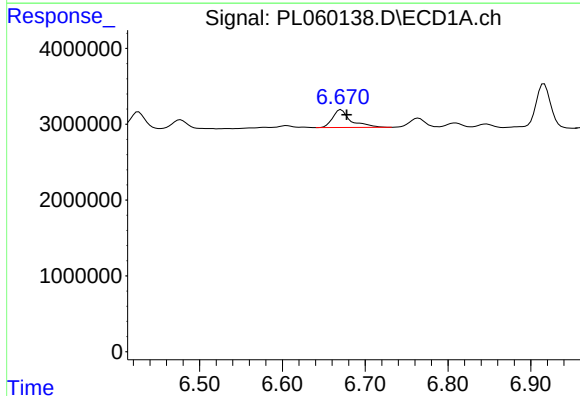


#19 Endosulfan Sulfate

R.T.: 6.671 min
Delta R.T.: -0.007 min
Response: 3563780
Conc: 2.17 ng/ml

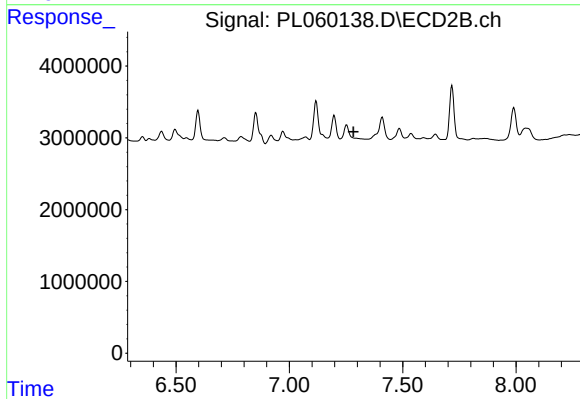

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.284 min
Response: 0
Conc: N.D.

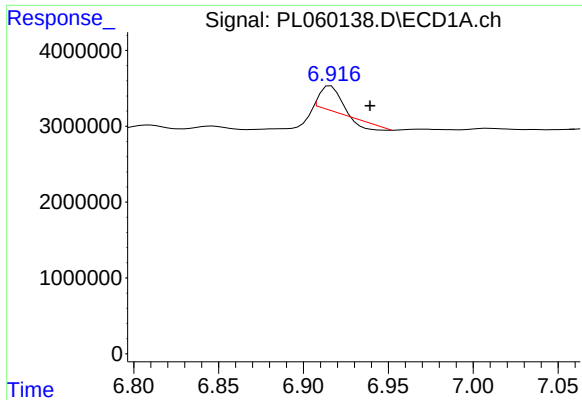

#20 Methoxychlor


R.T.: 6.916 min
Delta R.T.: -0.023 min
Response: 1917158
Conc: 2.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
339-GRID-B3-B4

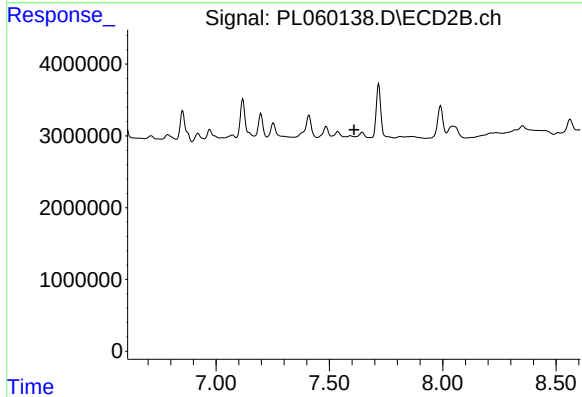


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.609 min
Response: 0
Conc: N.D.

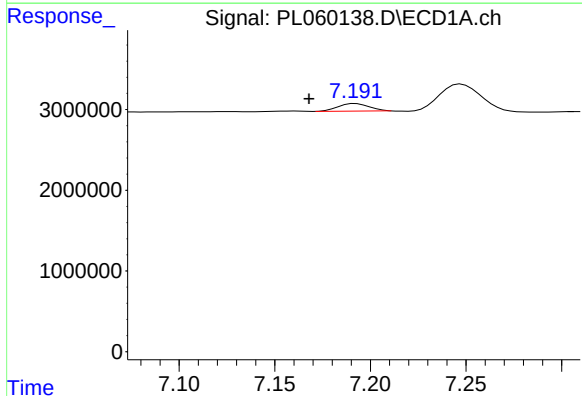


#21 Endrin ketone

R.T.: 7.192 min
Delta R.T.: 0.024 min
Response: 1078708
Conc: 0.57 ng/ml

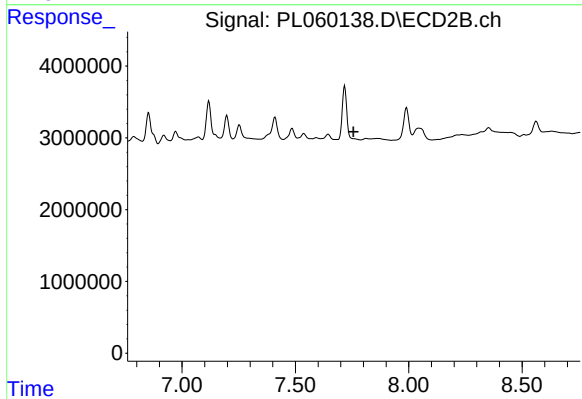

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.756 min
Response: 0
Conc: N.D.

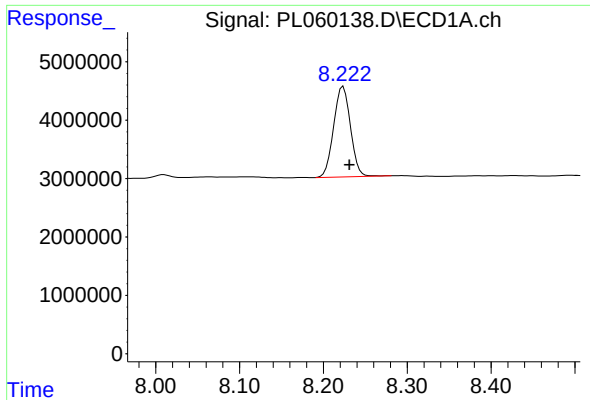

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.007 min
Response: 21592364
Conc: 13.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
339-GRID-B3-B4

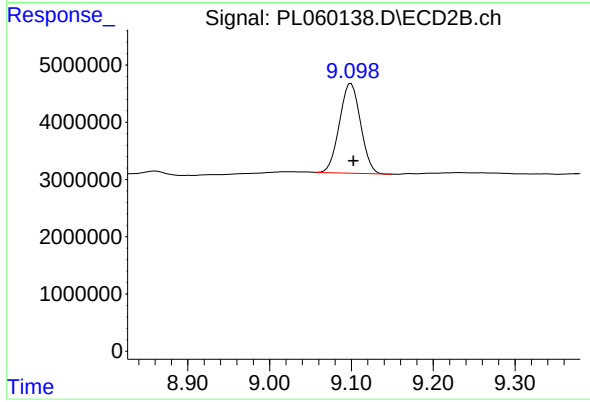

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: -0.003 min
Response: 27952023
Conc: 13.37 ng/ml