

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072320\
 Data File : PL060145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2020 16:53
 Operator : DD\AJ
 Sample : PB130432BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB130432BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 02:28:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	42909411	58433212	22.184	22.049
28)	SA Decachlor...	8.224	9.099	31610726	41662185	19.215	19.921
Target Compounds							
10)	B gamma-Chl...	0.000	6.097f	0	6150778	N.D.	2.148 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072320\
Data File : PL060145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2020 16:53
Operator : DD\AJ
Sample : PB130432BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB130432BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 02:28:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

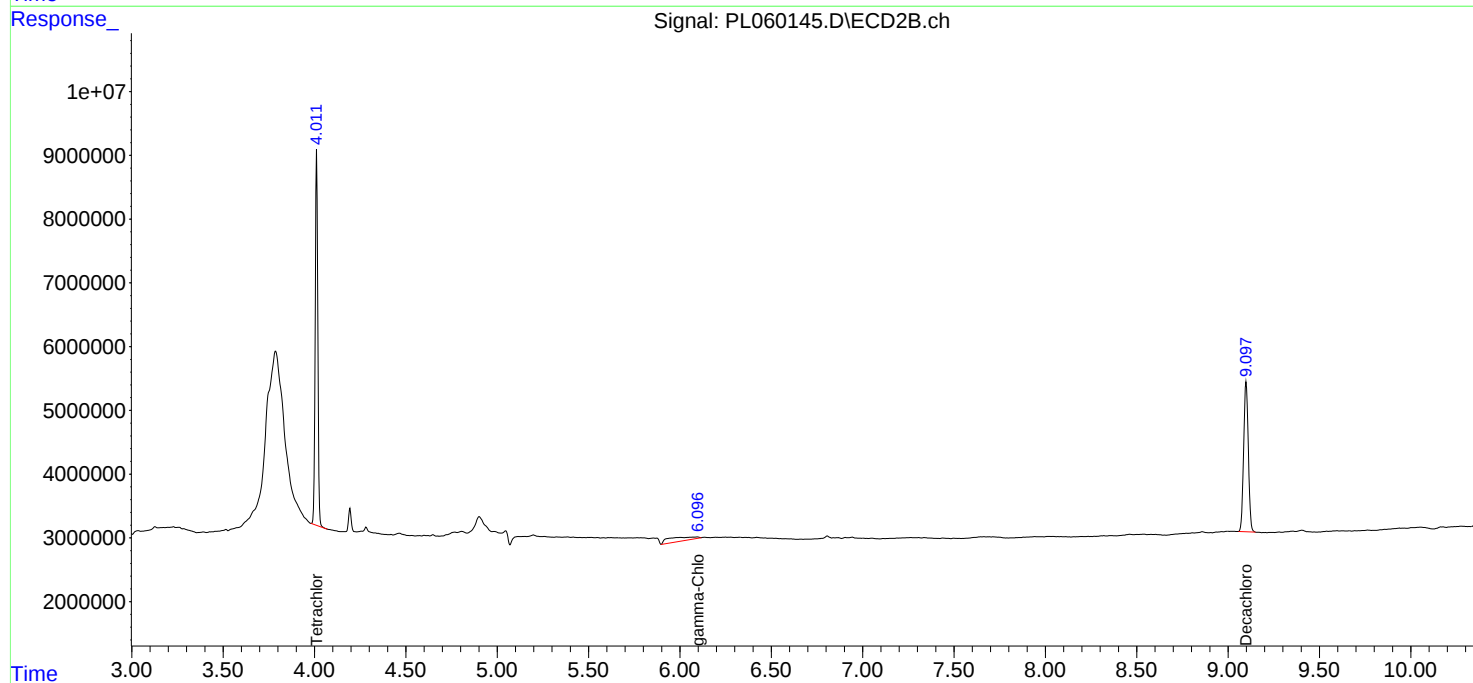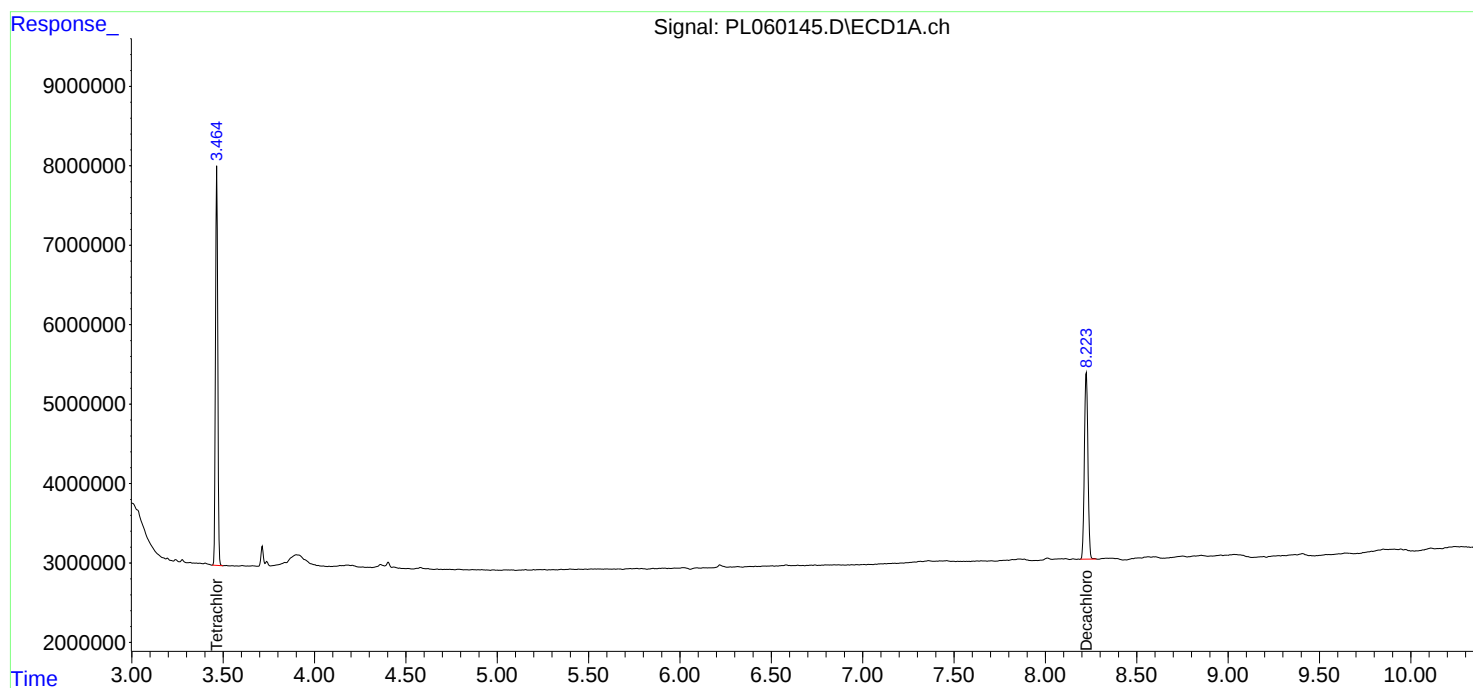


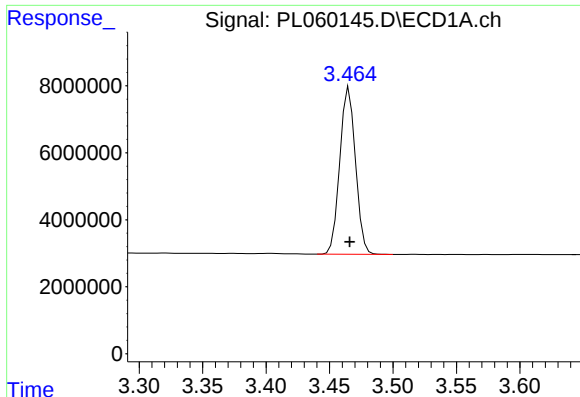

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 42909411
Conc: 22.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB130432BL

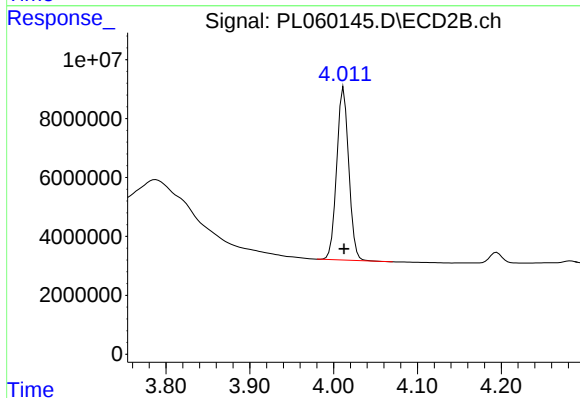


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 58433212
Conc: 22.05 ng/ml

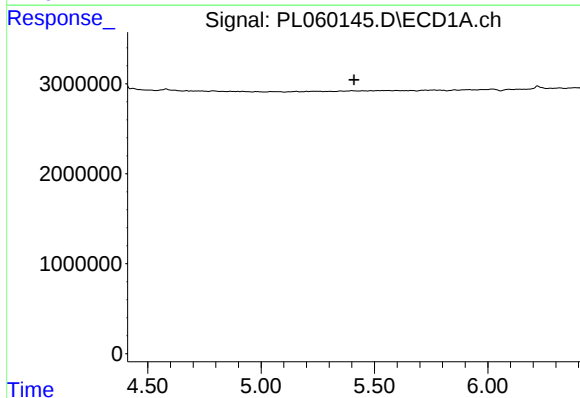


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.410 min
Response: 0
Conc: N.D.

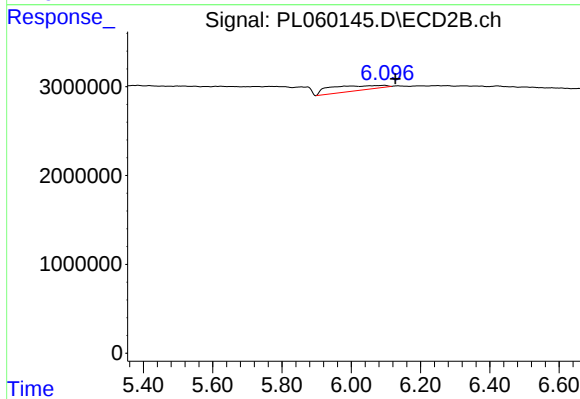

#10 gamma-Chlordane


R.T.: 6.097 min
Delta R.T.: -0.030 min
Response: 6150778
Conc: 2.15 ng/ml

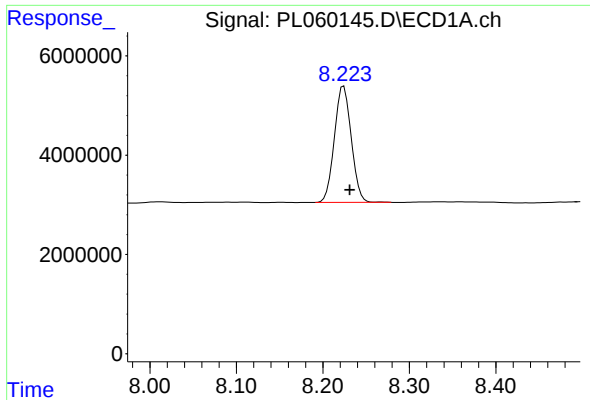

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.007 min
Response: 31610726
Conc: 19.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB130432BL

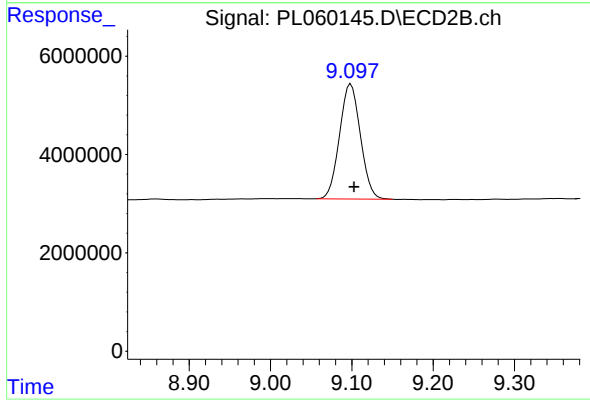

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.004 min
Response: 41662185
Conc: 19.92 ng/ml